
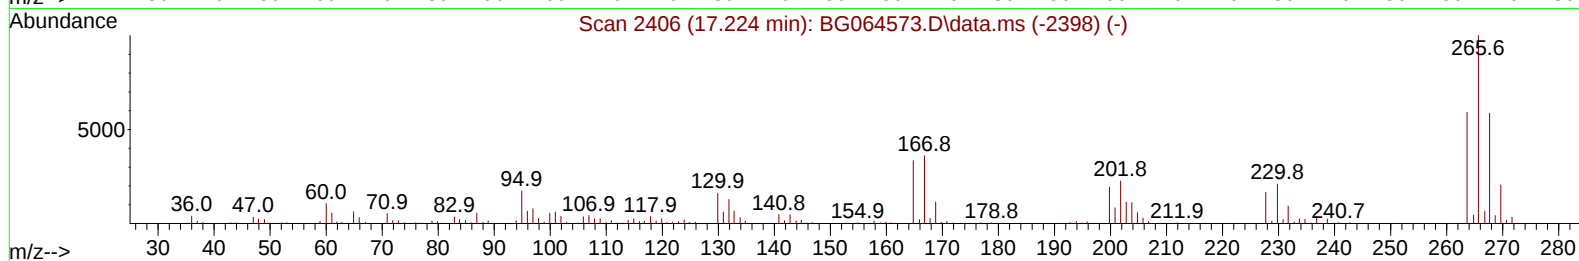
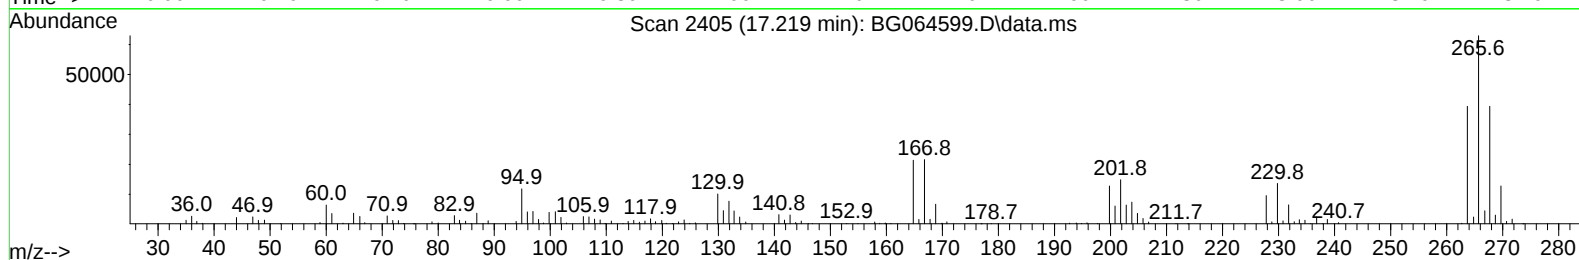


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102825\
Data File : BG064599.D
Acq On : 28 Oct 2025 13:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 13:46:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 16:40:26 2025
Response via : Initial Calibration

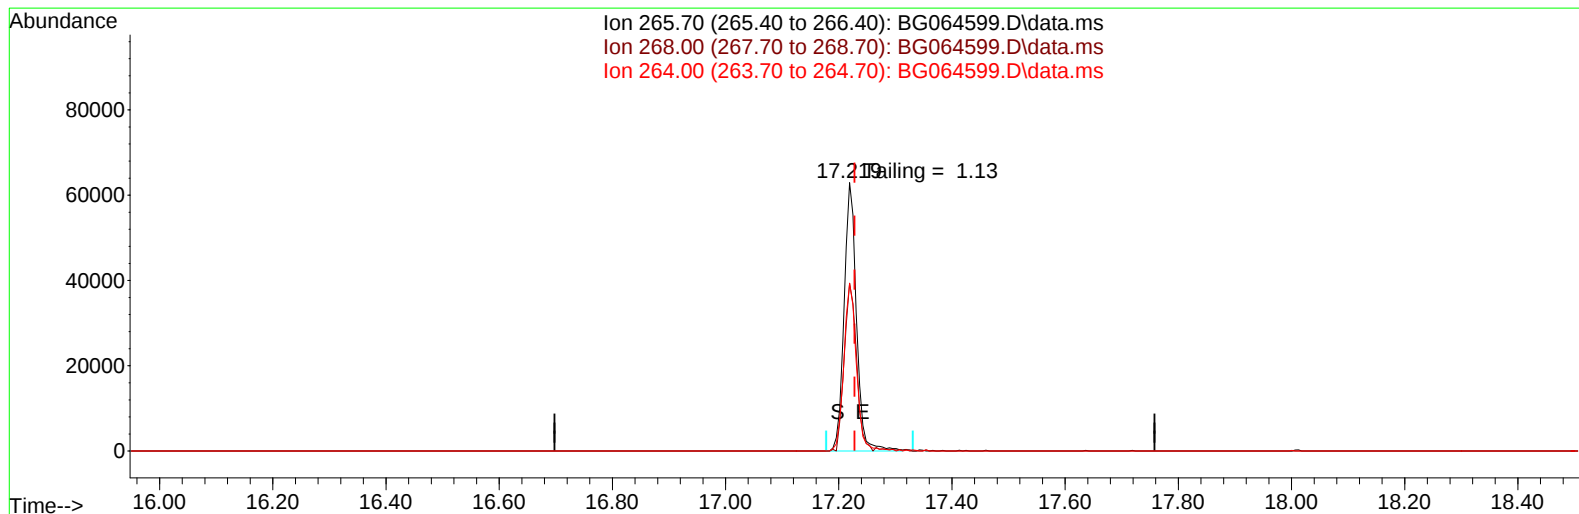

TIC: BG064599.D\data.ms

(70) Pentachlorophenol (C)




17.219min (-0.009) 17647.50 ng

response 95812

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	67.39
264.00	59.10	62.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102825\
Data File : BG064599.D
Acq On : 28 Oct 2025 13:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 13:46:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 16:40:26 2025
Response via : Initial Calibration

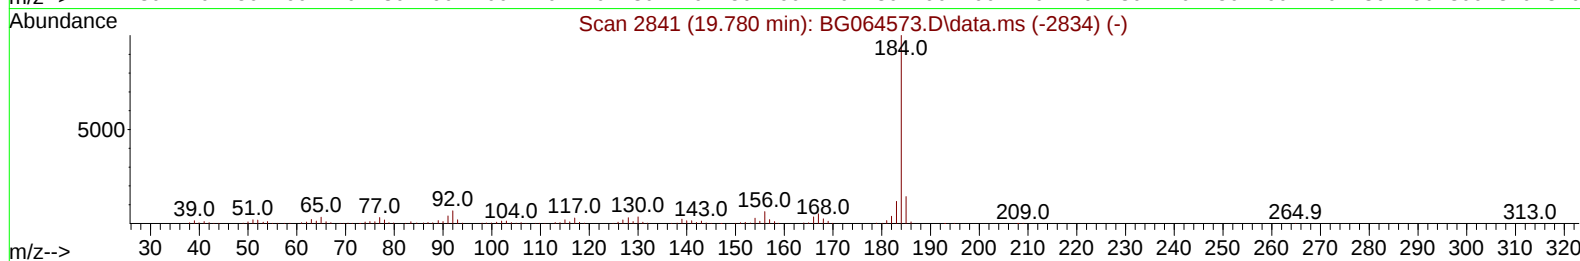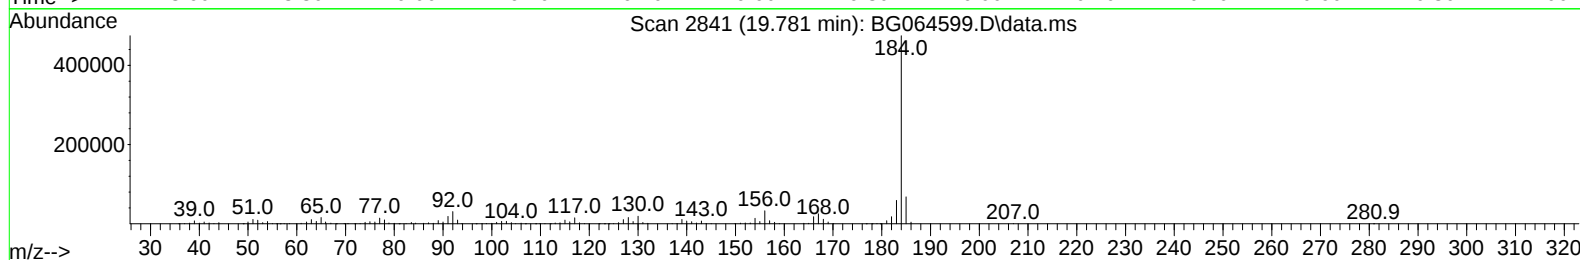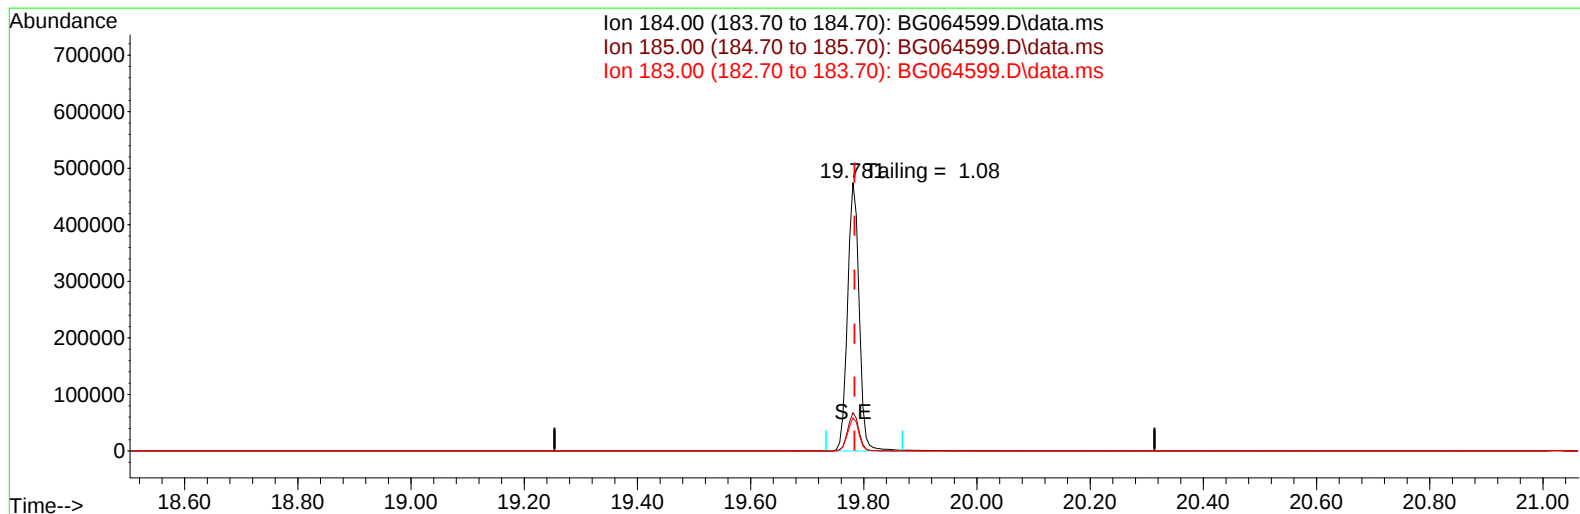

TIC: BG064599.D\data.ms

(77) Benzidine

19.781min (-0.003) 0.00 ng

response 671639

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.33
183.00	11.80	12.43
0.00	0.00	0.00