

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102825\
 Data File : BG064614.D
 Acq On : 28 Oct 2025 23:20
 Operator : RC/JU
 Sample : Q3460-17 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 WC-5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG064614.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.201	13	19	27	rBV4	11347	26704	3.00%	0.440%
2	3.278	27	32	45	rVB	80979	156899	17.63%	2.586%
3	3.818	118	124	138	rBV	57603	107472	12.08%	1.772%
4	4.335	204	212	218	rBV3	8355	16081	1.81%	0.265%
5	5.745	445	452	460	rVB	104504	177101	19.90%	2.919%
6	7.343	717	724	733	rBV	104816	186933	21.01%	3.081%
7	8.219	866	873	880	rBV	137578	242873	27.30%	4.003%
8	9.376	1060	1070	1077	rBV	62966	105737	11.88%	1.743%
9	11.039	1346	1353	1362	rVB	200106	362250	40.71%	5.971%
10	13.466	1759	1766	1772	rBV	185285	279893	31.46%	4.614%
11	14.841	1992	2000	2007	rBV	392041	610202	68.58%	10.058%
12	16.180	2221	2228	2233	rBV	22956	33222	3.73%	0.548%
13	16.309	2245	2250	2260	rVB2	168601	255240	28.69%	4.207%
14	17.573	2458	2465	2471	rBV2	581209	889744	100.00%	14.666%
15	17.614	2471	2472	2479	rVB	15556	15999	1.80%	0.264%
16	18.448	2610	2614	2618	rBV2	20661	29467	3.31%	0.486%
17	18.636	2640	2646	2650	rBV6	6433	11261	1.27%	0.186%
18	19.611	2804	2812	2817	rBV	49043	71792	8.07%	1.183%
19	19.711	2824	2829	2833	rBV5	10084	13245	1.49%	0.218%
20	19.970	2864	2873	2881	rBV2	43906	85485	9.61%	1.409%
21	20.164	2898	2906	2912	rBV	349299	467808	52.58%	7.711%
22	20.458	2952	2956	2960	rVB6	8946	14143	1.59%	0.233%
23	20.563	2969	2974	2978	rVB8	6025	9051	1.02%	0.149%
24	20.610	2980	2982	2987	rVB6	8185	10047	1.13%	0.166%
25	21.468	3124	3128	3130	rBV5	7657	12092	1.36%	0.199%
26	21.733	3171	3173	3178	rVB5	8015	9559	1.07%	0.158%
27	21.850	3185	3193	3199	rBV	476741	867005	97.44%	14.292%
28	24.136	3575	3582	3588	rBV2	16857	47710	5.36%	0.786%
29	24.282	3603	3607	3613	rVB4	12589	22033	2.48%	0.363%
30	25.029	3728	3734	3739	rBV3	14882	31580	3.55%	0.521%
31	25.187	3751	3761	3771	rBV	286201	853185	95.89%	14.064%
32	27.937	4220	4229	4233	rBV8	16552	44763	5.03%	0.738%


Sum of corrected areas: 6066576

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102825\
Data File : BG064614.D
Acq On : 28 Oct 2025 23:20
Operator : RC/JU
Sample : Q3460-17 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WC-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

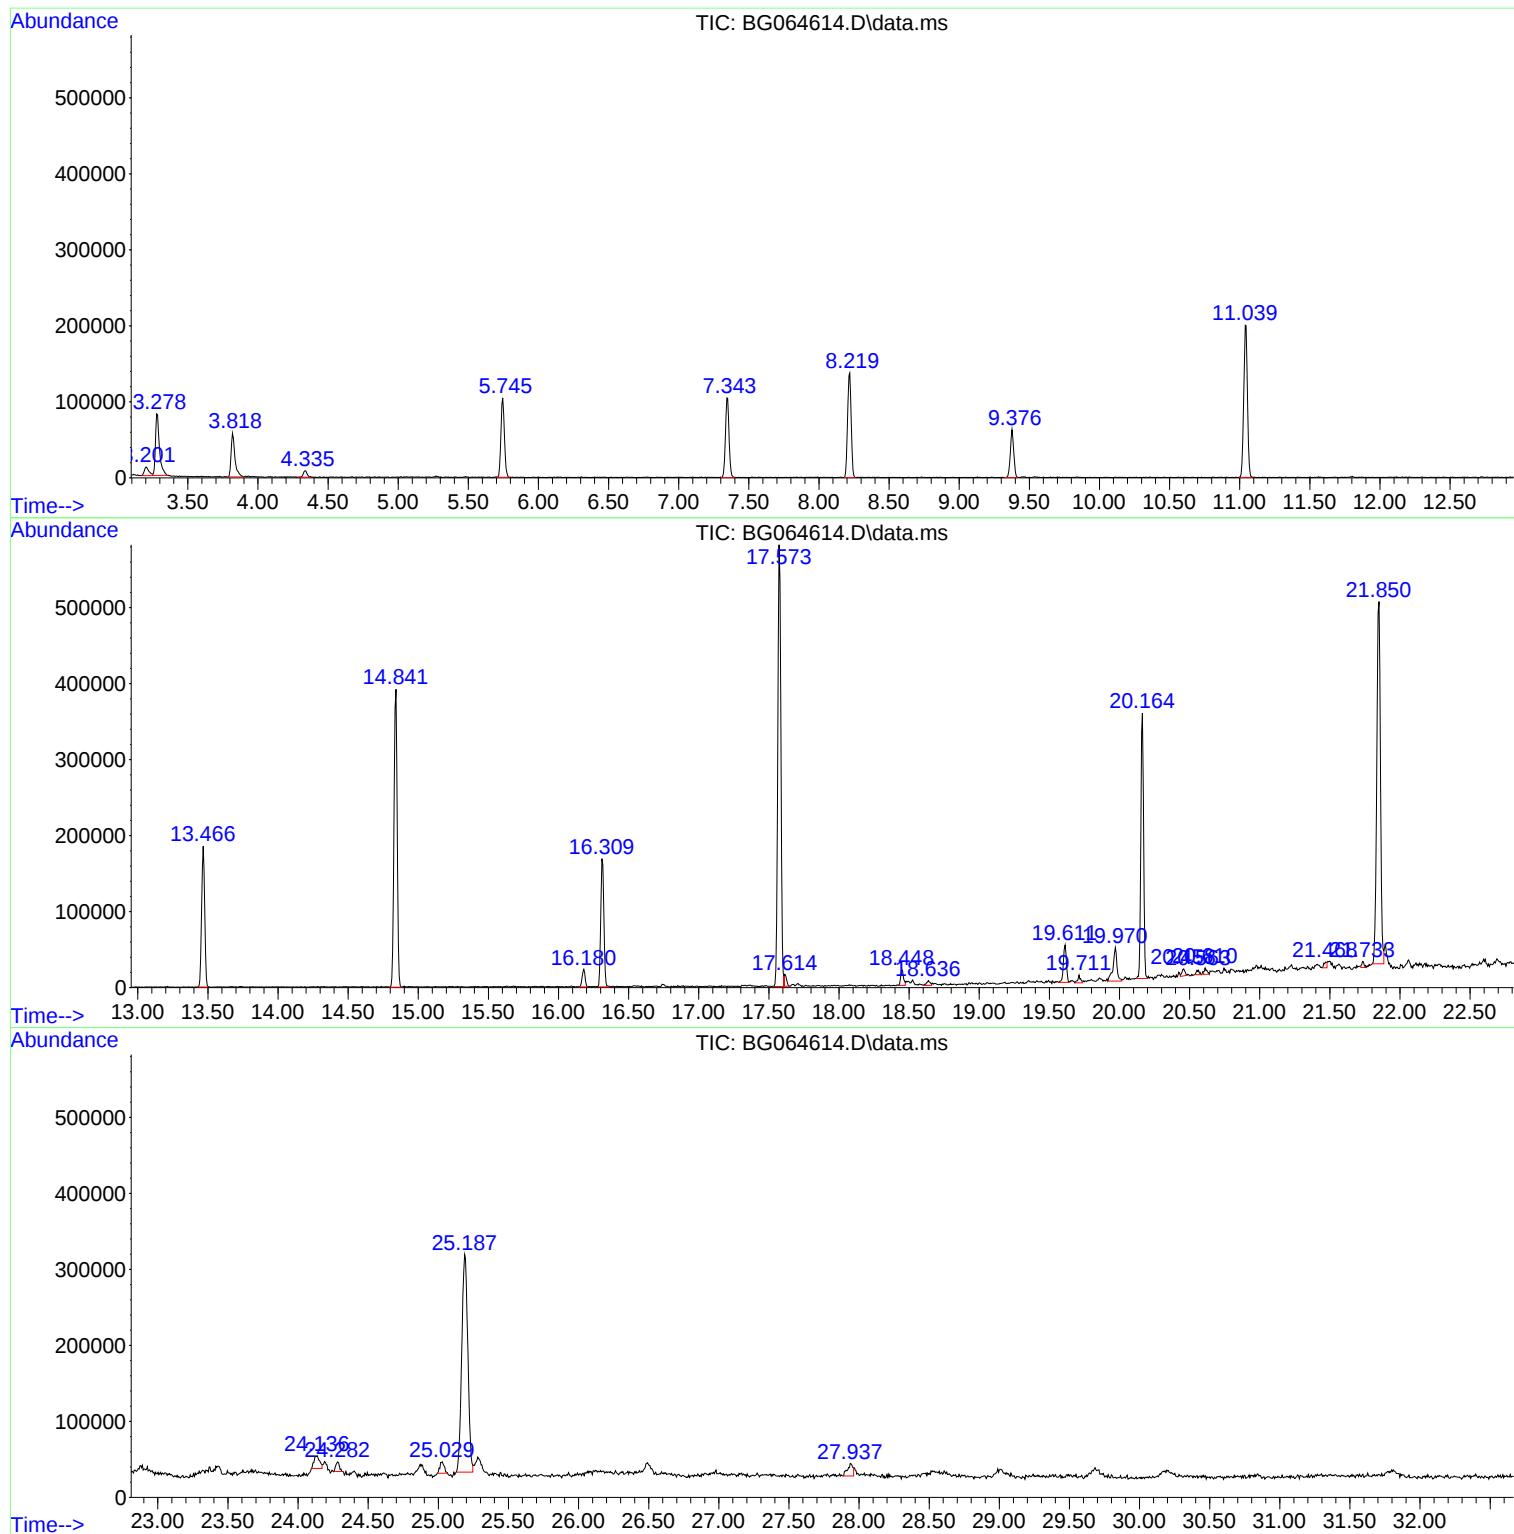

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102825\
Data File : BG064614.D
Acq On : 28 Oct 2025 23:20
Operator : RC/JU
Sample : Q3460-17 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WC-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102825\
Data File : BG064614.D
Acq On : 28 Oct 2025 23:20
Operator : RC/JU
Sample : Q3460-17 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WC-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc