
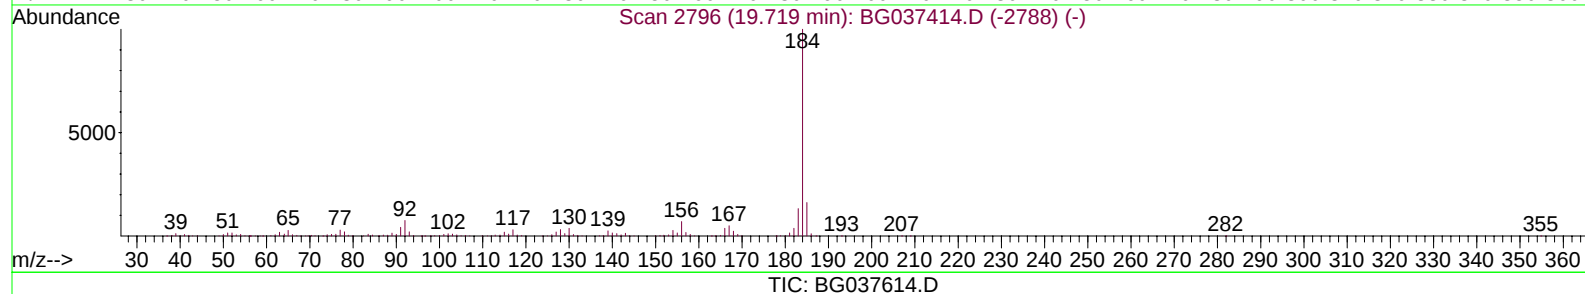
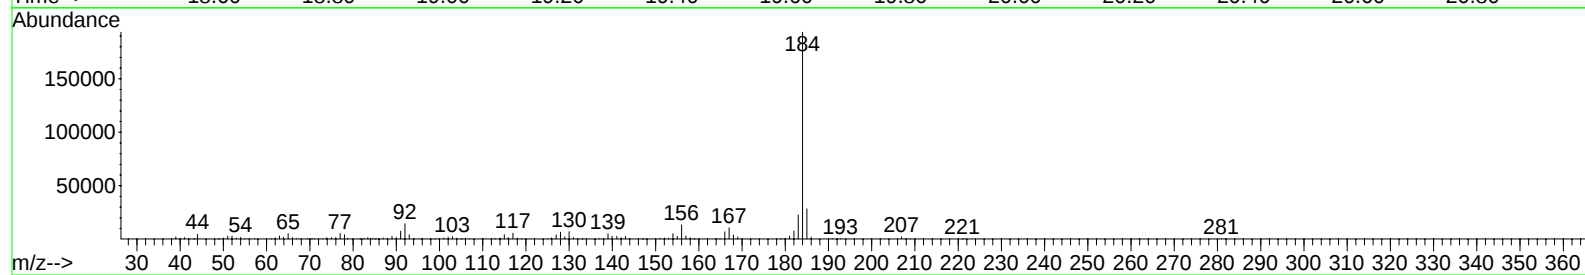


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG102918\
Data File : BG037614.D
Acq On : 29 Oct 2018 9:21
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 01 08:10:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

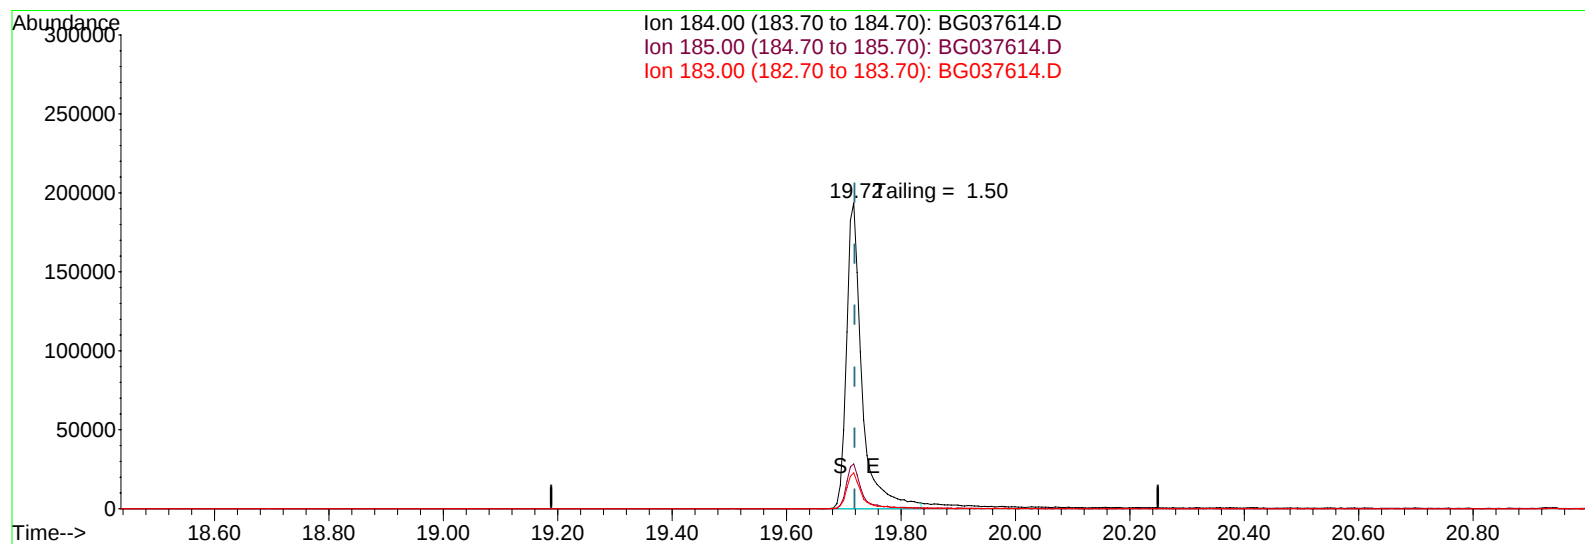

TIC: BG037614.D

(77) Benzidine




19.717min (-0.002) 65139.67ng

response 378751

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.63
183.00	12.70	11.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG102918\
Data File : BG037614.D
Acq On : 29 Oct 2018 9:21
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 01 08:10:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

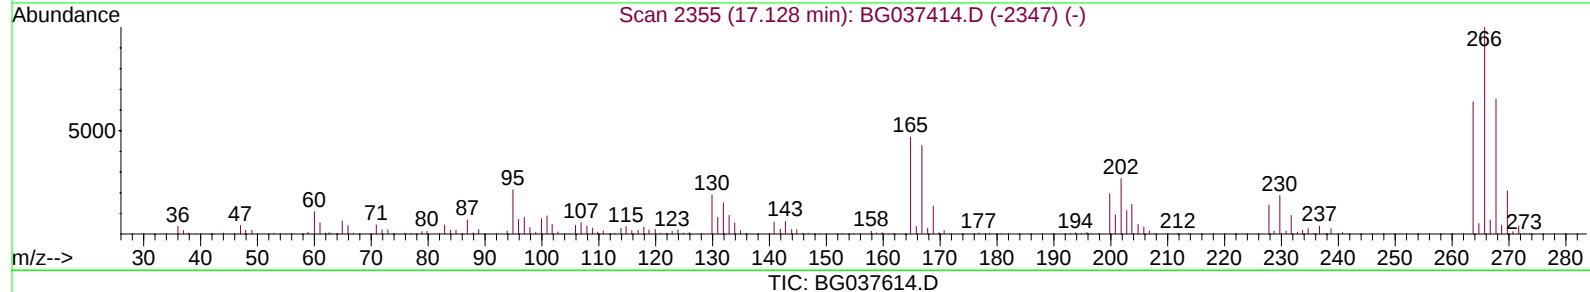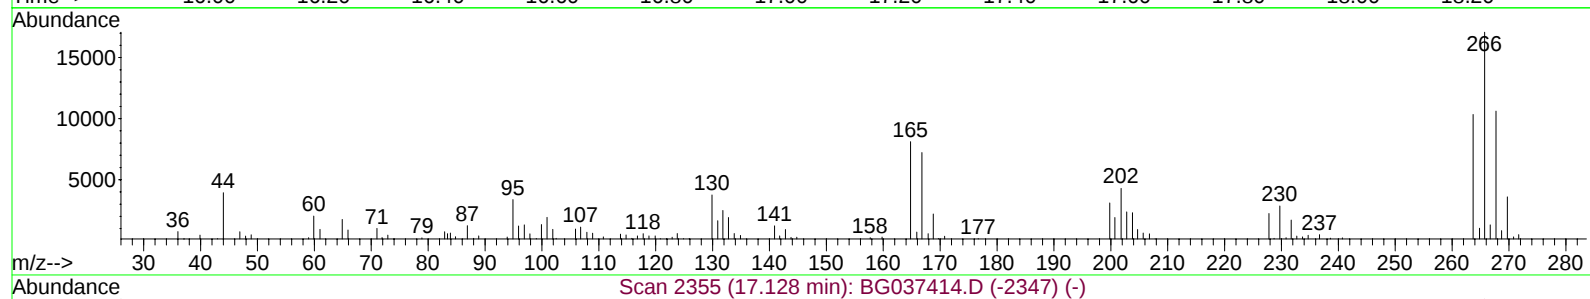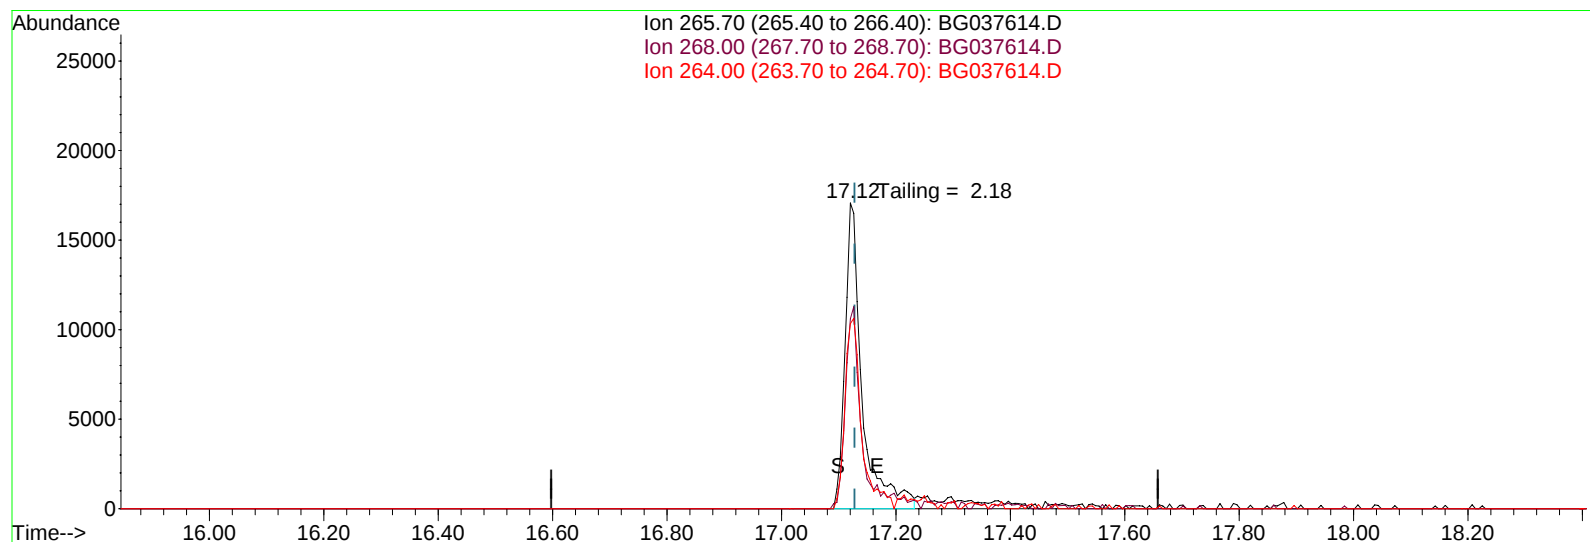

(70) Pentachlorophenol (C)

17.120min (-0.008) 83259.04ng

response 34276

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	67.03
264.00	73.60	60.57
0.00	0.00	0.00