
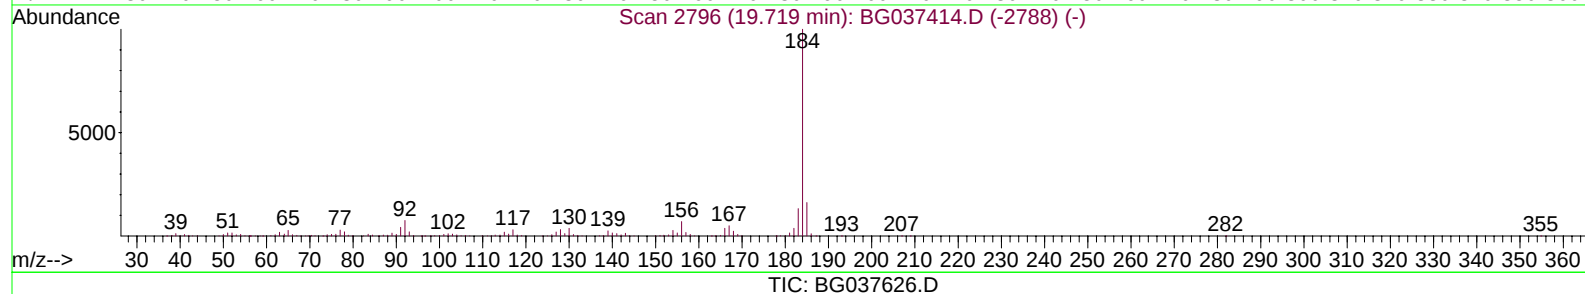
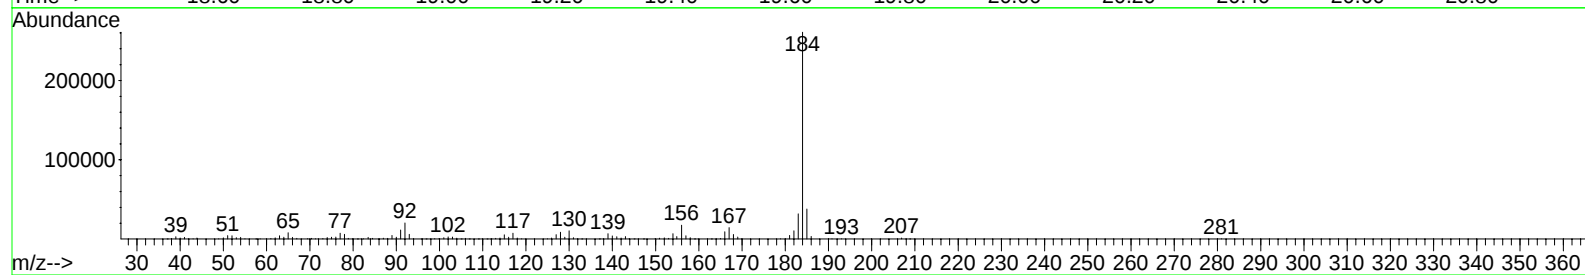


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG102918\
Data File : BG037626.D
Acq On : 29 Oct 2018 17:12
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 01 08:18:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

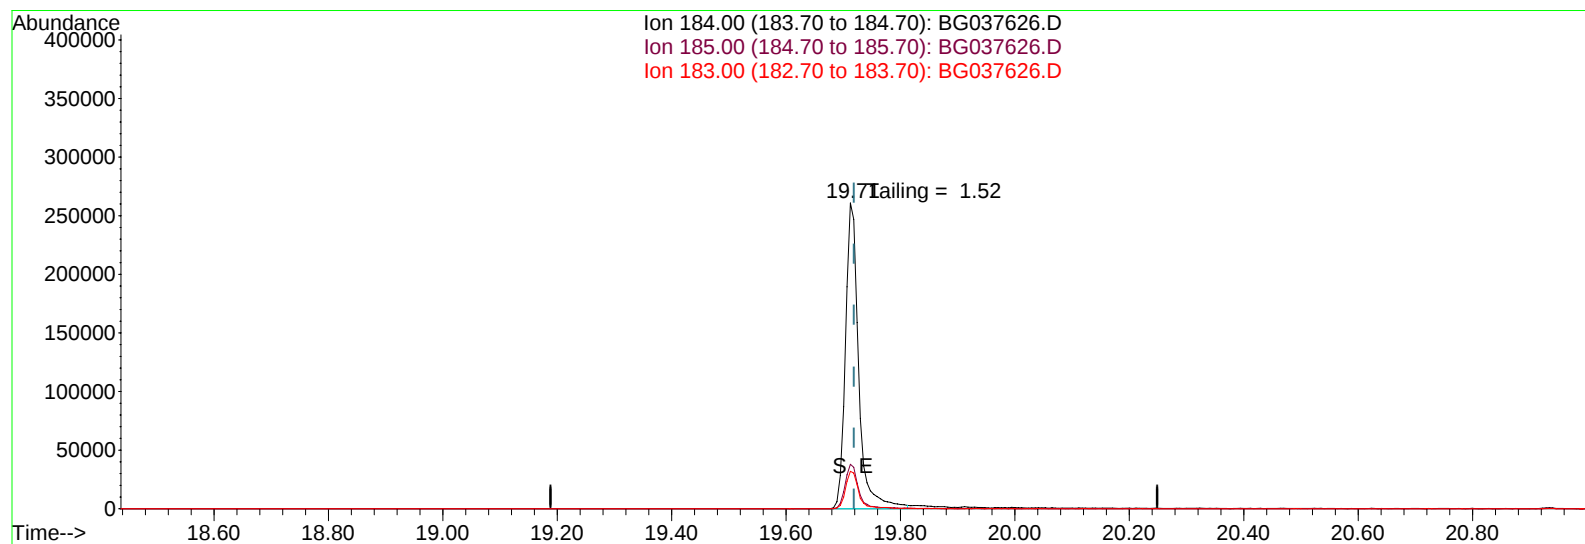

TIC: BG037626.D

(77) Benzidine




19.712min (-0.007) 0.00ng

response 422755

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.54
183.00	12.70	12.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG102918\
Data File : BG037626.D
Acq On : 29 Oct 2018 17:12
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 01 08:18:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

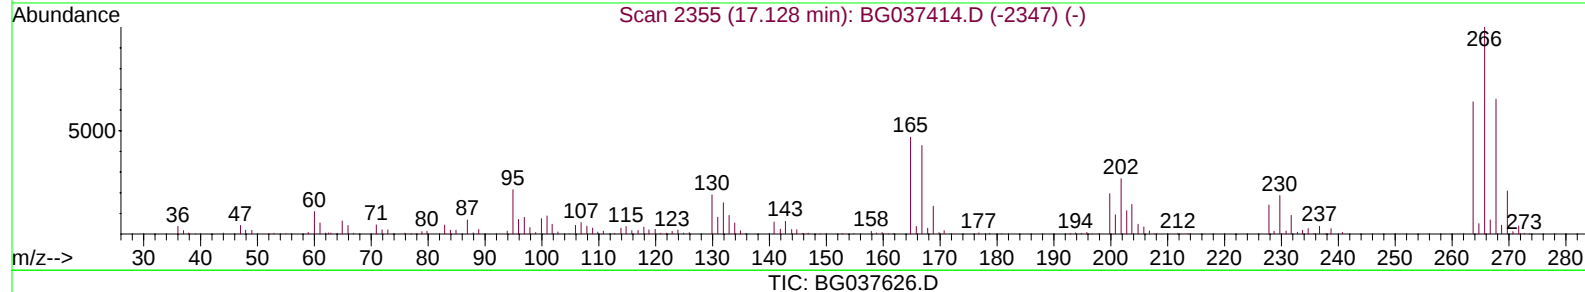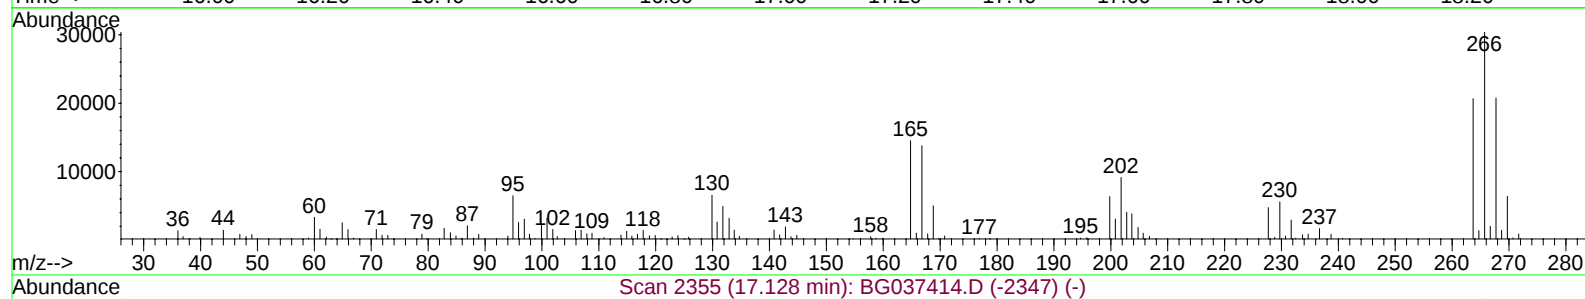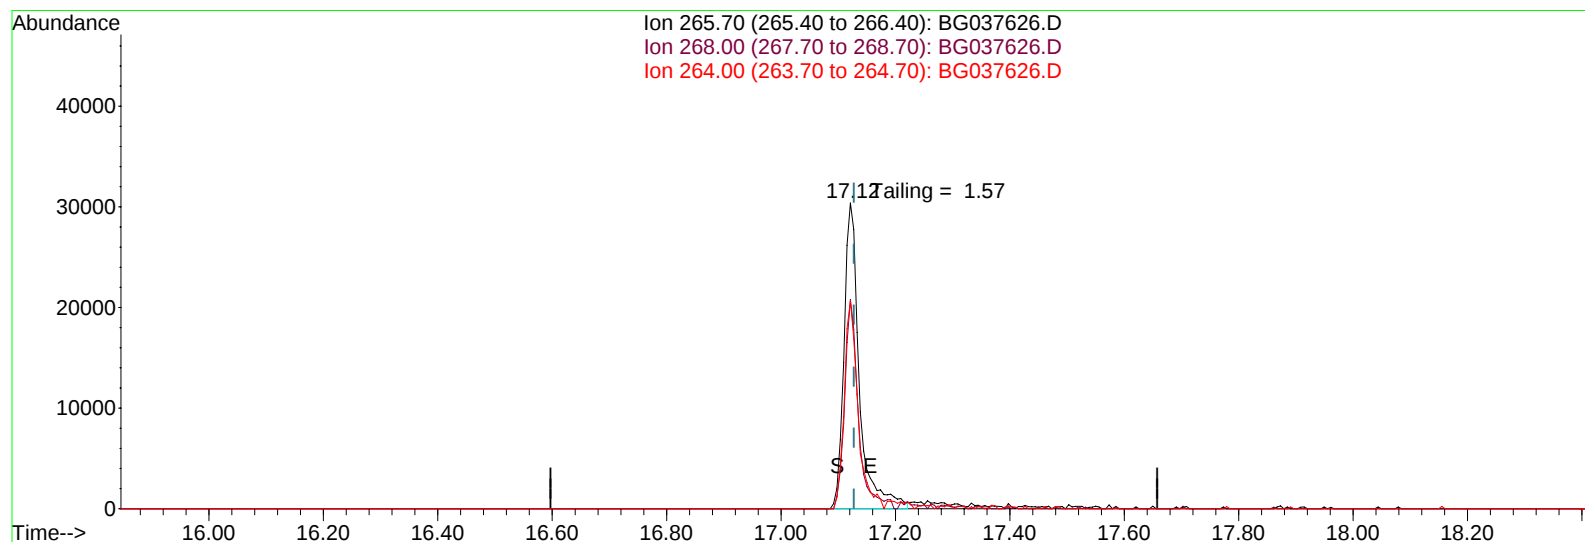

(70) Pentachlorophenol (C)

17.121min (-0.007) 36187.83ng

response 57384

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	73.03
264.00	73.60	72.49
0.00	0.00	0.00