

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102918\
 Data File : BG037630.D
 Acq On : 29 Oct 2018 19:48
 Operator : JU/SJ
 Sample : J5691-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-9

Quant Time: Oct 30 05:12:14 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 18 14:06:42 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	57773	20.00	ng	0.00
21) Naphthalene-d8	10.92	136	257009	20.00	ng	0.00
39) Acenaphthene-d10	14.73	164	174512	20.00	ng	0.00
64) Phenanthrene-d10	17.48	188	406346	20.00	ng	0.00
76) Chrysene-d12	21.77	240	369634	20.00	ng	0.00
87) Perylene-d12	25.10	264	370734	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	409324	118.45	ng	0.00
7) Phenol-d6	7.24	99	601437	115.10	ng	0.00
23) Nitrobenzene-d5	9.28	82	342780	74.71	ng	0.00
42) 2,4,6-Tribromophenol	16.22	330	209870	110.26	ng	0.00
45) 2-Fluorobiphenyl	13.35	172	783994	67.74	ng	-0.01
79) Terphenyl-d14	20.08	244	1111405	64.25	ng	0.00
Target Compounds						
10) Phenol	7.27	94	35297	6.402	ng	99
50) Dimethylphthalate	14.18	163	146902	10.881	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102918\
Data File : BG037630.D
Acq On : 29 Oct 2018 19:48
Operator : JU/SJ
Sample : J5691-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-9

Quant Time: Oct 30 05:12:14 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

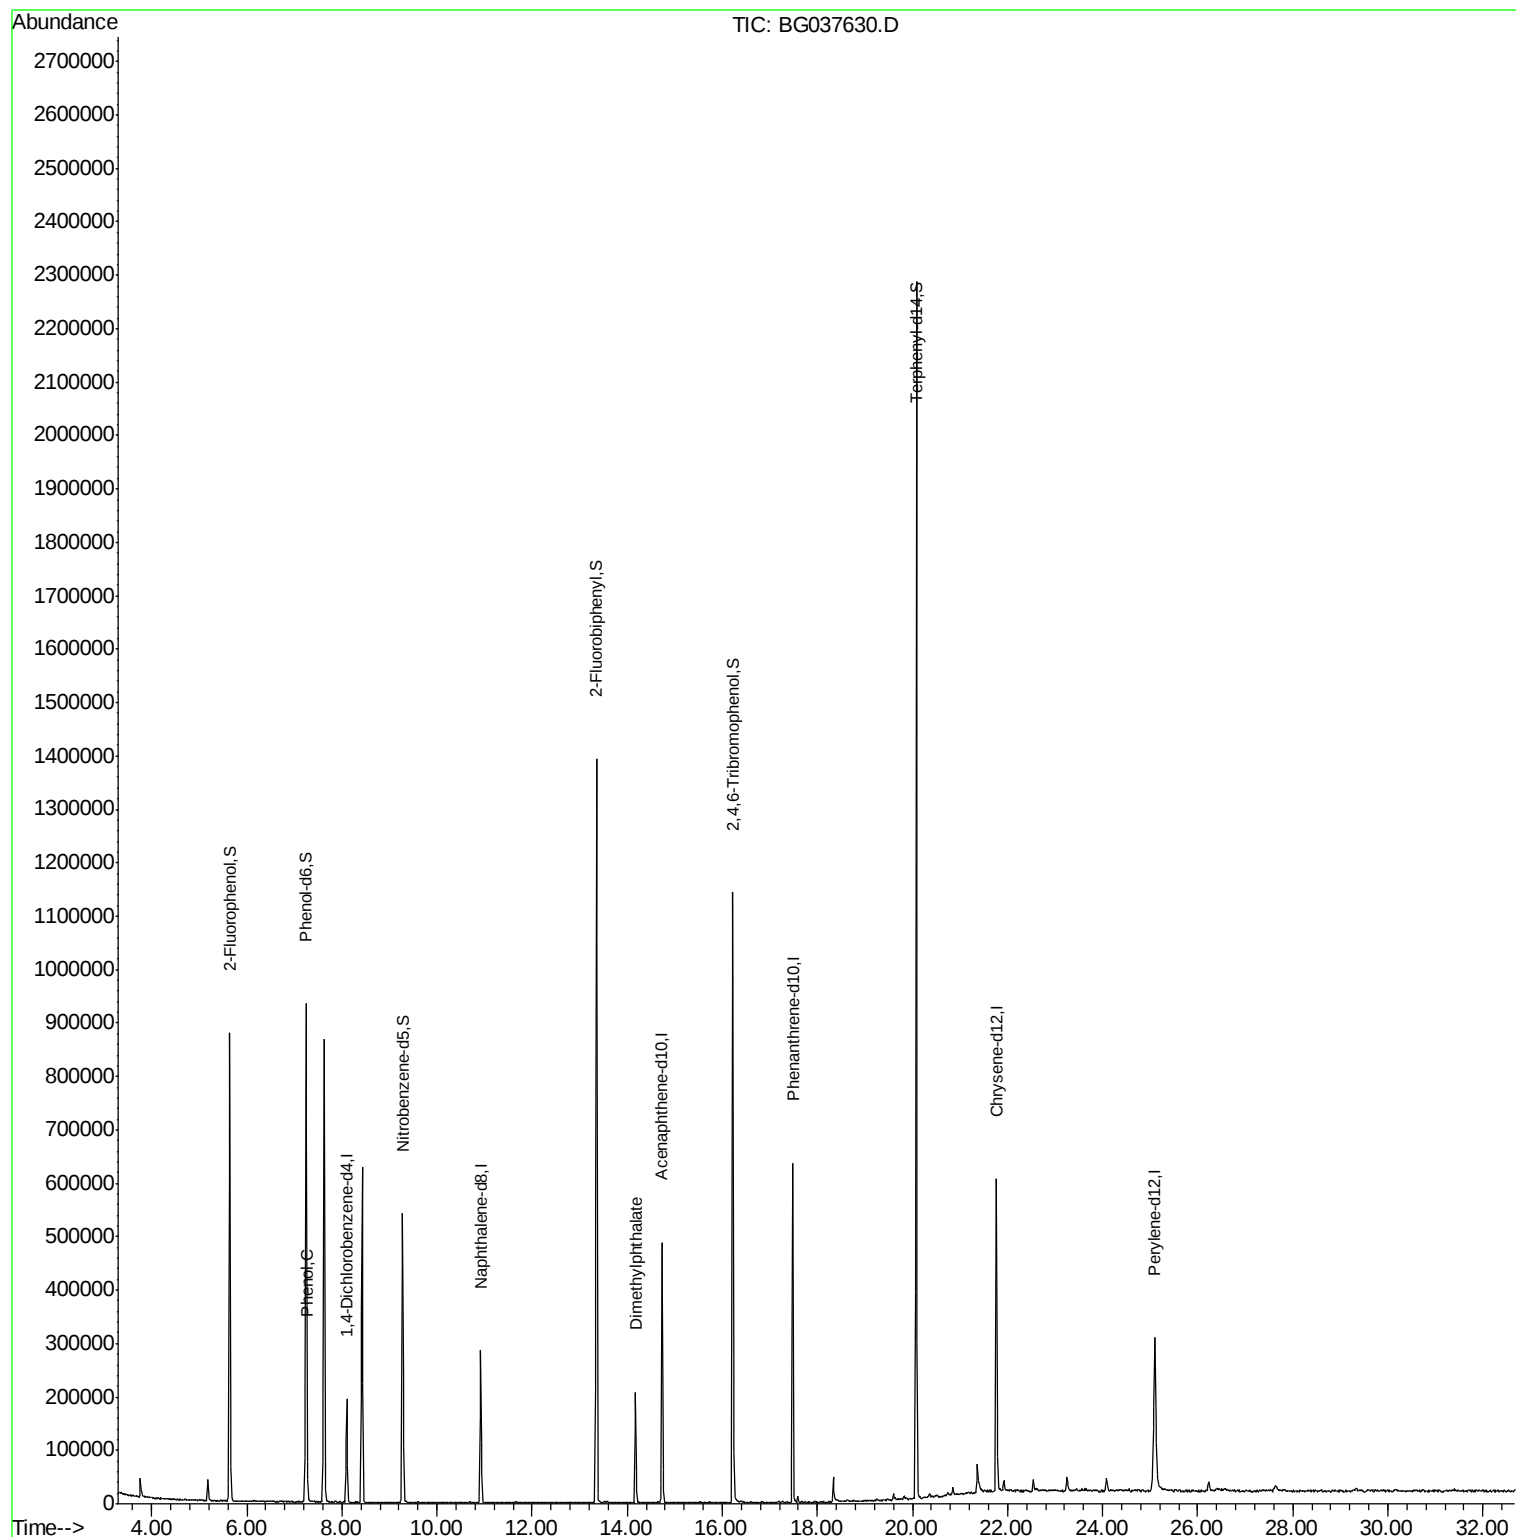

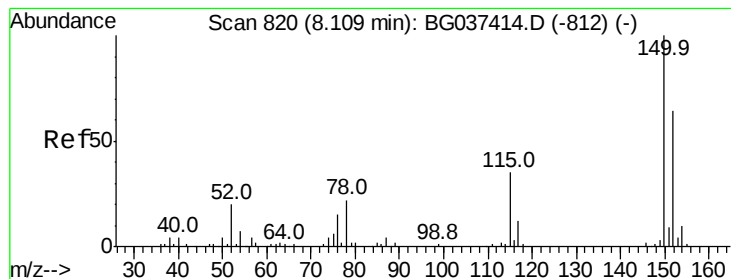


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.10 min Scan# 819
Delta R.T. -0.01 min
Lab File: BG037630.D
Acq: 29 Oct 2018 19:48

Instrument :
BNA_G
ClientSampleId :
SB-9

Tot Ion:152 Resp: 57773
Ion Ratio Lower Upper
152 100
150 158.0 126.0 189.0
115 59.9 45.5 68.3

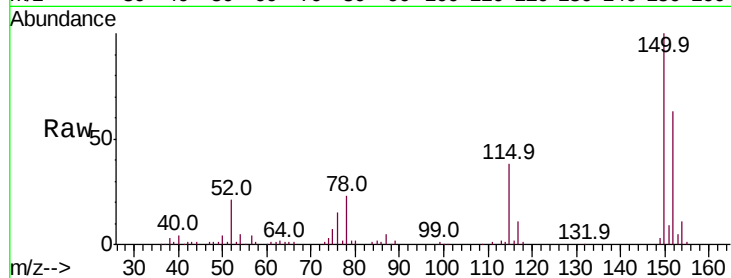


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

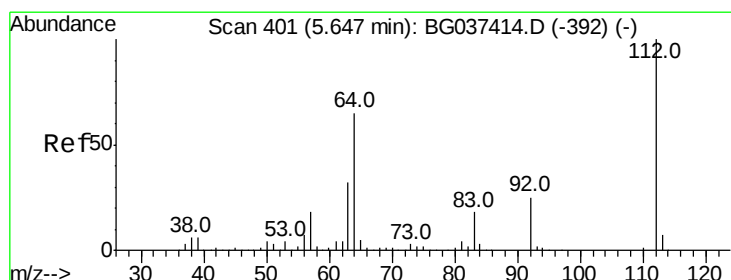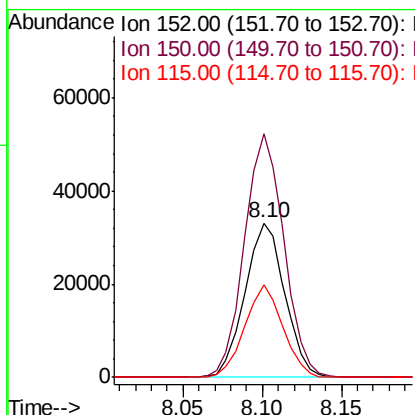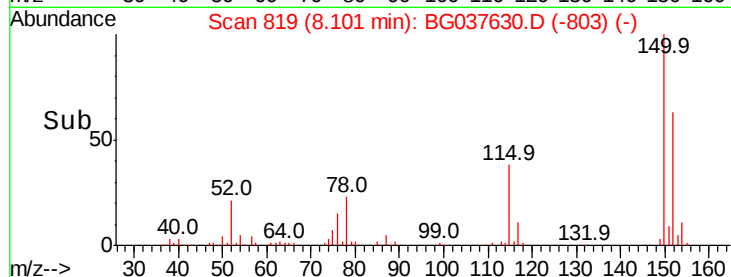



#5


2-Fluorophenol
Concen: 118.451 ng
RT: 5.64 min Scan# 401
Delta R.T. -0.00 min
Lab File: BG037630.D
Acq: 29 Oct 2018 19:48

Tgt Ion:112 Resp: 409324
Ion Ratio Lower Upper
112 100
64 64.8 53.1 79.7
63 33.2 27.3 40.9

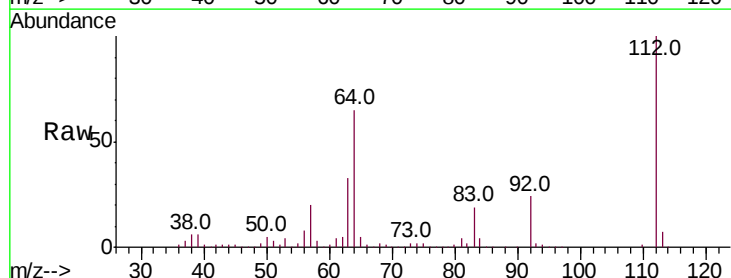

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

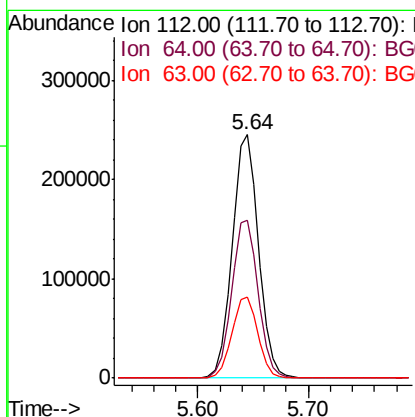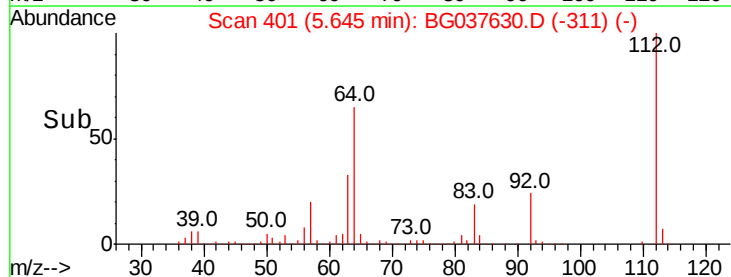

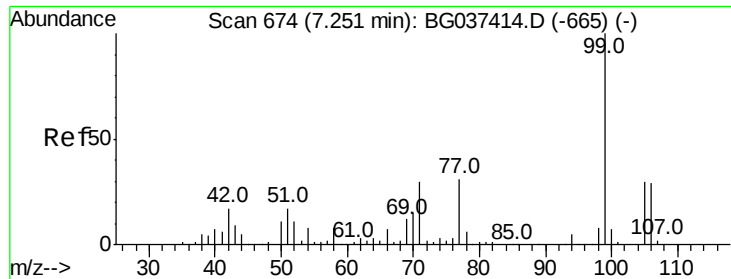

#7

Phenol-d6

Concen: 115.100 ng

RT: 7.24 min Scan# 673

Delta R.T. -0.01 min

Lab File: BG037630.D

Acq: 29 Oct 2018 19:48

Instrument :

BNA_G

ClientSampled :

SB-9


Tot Ion: 99 Resp: 601437

Ion Ratio Lower Upper




99 100

42 17.7 15.0 22.4

71 32.0 25.5 38.3

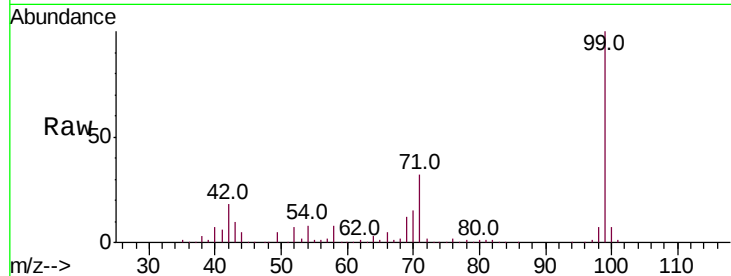

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

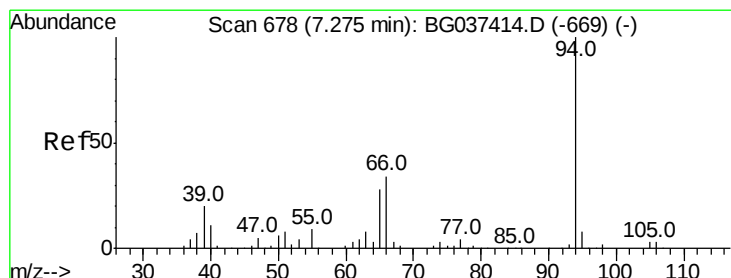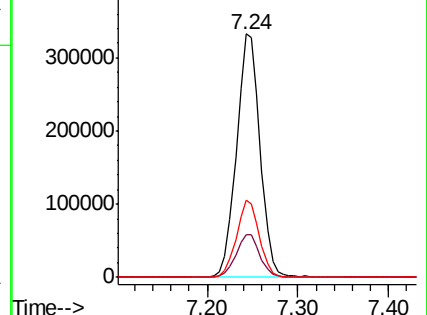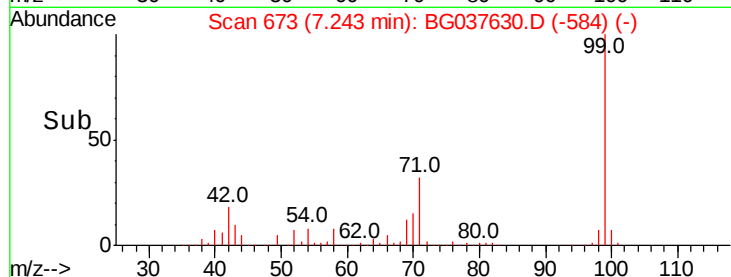

#10

Phenol

Concen: 6.402 ng

RT: 7.27 min Scan# 678

Delta R.T. -0.00 min

Lab File: BG037630.D

Acq: 29 Oct 2018 19:48


Tgt Ion: 94 Resp: 35297

Ion Ratio Lower Upper



94 100

65 30.4 9.7 49.7

66 36.6 15.9 55.9

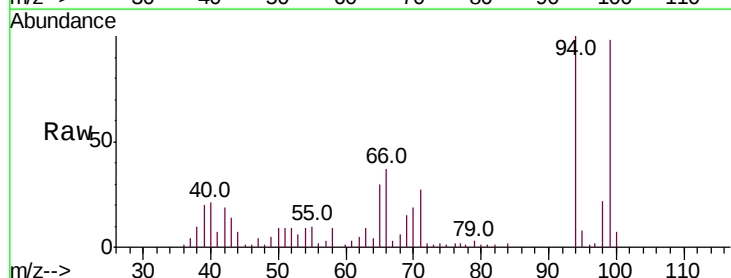

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC



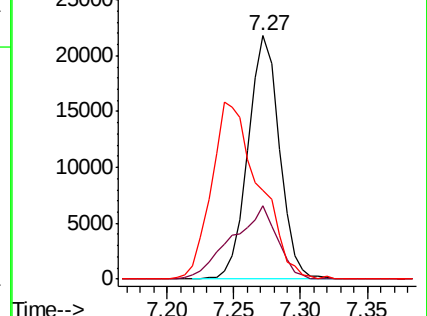
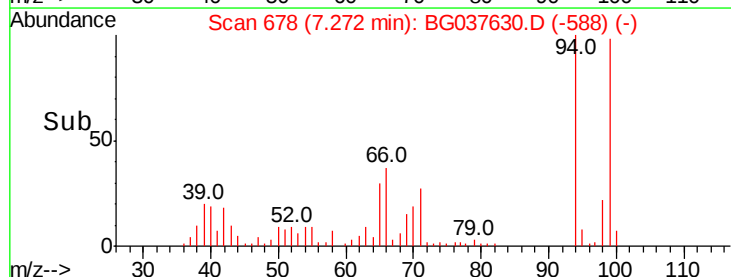




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.92 min Scan# 1299
Delta R.T. -0.01 min
Lab File: BG037630.D
Acq: 29 Oct 2018 19:48




Instrument :
BNA_G
ClientSampleId :
SB-9

Tot Ion:	136	Resp:	257009
Ion	Ratio	Lower	Upper
136	100		
137	11.4	9.6	14.4
54	10.2	7.9	11.9
68	6.3	4.8	7.2

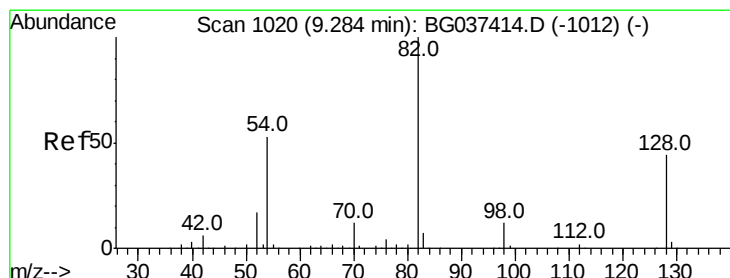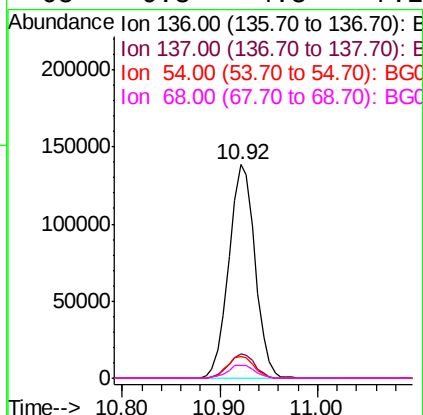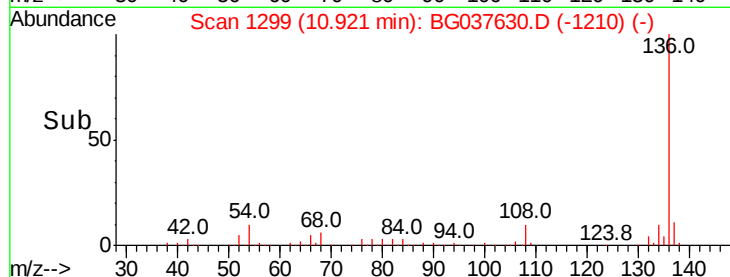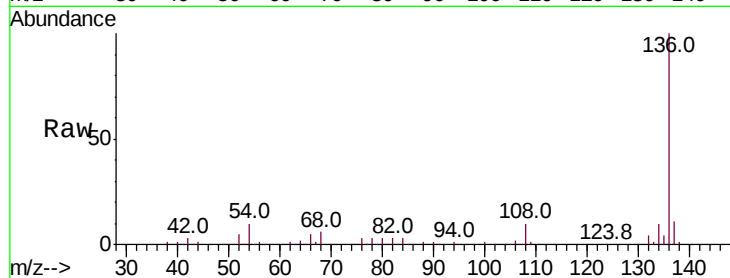

#23
Nitrobenzene-d5
Concen: 74.714 ng
RT: 9.28 min Scan# 1019
Delta R.T. -0.01 min
Lab File: BG037630.D
Acq: 29 Oct 2018 19:48

Tgt Ion:	82	Resp:	342780
Ion	Ratio	Lower	Upper
82	100		
128	43.9	34.6	51.8
54	53.2	45.3	67.9

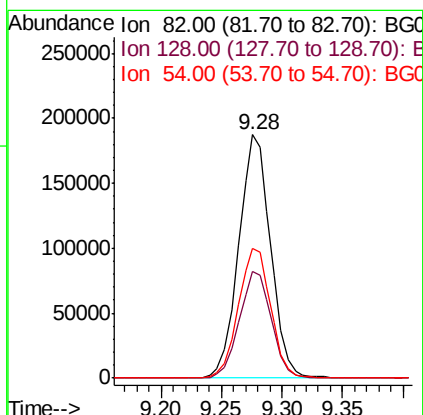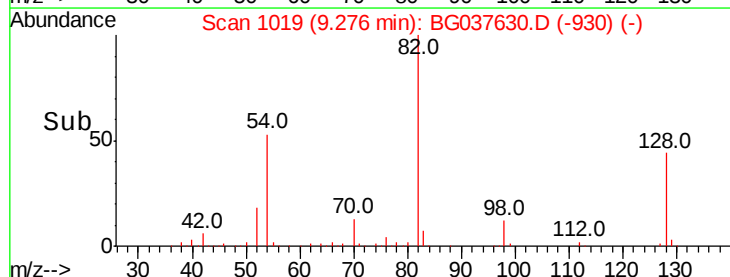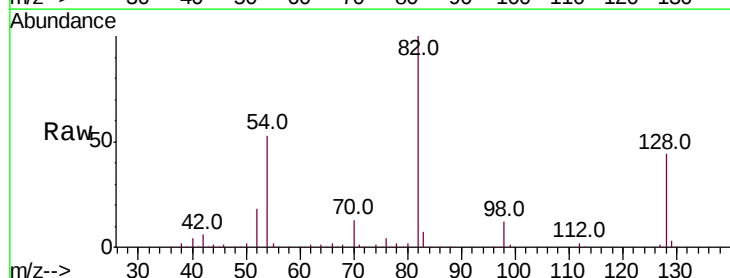



#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.73 min Scan# 1948

Delta R.T. -0.01 min

Lab File: BG037630.D

Acq: 29 Oct 2018 19:48

Instrument :

BNA_G

ClientSampleId :

SB-9


Tot Ion:164 Resp: 174512

Ion Ratio Lower Upper

164 100

162 103.7 81.3 121.9




160 45.5 36.3 54.5

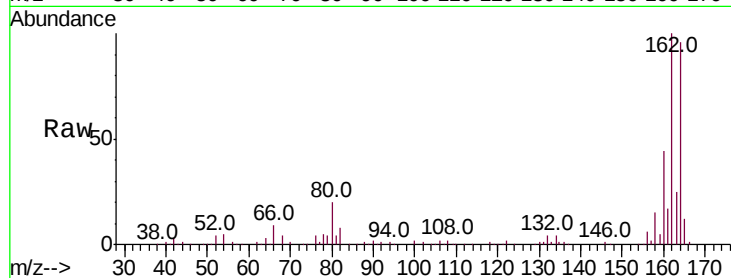

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

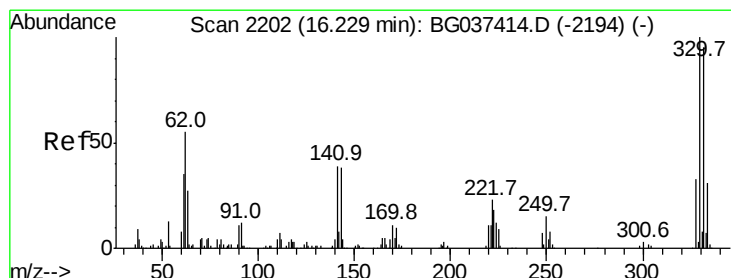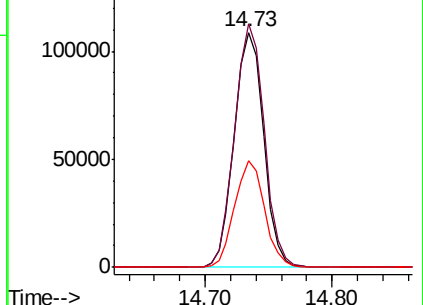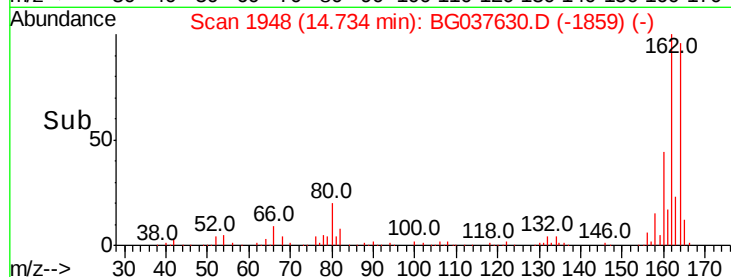

#42

2,4,6-Tribromophenol

Concen: 110.262 ng

RT: 16.22 min Scan# 2201

Delta R.T. -0.01 min

Lab File: BG037630.D

Acq: 29 Oct 2018 19:48


Tgt Ion:330 Resp: 209870

Ion Ratio Lower Upper

330 100

332 96.1 78.4 117.6



141 40.3 32.2 48.2

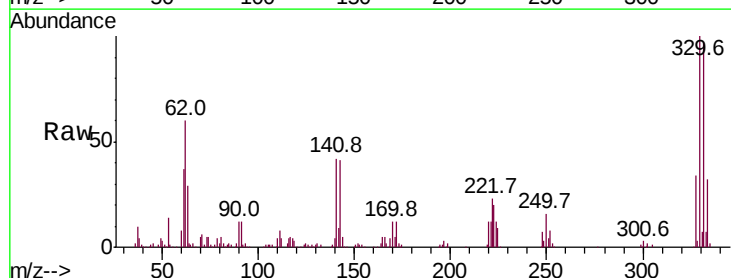

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



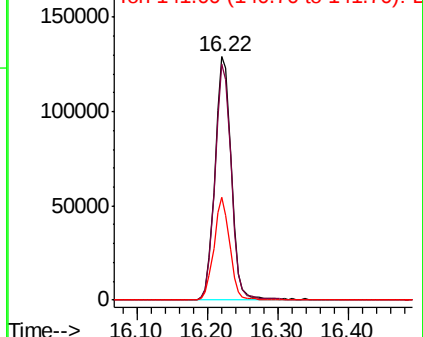
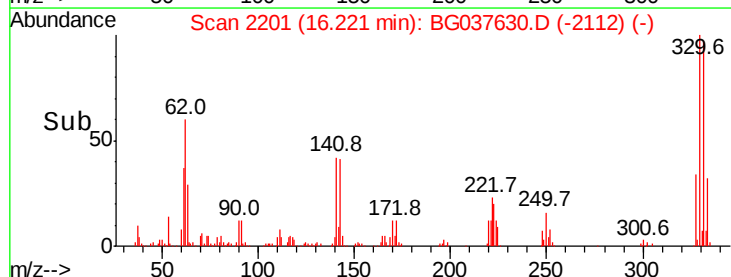




#45
 2-Fluorobiphenyl
 Concen: 67.744 ng
 RT: 13.35 min Scan# 1713
 Delta R.T. -0.01 min
 Lab File: BG037630.D
 Acq: 29 Oct 2018 19:48




Instrument :
 BNA_G
 ClientSampleId :
 SB-9


Tot Ion	Ratio	Lower	Upper
172	100		
171	36.8	31.0	46.4
170	24.6	20.2	30.2

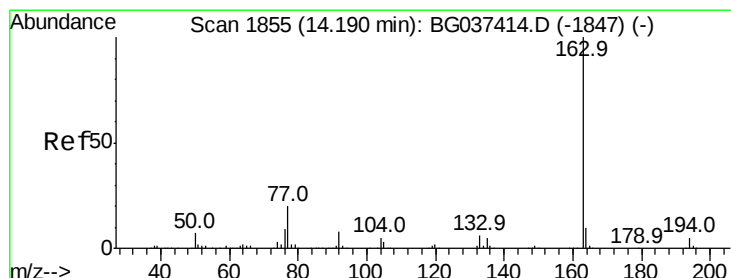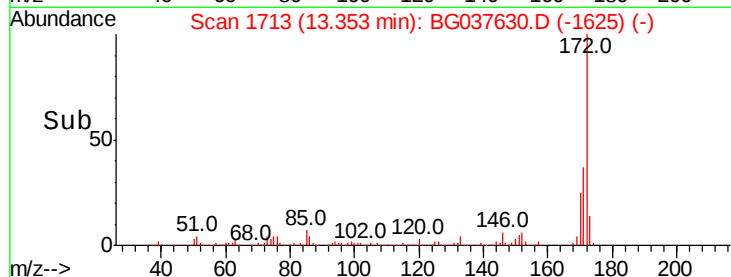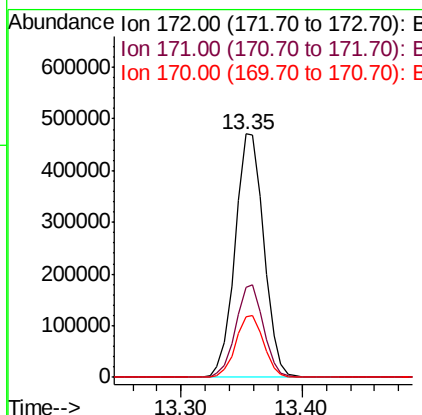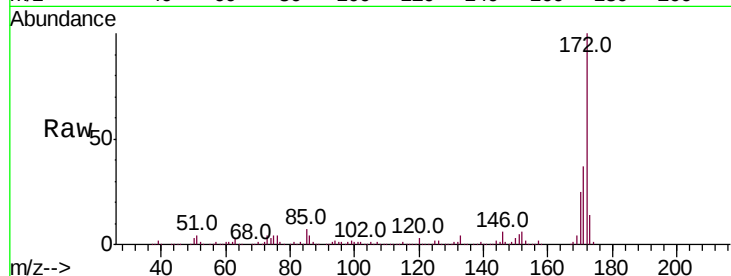

#50
 Dimethylphthalate
 Concen: 10.881 ng
 RT: 14.18 min Scan# 1853
 Delta R.T. -0.01 min
 Lab File: BG037630.D
 Acq: 29 Oct 2018 19:48

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.4	3.5	5.3
164	9.9	8.5	12.7

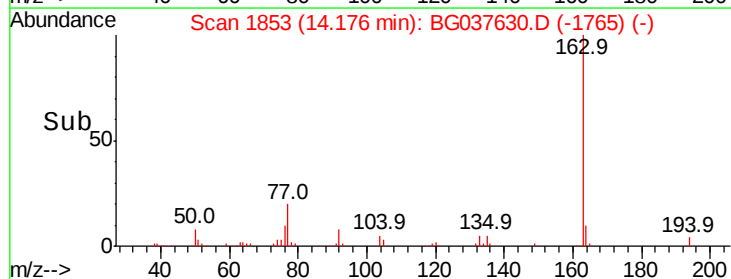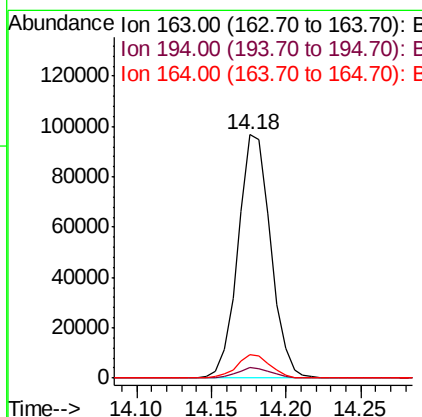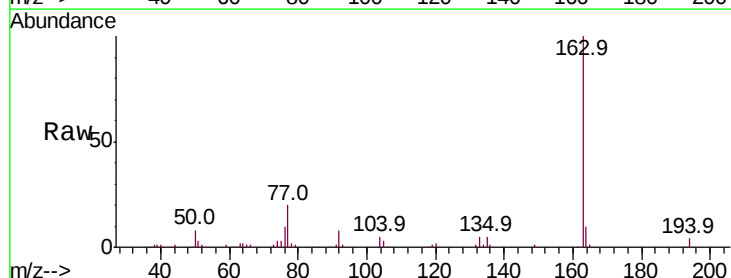


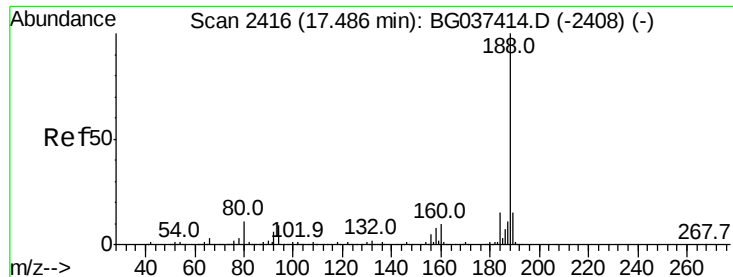




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.48 min Scan# 2416
Delta R.T. -0.00 min
Lab File: BG037630.D
Acq: 29 Oct 2018 19:48

Instrument :
BNA_G
ClientSampleId :
SB-9

Tot Ion:188 Resp: 406346
Ion Ratio Lower Upper
188 100
94 9.0 7.2 10.8
80 9.8 7.7 11.5

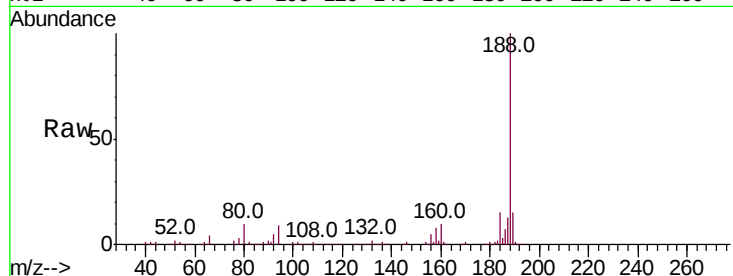


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BG
Ion 80.00 (79.70 to 80.70): BG

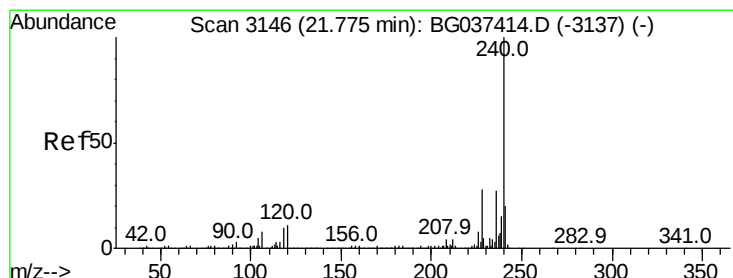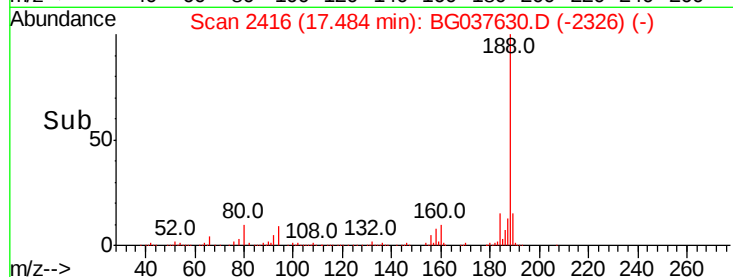
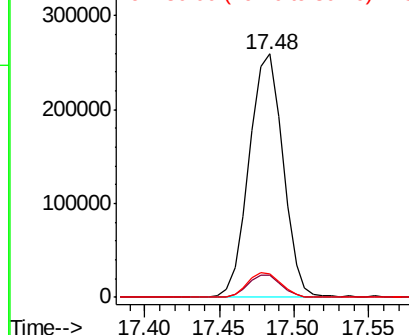



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.77 min Scan# 3145
Delta R.T. -0.01 min
Lab File: BG037630.D
Acq: 29 Oct 2018 19:48

Tgt Ion:240 Resp: 369634
Ion Ratio Lower Upper
240 100
120 10.9 8.1 12.1
236 27.6 21.4 32.0

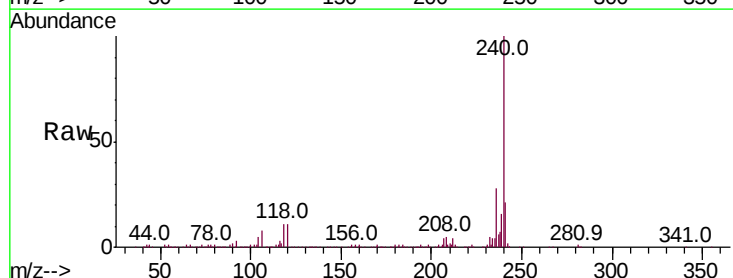

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

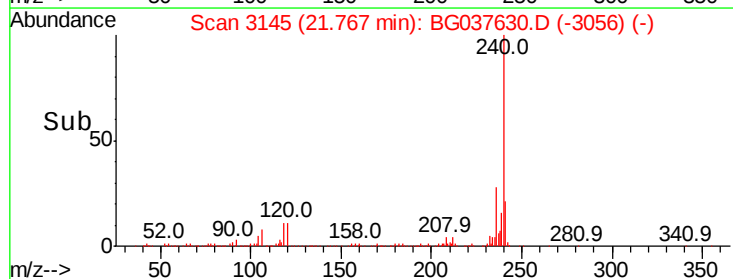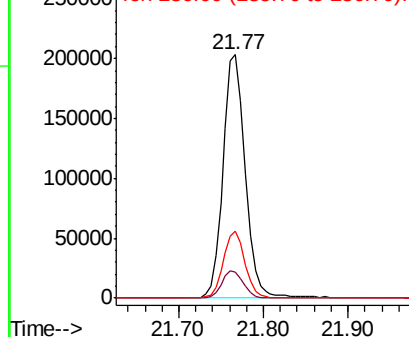

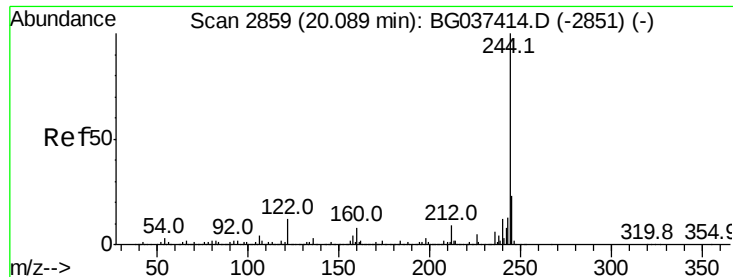

#79

Terphenyl-d14

Concen: 64.248 ng

RT: 20.08 min Scan# 2858

Delta R.T. -0.01 min

Lab File: BG037630.D

Acq: 29 Oct 2018 19:48

Instrument :

BNA_G

ClientSampled :

SB-9


Tot Ion:244 Resp: 1111405

Ion Ratio Lower Upper




244 100

212 8.1 6.5 9.7

122 11.6 9.0 13.4

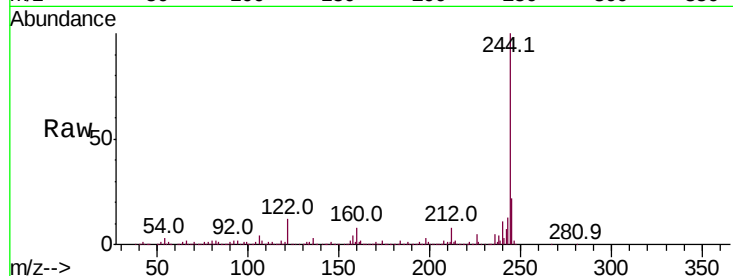

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

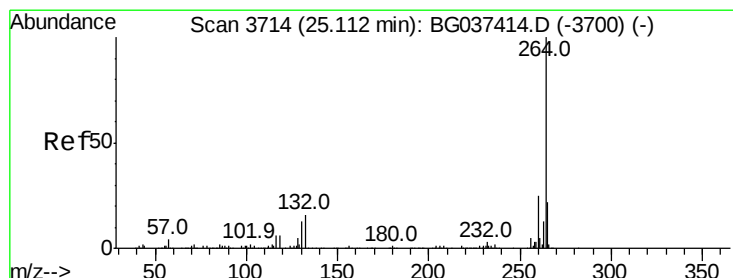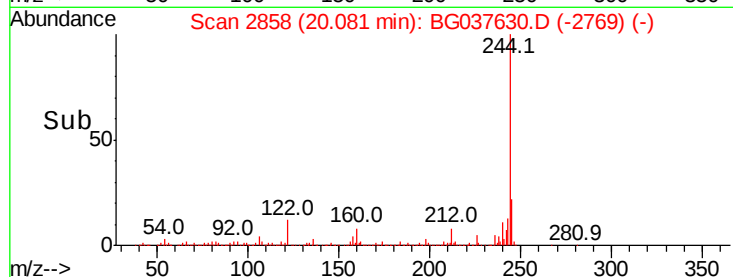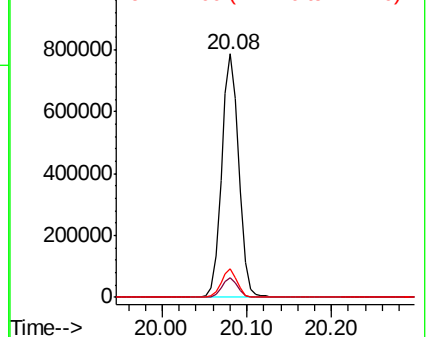

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.10 min Scan# 3712

Delta R.T. -0.01 min

Lab File: BG037630.D

Acq: 29 Oct 2018 19:48


Tgt Ion:264 Resp: 370734

Ion Ratio Lower Upper

264 100

260 24.7 18.2 27.4

265 23.1 17.9 26.9

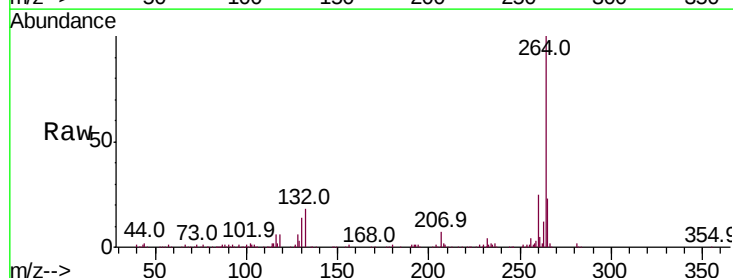

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

