


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG102918\
 Data File : BG037626.D
 Acq On : 29 Oct 2018 17:12
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 18 14:06:42 2018

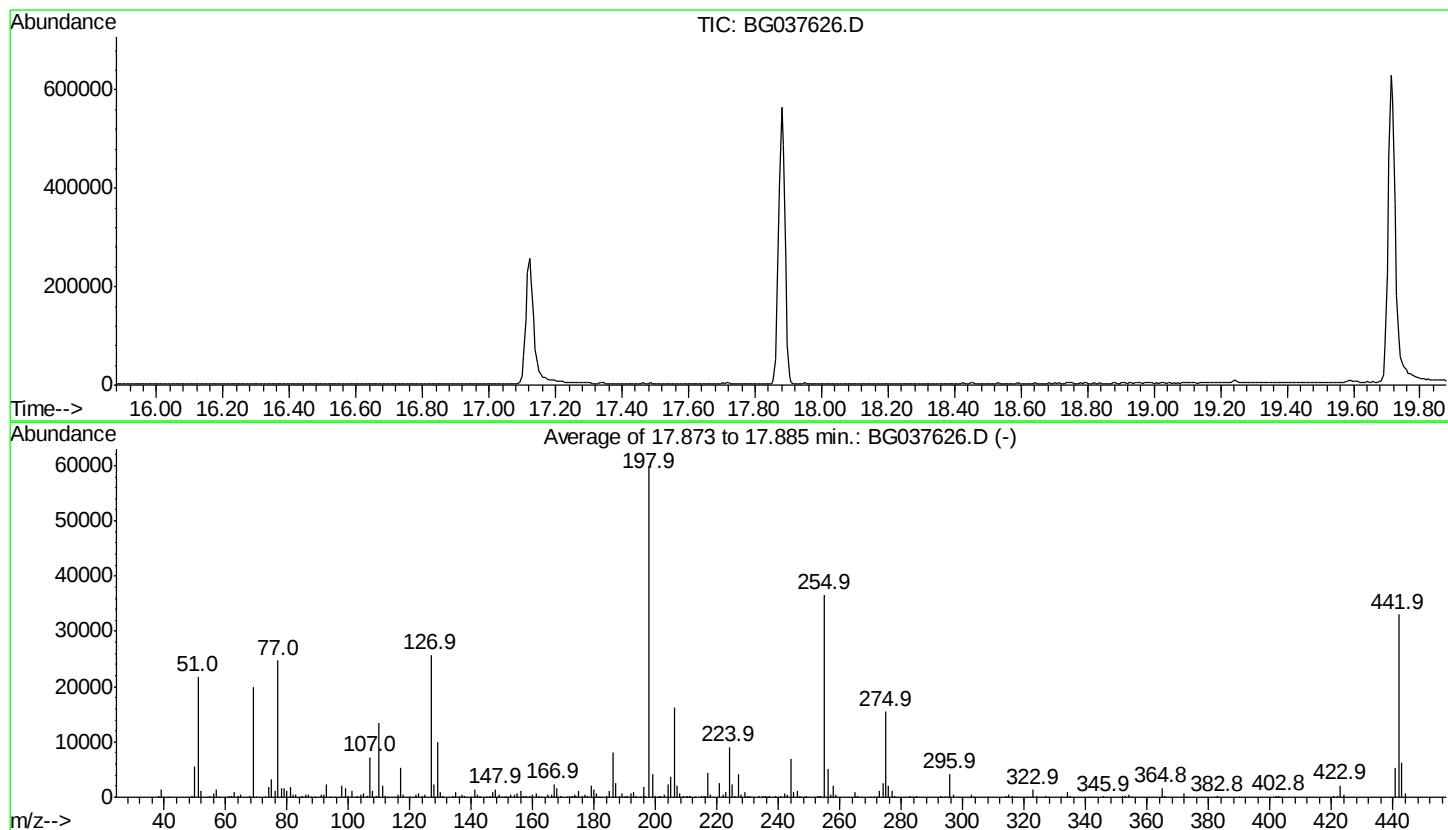

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	21882	PASS
68	69	0.00	2	1.5	299	PASS
69	198	0.00	100	33.3	19952	PASS
70	69	0.00	2	0.4	79	PASS
127	198	10	80	42.9	25744	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59978	PASS
199	198	5	9	6.9	4127	PASS
275	198	10	60	25.7	15404	PASS
365	198	1	100	2.8	1707	PASS
441	198	0.01	100	8.7	5227	PASS
442	198	50	100	55.2	33082	PASS
443	442	15	24	18.6	6157	PASS