

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102919\
 Data File : BG043374.D
 Acq On : 29 Oct 2019 15:06
 Operator : JU
 Sample : PB124325BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB124325BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.127	342	347	355	rBV	122003	191334	5.36%	1.218%
2	5.615	423	430	443	rBV	615657	1082058	30.33%	6.891%
3	7.213	694	702	721	rBV	653372	1200632	33.65%	7.646%
4	7.565	753	762	773	rBV	675787	1209833	33.91%	7.704%
5	8.024	831	840	852	rBV	126223	228254	6.40%	1.454%
6	8.347	887	895	905	rBV	530253	943989	26.46%	6.011%
7	9.187	1029	1038	1054	rBV	342750	712436	19.97%	4.537%
8	10.826	1310	1317	1331	rBV	131627	287468	8.06%	1.831%
9	13.276	1726	1734	1745	rBV	1110047	1880265	52.70%	11.974%
10	14.651	1959	1968	1980	rBV2	262280	470695	13.19%	2.997%
11	16.138	2215	2221	2244	rBV	928166	1693866	47.48%	10.787%
12	17.395	2424	2435	2454	rBV	327248	596999	16.73%	3.802%
13	20.004	2873	2879	2894	rBV	2519947	3567540	100.00%	22.718%
14	21.660	3154	3161	3171	rBV2	365406	742795	20.82%	4.730%
15	23.135	3407	3412	3420	rVB2	19735	37741	1.06%	0.240%
16	23.934	3540	3548	3558	rBV4	19775	46048	1.29%	0.293%
17	24.857	3695	3705	3722	rBV	254561	811294	22.74%	5.166%


Sum of corrected areas: 15703247

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102919\
Data File : BG043374.D
Acq On : 29 Oct 2019 15:06
Operator : JU
Sample : PB124325BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB124325BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

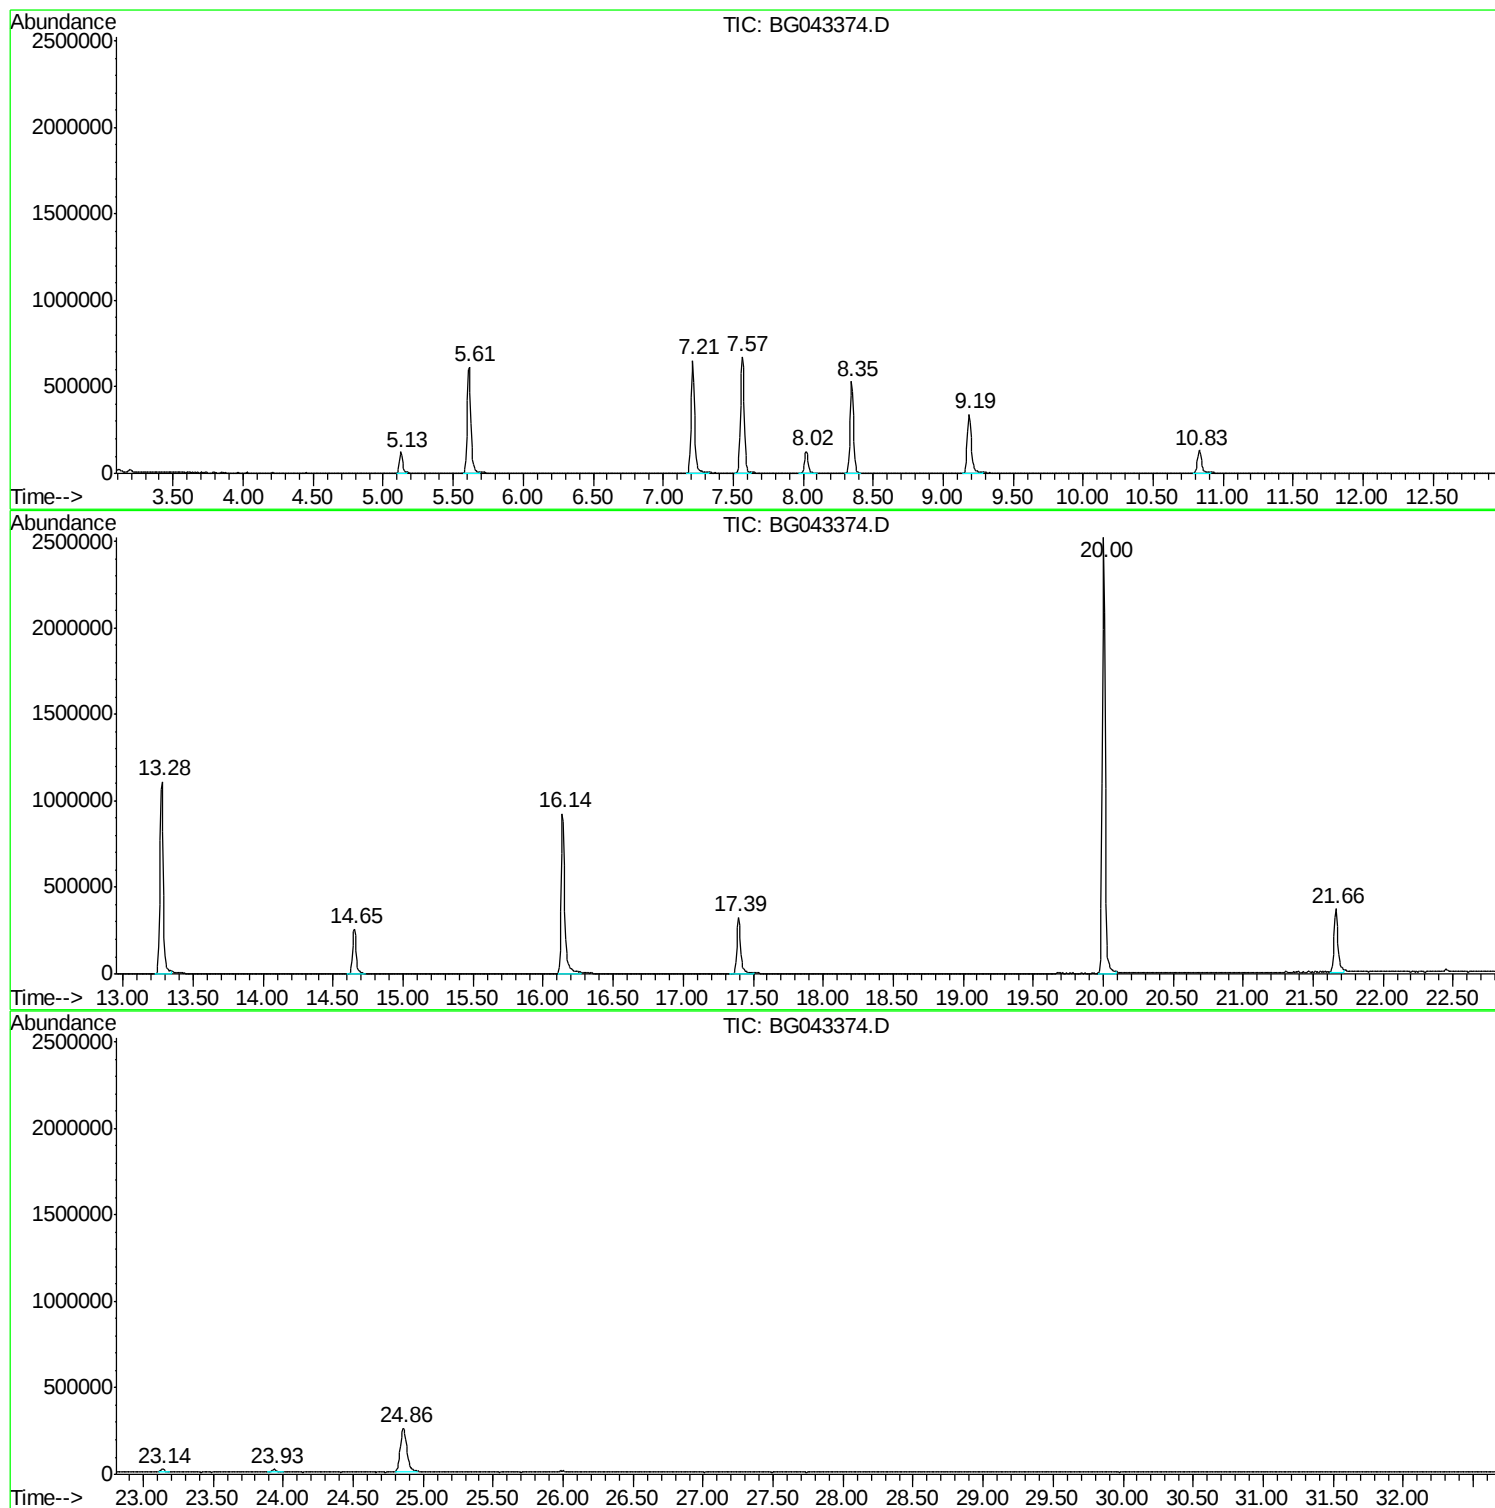

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102919\
Data File : BG043374.D
Acq On : 29 Oct 2019 15:06
Operator : JU
Sample : PB124325BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB124325BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown5.13 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.13	16.77 ng	191334	1,4-Dichlorobenzene-d4	8.02

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	40
2		2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	38
3		Butyl aldoxime, 3-methyl-, syn-	101	C5H11NO	005780-40-5	23
4		Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9
5		(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	9

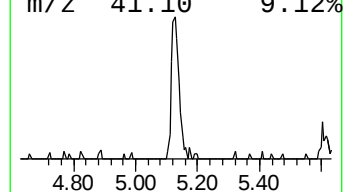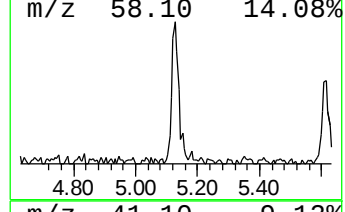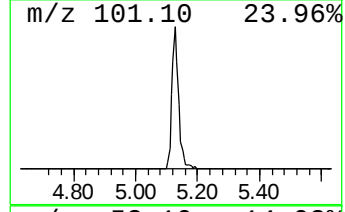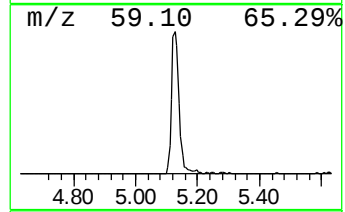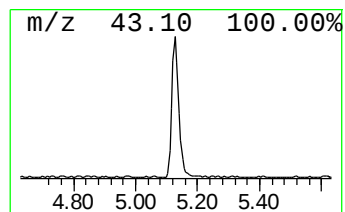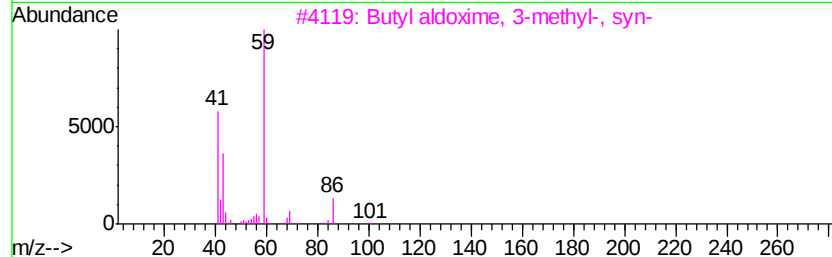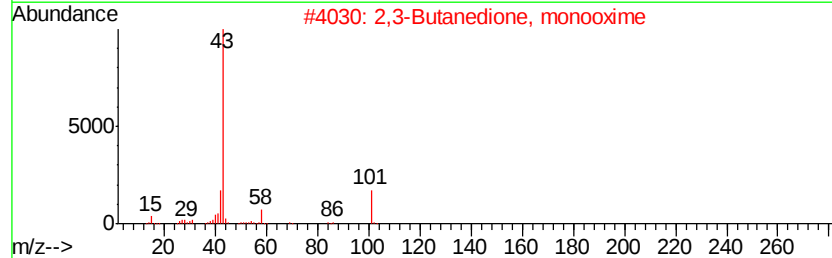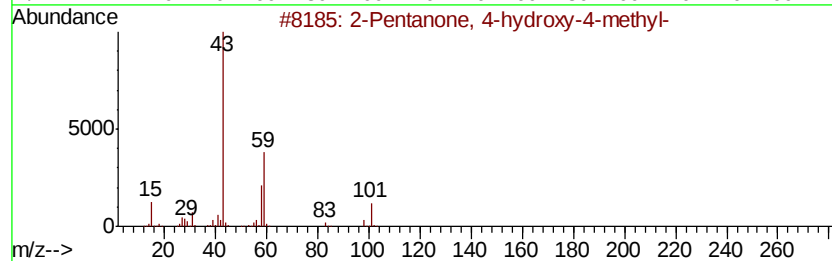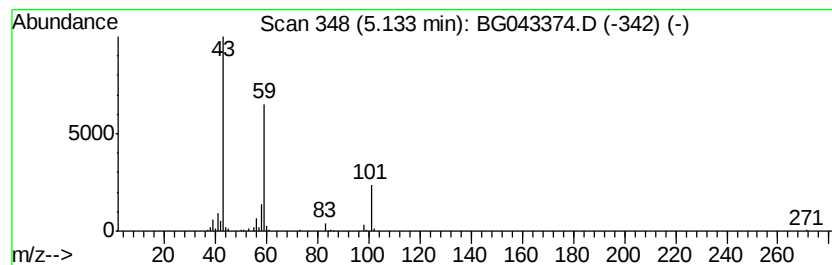

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102919\
Data File : BG043374.D
Acq On : 29 Oct 2019 15:06
Operator : JU
Sample : PB124325BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB124325BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.57 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.57	106.01 ng	1209830	1,4-Dichlorobenzene-d4	8.02

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	27
3		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
4		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	17
5		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12

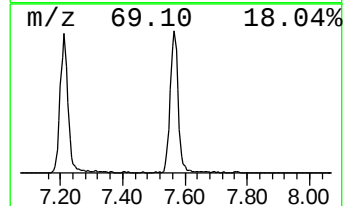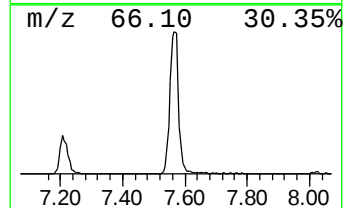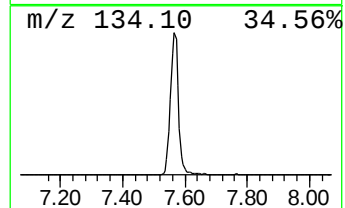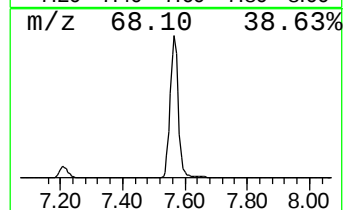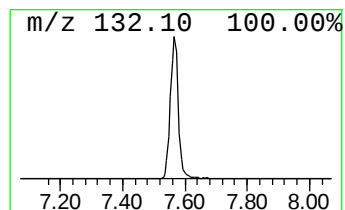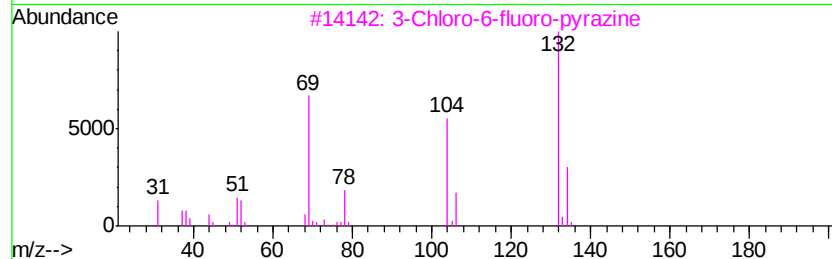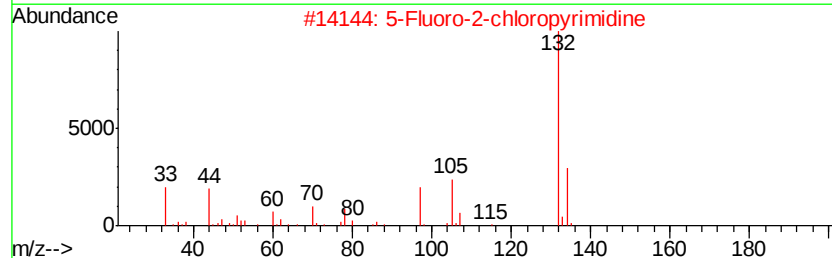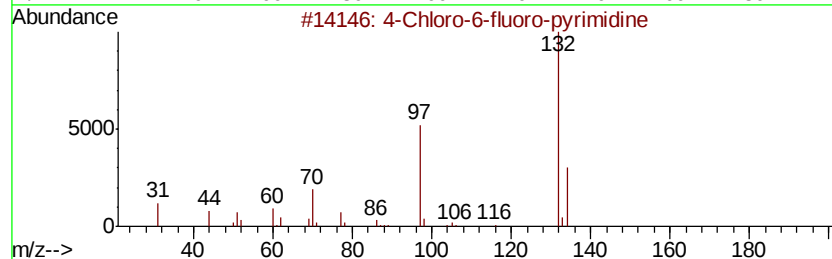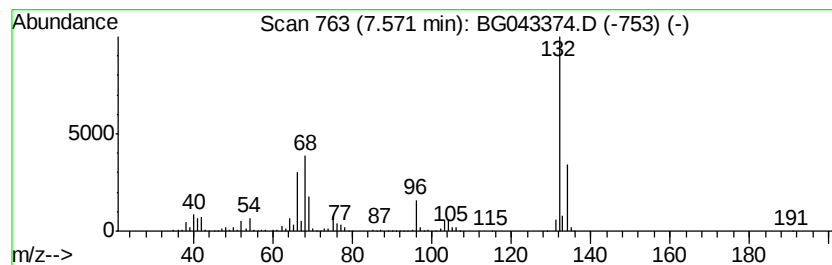

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG102919\
Data File : BG043374.D
Acq On : 29 Oct 2019 15:06
Operator : JU
Sample : PB124325BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB124325BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown5.13	5.13	16.8	ng	191334	1	8.02	228254	20.0
unknown7.57	7.57	106.0	ng	1209830	1	8.02	228254	20.0