


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG102919\
 Data File : BG043368.D
 Acq On : 29 Oct 2019 10:18
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 21 16:37:43 2019

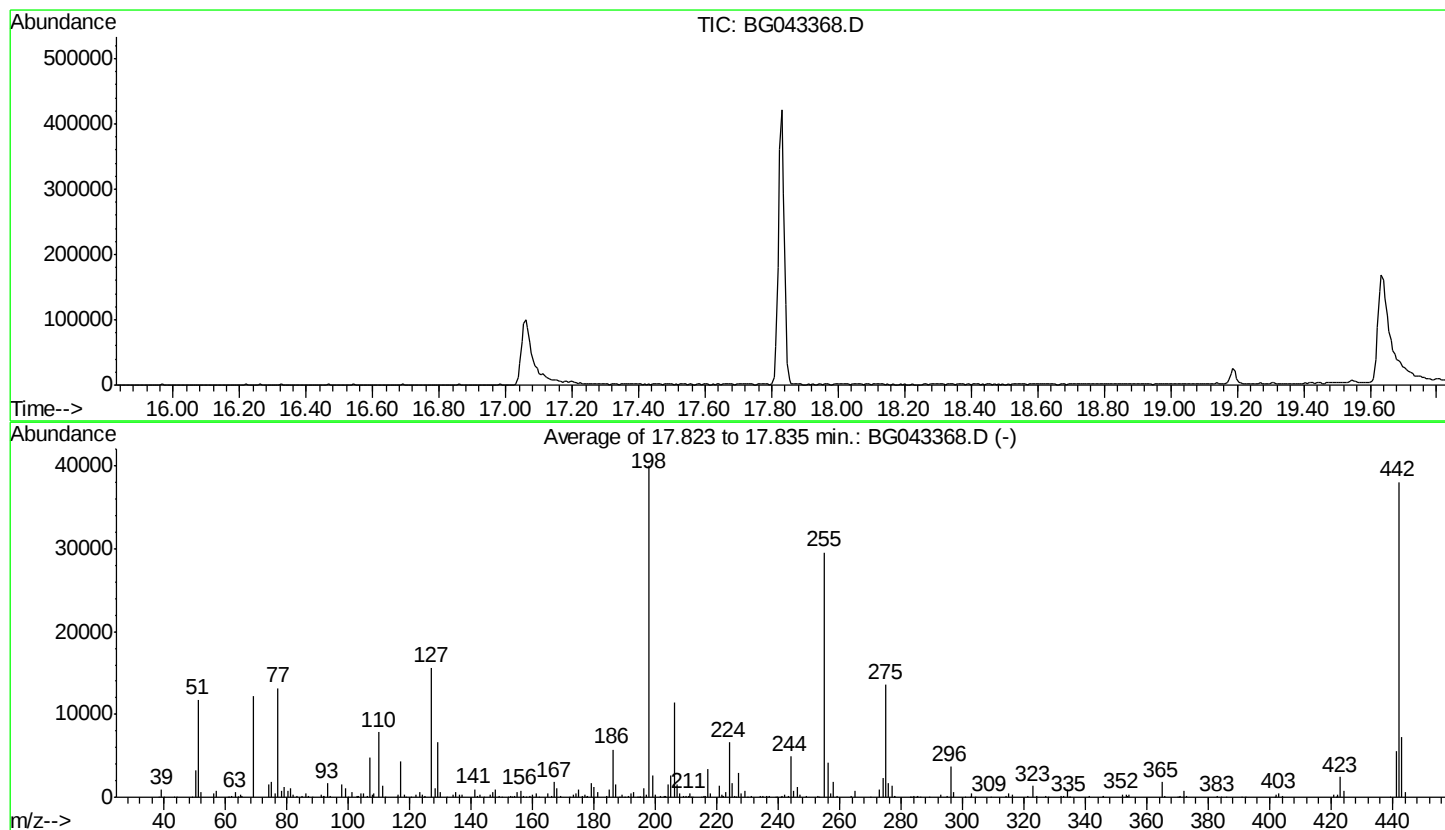

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	11787	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.4	12167	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.1	15656	PASS
197	198	0.00	2	0.8	301	PASS
198	198	100	100	100.0	40037	PASS
199	198	5	9	6.4	2567	PASS
275	198	10	60	33.9	13557	PASS
365	198	1	100	4.6	1833	PASS
441	198	0.01	100	14.0	5592	PASS
442	198	50	100	95.0	38050	PASS
443	442	15	24	19.1	7281	PASS