


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102919\
 Data File : BG043385.D
 Acq On : 29 Oct 2019 23:27
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 21 16:37:43 2019

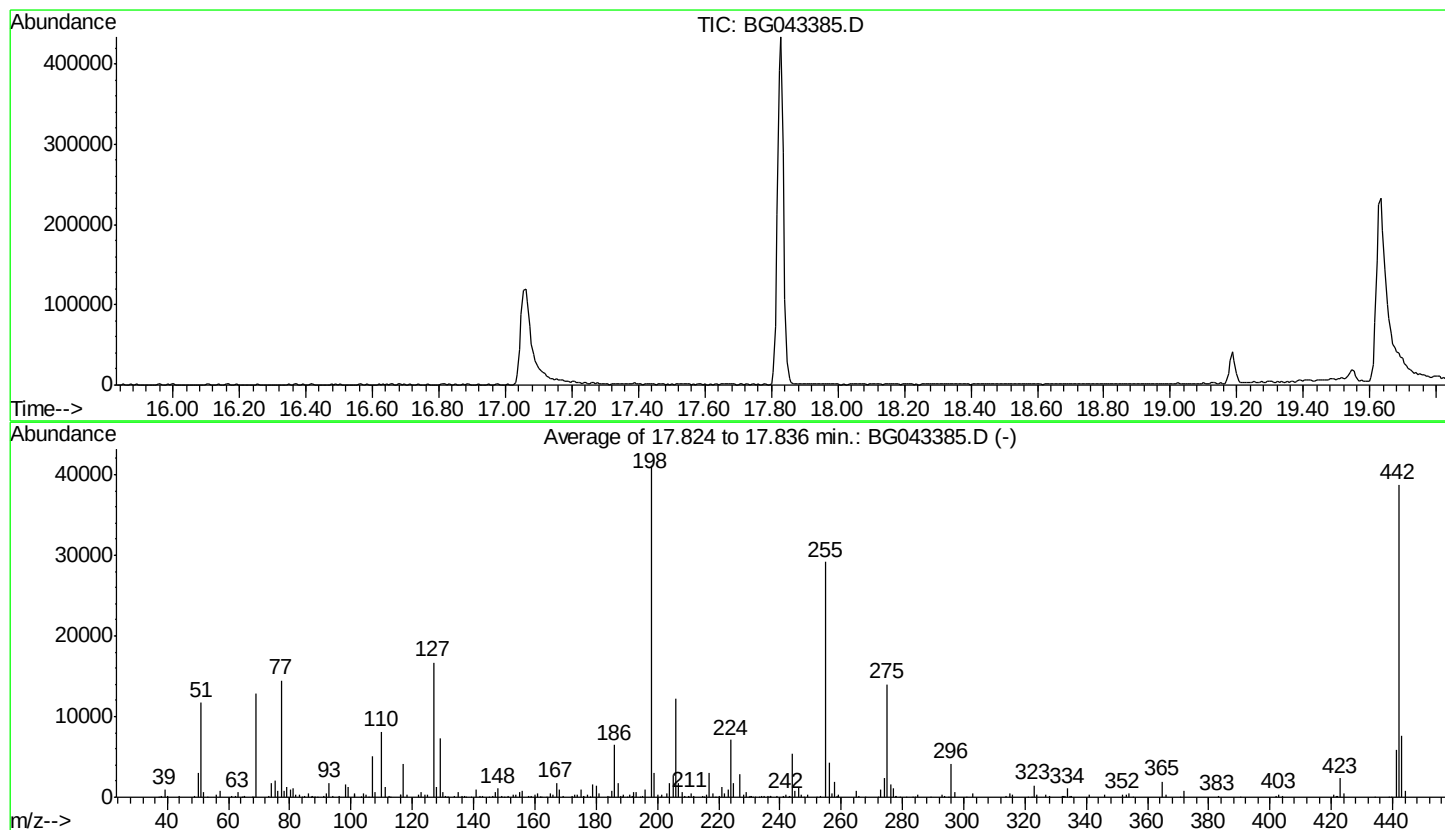

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.5	11699	PASS
68	69	0.00	2	0.6	79	PASS
69	198	0.00	100	31.4	12896	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.7	16708	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	41098	PASS
199	198	5	9	7.2	2977	PASS
275	198	10	60	34.1	14019	PASS
365	198	1	100	4.6	1910	PASS
441	198	0.01	100	14.4	5938	PASS
442	198	50	100	94.2	38722	PASS
443	442	15	24	19.8	7685	PASS