

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102920\
 Data File : BG047121.D
 Acq On : 29 Oct 2020 16:38
 Operator : CG/JU
 Sample : L4499-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW2B8

Quant Time: Oct 29 16:20:00 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG102220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 29 16:49:45 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	52177	20.00	ng/ul	0.00
18) Naphthalene-d8	10.87	136	207183	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.69	164	155851	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.43	188	374152	20.00	ng/ul	0.00
78) Chrysene-d12	21.70	240	393285	20.00	ng/ul	0.00
86) Perylene-d12	24.95	264	401216	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.46	96	6212	4.80	ng/uL	0.00
5) Phenol-d5	7.21	99	156825	34.63	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.38	67	82862	31.81	ng/ul	0.00
9) 2-Chlorophenol-d4	7.59	132	116706	33.14	ng/ul	0.00
13) 4-Methylphenol-d8	8.76	113	125383	34.70	ng/ul	0.00
19) Nitrobenzene-d5	9.22	128	57662	33.20	ng/ul	0.00
22) 2-Nitrophenol-d4	9.95	143	66029	32.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.49	165	132178	33.39	ng/ul	0.00
29) 4-Chloroaniline-d4	11.00	131	148517	44.00	ng/ul	0.00
44) Dimethylphthalate-d6	14.09	166	427107	33.33	ng/ul	0.00
47) Acenaphthylene-d8	14.38	160	499101	32.92	ng/ul	0.00
52) 4-Nitrophenol-d4	14.88	143	65609	32.52	ng/ul	0.00
58) Fluorene-d10	15.68	176	374843	31.50	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.79	200	74183	28.75	ng/ul	0.00
71) Anthracene-d10	17.53	188	590993	32.59	ng/ul	0.00
79) Pyrene-d10	19.82	212	730601	32.57	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.73	264	716983	32.51	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	14.14	163	53730	4.178	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102920\
Data File : BG047121.D
Acq On : 29 Oct 2020 16:38
Operator : CG/JU
Sample : L4499-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW2B8

Quant Time: Oct 29 16:20:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG102220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 29 16:49:45 2020
Response via : Initial Calibration

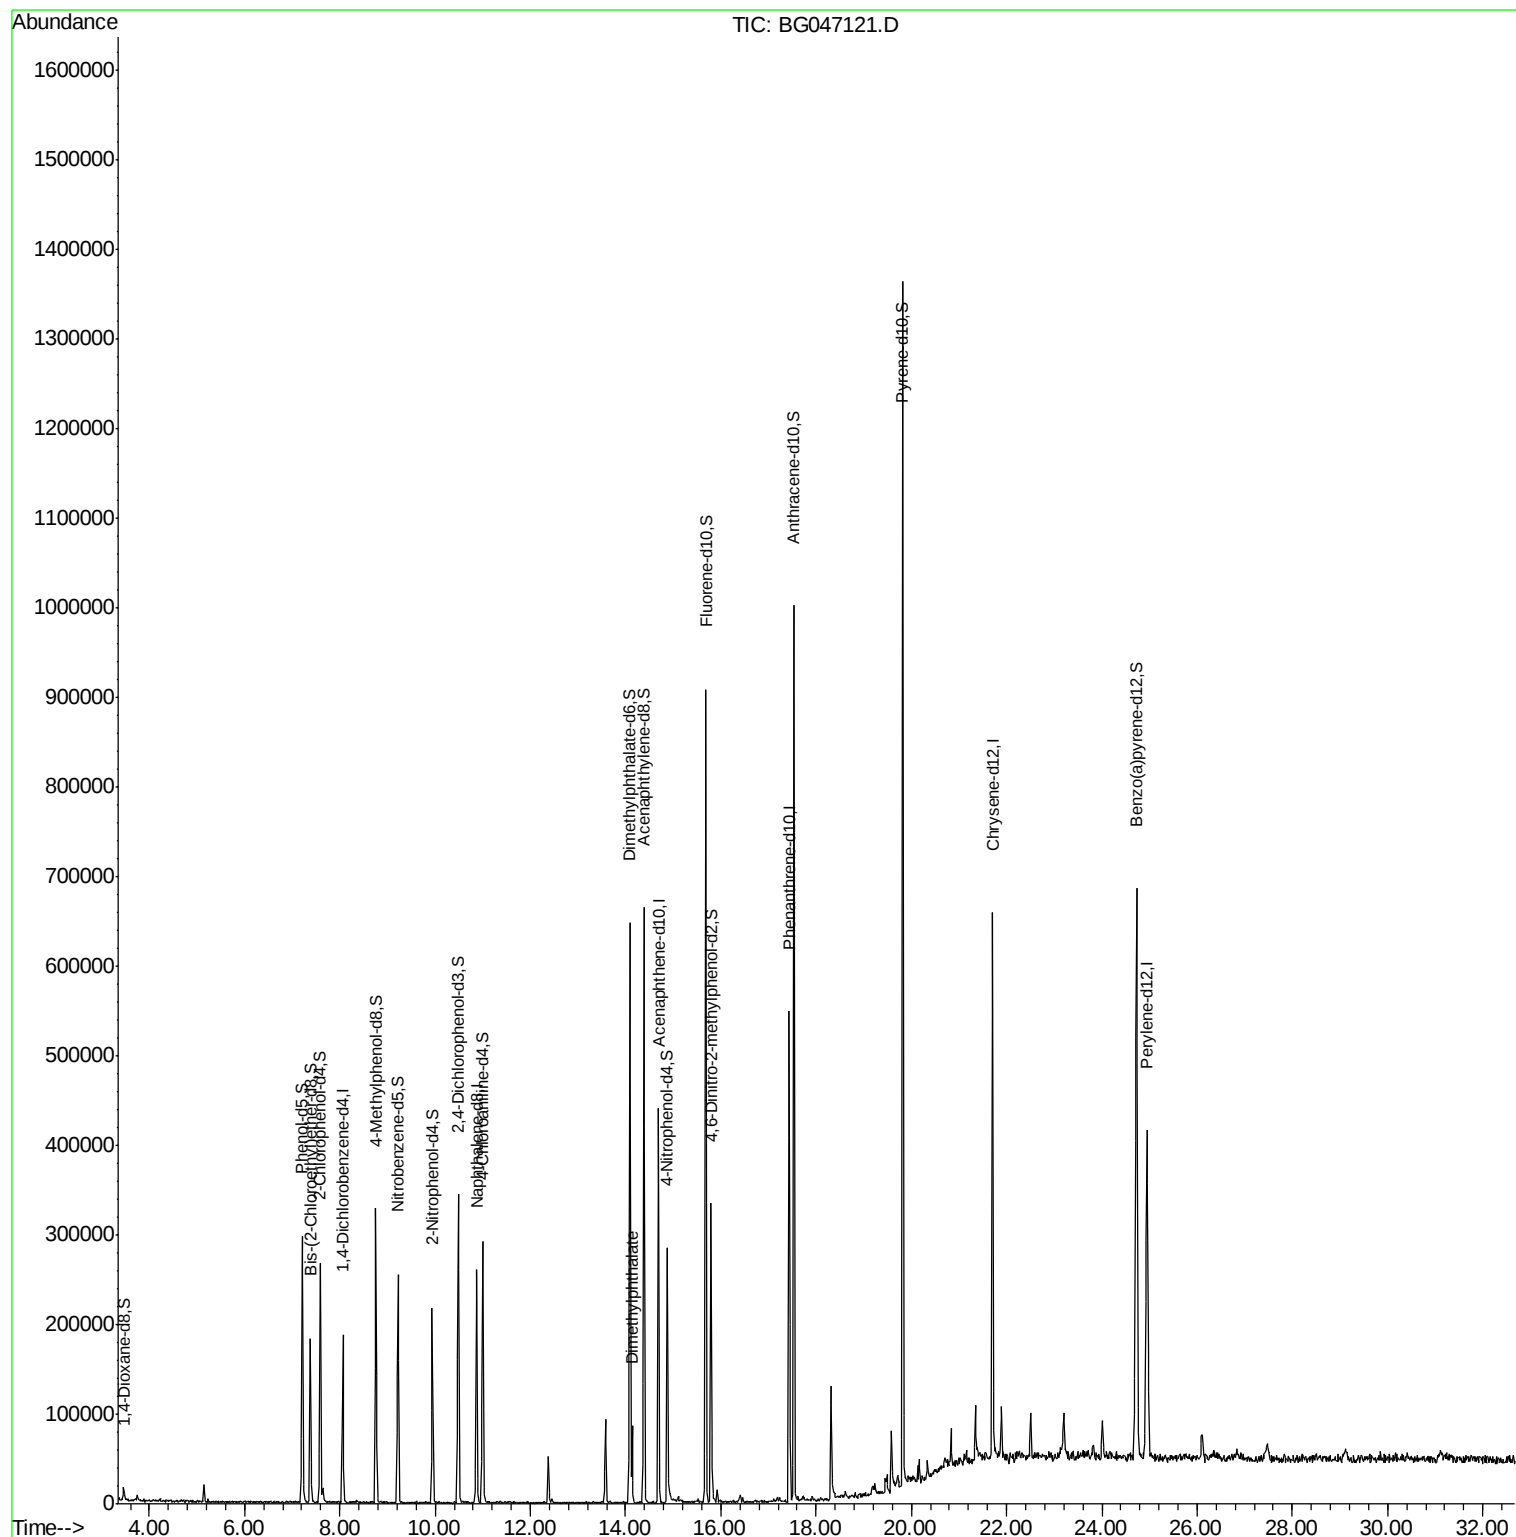

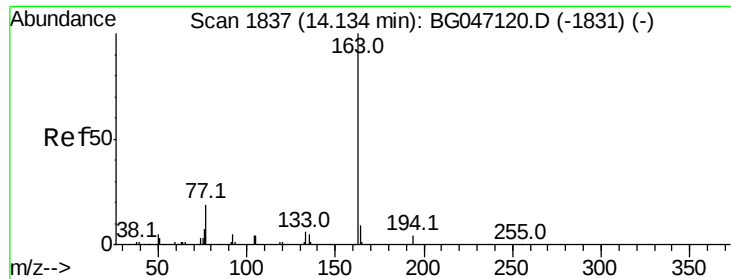

#45

Dimethylphthalate

Concen: 4.178 ng/ul

RT: 14.14 min Scan# 1838

Delta R.T. 0.00 min

Lab File: BG047121.D

Acq: 29 Oct 2020 16:38

Instrument :

BNA_G

ClientSampleId :

EW2B8


Tot Ion:163 Resp: 53730

Ion Ratio Lower Upper

163 100

194 4.9 3.7 5.5

164 9.6 7.9 11.9

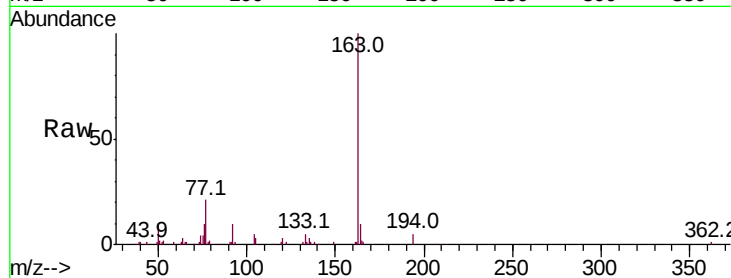

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

