
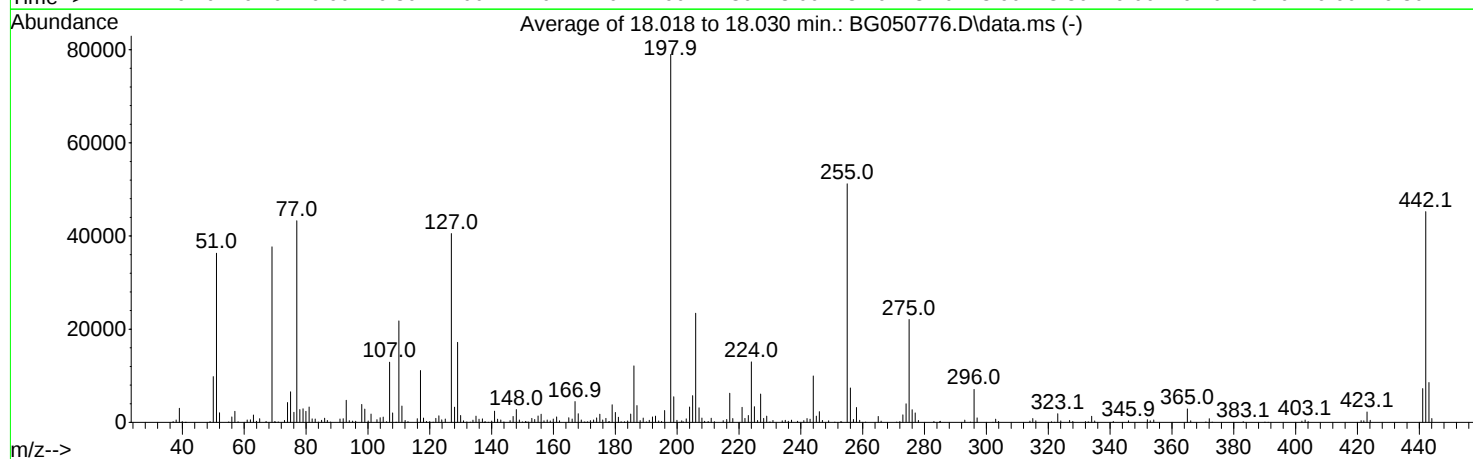


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102921\
 Data File : BG050776.D
 Acq On : 29 Oct 2021 12:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 14 10:56:22 2021

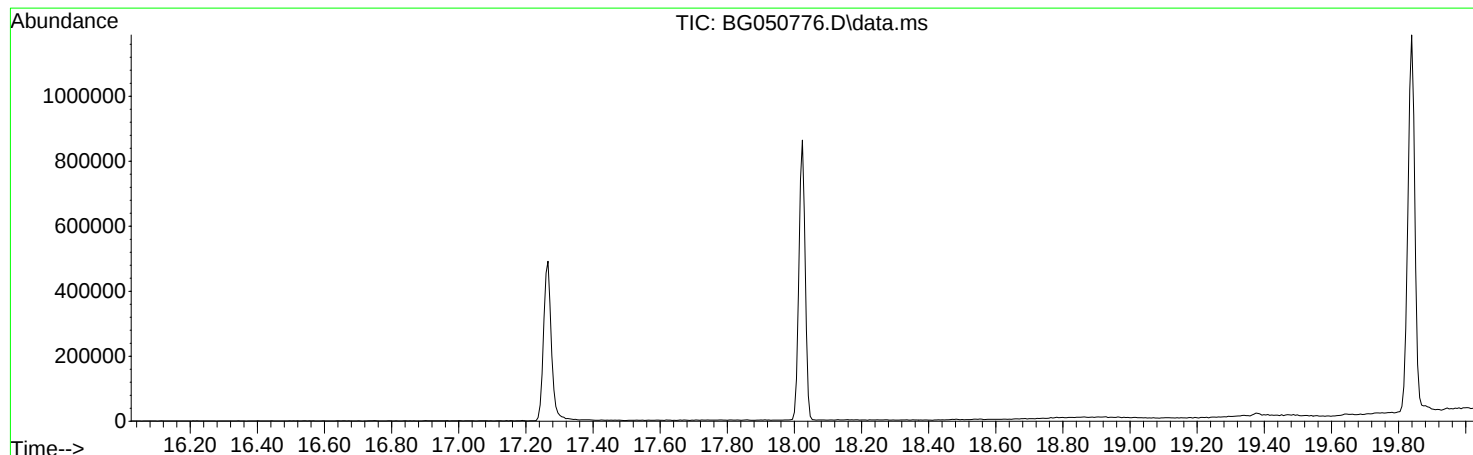

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.0	36315	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	47.7	37685	PASS
70	69	0.00	2	0.5	201	PASS
127	198	10	80	51.3	40528	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	78960	PASS
199	198	5	9	7.0	5510	PASS
275	198	10	60	28.0	22077	PASS
365	198	1	100	3.6	2879	PASS
441	198	0.01	100	9.2	7232	PASS
442	442	50	100	100.0	45237	PASS
443	442	15	24	18.9	8541	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/29/2021	BNA_G	<u>BG050776.D</u>
Compound Name	Response	Retention Time
DDT	254975	21.07
DDD	13071	20.62
DDE	219	20.11
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13290	268265	4.95

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102921\
 Data File : BG050776.D
 Acq On : 29 Oct 2021 12:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Oct 29 16:29:58 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 14 10:56:22 2021
 Response via : Initial Calibration

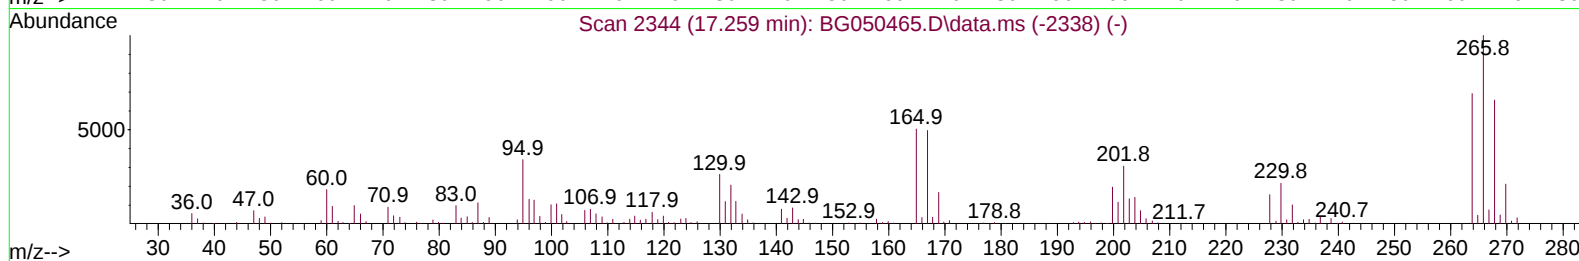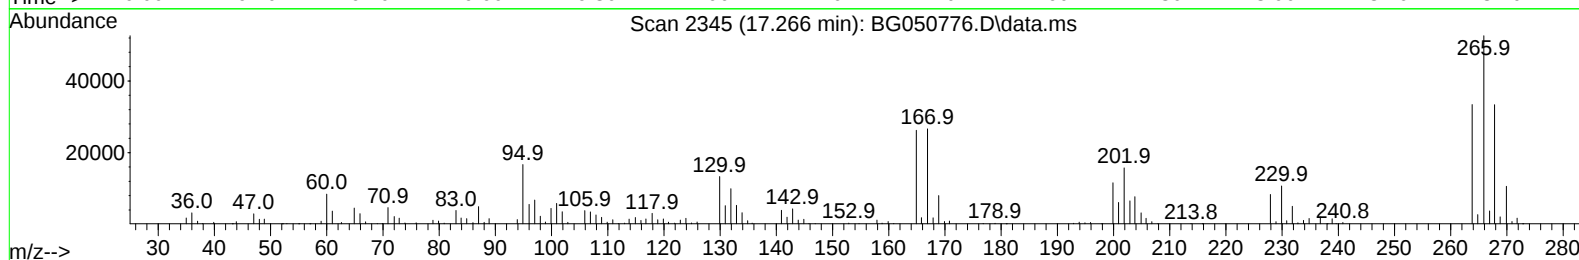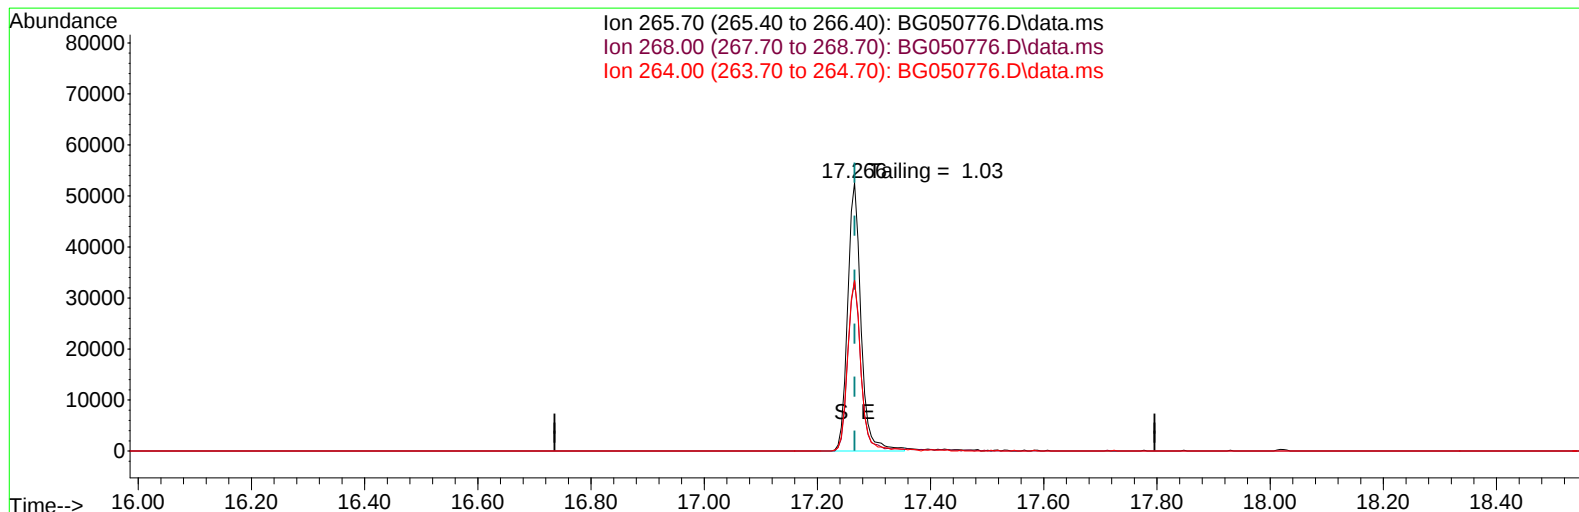

TIC: BG050776.D\data.ms

(70) Pentachlorophenol (C)

17.266min (+ 0.000) 235270.82 ng




response 86618

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.46
264.00	61.30	63.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102921\
Data File : BG050776.D
Acq On : 29 Oct 2021 12:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 29 16:29:58 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

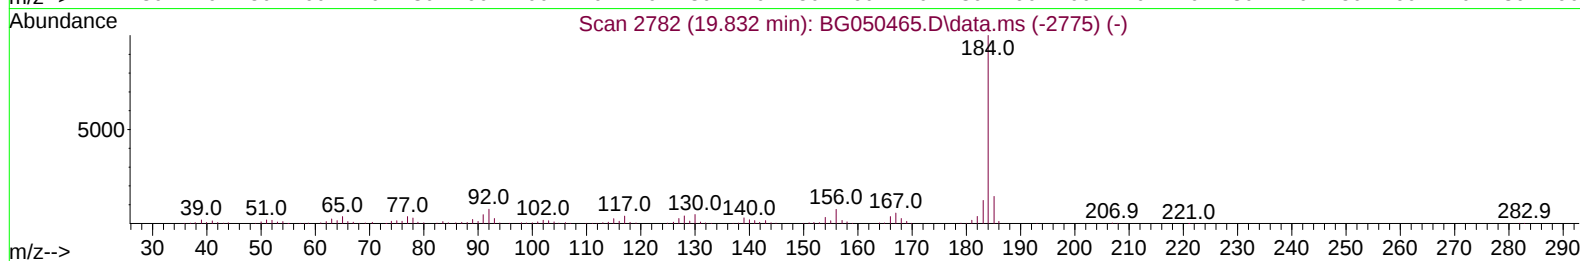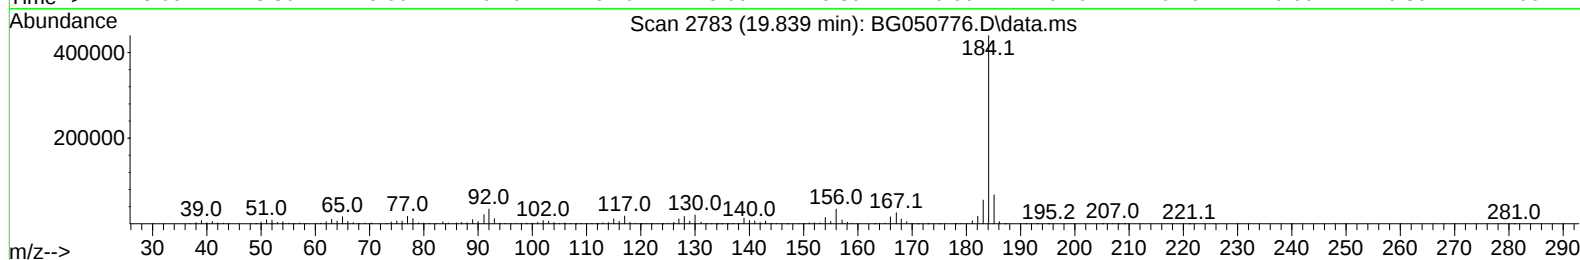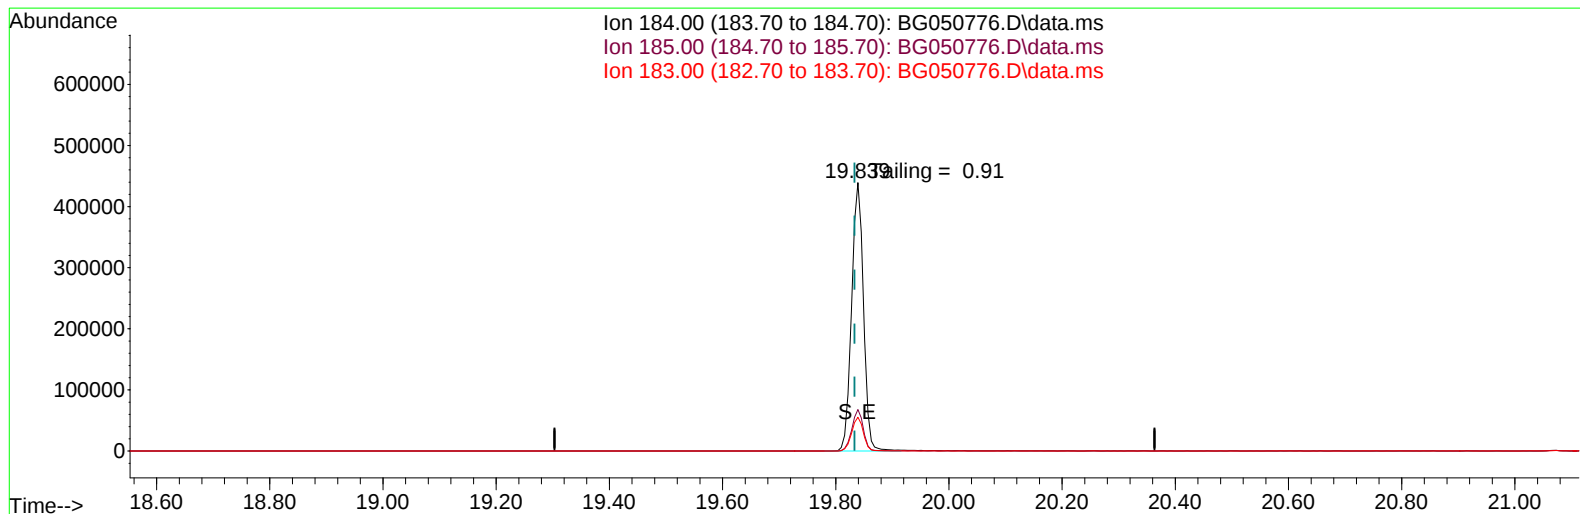

TIC: BG050776.D\data.ms

(77) Benzidine

19.839min (+ 0.006) 17409.17 ng

response 640990

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.43
183.00	11.70	12.62
0.00	0.00	0.00