
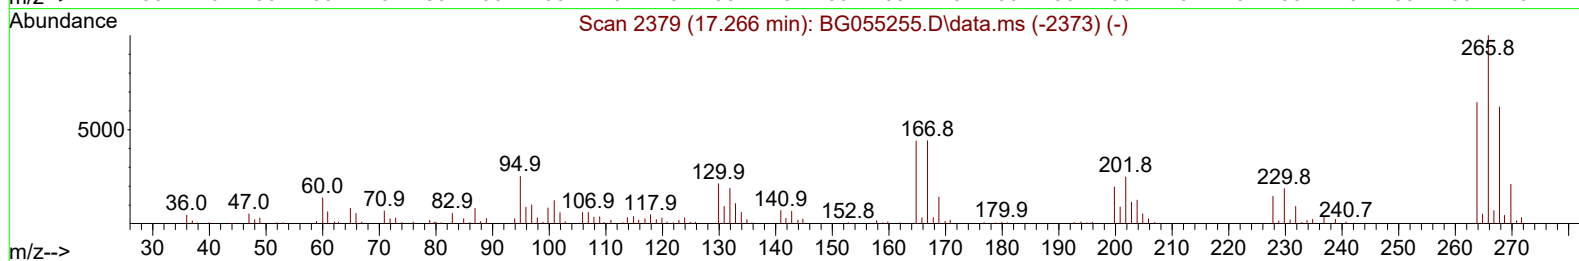
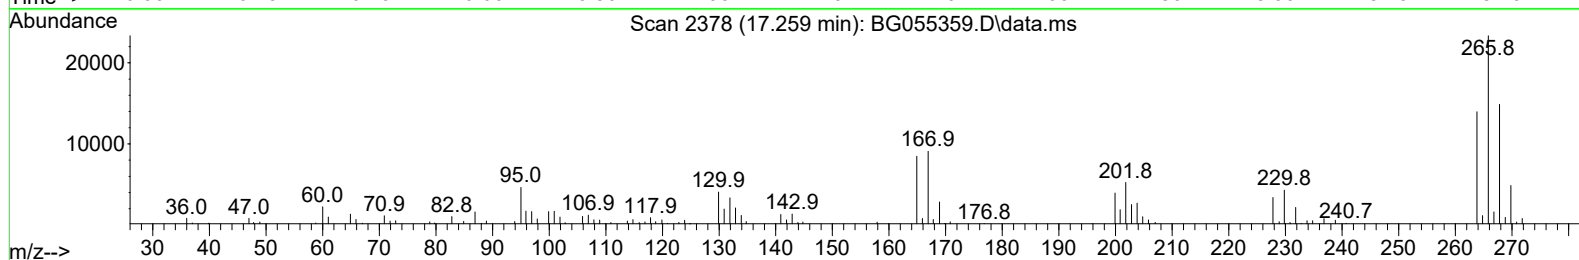


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG102922\  
Data File : BG055359.D  
Acq On : 29 Oct 2022 10:27  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 29 11:04:51 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG102422.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Oct 29 04:52:38 2022  
Response via : Initial Calibration

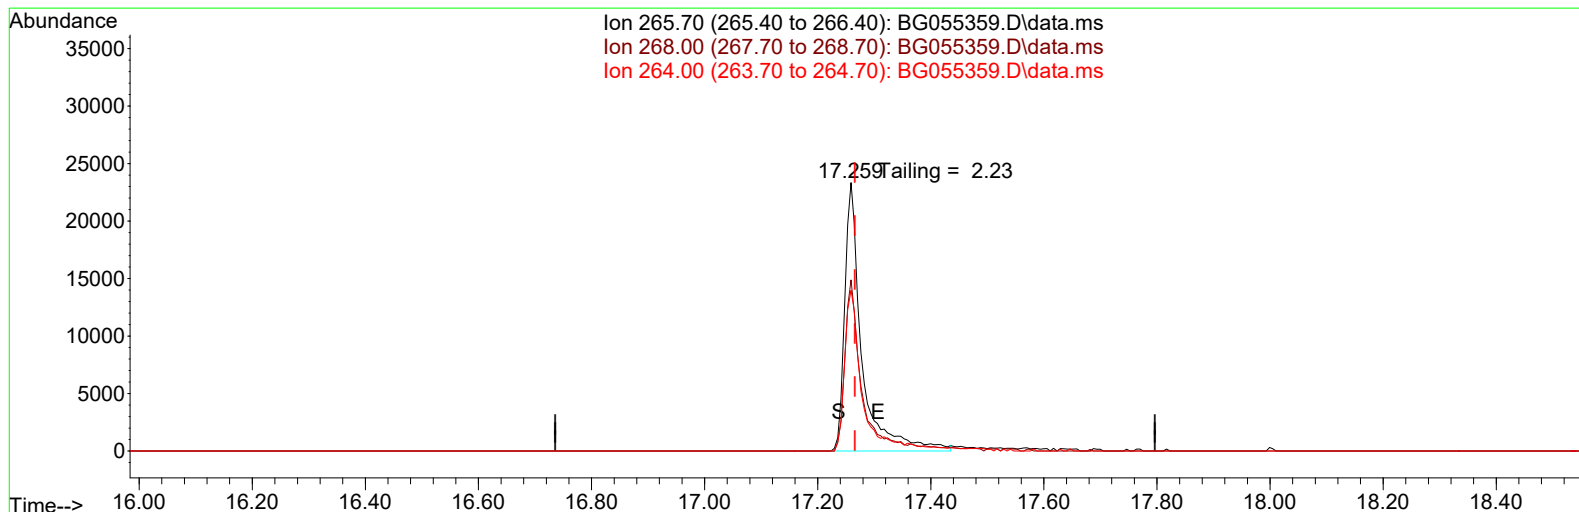

TIC: BG055359.D\data.ms




**(70) Pentachlorophenol (C)**

**17.259min (-0.007) 37945.18 ng**

**response 48396**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 66.50  | 63.76  |
| 264.00 | 64.40  | 59.85  |
| 0.00   | 0.00   | 0.00   |

Quant Time: Oct 29 11:04:51 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG102422.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Oct 29 04:52:38 2022  
Response via : Initial Calibration

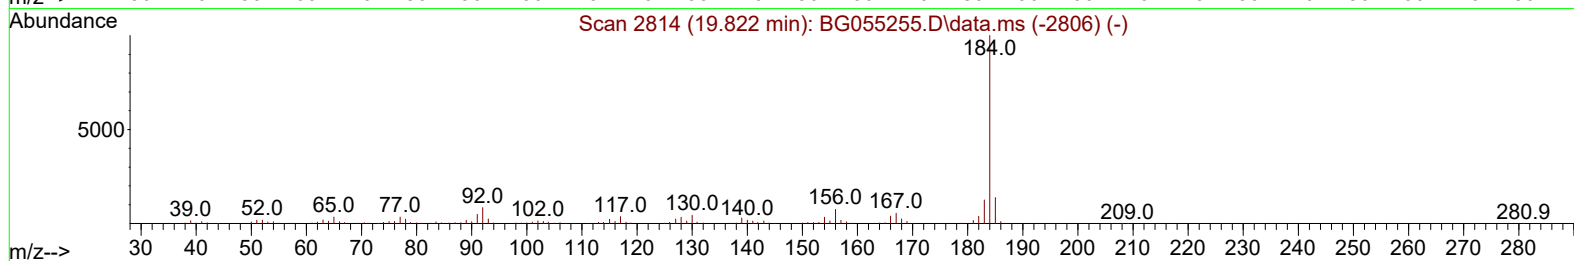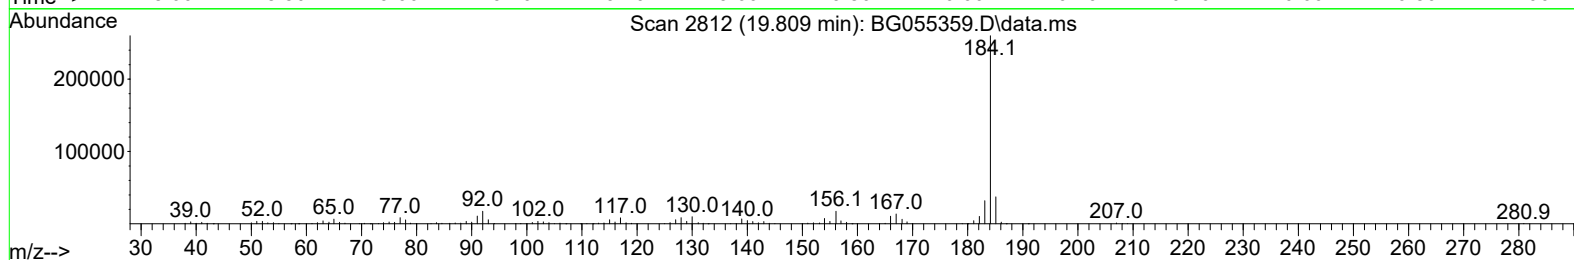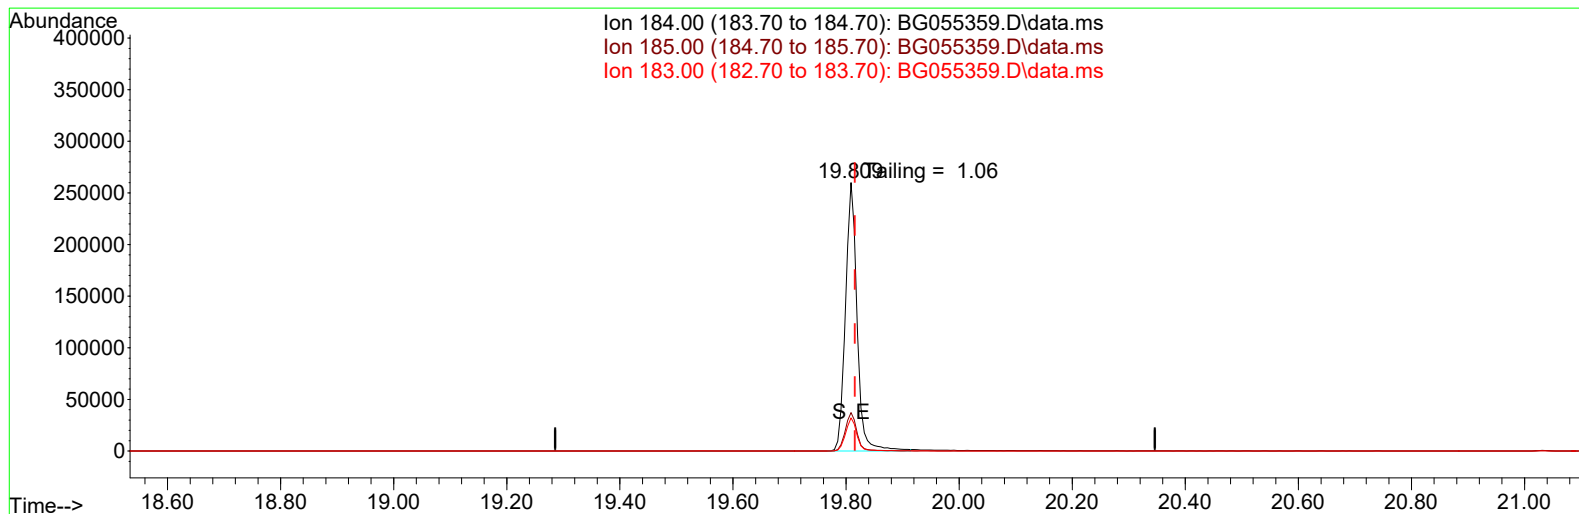

TIC: BG055359.D\data.ms

(77) Benzidine

19.809min (-0.007) 0.00 ng

**response**      **374555**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.80  | 14.35  |
| 183.00 | 12.50  | 12.34  |
| 0.00   | 0.00   | 0.00   |