
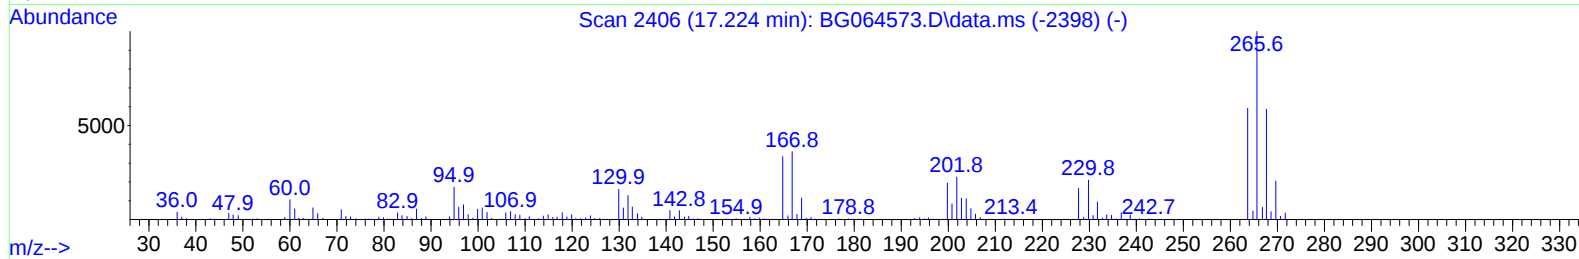
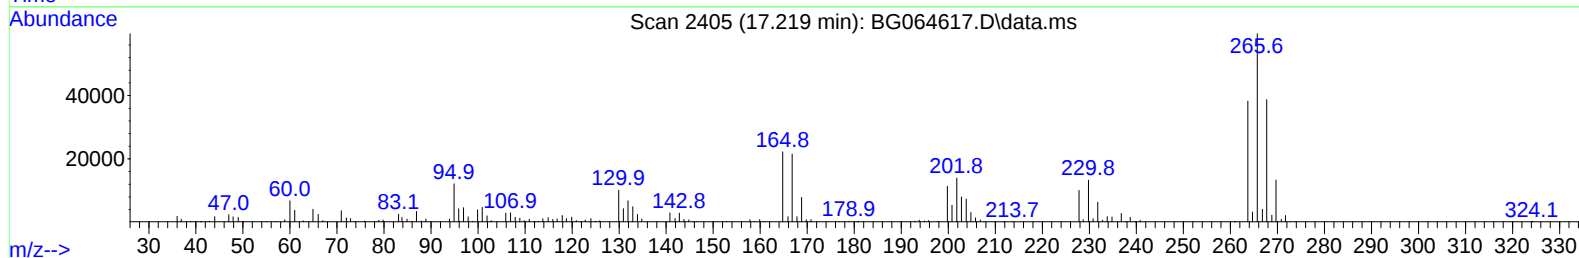


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102925\
Data File : BG064617.D
Acq On : 29 Oct 2025 10:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 29 11:21:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 16:40:26 2025
Response via : Initial Calibration

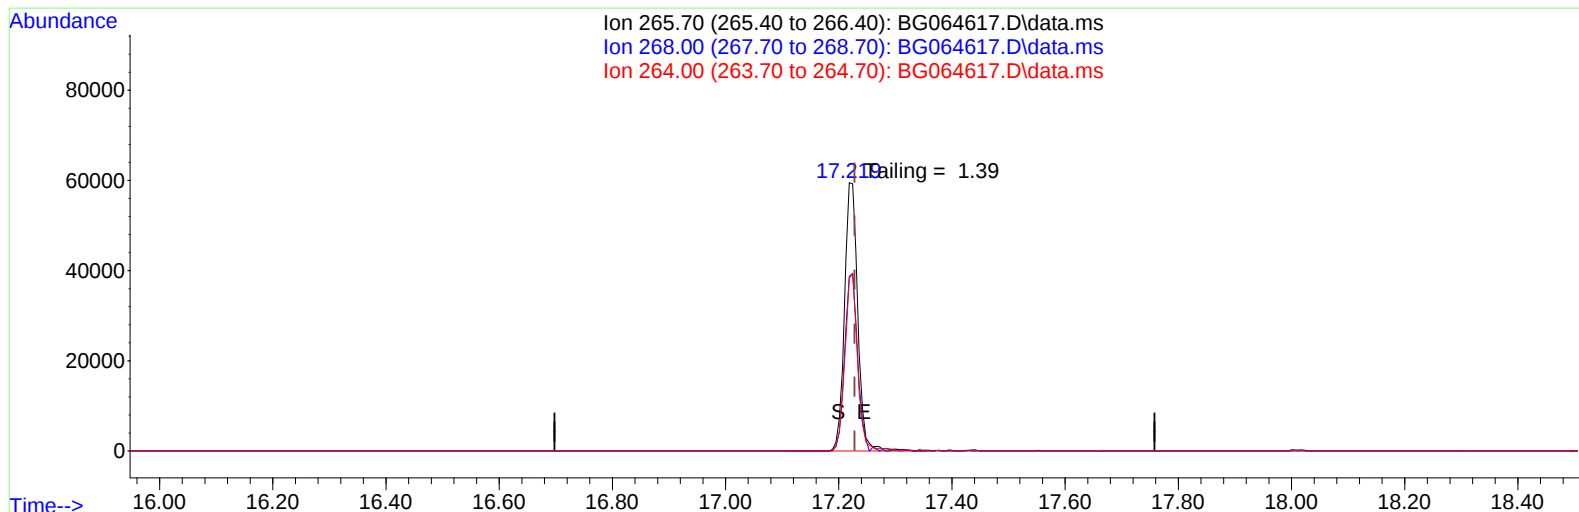

TIC: BG064617.D\data.ms

(70) Pentachlorophenol (C)




17.219min (-0.009) 35052.04 ng

response 97221

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	65.04
264.00	59.10	69.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102925\
Data File : BG064617.D
Acq On : 29 Oct 2025 10:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 29 11:21:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 16:40:26 2025
Response via : Initial Calibration

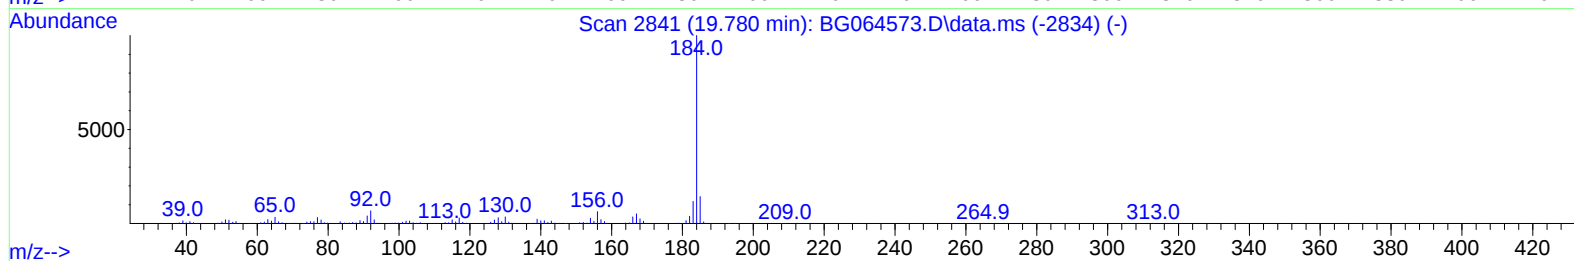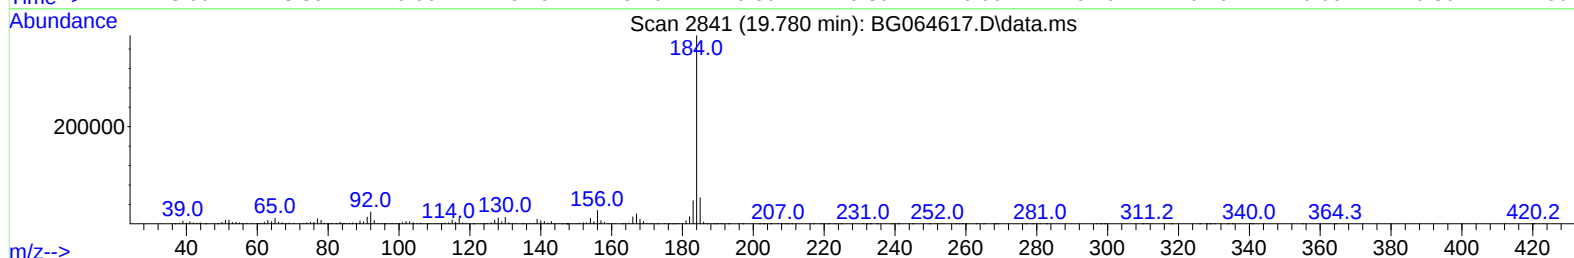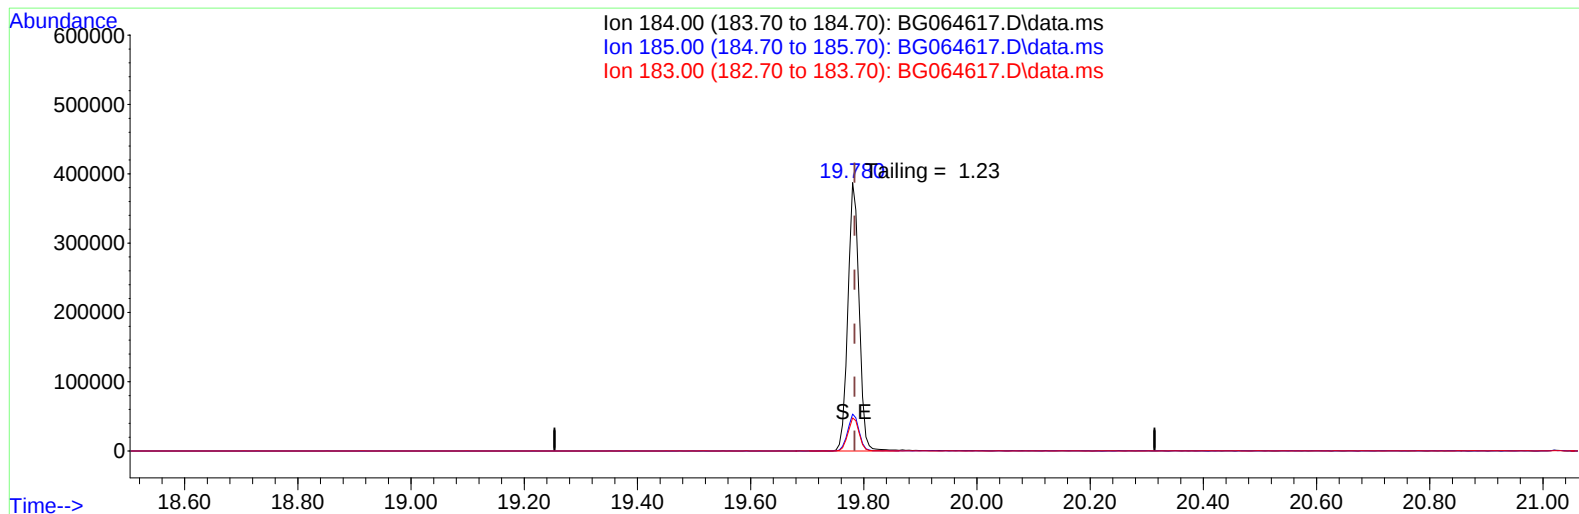

TIC: BG064617.D\data.ms

(77) Benzidine**19.780min (-0.003) 345166.57 ng****response 533588**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.80
183.00	11.80	12.33
0.00	0.00	0.00