
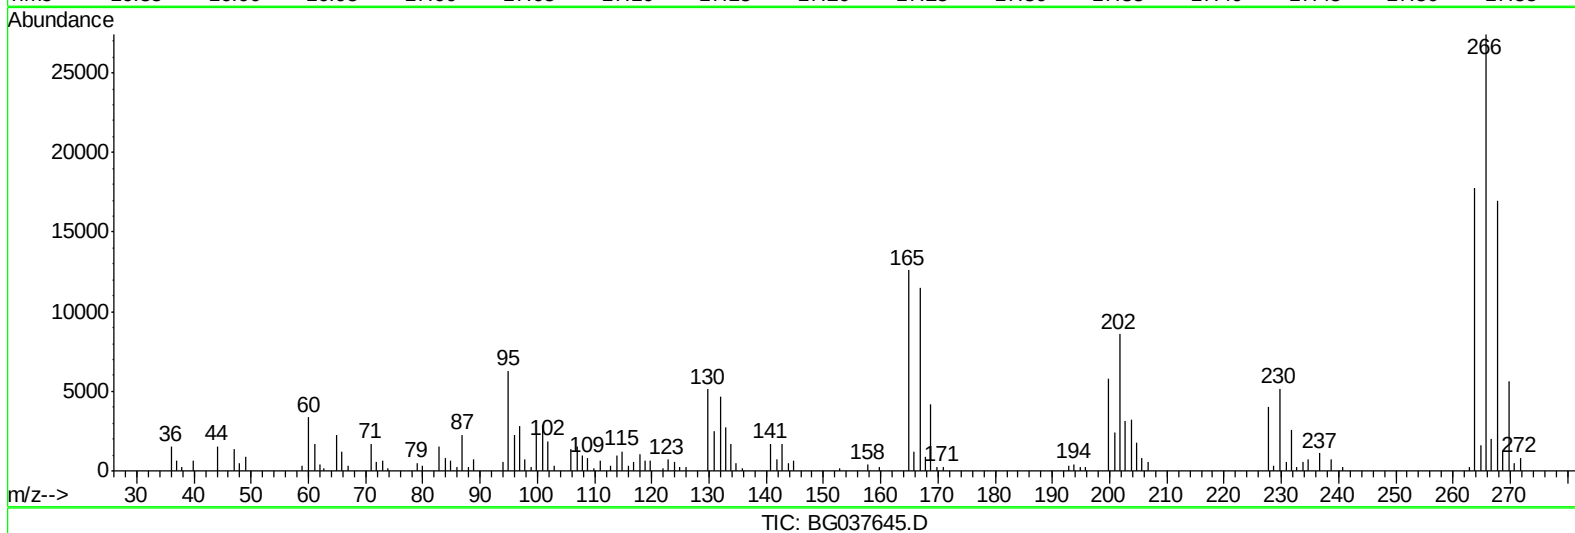


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG103018\
Data File : BG037645.D
Acq On : 30 Oct 2018 9:33
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 31 08:31:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

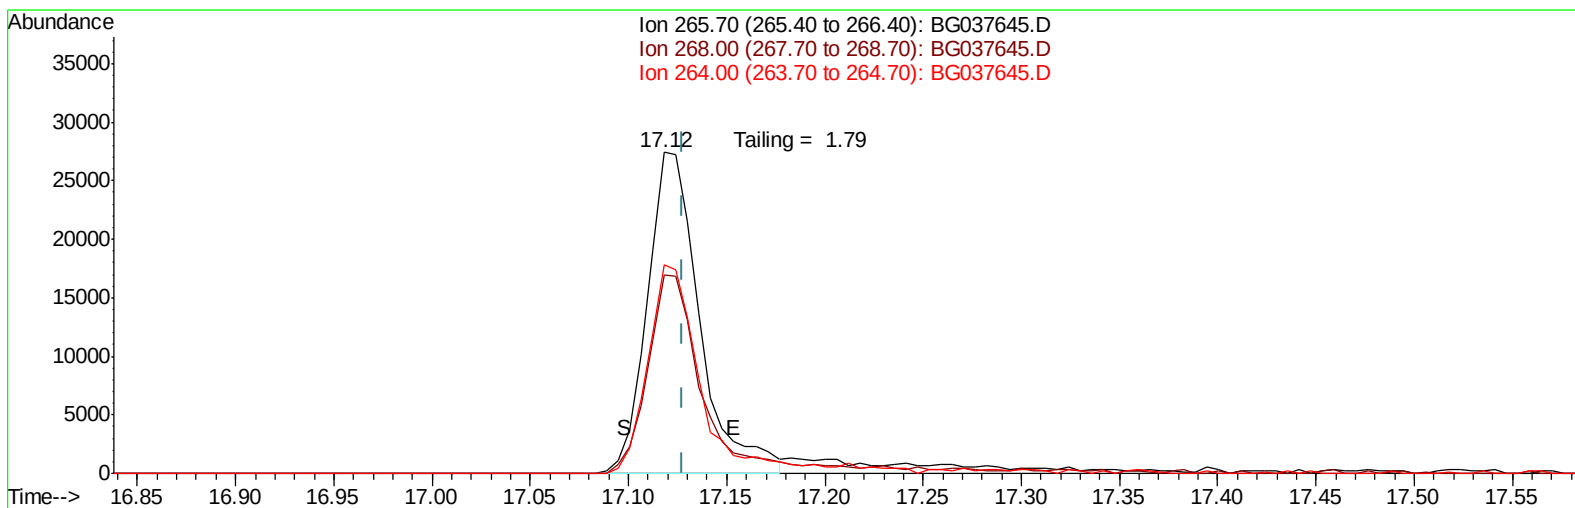

(70) Pentachlorophenol (C)



17.118min (-0.010) 19822.86ng

response 53951

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	66.59
264.00	73.60	64.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG103018\
Data File : BG037645.D
Acq On : 30 Oct 2018 9:33
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 31 08:31:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

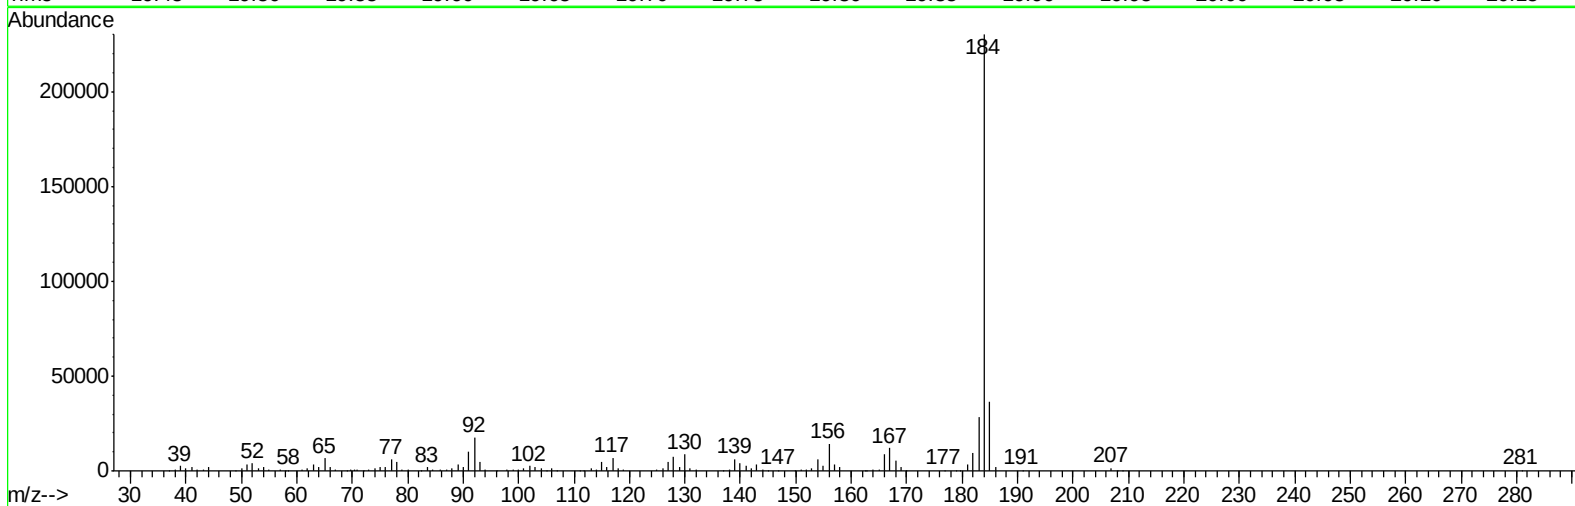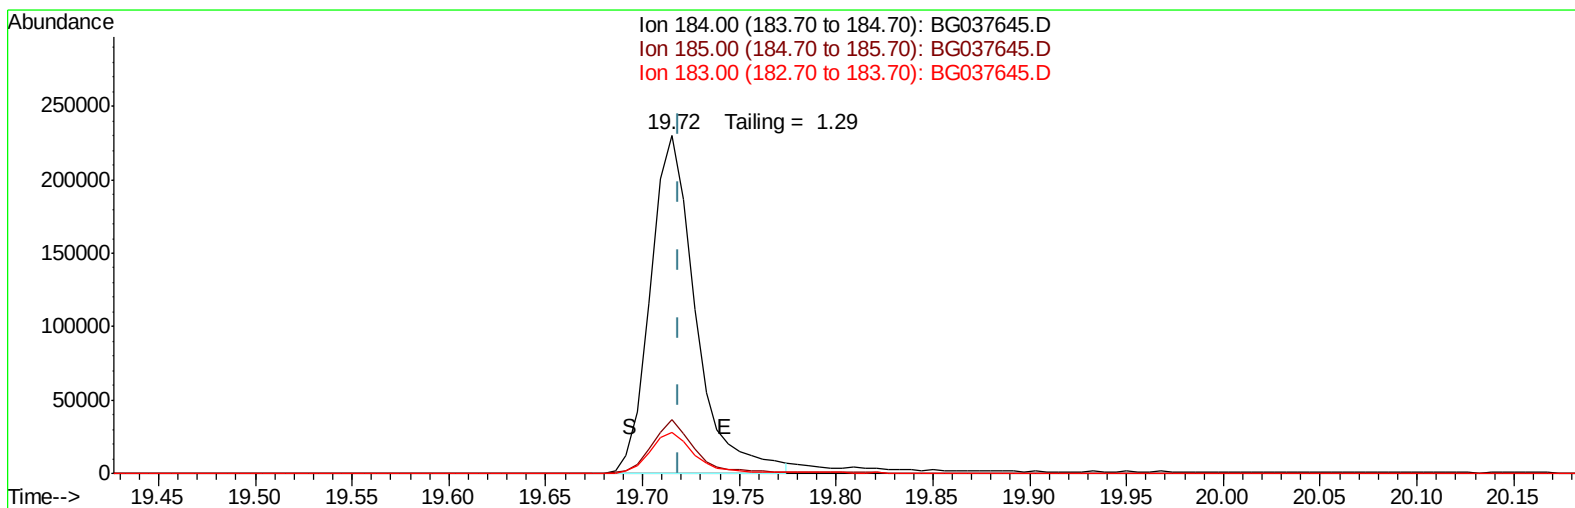

TIC: BG037645.D

(77) Benzidine

19.715min (-0.004) 0.00ng

response 395246

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.86
183.00	12.70	12.32
0.00	0.00	0.00