


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103018\
 Data File : BG037664.D
 Acq On : 30 Oct 2018 22:31
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 18 14:06:42 2018

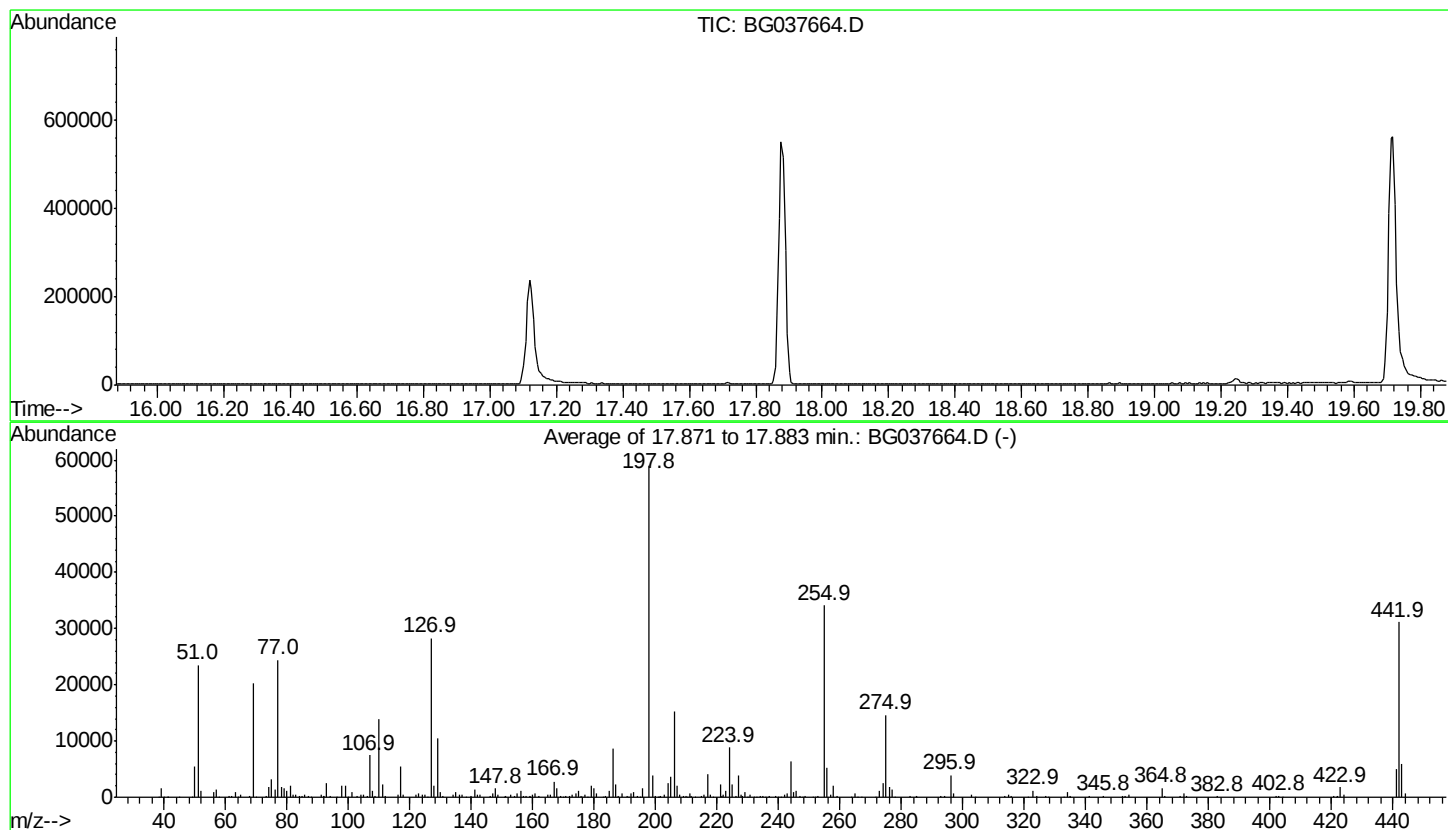

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	23514	PASS
68	69	0.00	2	0.6	126	PASS
69	198	0.00	100	34.2	20170	PASS
70	69	0.00	2	0.3	67	PASS
127	198	10	80	48.1	28346	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58986	PASS
199	198	5	9	6.7	3944	PASS
275	198	10	60	24.8	14623	PASS
365	198	1	100	2.9	1695	PASS
441	198	0.01	100	8.4	4932	PASS
442	198	50	100	52.8	31117	PASS
443	442	15	24	19.3	6002	PASS