

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059550.D
 Acq On : 30 Oct 2023 18:08
 Operator : MA/JU
 Sample : PB156396BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK396

Quant Time: Oct 31 05:04:37 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.358	152	66129	20.000	ng/ul	0.00
20) Naphthalene-d8	11.208	136	314725	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.986	164	274698	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.842	188	954766	20.000	ng/ul	0.10
79) Chrysene-d12	22.078	240	475822	20.000	ng/ul	0.00
88) Perylene-d12	25.685	264	524562	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.652	96	11664	6.599	ng/uL	0.00
4) Pyridine-d5	4.093	84	147275	29.818	ng/ul	0.00
7) Phenol-d5	7.465	99	204272	30.060	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.677	67	89377	28.635	ng/ul	0.00
11) 2-Chlorophenol-d4	7.871	132	166995	30.291	ng/ul	0.00
15) 4-Methylphenol-d8	9.040	113	164783	30.565	ng/ul	0.00
21) Nitrobenzene-d5	9.557	128	77858	34.792	ng/ul	0.00
24) 2-Nitrophenol-d4	10.280	143	85721	37.314	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.803	165	156154	30.851	ng/ul	0.00
31) 4-Chloroaniline-d4	11.349	131	250122	30.019	ng/ul	0.00
46) Dimethylphthalate-d6	14.387	166	611536	24.573	ng/ul	0.00
49) Acenaphthylene-d8	14.692	160	864525	29.601	ng/ul	0.00
54) 4-Nitrophenol-d4	15.151	143	136065	31.882	ng/ul	0.00
60) Fluorene-d10	15.979	176	594644	27.959	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.214	200	131	0.029	ng/ul	0.13
73) Anthracene-d10	17.842	188	954766	18.458	ng/ul	0.00
81) Pyrene-d10	20.109	212	1001402	30.278	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.438	264	899838	29.131	ng/ul	0.00
Target Compounds						
17) N-Nitroso-di-n-propyla...	9.052	70	4799	1.198	ng/ul#	Qvalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
Data File : BG059550.D
Acq On : 30 Oct 2023 18:08
Operator : MA/JU
Sample : PB156396BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK396


Quant Time: Oct 31 05:04:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 28 03:56:42 2023
Response via : Initial Calibration

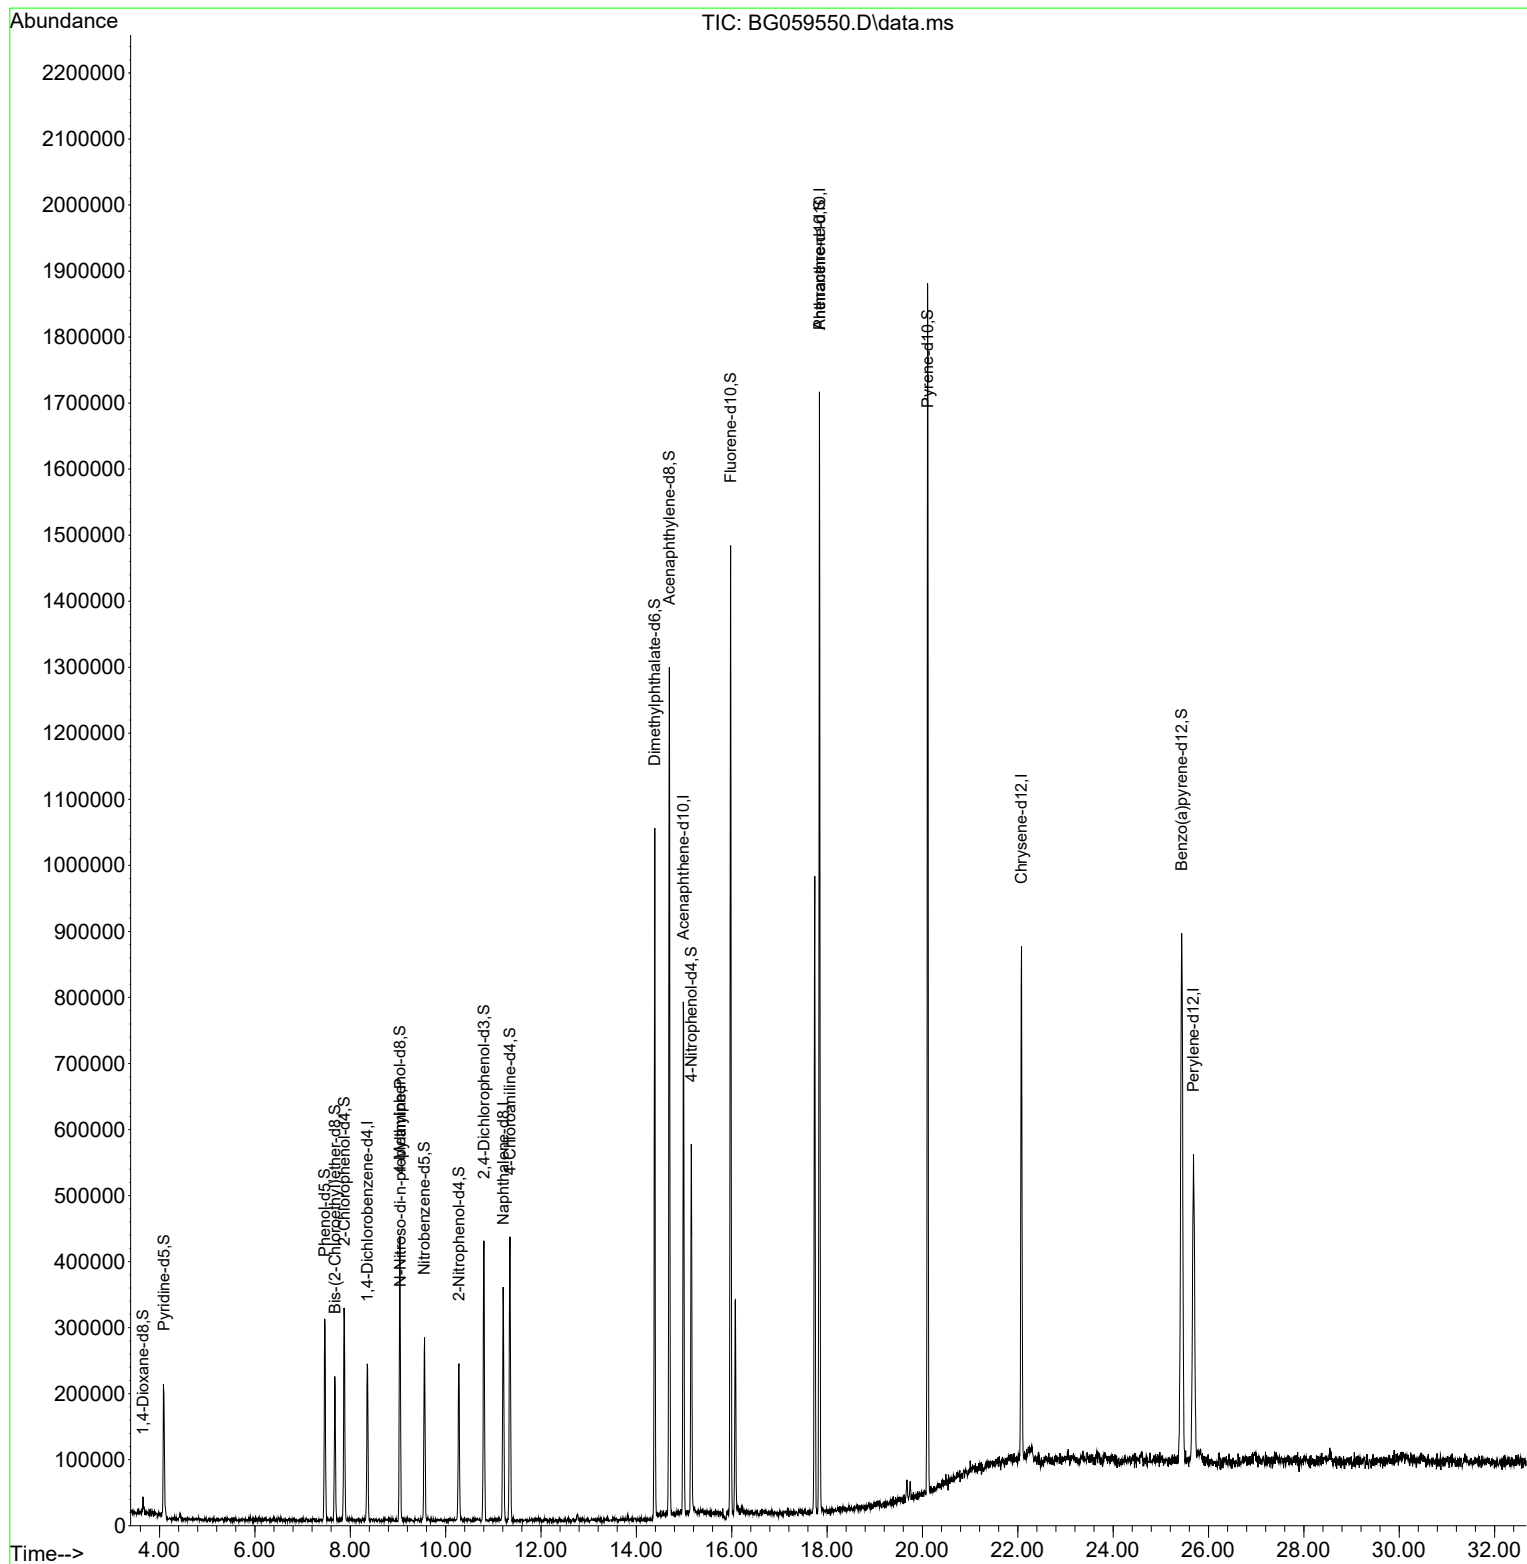

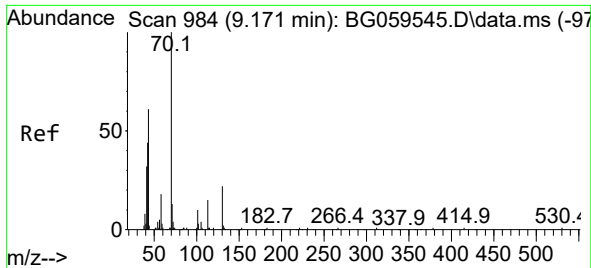

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.198 ng/ul
 RT: 9.052 min Scan# 90
 Delta R.T. -0.120 min
 Lab File: BG059550.D
 Acq: 30 Oct 2023 18:08

Instrument :
 BNA_G
 ClientSampleId :
 SBLK396

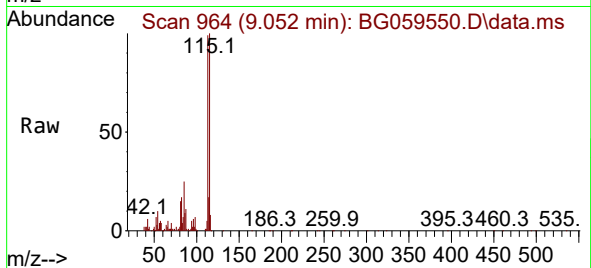

Tgt Ion: 70 Resp: 4799

Ion	Ratio	Lower	Upper
70	100		
42	141.4	33.8	50.8#
101	0.0	5.4	8.0#
130	0.0	18.2	27.4#

