




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059545.D
 Acq On : 30 Oct 2023 12:03
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:06:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
 Supervised By :mohammad ahmed 11/01/2023

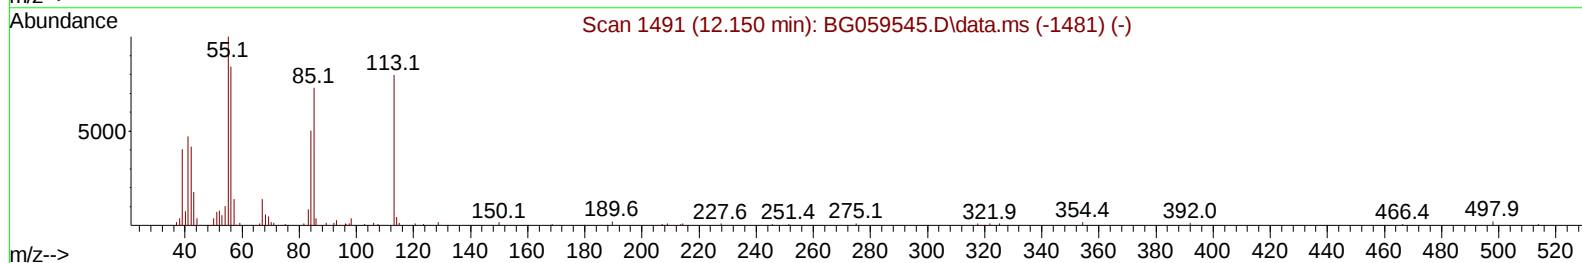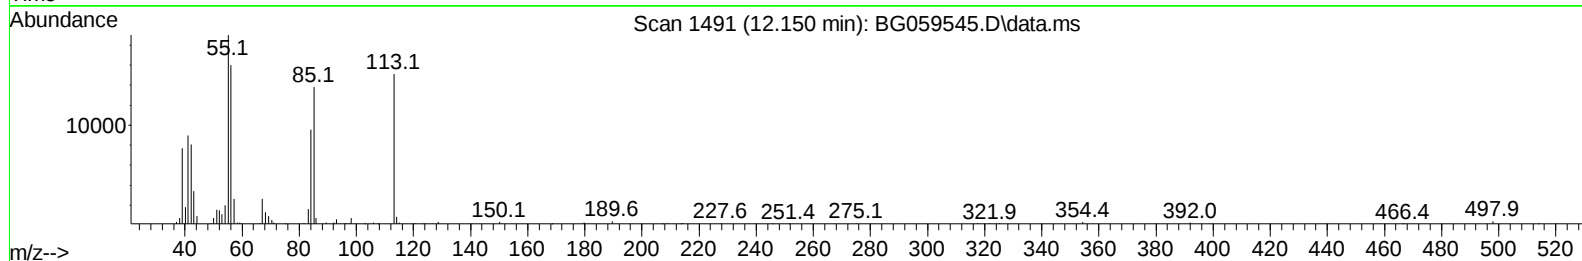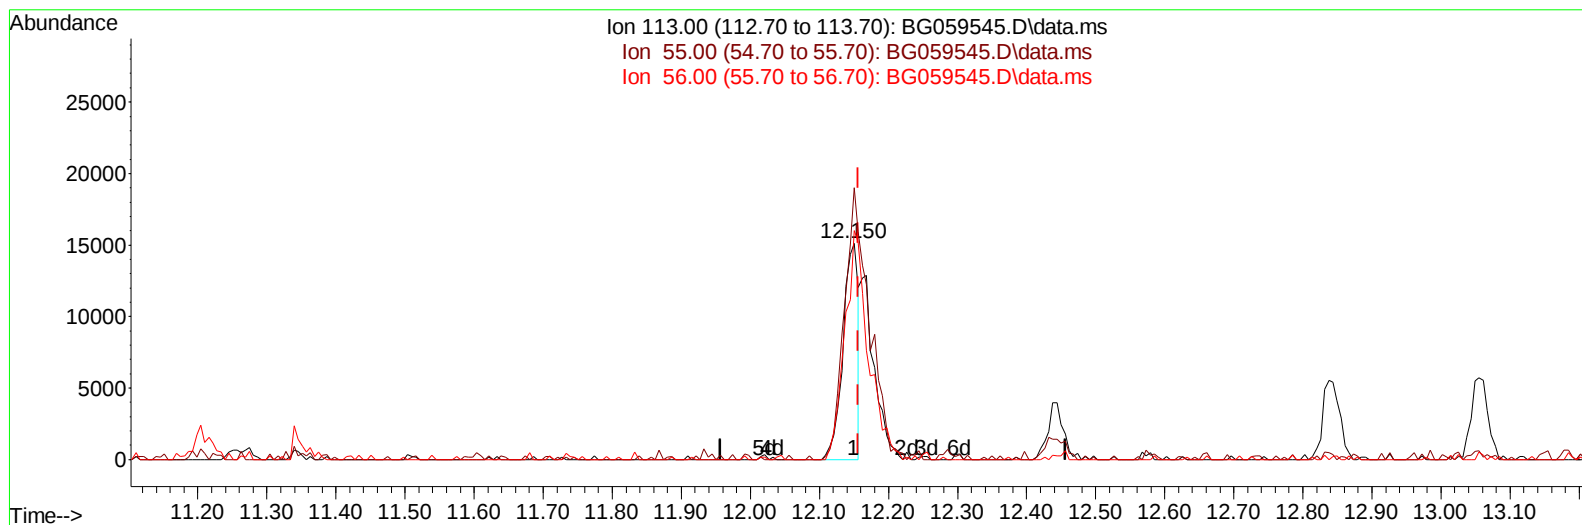

TIC: BG059545.D\data.ms

(34) Caprolactam

12.150min (-0.007) 10.99 ng/ul

response 23320

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	108.60	125.54
56.00	80.50	105.76#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059545.D
 Acq On : 30 Oct 2023 12:03
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:06:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
 Supervised By :mohammad ahmed 11/01/2023

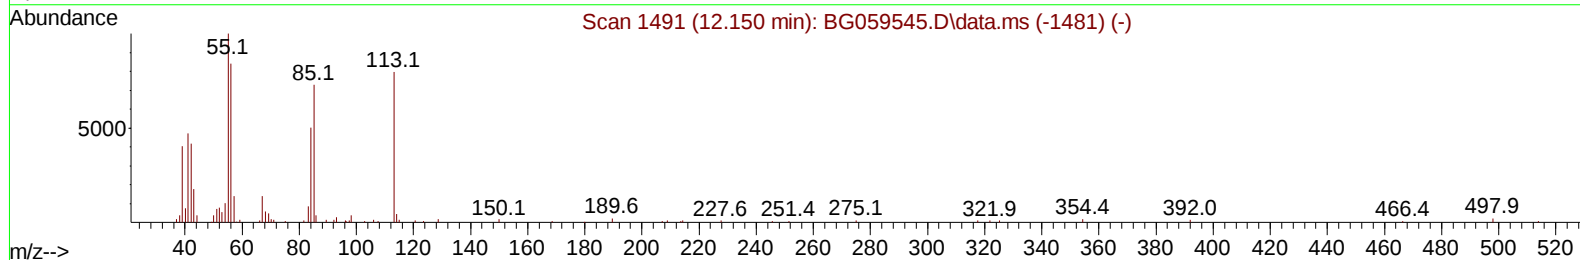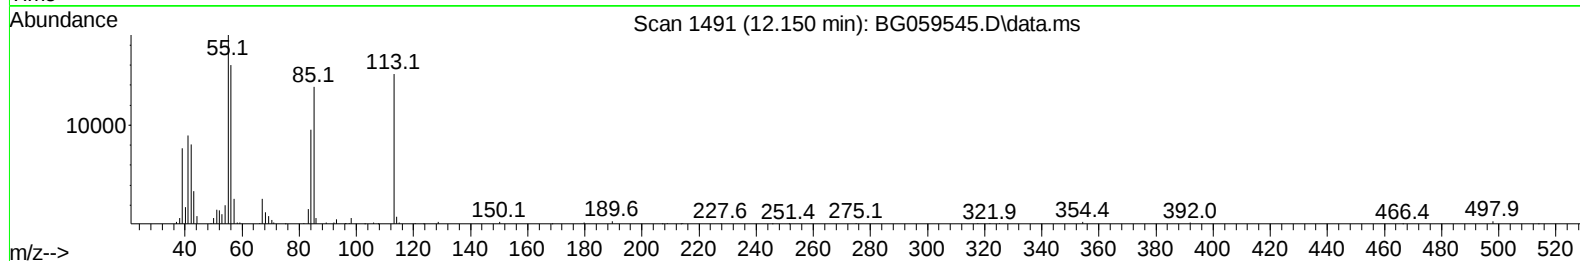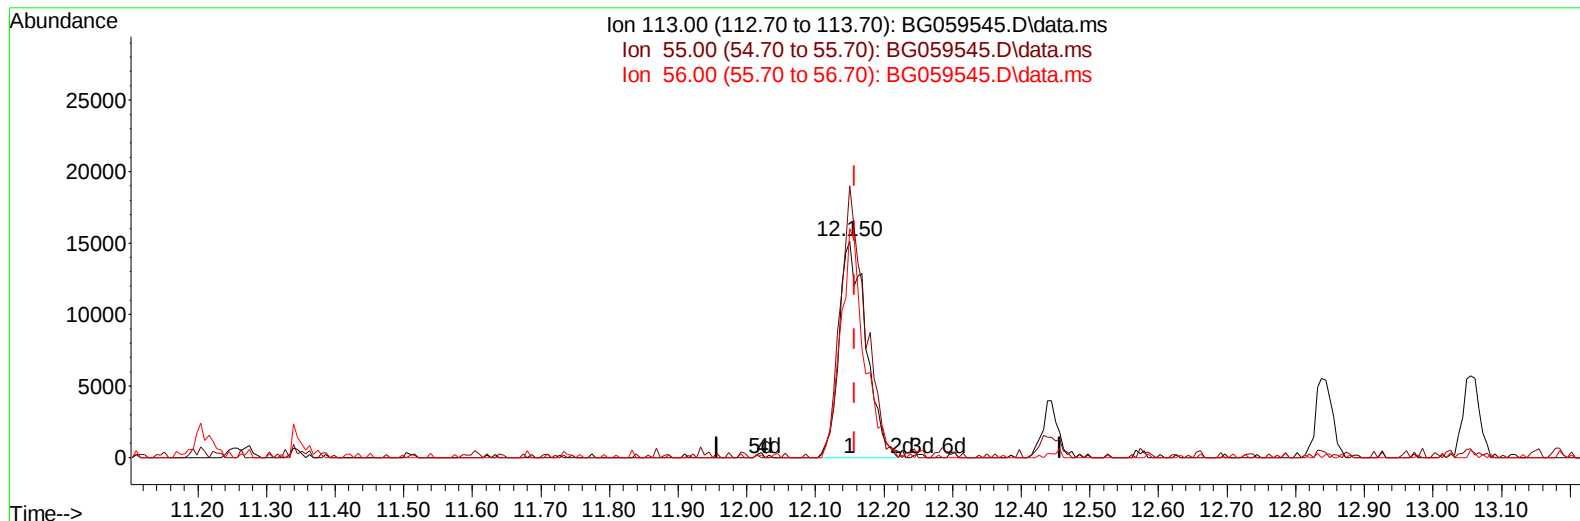

TIC: BG059545.D\data.ms

(34) Caprolactam

12.150min (-0.007) 19.39 ng/ul m

response 41162

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	108.60	125.54
56.00	80.50	105.76#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059545.D
 Acq On : 30 Oct 2023 12:03
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:06:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
 Supervised By :mohammad ahmed 11/01/2023

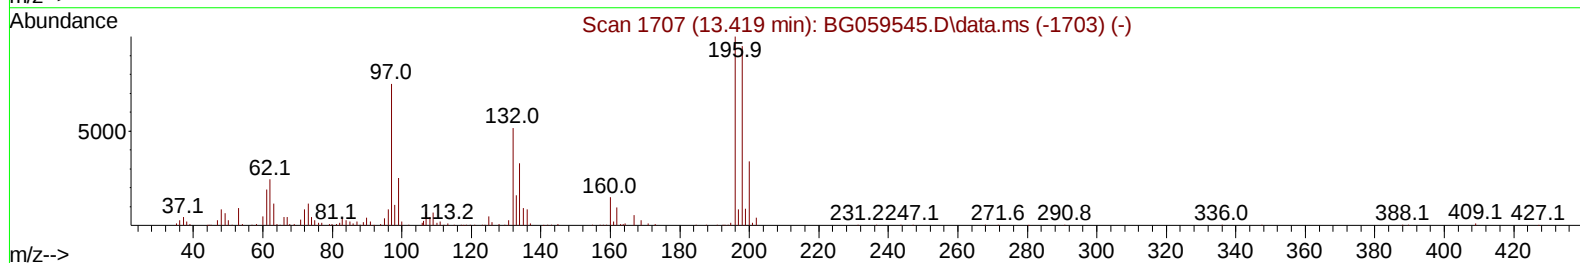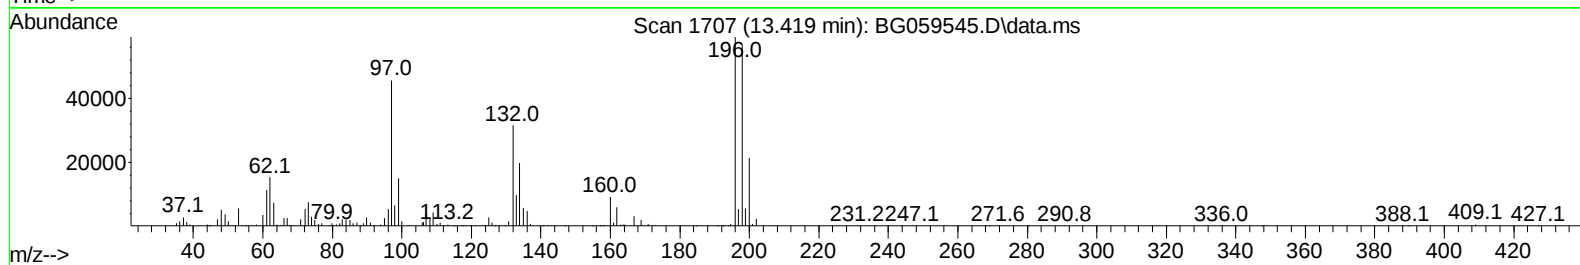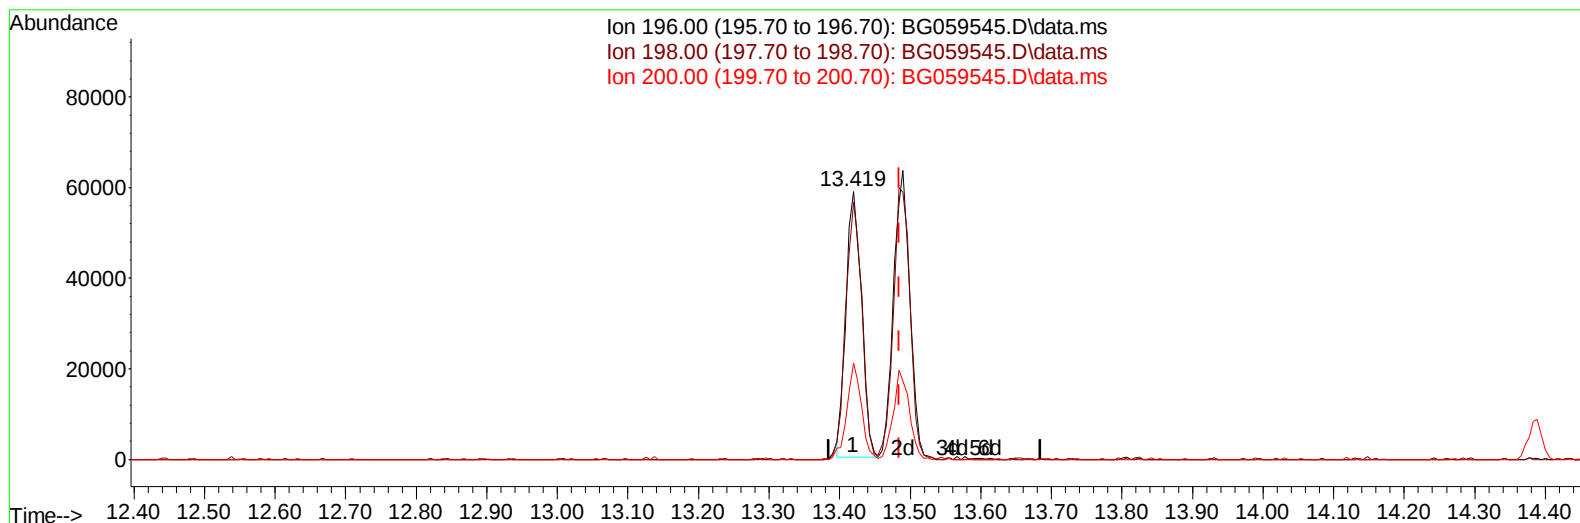

TIC: BG059545.D\data.ms

(42) 2,4,5-Trichlorophenol

13.419min (-0.065) 17.94 ng/u1

response 90013

Ion	Exp%	Act%
196.00	100.00	100.00
198.00	99.70	96.02
200.00	35.00	36.04
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059545.D
 Acq On : 30 Oct 2023 12:03
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:06:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
 Supervised By :mohammad ahmed 11/01/2023

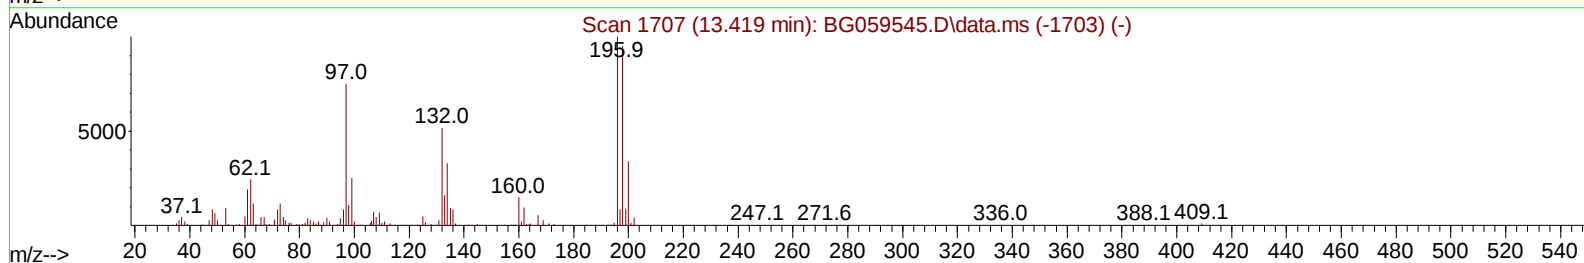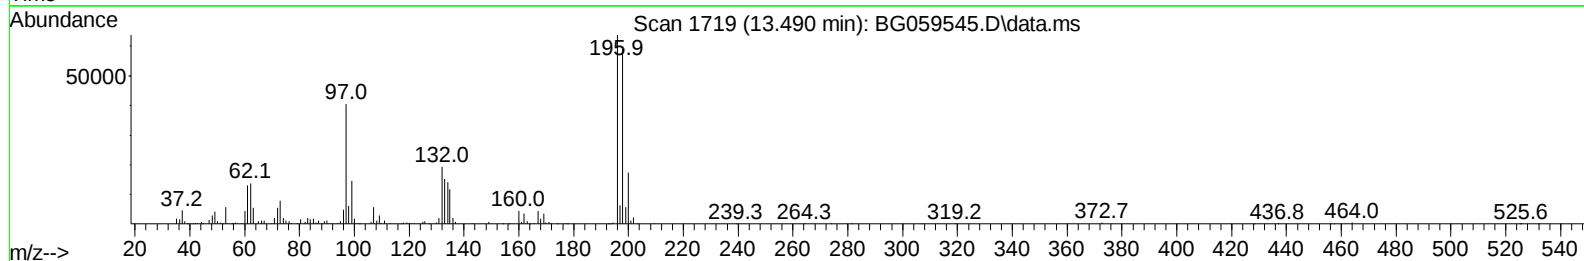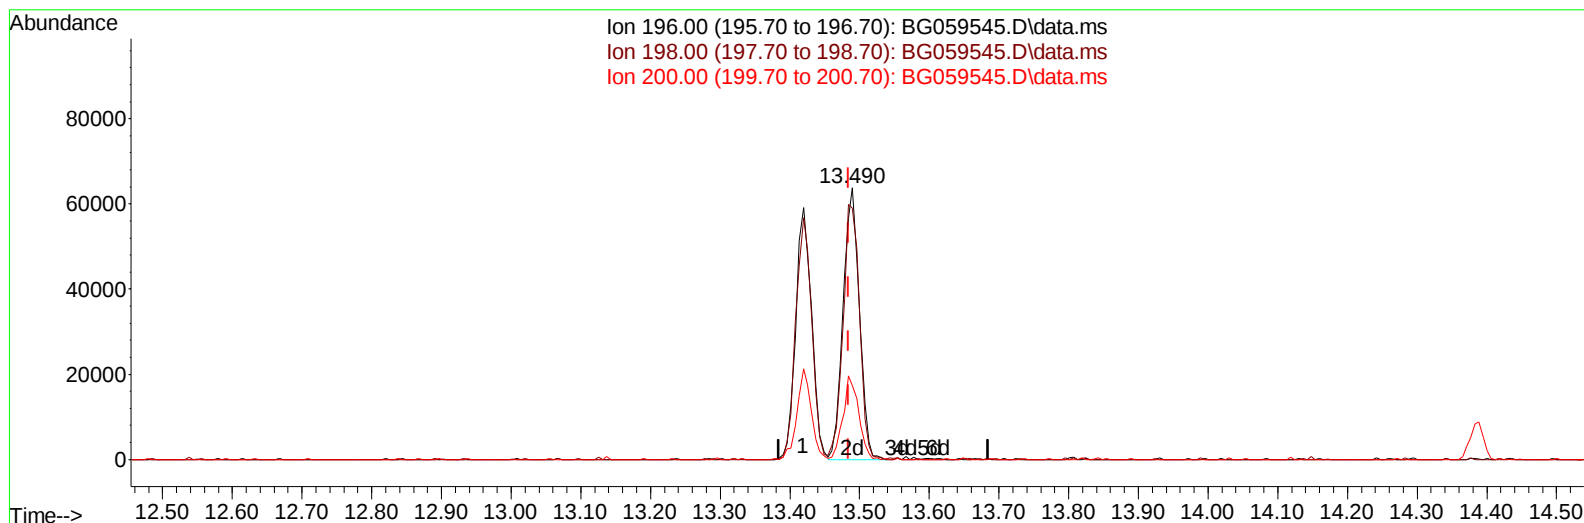

TIC: BG059545.D\data.ms

(42) 2,4,5-Trichlorophenol

13.490min (+ 0.005) 20.55 ng/ul m

response 103134

Ion	Exp%	Act%
196.00	100.00	100.00
198.00	99.70	92.47
200.00	35.00	27.18#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059545.D
 Acq On : 30 Oct 2023 12:03
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:06:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
 Supervised By :mohammad ahmed 11/01/2023

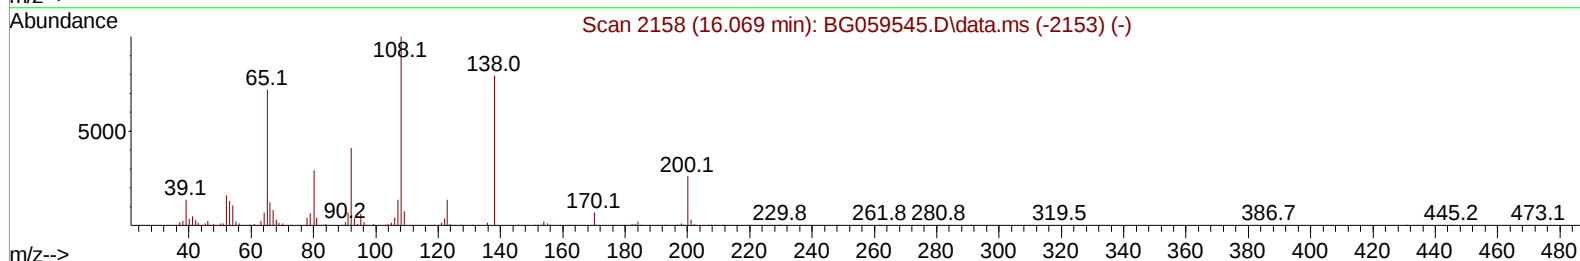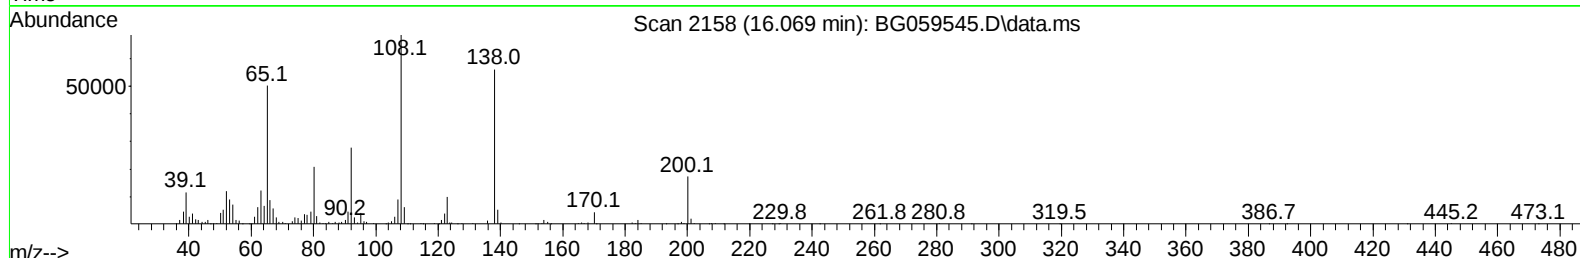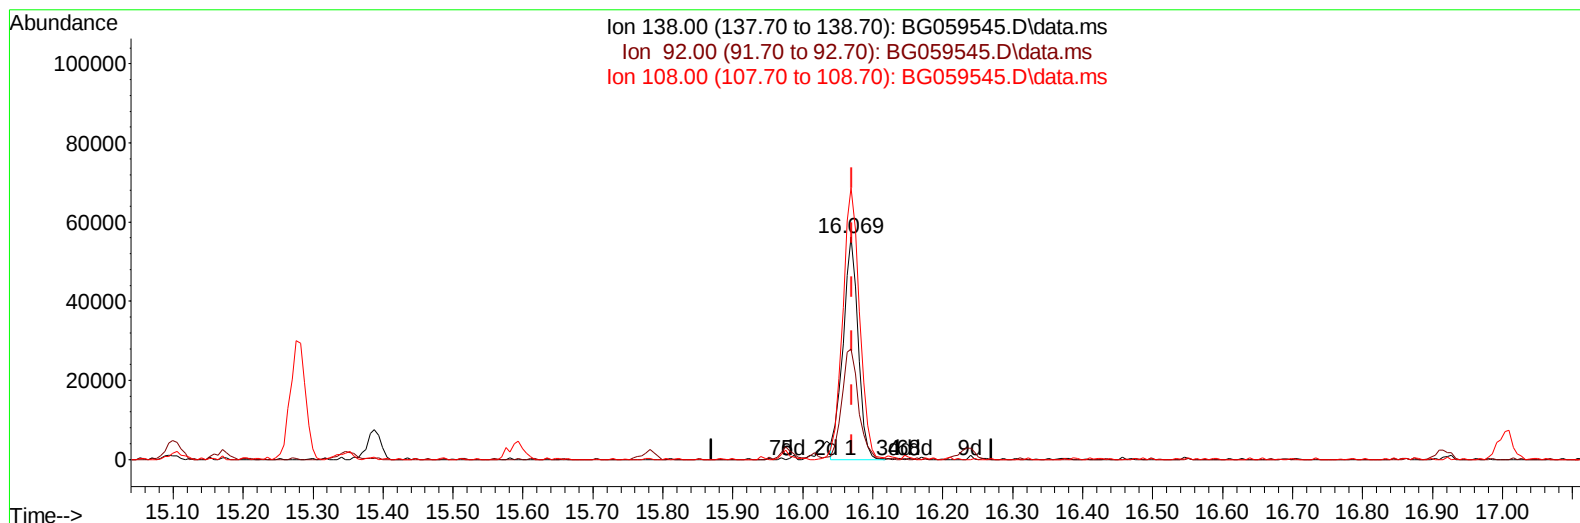

TIC: BG059545.D\data.ms

(63) 4-Nitroaniline

16.069min (-0.001) 20.34 ng/ul

response 84301

Ion	Exp%	Act%
138.00	100.00	100.00
92.00	62.30	49.64#
108.00	126.10	122.16
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059545.D
 Acq On : 30 Oct 2023 12:03
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:06:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
 Supervised By :mohammad ahmed 11/01/2023

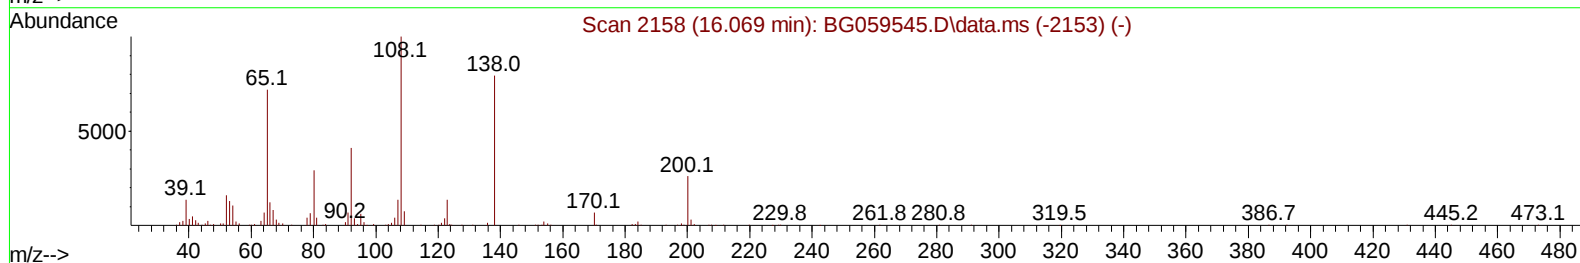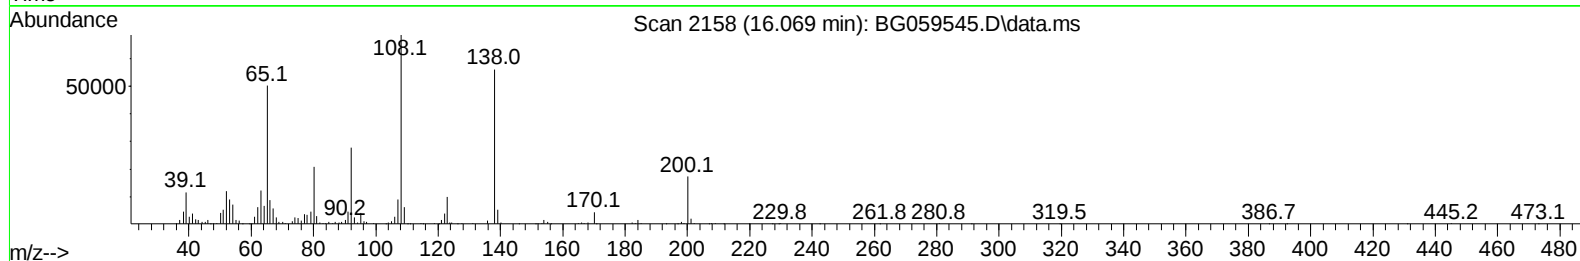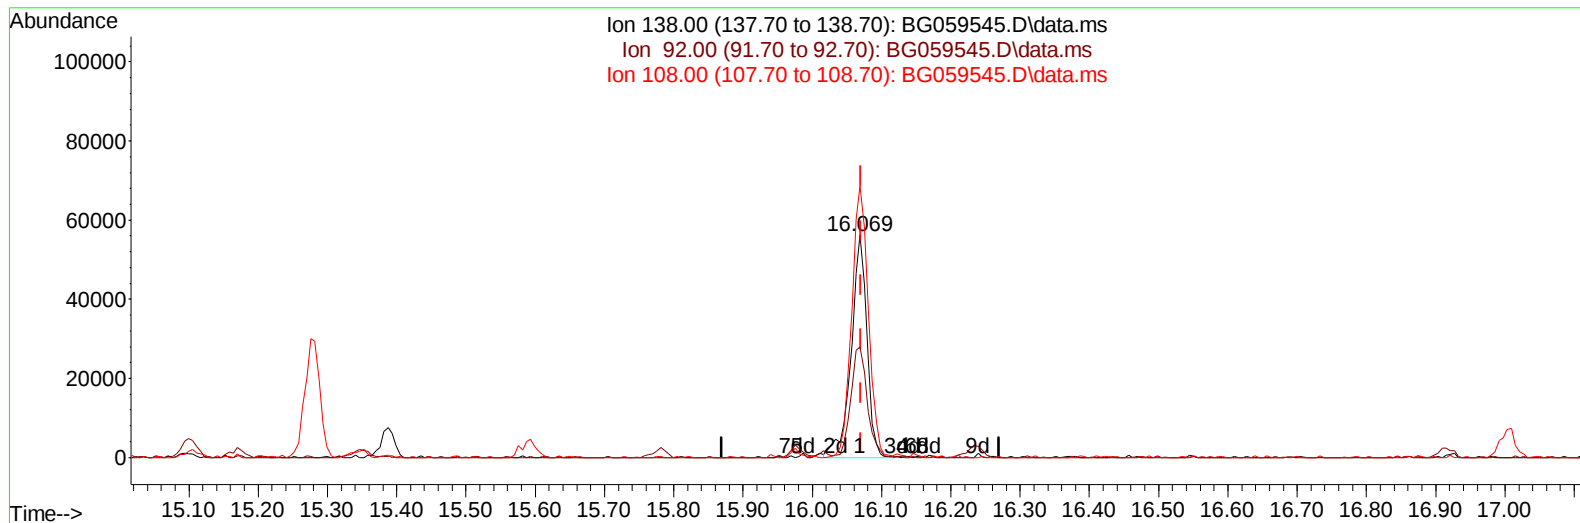

TIC: BG059545.D\data.ms

(63) 4-Nitroaniline

16.069min (-0.001) 21.50 ng/ul m

response 89124

Ion	Exp%	Act%
138.00	100.00	100.00
92.00	62.30	49.64#
108.00	126.10	122.16
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059545.D
 Acq On : 30 Oct 2023 12:03
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:06:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
 Supervised By :mohammad ahmed 11/01/2023

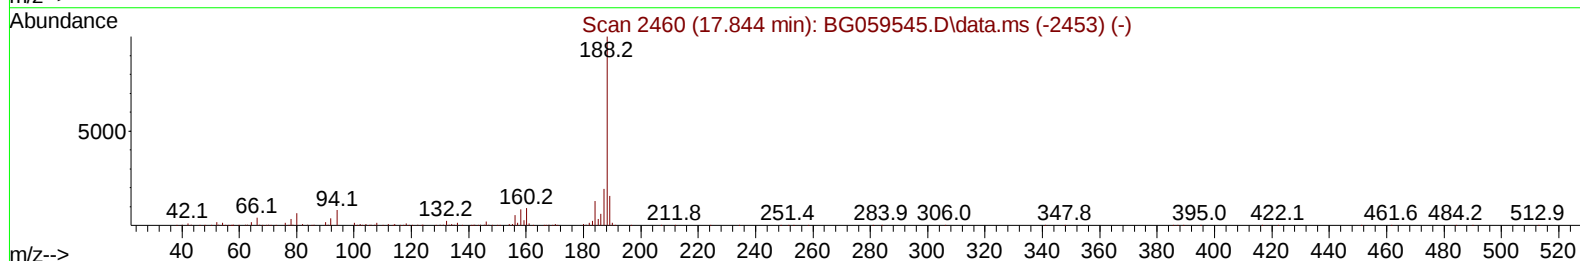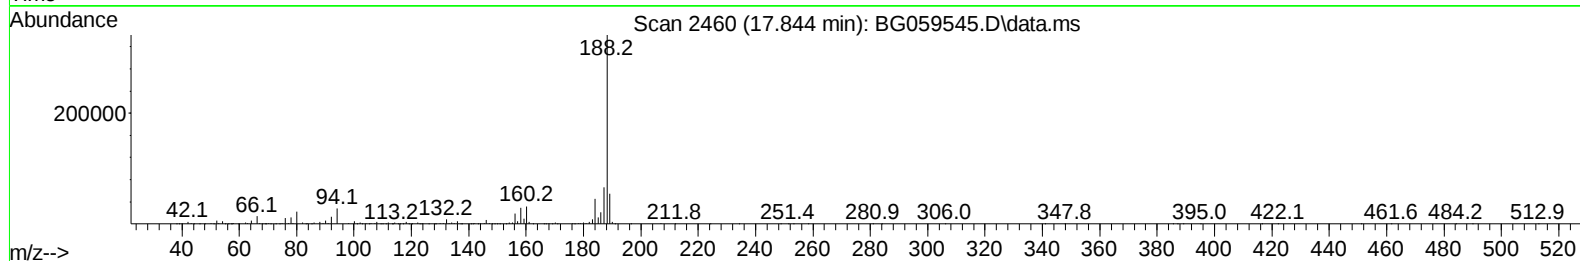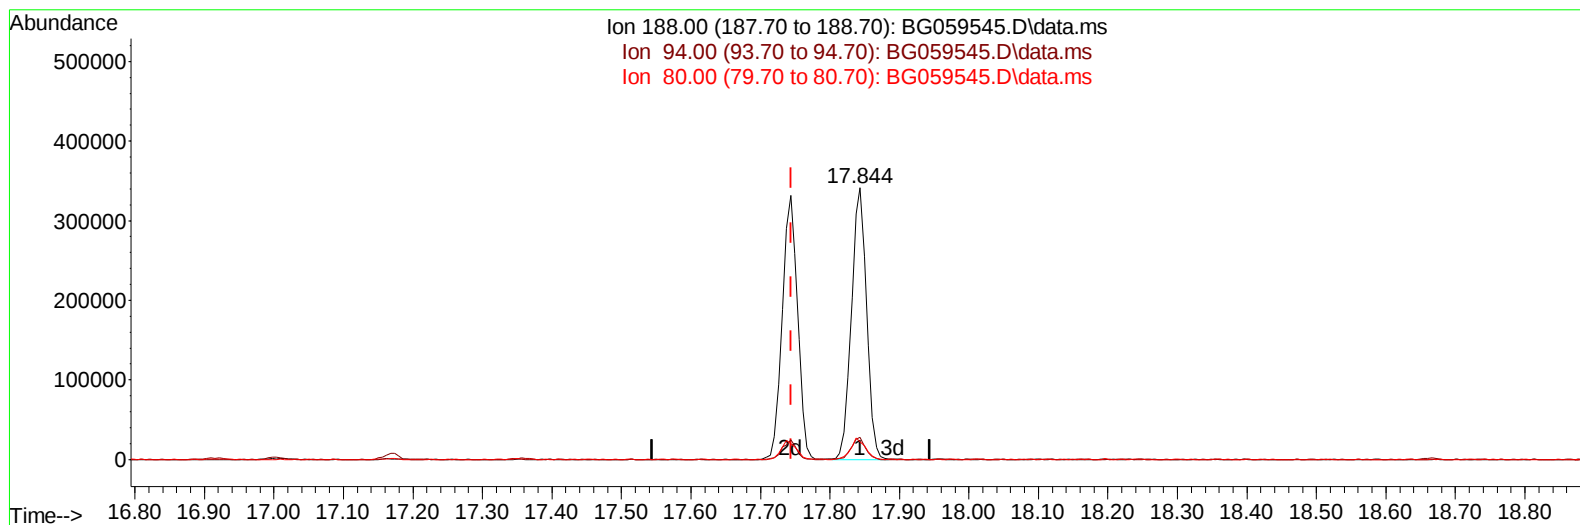

TIC: BG059545.D\data.ms

(64) Phenanthrene-d10 (I)

17.844min (+ 0.099) 20.00 ng/u1

response 518767

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.50	8.14
80.00	7.80	6.62
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059545.D
 Acq On : 30 Oct 2023 12:03
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:06:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
 Supervised By :mohammad ahmed 11/01/2023

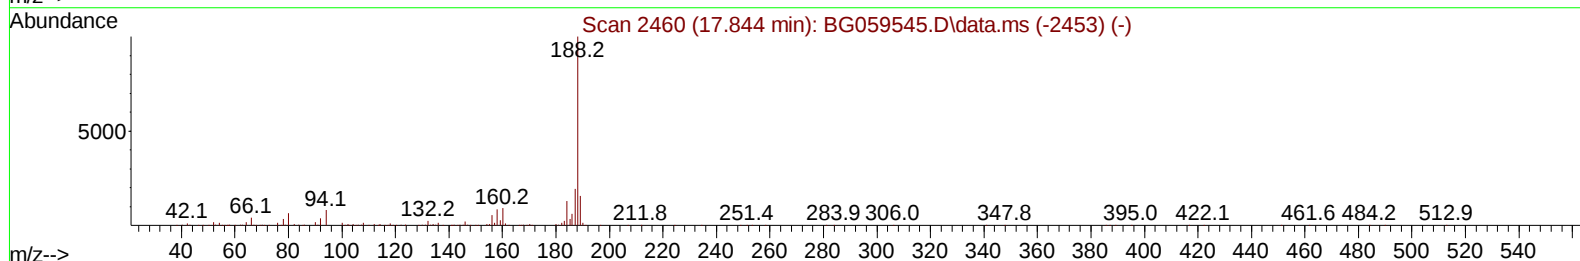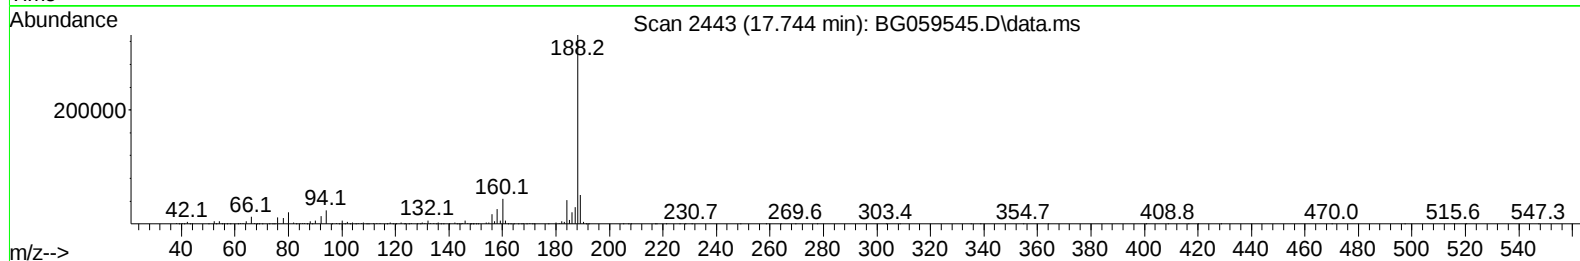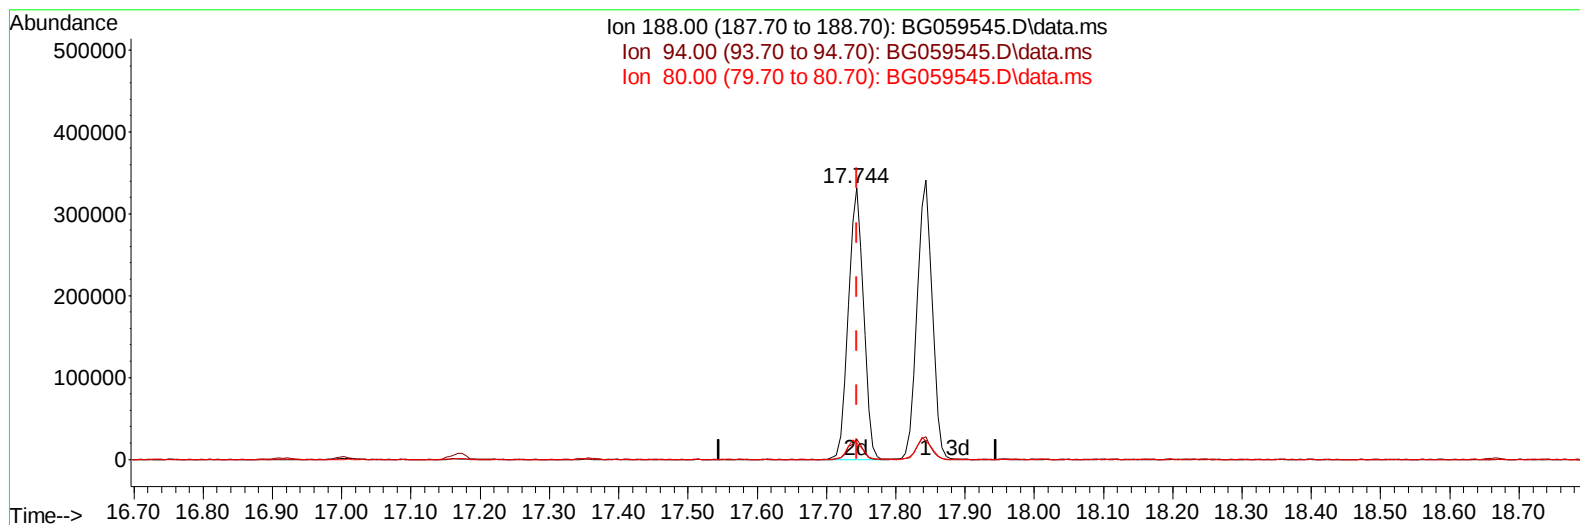

TIC: BG059545.D\data.ms

(64) Phenanthrene-d10 (I)

17.744min (-0.001) 20.00 ng/ul m

response 505095

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.50	7.34
80.00	7.80	6.04#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
Data File : BG059545.D
Acq On : 30 Oct 2023 12:03
Operator : MA/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
LabSampleId :
SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:08:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 28 03:56:42 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
Supervised By :mohammad ahmed 11/01/2023

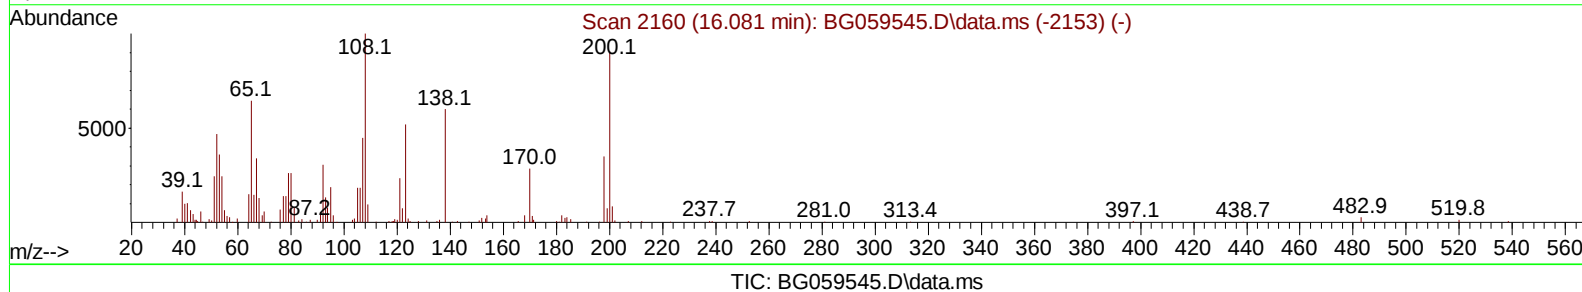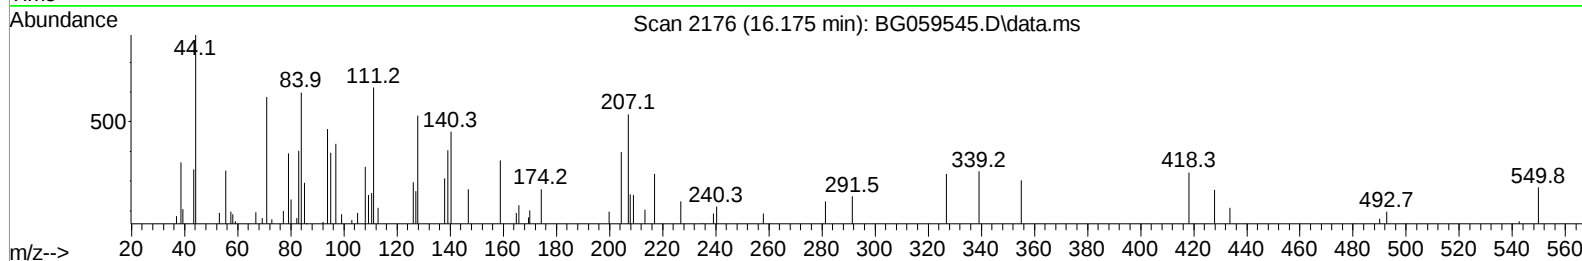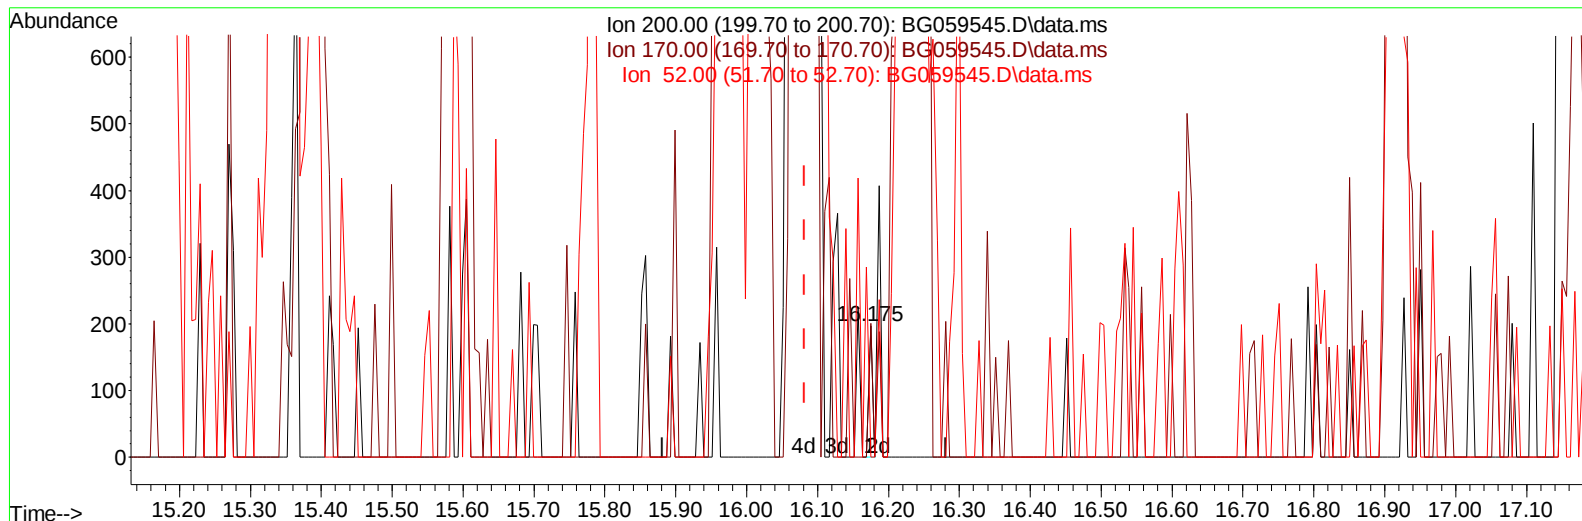

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

16.175min (+ 0.093) 0.03 ng/u1

response 69

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	21.90	102.03#
52.00	40.40	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059545.D
 Acq On : 30 Oct 2023 12:03
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:08:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
 Supervised By :mohammad ahmed 11/01/2023

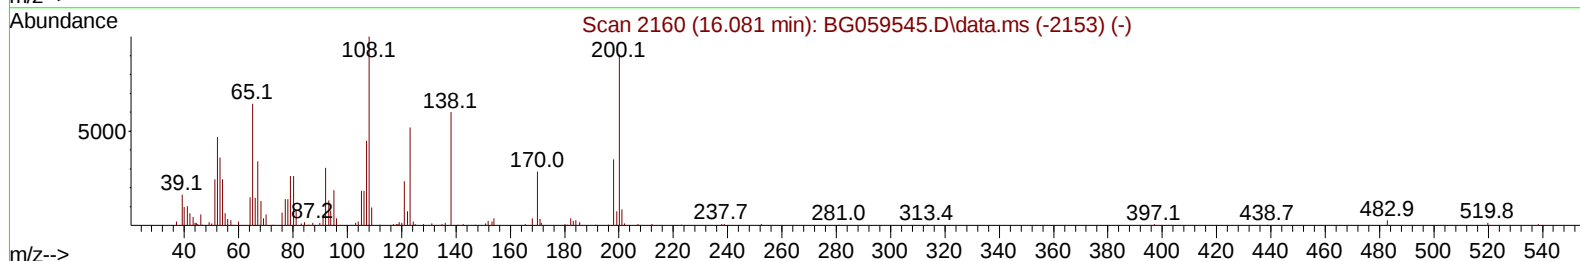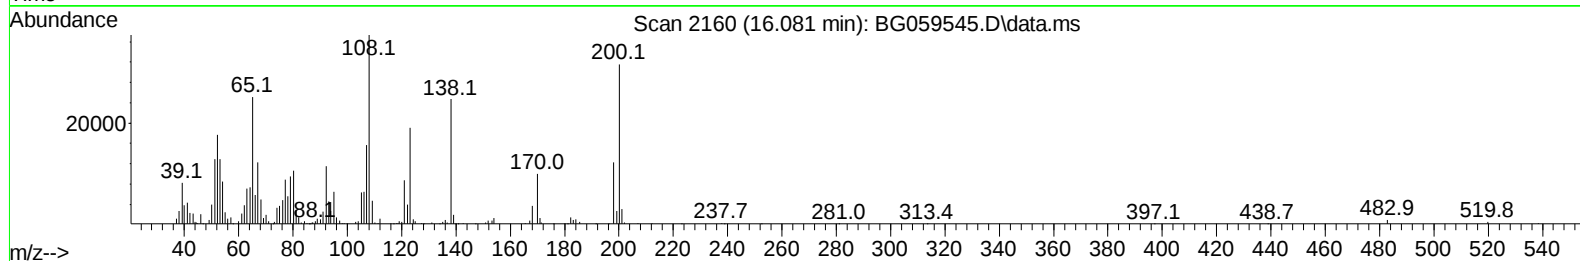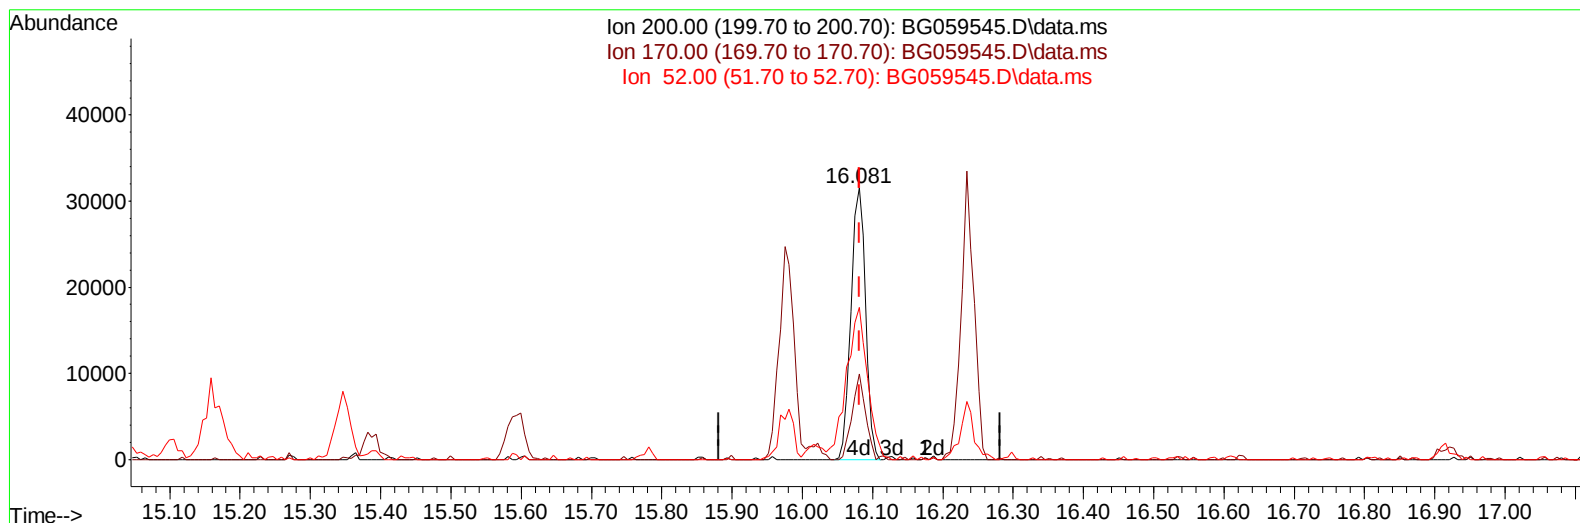

TIC: BG059545.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

16.081min (-0.001) 18.94 ng/ul m

response 45305

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	21.90	31.49#
52.00	40.40	56.09#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059545.D
 Acq On : 30 Oct 2023 12:03
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:08:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
 Supervised By :mohammad ahmed 11/01/2023

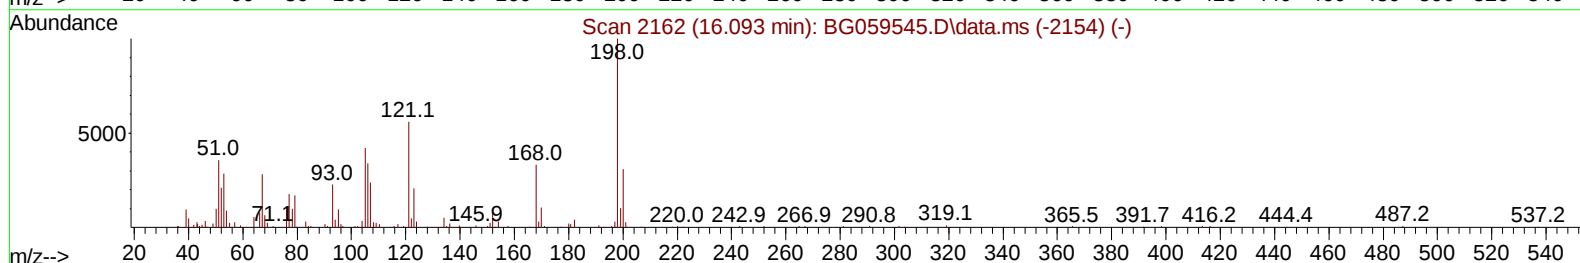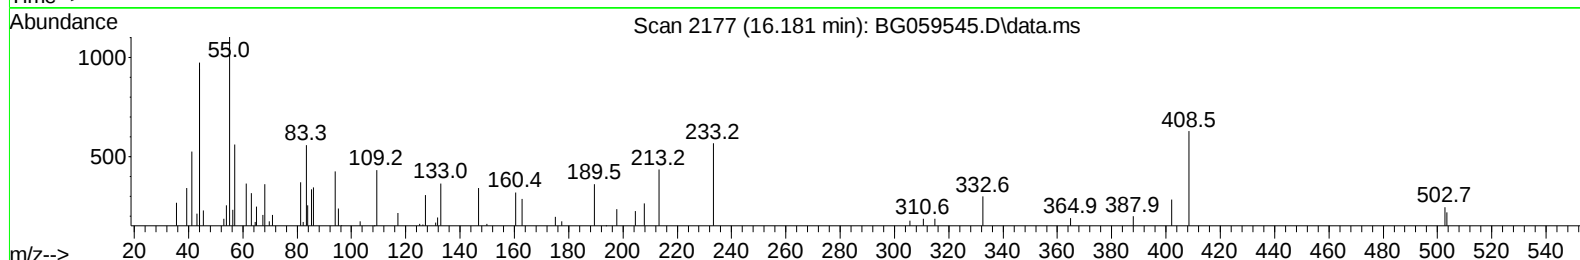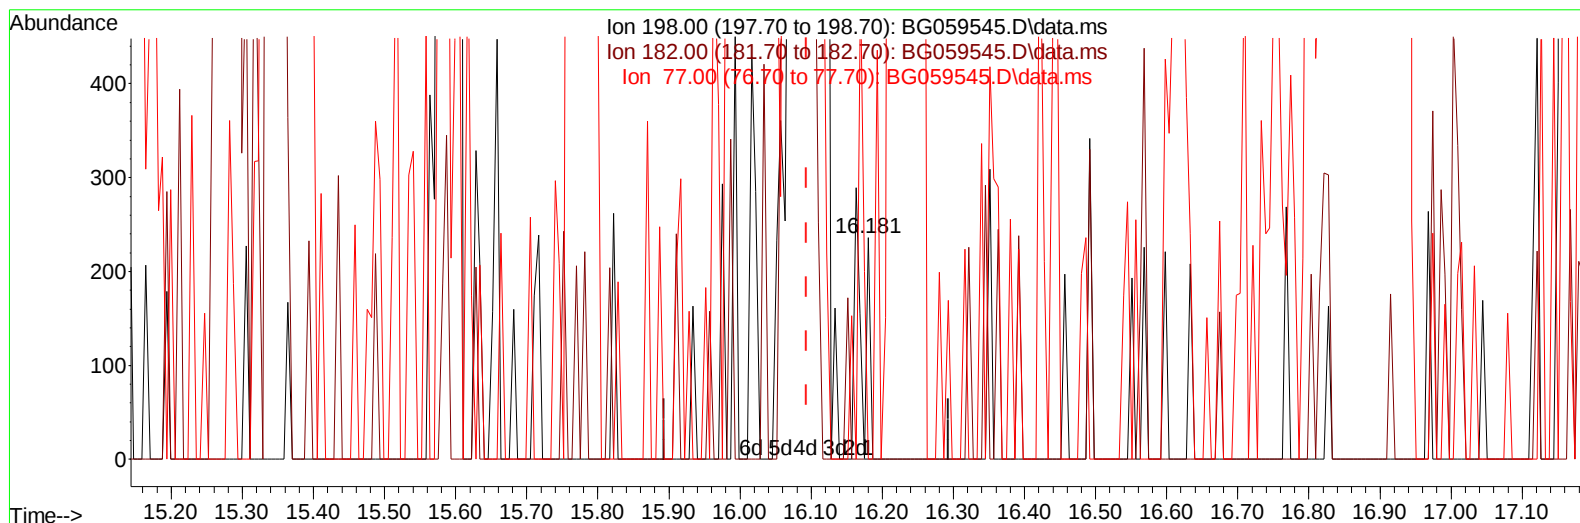

TIC: BG059545.D\data.ms

(66) 4,6-Dinitro-2-methylphenol

16.181min (+ 0.087) 0.03 ng/ul

response 83

Ion	Exp%	Act%
198.00	100.00	100.00
182.00	1.70	0.00#
77.00	19.80	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059545.D
 Acq On : 30 Oct 2023 12:03
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:08:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
 Supervised By :mohammad ahmed 11/01/2023

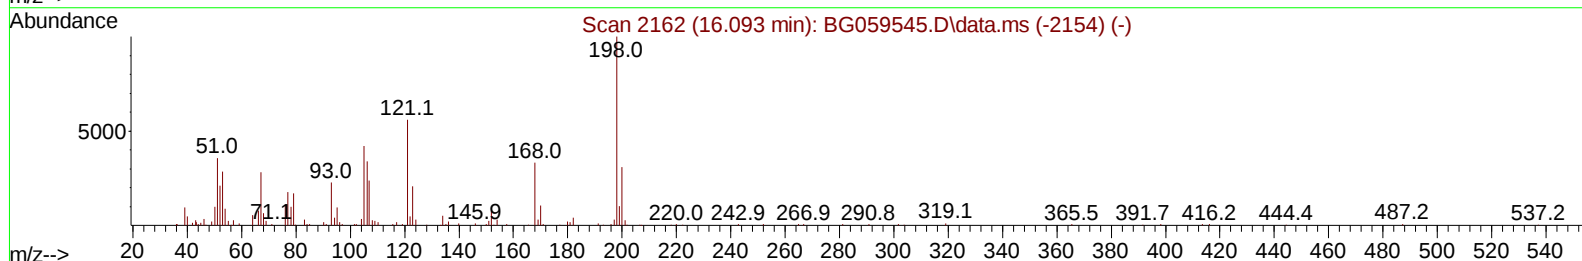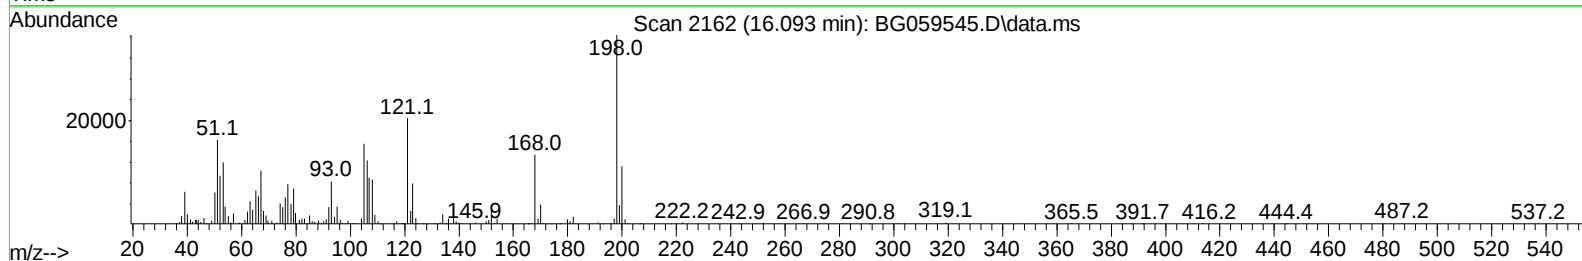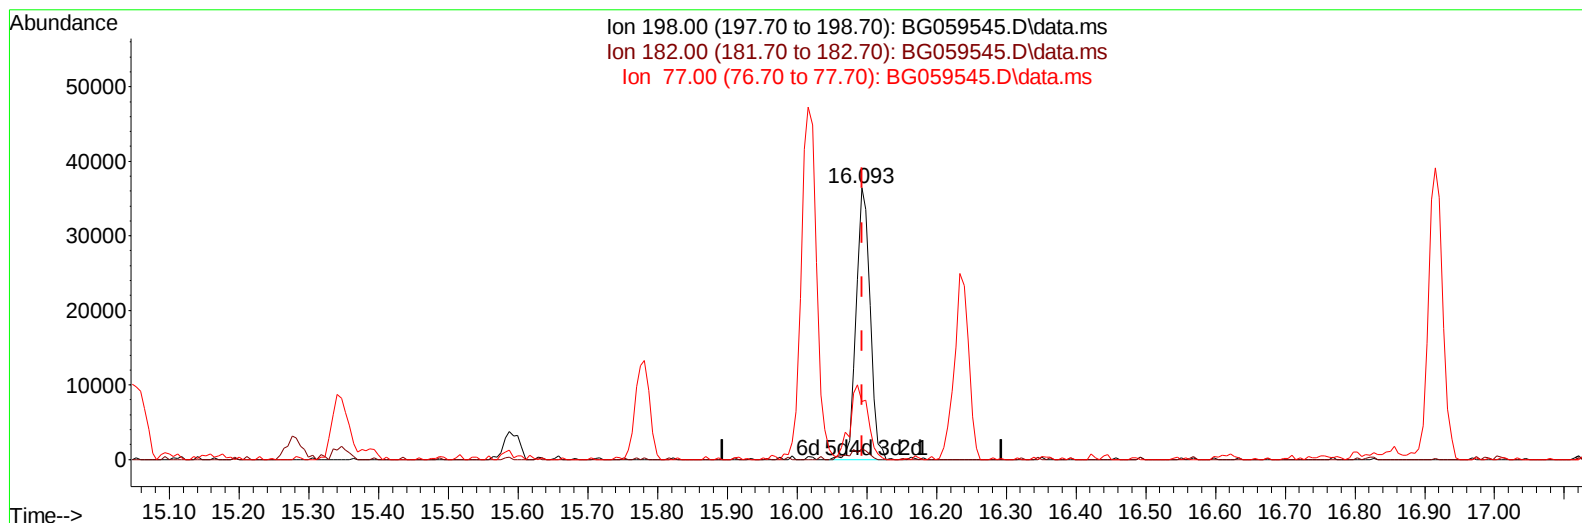

TIC: BG059545.D\data.ms

(66) 4,6-Dinitro-2-methylphenol

16.093min (-0.001) 19.98 ng/ul m

response 50374

Ion	Exp%	Act%
198.00	100.00	100.00
182.00	1.70	4.00#
77.00	19.80	21.43
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059545.D
 Acq On : 30 Oct 2023 12:03
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:08:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
 Supervised By :mohammad ahmed 11/01/2023

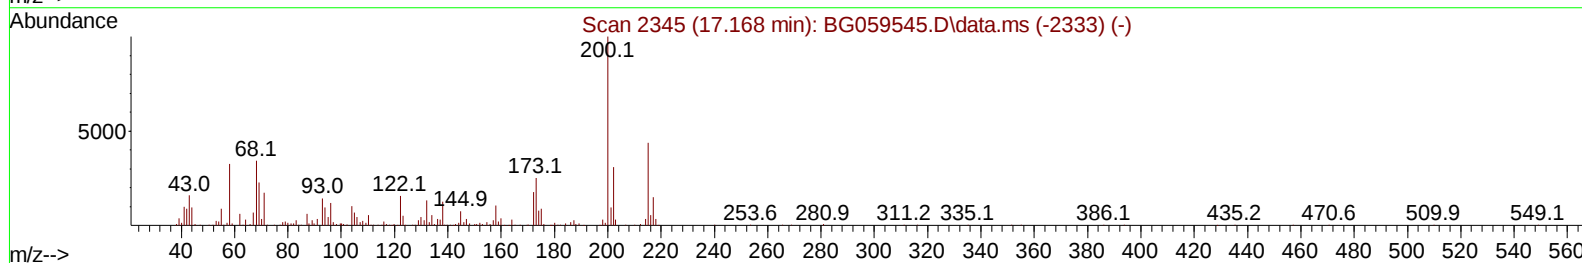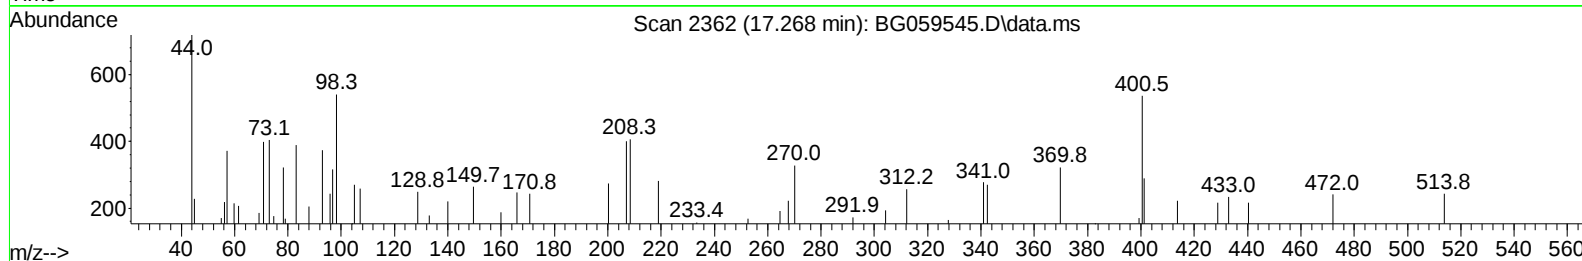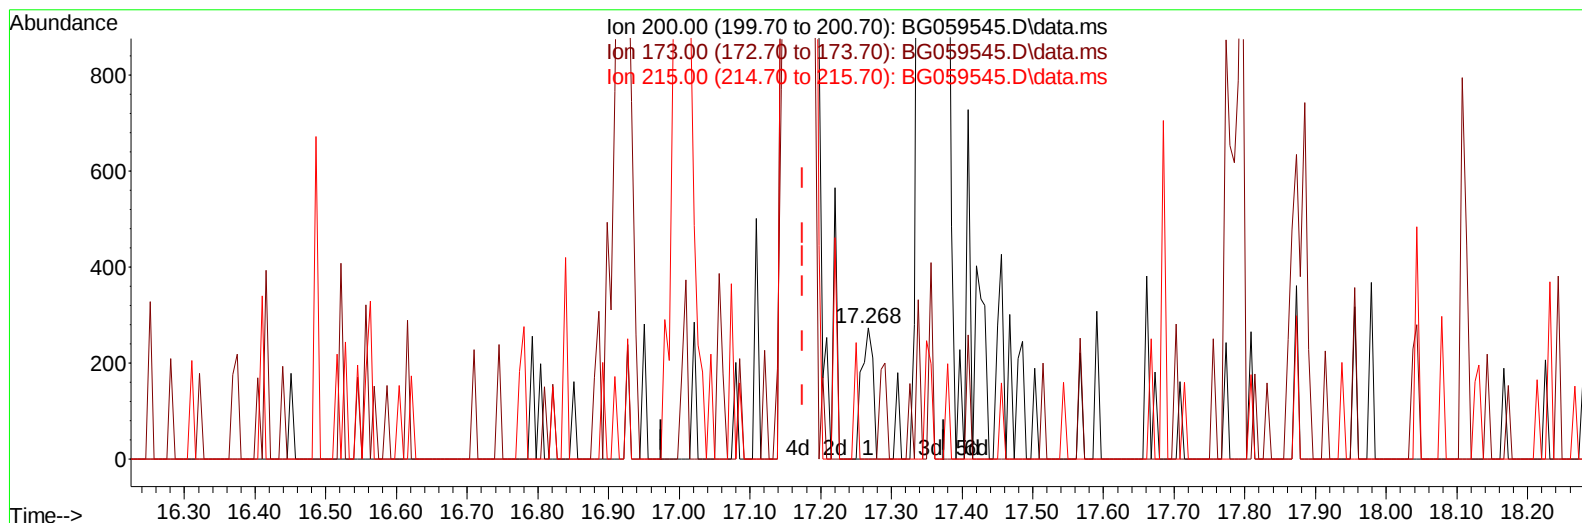

TIC: BG059545.D\data.ms

(70) Atrazine

17.268min (+ 0.093) 0.06 ng/ul

response 306

Ion	Exp%	Act%
200.00	100.00	100.00
173.00	32.10	0.00#
215.00	40.10	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
Data File : BG059545.D
Acq On : 30 Oct 2023 12:03
Operator : MA/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
LabSampleId :
SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:08:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 28 03:56:42 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
Supervised By :mohammad ahmed 11/01/2023

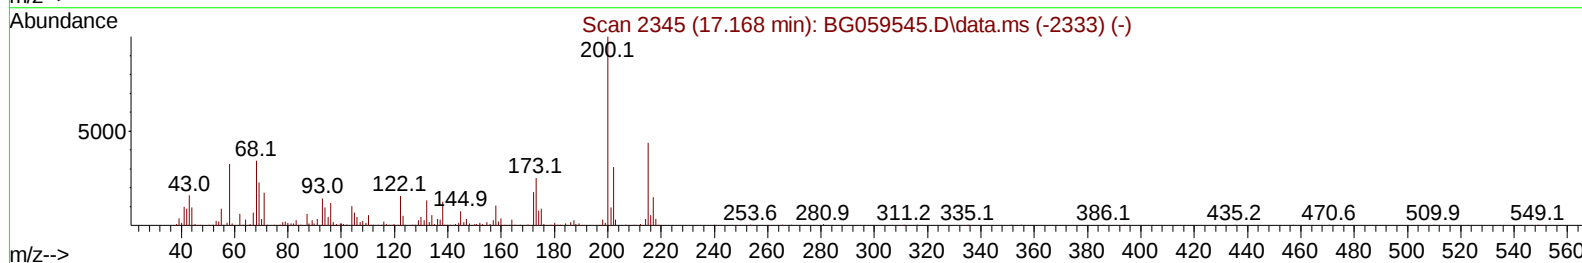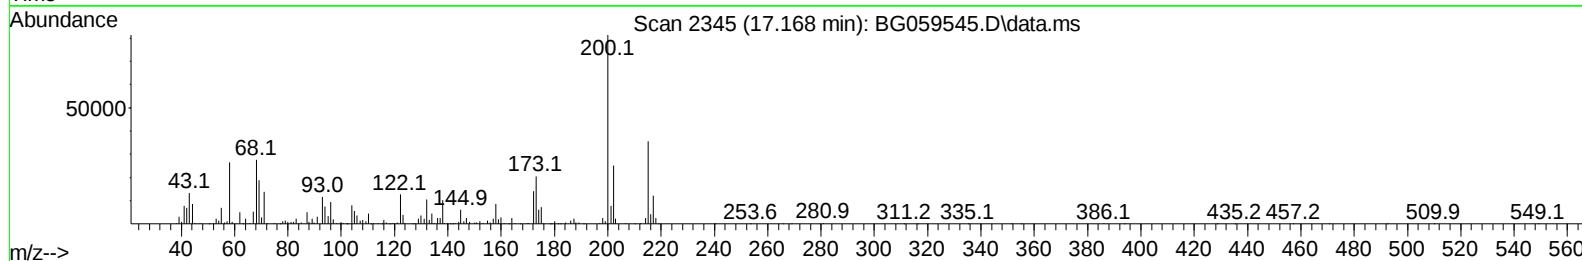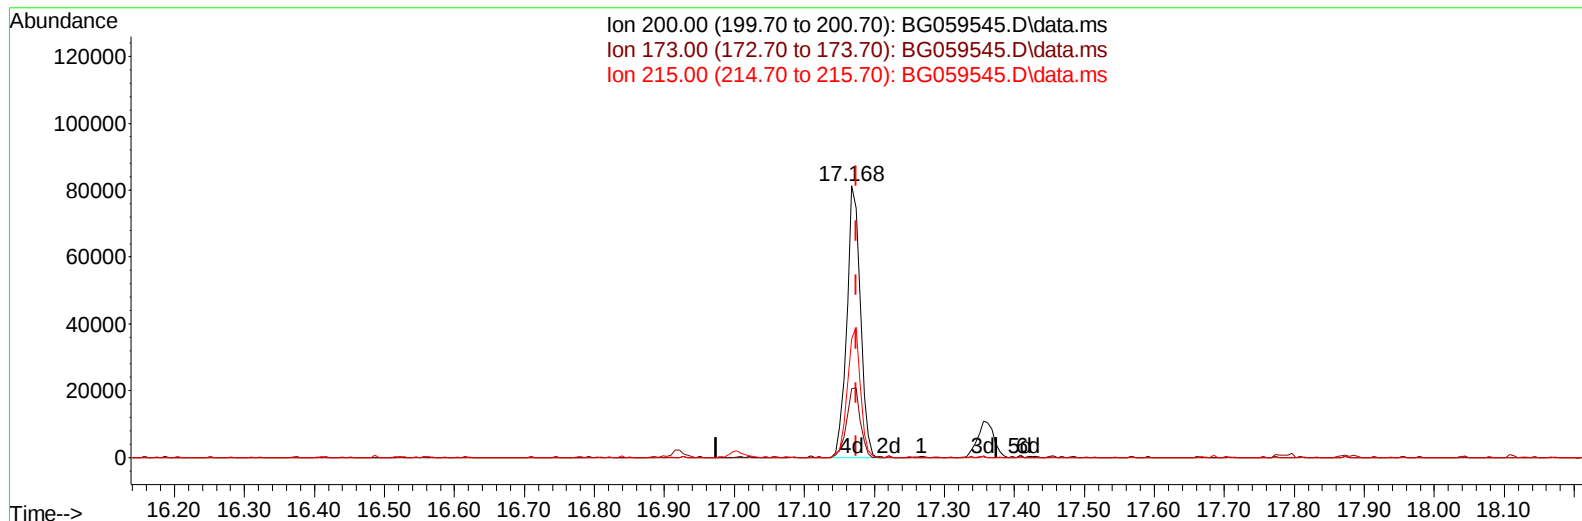

TIC: BG059545.D\data.ms

(70) Atrazine

17.168min (-0.007) 20.46 ng/ul m

response 109438

Ion	Exp%	Act%
200.00	100.00	100.00
173.00	32.10	25.26#
215.00	40.10	43.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
Data File : BG059545.D
Acq On : 30 Oct 2023 12:03
Operator : MA/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :

BNA_G




LabSampleId :

SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:08:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 28 03:56:42 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
Supervised By :mohammad ahmed 11/01/2023

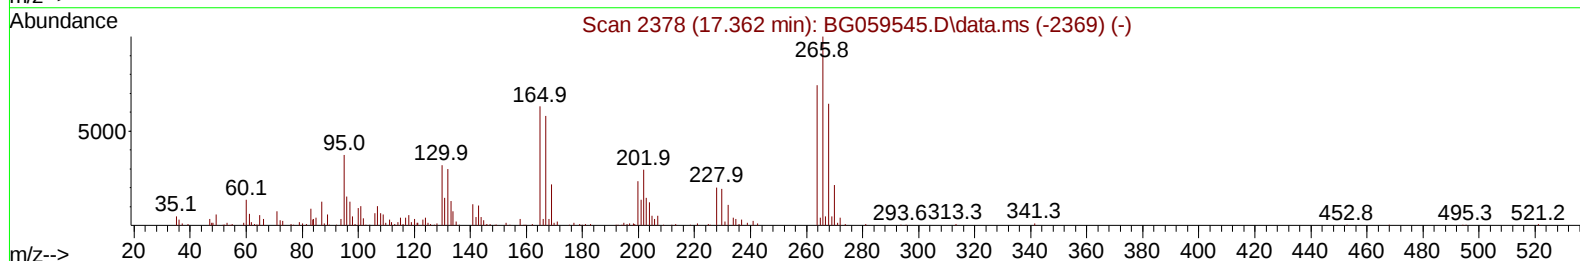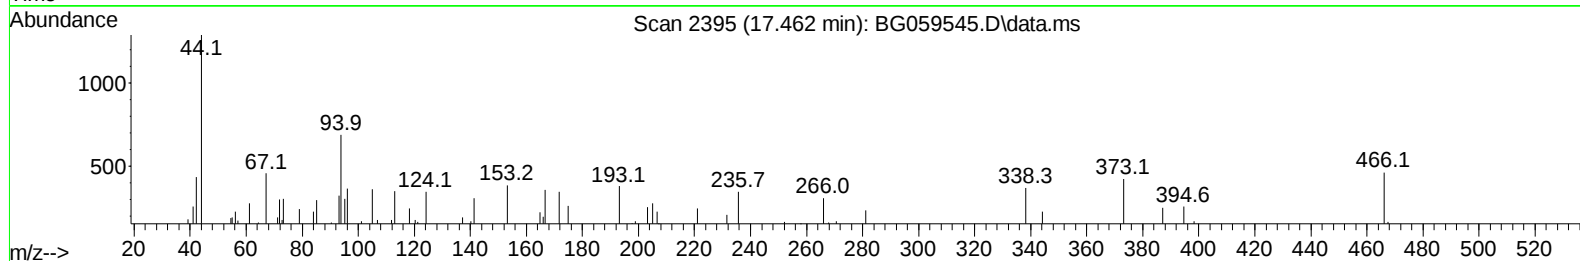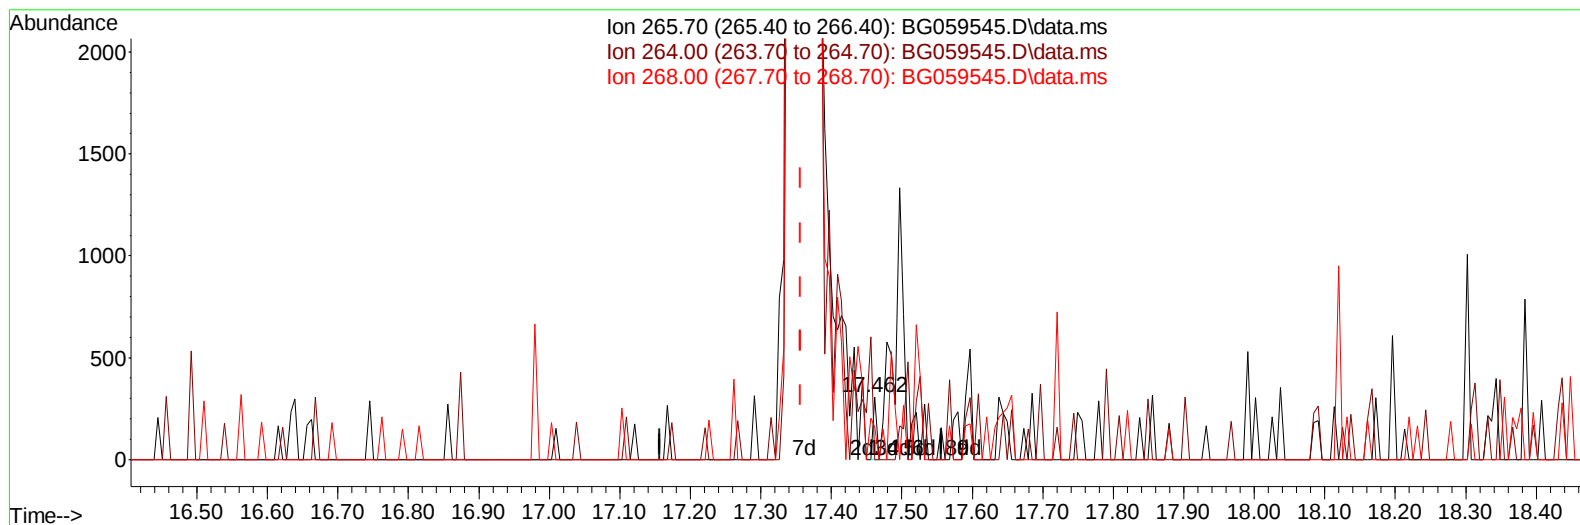

TIC: BG059545.D\data.ms

(71) Pentachlorophenol (C)

17.462min (+ 0.105) 0.03 ng/u1

response 108

Ion	Exp%	Act%
265.70	100.00	100.00
264.00	57.70	0.00#
268.00	58.00	51.47
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059545.D
 Acq On : 30 Oct 2023 12:03
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:08:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
 Supervised By :mohammad ahmed 11/01/2023

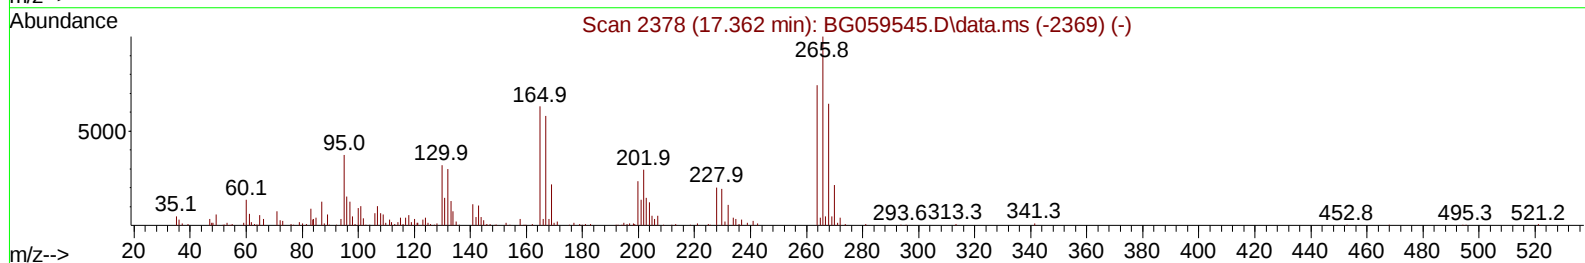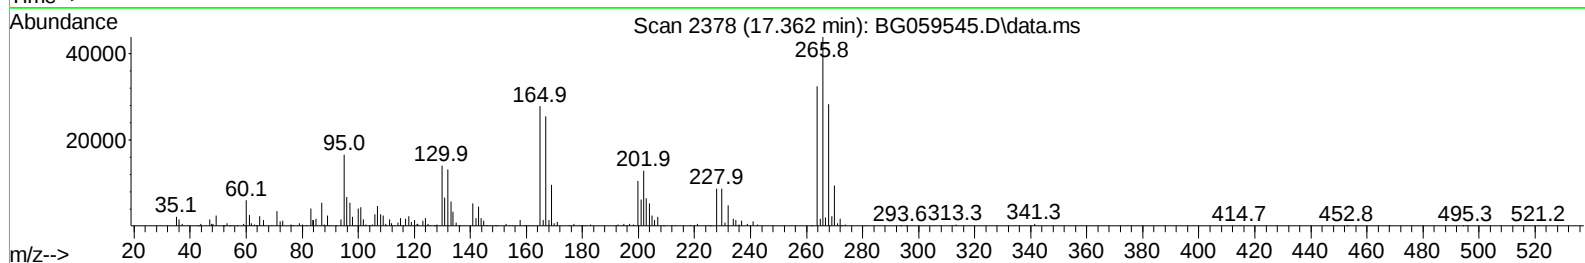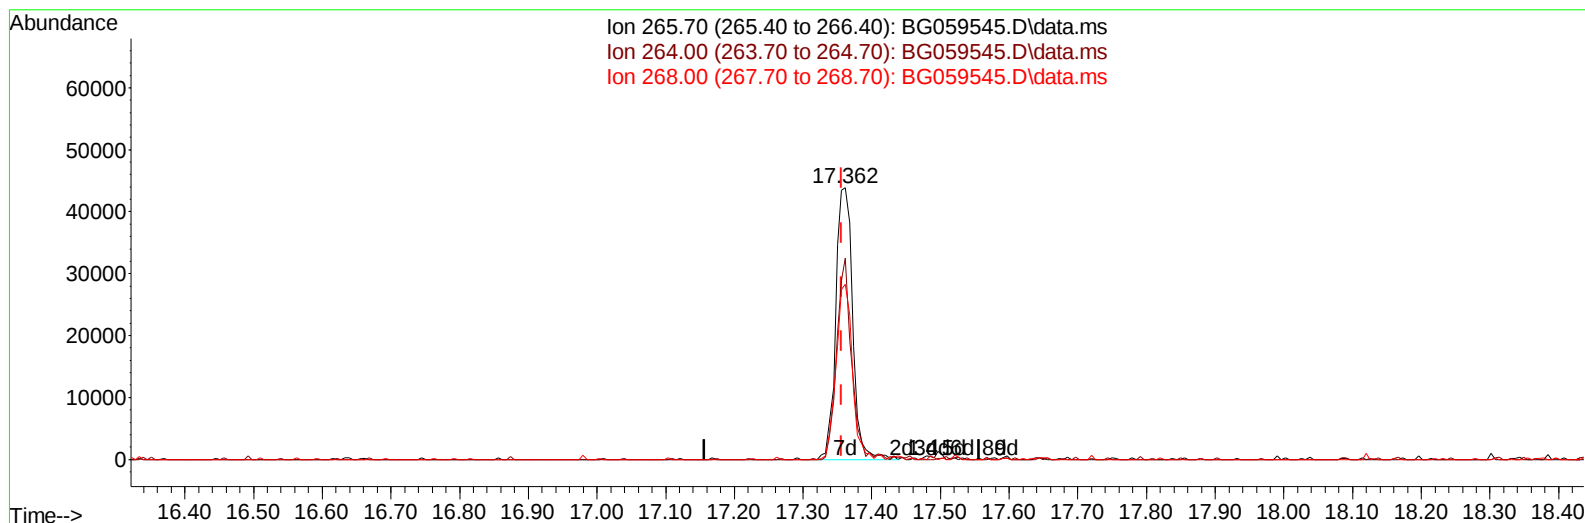

TIC: BG059545.D\data.ms

(71) Pentachlorophenol (C)

17.362min (+ 0.005) 22.53 ng/ul m

response 75184

Ion	Exp%	Act%
265.70	100.00	100.00
264.00	57.70	74.16#
268.00	58.00	64.54
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059545.D
 Acq On : 30 Oct 2023 12:03
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:08:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
 Supervised By :mohammad ahmed 11/01/2023

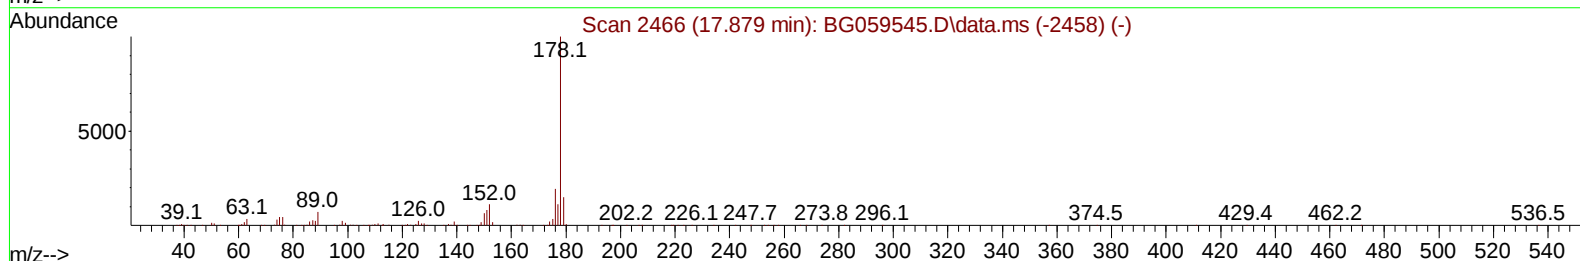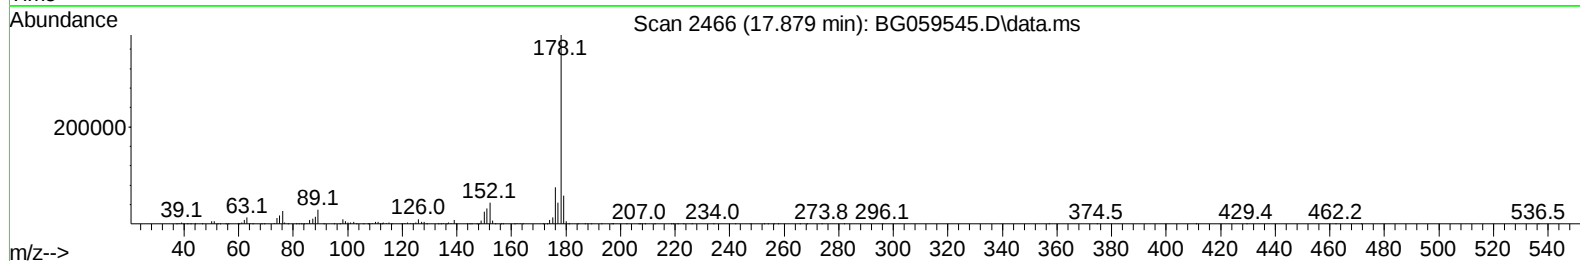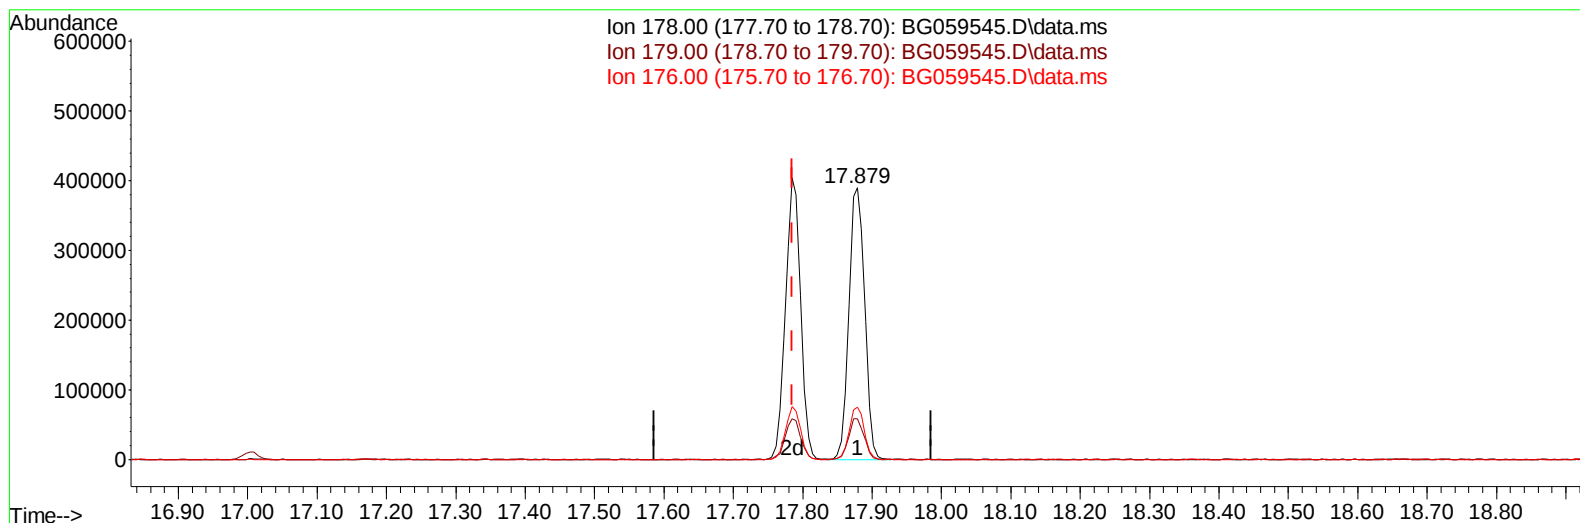

TIC: BG059545.D\data.ms

(72) Phenanthrene

17.879min (+ 0.093) 18.77 ng/u1

response 616223

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	14.10	14.97
176.00	19.20	19.33
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059545.D
 Acq On : 30 Oct 2023 12:03
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:08:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
 Supervised By :mohammad ahmed 11/01/2023

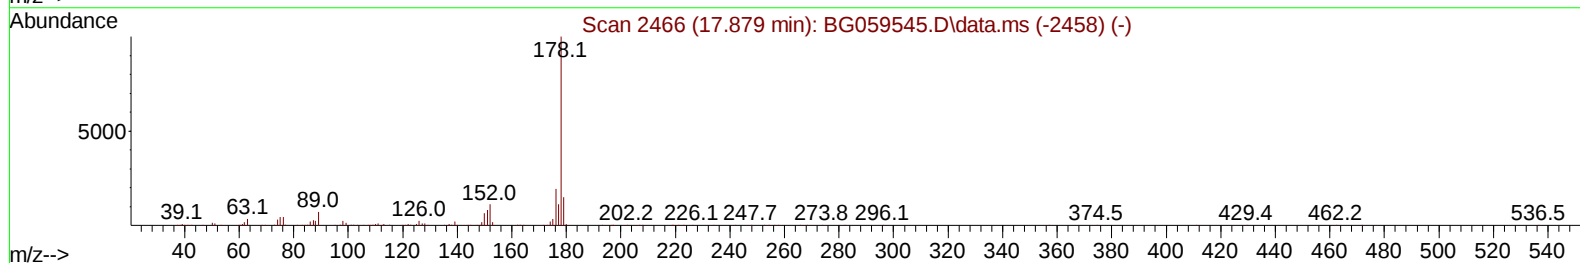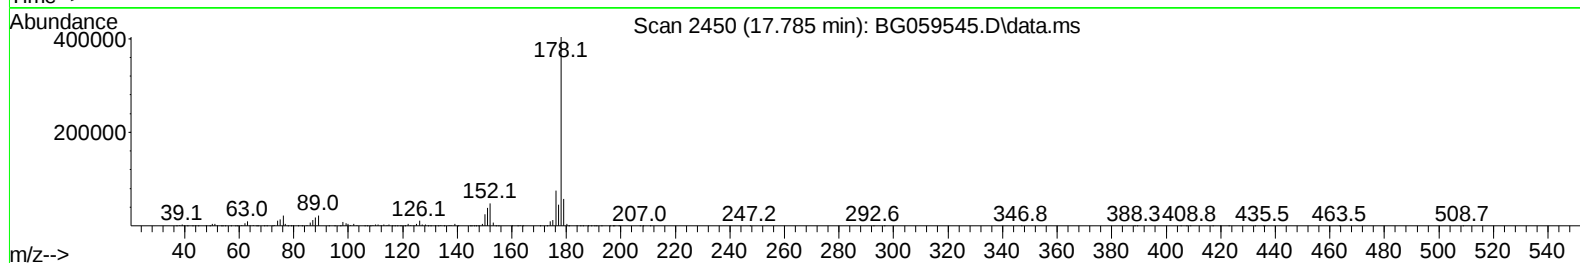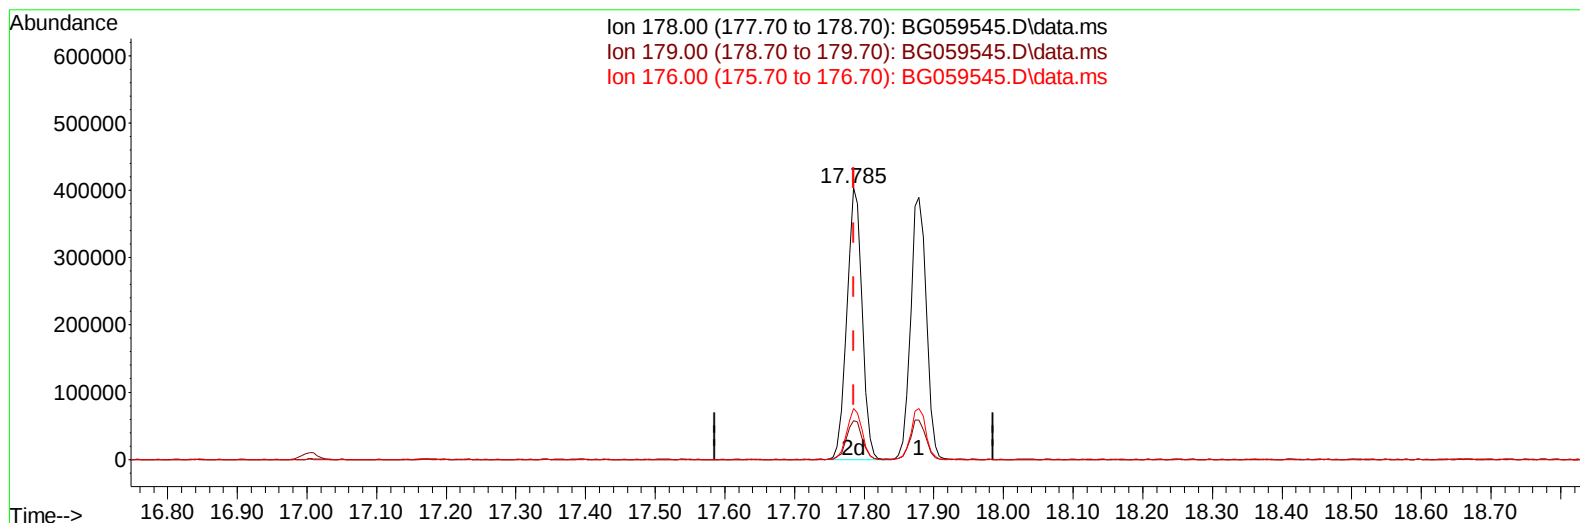

TIC: BG059545.D\data.ms

(72) Phenanthrene

17.785min (-0.001) 18.58 ng/ul m

response 610148

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	14.10	14.38
176.00	19.20	18.83
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059545.D
 Acq On : 30 Oct 2023 12:03
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:08:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
 Supervised By :mohammad ahmed 11/01/2023

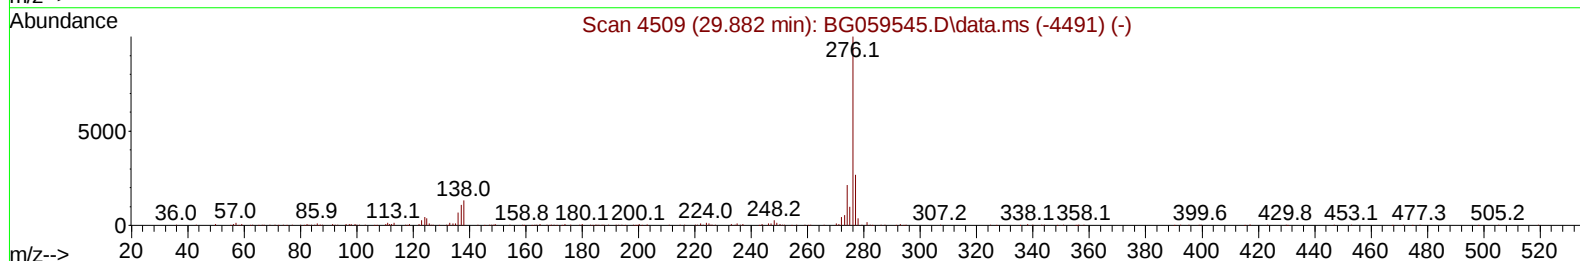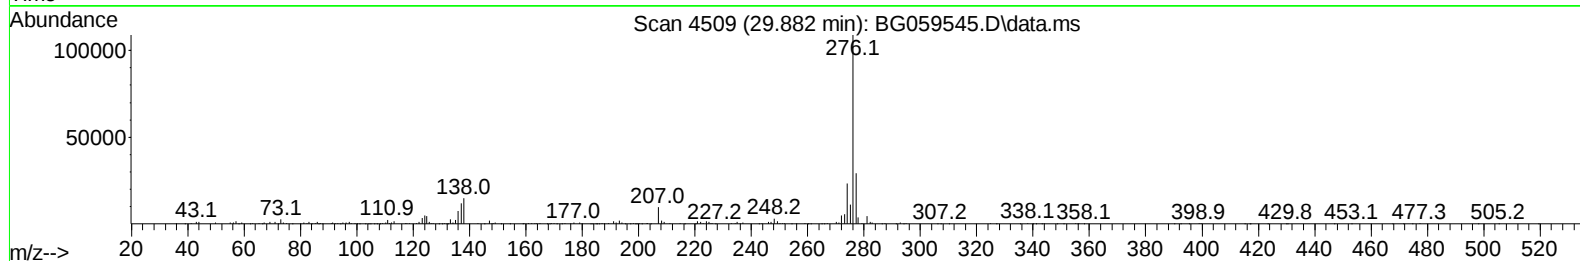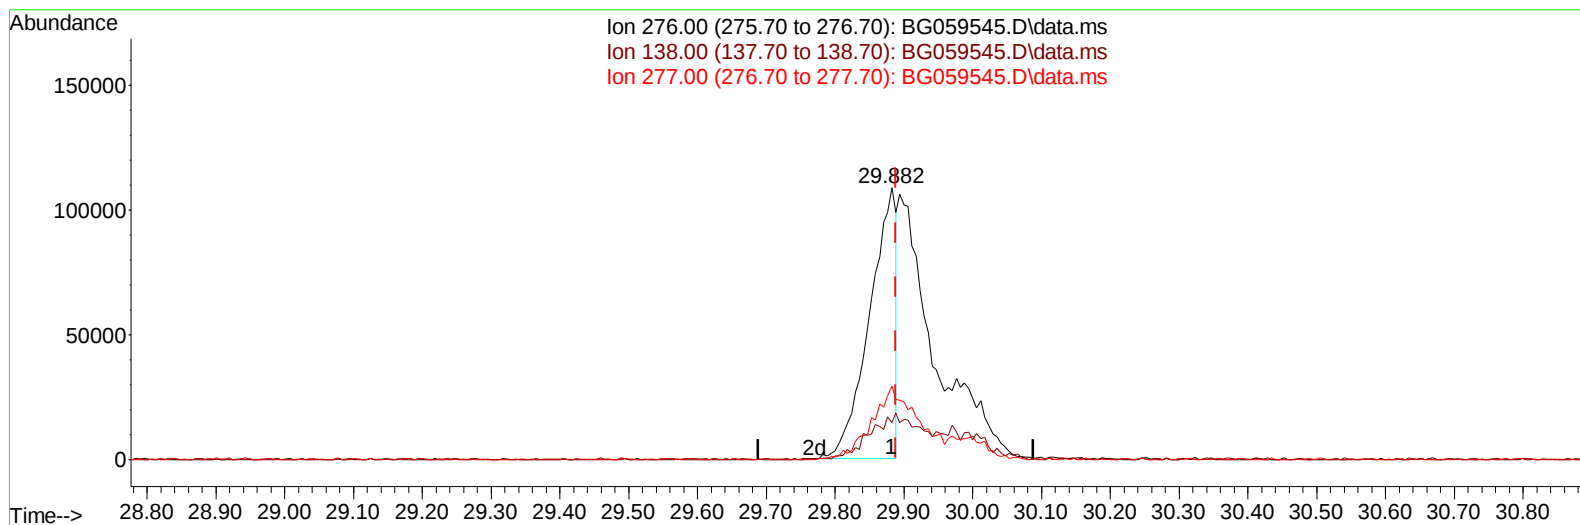

TIC: BG059545.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

29.882min (-0.007) 8.03 ng/u1

response 291845

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	19.10	13.59#
277.00	20.50	27.03#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
Data File : BG059545.D
Acq On : 30 Oct 2023 12:03
Operator : MA/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
LabSampleId :
SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:08:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 28 03:56:42 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
Supervised By :mohammad ahmed 11/01/2023

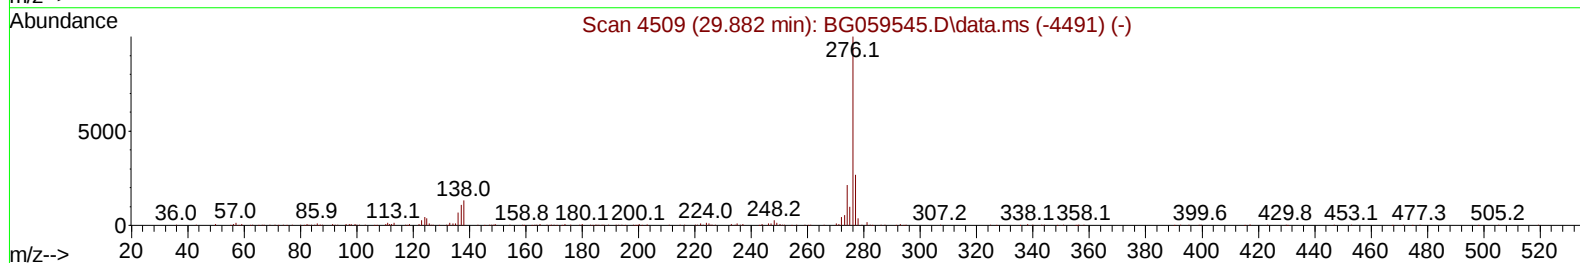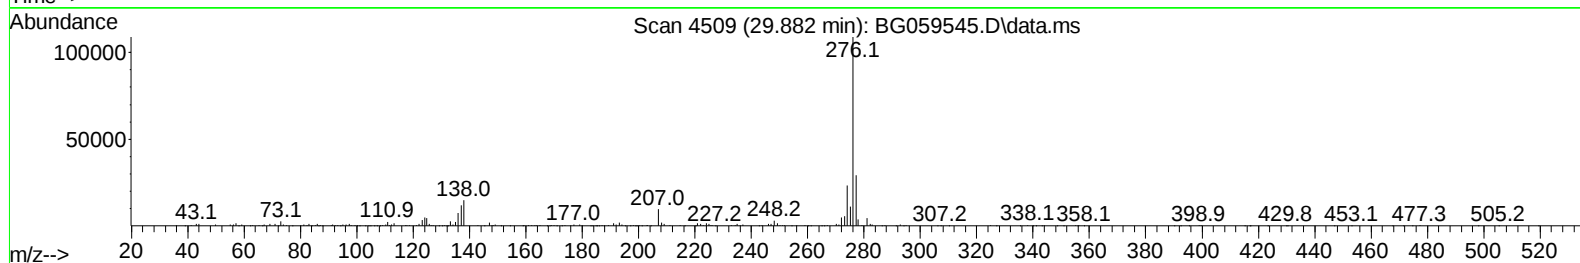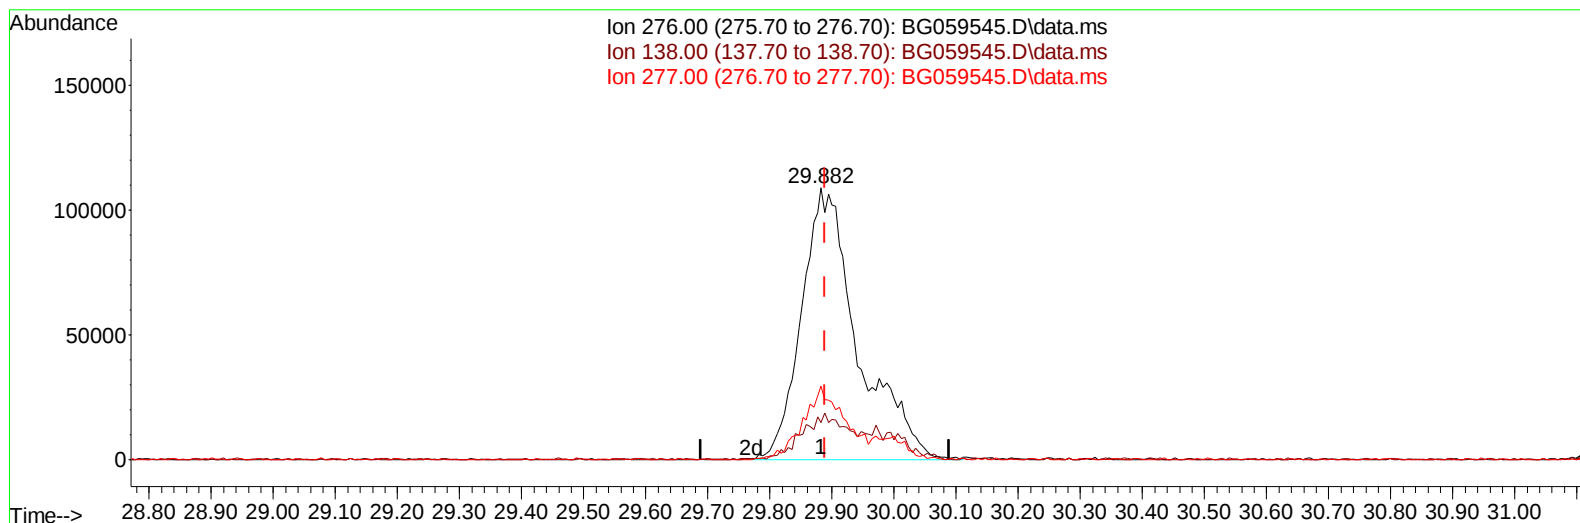

TIC: BG059545.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

29.882min (-0.007) 18.81 ng/ul m

response 683703

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	19.10	13.59#
277.00	20.50	27.03#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059545.D
 Acq On : 30 Oct 2023 12:03
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:08:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
 Supervised By :mohammad ahmed 11/01/2023

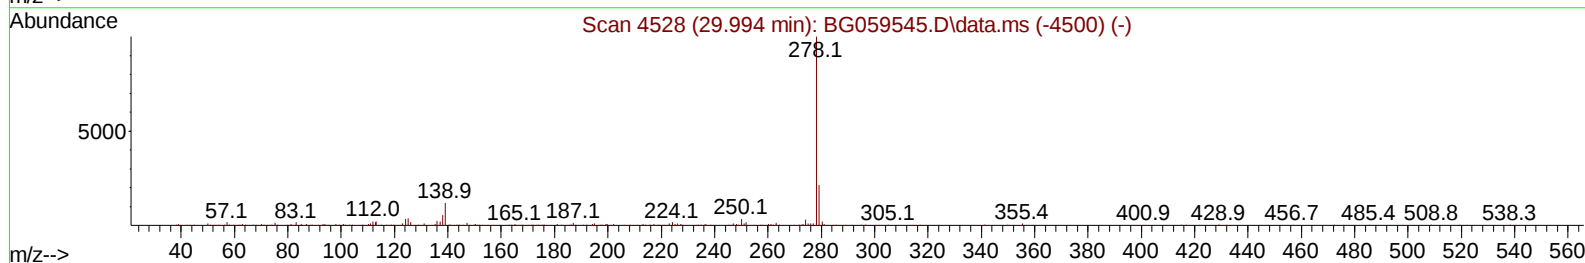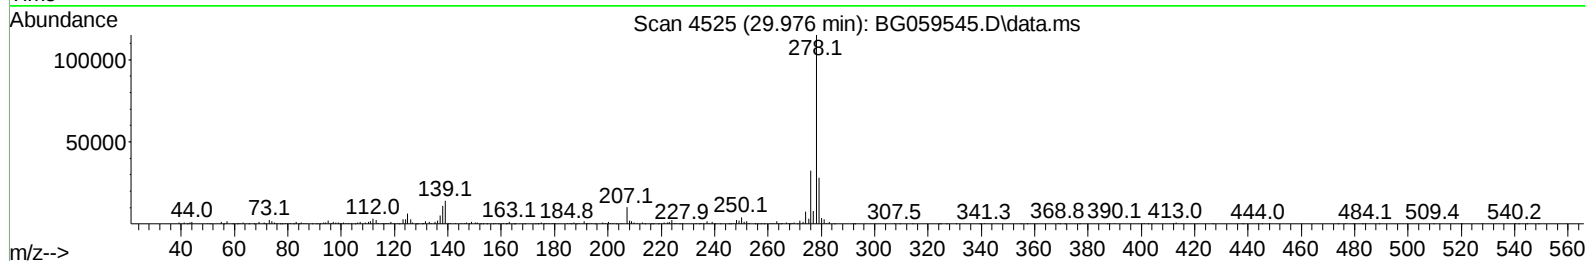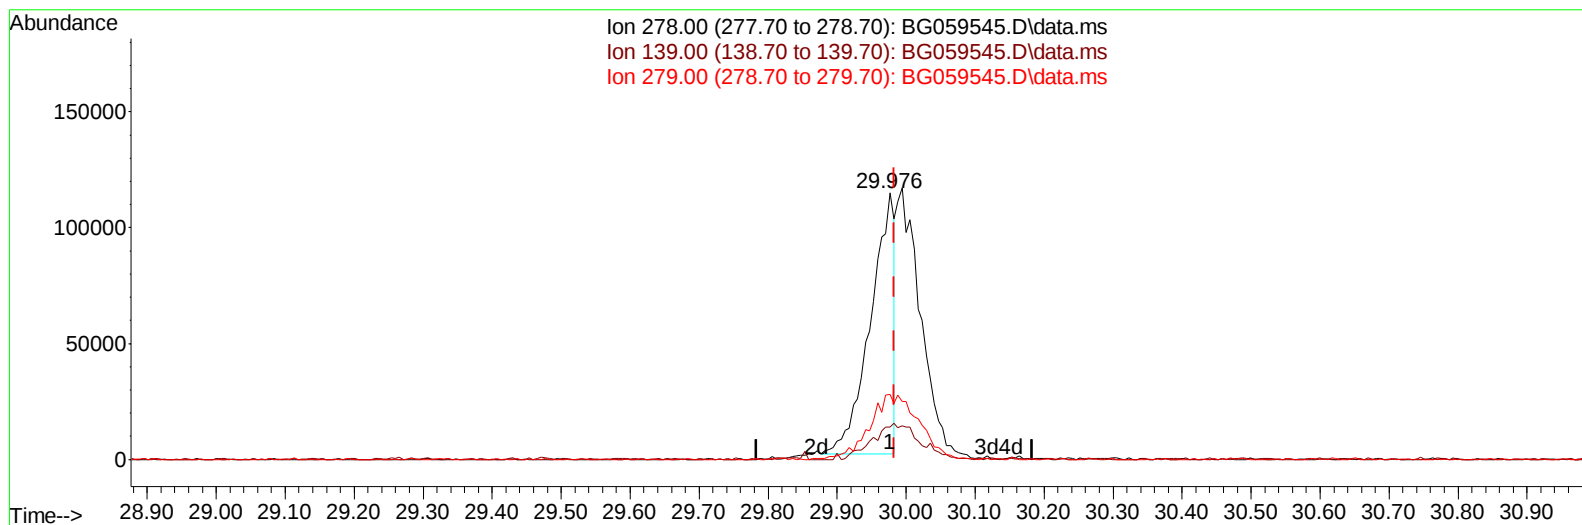

TIC: BG059545.D\data.ms

(95) Dibenzo(a,h)anthracene

29.976min (-0.007) 9.05 ng/u1

response 271670

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	13.80	12.21
279.00	22.90	24.42
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059545.D
 Acq On : 30 Oct 2023 12:03
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:08:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
 Supervised By :mohammad ahmed 11/01/2023

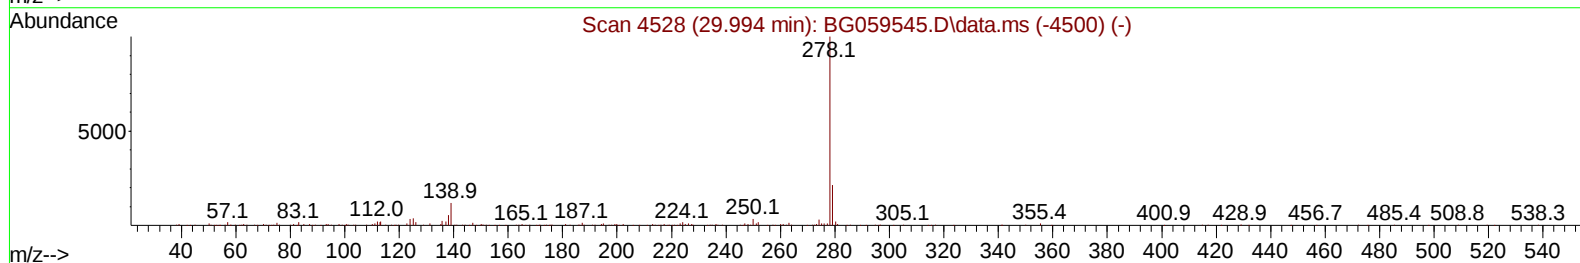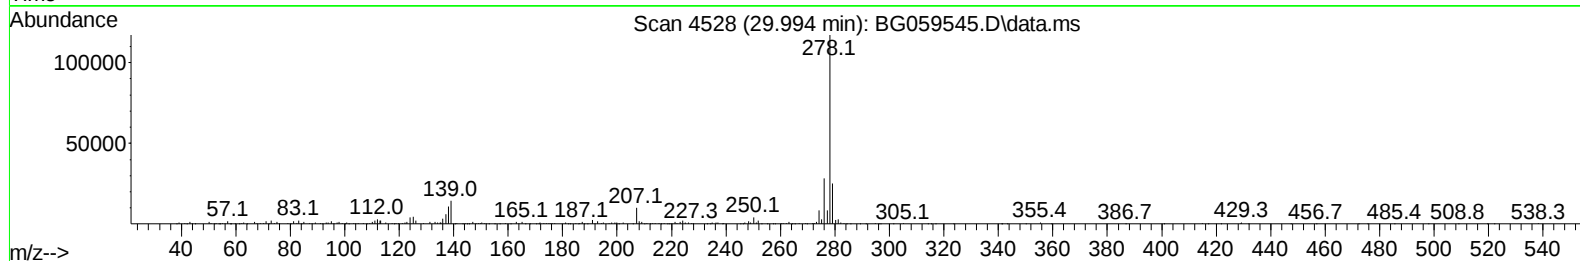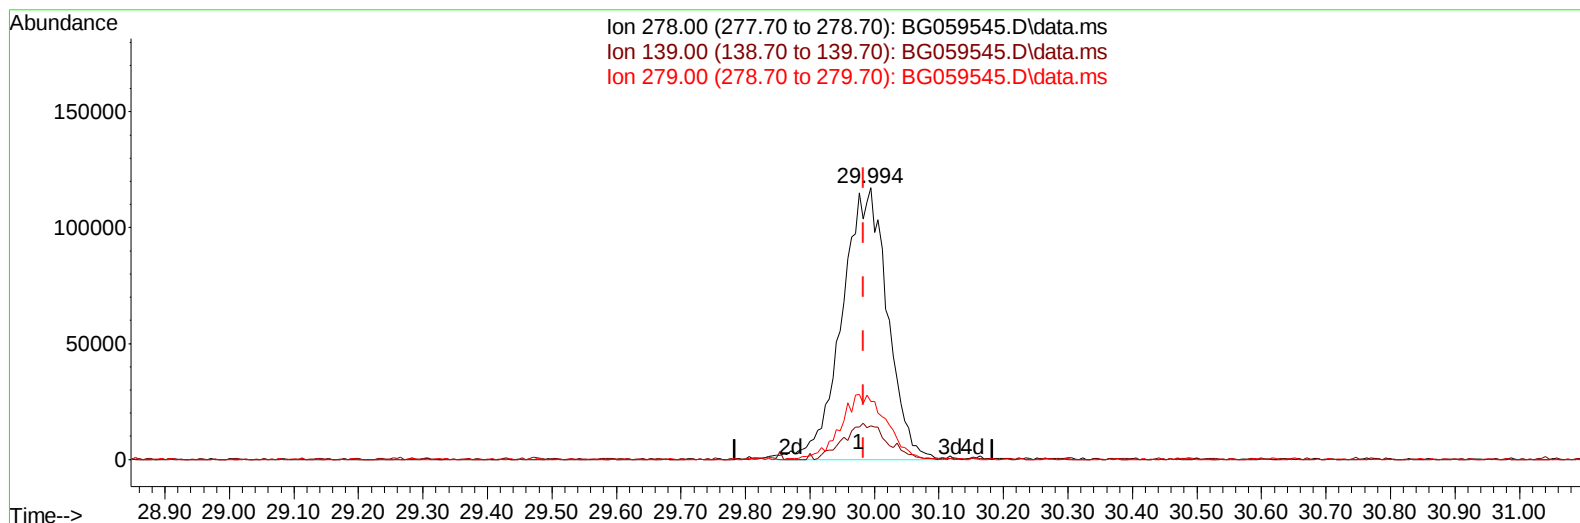

TIC: BG059545.D\data.ms

(95) Dibenzo(a,h)anthracene

29.994min (+ 0.011) 19.14 ng/ul m

response 574366

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	13.80	12.40
279.00	22.90	21.36
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059545.D
 Acq On : 30 Oct 2023 12:03
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:08:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
 Supervised By :mohammad ahmed 11/01/2023

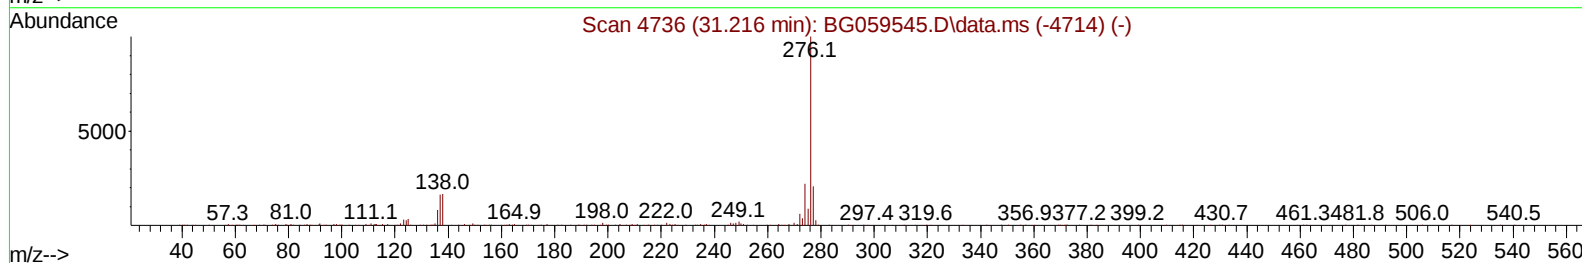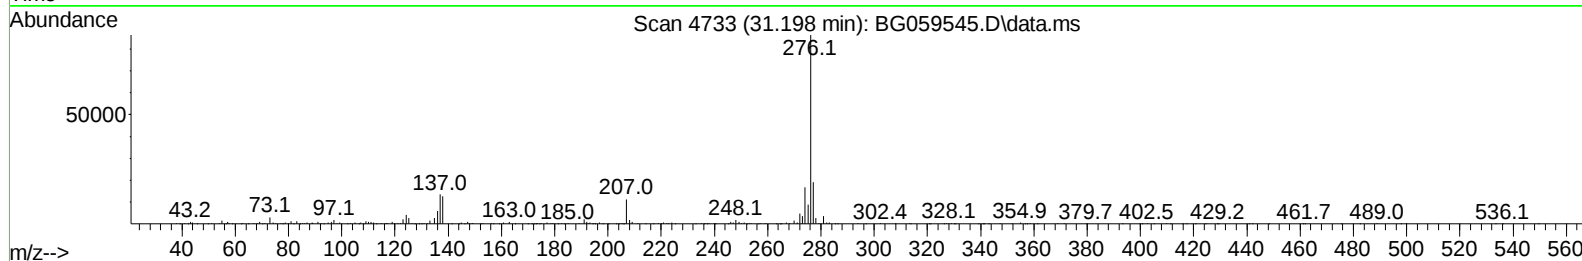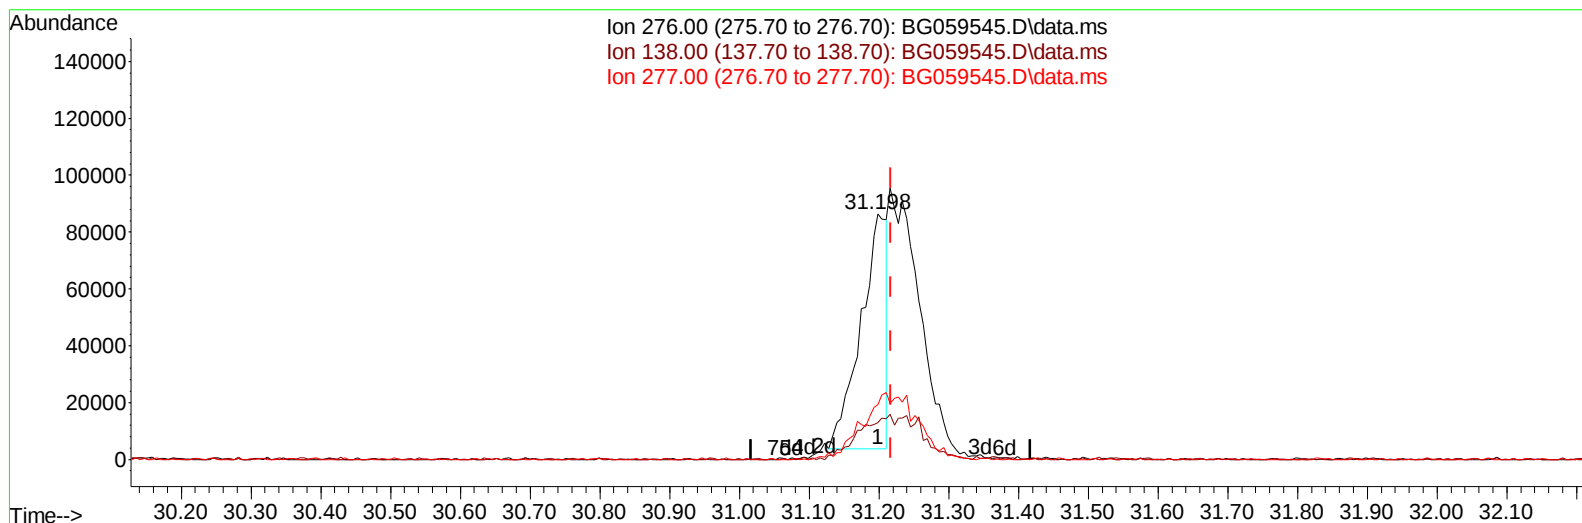

TIC: BG059545.D\data.ms

(96) Benzo(g,h,i)perylene

31.198min (-0.018) 7.15 ng/u1

response 212785

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	20.20	14.91#
277.00	22.80	22.23
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059545.D
 Acq On : 30 Oct 2023 12:03
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:08:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
 Supervised By :mohammad ahmed 11/01/2023

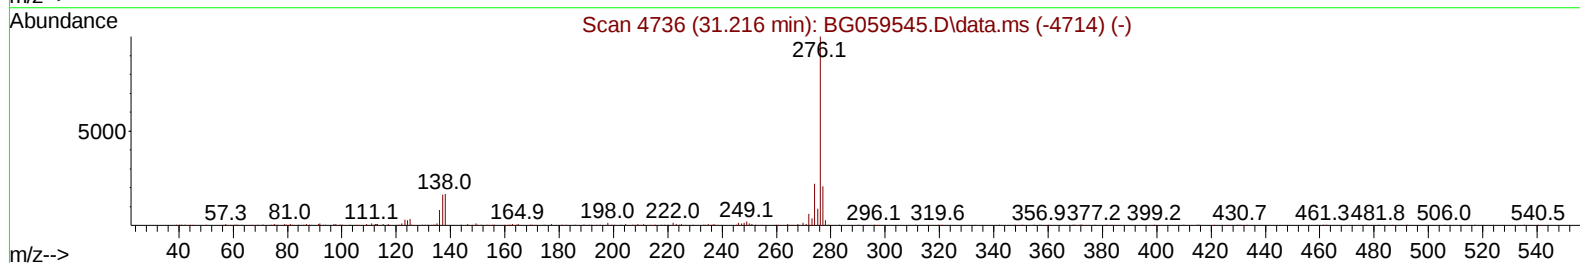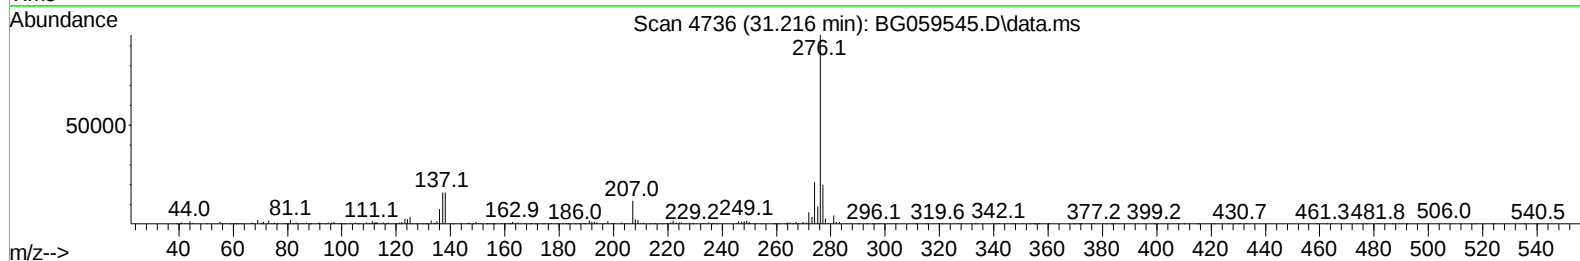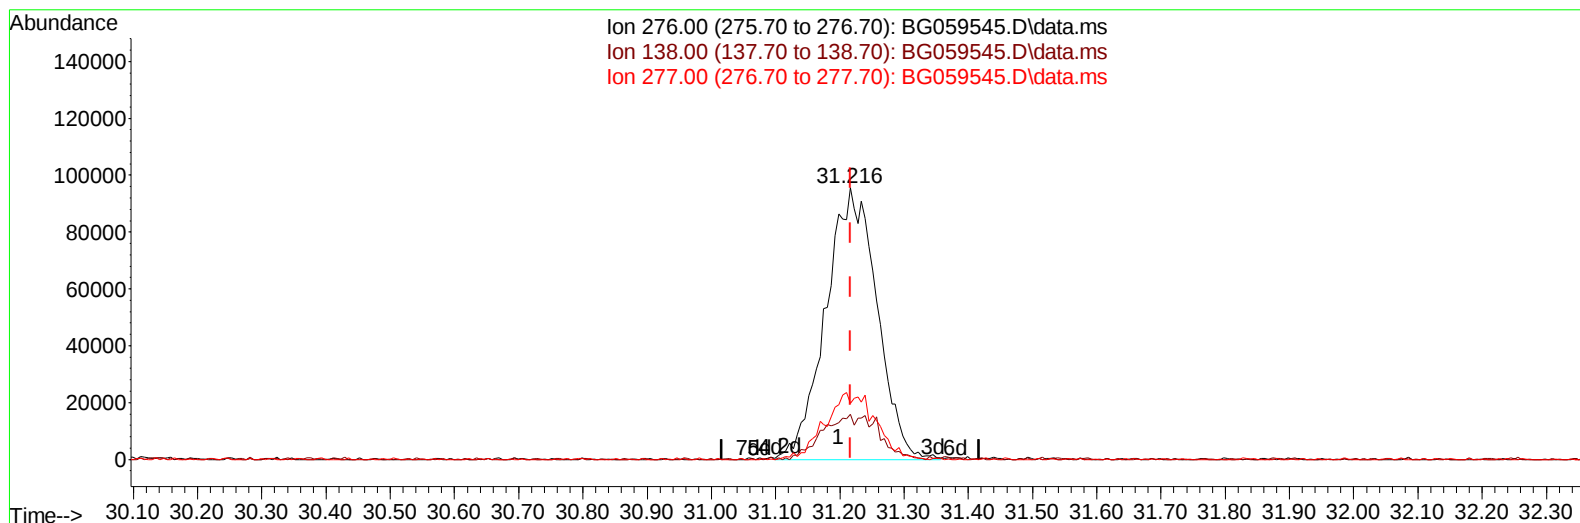

TIC: BG059545.D\data.ms

(96) Benzo(g,h,i)perylene

31.216min (-0.001) 17.79 ng/ul m

response 529154

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	20.20	16.73
277.00	22.80	20.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059545.D
 Acq On : 30 Oct 2023 12:03
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:10:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
 Supervised By :mohammad ahmed 11/01/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.361	152	80052	20.000	ng/ul	0.00
20) Naphthalene-d8	11.210	136	372908	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.988	164	232098	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.744	188	505095m	20.000	ng/ul	0.00
79) Chrysene-d12	22.080	240	383431	20.000	ng/ul	0.00
88) Perylene-d12	25.699	264	418509	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.660	96	13563	6.339	ng/uL	0.00
4) Pyridine-d5	4.095	84	101462	16.970	ng/ul	0.00
7) Phenol-d5	7.473	99	155049	18.848	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.679	67	69268	18.332	ng/ul	0.00
11) 2-Chlorophenol-d4	7.879	132	127875	19.161	ng/ul	0.00
15) 4-Methylphenol-d8	9.042	113	130502	19.996	ng/ul	0.00
21) Nitrobenzene-d5	9.565	128	60820	22.938	ng/ul	0.00
24) 2-Nitrophenol-d4	10.276	143	62957	23.129	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.805	165	127595	21.276	ng/ul	0.00
31) 4-Chloroaniline-d4	11.351	131	202056	20.467	ng/ul	0.00
46) Dimethylphthalate-d6	14.383	166	382507	18.191	ng/ul	0.00
49) Acenaphthylene-d8	14.694	160	461458	18.700	ng/ul	0.00
54) 4-Nitrophenol-d4	15.158	143	71338	19.784	ng/ul	0.00
60) Fluorene-d10	15.981	176	325413	18.108	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.081	200	45305m	18.940	ng/ul	0.00
73) Anthracene-d10	17.844	188	518000	18.930	ng/ul	0.00
81) Pyrene-d10	20.111	212	527768	19.802	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.435	264	465498	18.889	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.695	88	15390	6.427	ng/uL	96
5) Pyridine	4.113	79	102938	17.454	ng/ul	92
6) Benzaldehyde	7.509	77	79728	21.518	ng/ul	94
8) Phenol	7.503	94	146567	18.899	ng/ul	98
10) Bis(2-Chloroethyl)ether	7.773	93	101511	17.849	ng/ul	95
12) 2-Chlorophenol	7.914	128	136020	20.559	ng/ul#	84
13) 2-Methylphenol	8.778	108	124567	19.268	ng/ul	95
14) 2,2'-oxybis(1-Chloropr...	8.878	45	91886	17.169	ng/ul#	87
16) Acetophenone	9.207	105	195317	18.985	ng/ul	97
17) N-Nitroso-di-n-propyla...	9.171	70	84053	17.340	ng/ul#	98
18) 4-Methylphenol	9.107	108	132399	19.248	ng/ul	95
19) Hexachloroethane	9.453	117	50111	19.070	ng/ul	95
22) Nitrobenzene	9.600	77	131880	23.043	ng/ul	91
23) Isophorone	10.111	82	254993	17.692	ng/ul#	86
25) 2-Nitrophenol	10.311	139	66422	22.689	ng/ul#	82
26) 2,4-Dimethylphenol	10.335	107	155875	20.243	ng/ul	91
27) Bis(2-Chloroethoxy)met...	10.599	93	148118	18.457	ng/ul	95
29) 2,4-Dichlorophenol	10.834	162	121665	20.969	ng/ul#	89
30) Naphthalene	11.263	128	438514	18.867	ng/ul	97
32) 4-Chloroaniline	11.375	127	182085	19.417	ng/ul#	86
33) Hexachlorobutadiene	11.492	225	65031	18.683	ng/ul	99
34) Caprolactam	12.150	113	41162m	19.392	ng/ul	
35) 4-Chloro-3-methylphenol	12.438	107	144712	20.904	ng/ul	88

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059545.D
 Acq On : 30 Oct 2023 12:03
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Oct 31 05:10:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/01/2023
 Supervised By :mohammad ahmed 11/01/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
36) 2-Methylnaphthalene	12.838	142	313273	19.592	ng/ul	98
37) 1-Methylnaphthalene	13.055	142	316337	19.862	ng/ul#	94
39) 1,2,4,5-Tetrachloroben...	13.178	216	135018	20.169	ng/ul	98
40) Hexachlorocyclopentadiene	13.137	237	67457	17.286	ng/ul	98
41) 2,4,6-Trichlorophenol	13.419	196	93710	20.216	ng/ul#	90
42) 2,4,5-Trichlorophenol	13.490	196	103134m	20.551	ng/ul	
43) 1,1'-Biphenyl	13.831	154	414624	19.747	ng/ul	98
44) 2-Chloronaphthalene	13.883	162	310206	19.009	ng/ul	96
45) 2-Nitroaniline	14.089	65	72573	23.901	ng/ul	97
47) Dimethylphthalate	14.430	163	381333	18.356	ng/ul	97
48) 2,6-Dinitrotoluene	14.571	165	70779	22.585	ng/ul#	70
50) Acenaphthylene	14.724	152	535192	18.823	ng/ul	98
51) 3-Nitroaniline	14.912	138	88191	22.577	ng/ul#	79
52) Acenaphthene	15.053	153	327730	17.683	ng/ul	97
53) 2,4-Dinitrophenol	15.106	184	31811	17.865	ng/ul#	85
55) 4-Nitrophenol	15.176	109	86043	21.652	ng/ul	92
56) Dibenzofuran	15.388	168	446581	18.586	ng/ul	99
57) 2,4-Dinitrotoluene	15.346	165	97486	22.115	ng/ul	98
58) 2,3,4,6-Tetrachlorophenol	15.593	232	80236	20.371	ng/ul#	93
59) Diethylphthalate	15.781	149	409797	18.083	ng/ul	98
61) Fluorene	16.034	166	373091	17.987	ng/ul#	89
62) 4-Chlorophenyl-phenyle...	16.016	204	163167	18.406	ng/ul	94
63) 4-Nitroaniline	16.069	138	89124m	21.499	ng/ul	
66) 4,6-Dinitro-2-methylph...	16.093	198	50374m	19.982	ng/ul	
67) N-Nitrosodiphenylamine	16.234	169	325246	18.845	ng/ul	97
68) 4-Bromophenyl-phenylether	16.915	248	86340	17.082	ng/ul	93
69) Hexachlorobenzene	17.003	284	120550	20.637	ng/ul	96
70) Atrazine	17.168	200	109438m	20.463	ng/ul	
71) Pentachlorophenol	17.362	266	75184m	22.530	ng/ul	
72) Phenanthrene	17.785	178	610148m	18.582	ng/ul	
74) Anthracene	17.879	178	616223	18.586	ng/ul	96
75) 1,2,3,4-Tetrachloroben...	13.784	216	134994	20.070	ng/uL	96
76) Pentachlorobenzene	15.282	250	121508	19.037	ng/uL	98
77) Carbazole	18.149	167	567564	19.927	ng/ul	95
78) Di-n-butylphthalate	18.666	149	717672	18.339	ng/ul	99
80) Fluoranthene	19.777	202	648675	19.967	ng/ul	99
82) Pyrene	20.141	202	650218	19.268	ng/ul	97
83) Butylbenzylphthalate	21.010	149	304334	19.969	ng/ul	96
84) 3,3'-Dichlorobenzidine	21.968	252	207699	20.830	ng/ul#	91
85) Benzo(a)anthracene	22.062	228	581163	18.418	ng/ul	94
86) Bis(2-ethylhexyl)phtha...	21.909	149	446092	19.617	ng/ul#	96
87) Chrysene	22.133	228	540201	18.404	ng/ul	96
89) Di-n-octyl phthalate	23.261	149	738745	20.161	ng/ul	100
90) Benzo(b)fluoranthene	24.530	252	562280	18.535	ng/ul	95
91) Benzo(k)fluoranthene	24.606	252	569327	18.788	ng/ul	98
93) Benzo(a)pyrene	25.523	252	532906	18.586	ng/ul	95
94) Indeno(1,2,3-cd)pyrene	29.882	276	683703m	18.813	ng/ul	
95) Dibenzo(a,h)anthracene	29.994	278	574366m	19.136	ng/ul	
96) Benzo(g,h,i)perylene	31.216	276	529154m	17.790	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
BNA_G
LabSampleId :
SSTDCCC020

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/01/2023
Supervised By :mohammad ahmed 11/01/2023

