

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059546.D
 Acq On : 30 Oct 2023 12:57
 Operator : MA/JU
 Sample : PB156394BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK394

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059546.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.460	9	12	16	rVB4	7359	9370	0.40%	0.037%
2	3.495	16	18	19	rBV	6928	5623	0.24%	0.022%
3	3.654	41	45	51	rBV2	17521	28348	1.21%	0.113%
4	4.095	115	120	130	rBV	207831	344433	14.74%	1.372%
5	4.429	174	177	180	rBV4	11387	13677	0.59%	0.054%
6	4.529	190	194	196	rVB	4593	5252	0.22%	0.021%
7	4.559	196	199	201	rBV2	6667	5948	0.25%	0.024%
8	4.682	218	220	225	rBV3	6399	6379	0.27%	0.025%
9	4.870	248	252	259	rVB	6560	10796	0.46%	0.043%
10	5.117	290	294	298	rBV2	4711	7719	0.33%	0.031%
11	6.016	444	447	449	rBV2	5844	5190	0.22%	0.021%
12	6.169	469	473	474	rBV	5010	6163	0.26%	0.025%
13	6.345	502	503	505	rBV	6347	5851	0.25%	0.023%
14	6.445	518	520	523	rVB2	5643	6095	0.26%	0.024%
15	6.468	523	524	527	rBV	6320	5969	0.26%	0.024%
16	6.739	567	570	573	rVB	6087	6579	0.28%	0.026%
17	6.862	589	591	597	rBV	4950	6967	0.30%	0.028%
18	7.167	640	643	646	rBV	5122	6131	0.26%	0.024%
19	7.473	688	695	705	rVB	333622	576009	24.65%	2.295%
20	7.679	724	730	737	rBV	219479	369123	15.80%	1.471%
21	7.878	755	764	771	rBV	330880	592926	25.38%	2.362%
22	8.102	797	802	804	rBV	5521	7717	0.33%	0.031%
23	8.366	838	847	854	rVB	244595	429062	18.36%	1.709%
24	8.619	886	890	892	rVB	4859	5657	0.24%	0.023%
25	8.648	892	895	899	rVB	4710	6669	0.29%	0.027%
26	9.042	955	962	970	rVV	447674	777476	33.28%	3.097%
27	9.312	1005	1008	1010	rVV	4460	5424	0.23%	0.022%
28	9.335	1010	1012	1016	rVB	7020	7527	0.32%	0.030%
29	9.365	1016	1017	1022	rBV	4528	6072	0.26%	0.024%
30	9.559	1043	1050	1057	rVV	279982	512155	21.92%	2.040%
31	10.281	1166	1173	1182	rVB2	252065	464492	19.88%	1.850%
32	10.516	1210	1213	1217	rVB3	5929	6421	0.27%	0.026%
33	10.728	1247	1249	1252	rBV	5540	6980	0.30%	0.028%
34	10.804	1255	1262	1271	rVV	454150	814349	34.85%	3.244%
35	11.127	1313	1317	1318	rBV	4370	5188	0.22%	0.021%
36	11.216	1323	1332	1339	rBV	370509	702480	30.07%	2.799%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059546.D
 Acq On : 30 Oct 2023 12:57
 Operator : MA/JU
 Sample : PB156394BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK394

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

37	11.351	1345	1355	1362	rBV2	457970	867959	37.15%	3.458%
38	11.398	1362	1363	1367	rVB	6533	7631	0.33%	0.030%
39	11.574	1389	1393	1394	rBV	7115	6524	0.28%	0.026%
40	12.015	1463	1468	1470	rVV2	5212	6700	0.29%	0.027%

41	12.068	1476	1477	1481	rVB	4876	5351	0.23%	0.021%
42	12.150	1488	1491	1492	rBV	4391	5241	0.22%	0.021%
43	12.279	1512	1513	1517	rVB	8258	7636	0.33%	0.030%
44	12.320	1517	1520	1523	rBV	5305	7475	0.32%	0.030%
45	12.385	1528	1531	1535	rVB	6397	6945	0.30%	0.028%

46	12.449	1538	1542	1547	rVB	5107	8670	0.37%	0.035%
47	12.767	1595	1596	1601	rVB	15704	17378	0.74%	0.069%
48	12.937	1624	1625	1628	rBV2	5330	5563	0.24%	0.022%
49	13.149	1659	1661	1664	rVB	4937	5469	0.23%	0.022%
50	13.231	1673	1675	1678	rBV	7223	7578	0.32%	0.030%

51	13.284	1680	1684	1687	rVV4	6410	11147	0.48%	0.044%
52	13.348	1694	1695	1698	rVB2	6502	5607	0.24%	0.022%
53	13.395	1701	1703	1707	rVB	5689	8073	0.35%	0.032%
54	13.636	1742	1744	1746	rVV	6315	6117	0.26%	0.024%
55	13.666	1748	1749	1751	rBV2	6936	6500	0.28%	0.026%

56	13.713	1755	1757	1760	rVV4	4552	5361	0.23%	0.021%
57	13.813	1771	1774	1775	rVV	6425	7089	0.30%	0.028%
58	13.830	1775	1777	1781	rVB4	11799	10603	0.45%	0.042%
59	13.936	1792	1795	1798	rVB2	6024	5473	0.23%	0.022%
60	14.300	1855	1857	1860	rVV	4642	5419	0.23%	0.022%

61	14.388	1865	1872	1881	rVB	956938	1430797	61.24%	5.700%
62	14.694	1915	1924	1933	rVB	1121305	1769310	75.73%	7.049%
63	14.759	1933	1935	1938	rBV	6532	8477	0.36%	0.034%
64	14.888	1955	1957	1961	rVB2	7117	8354	0.36%	0.033%
65	14.929	1961	1964	1965	rBV2	7347	6254	0.27%	0.025%

66	14.994	1968	1975	1983	rBV	732093	1115686	47.75%	4.445%
67	15.158	1995	2003	2010	rBV	497876	782948	33.51%	3.119%
68	15.323	2029	2031	2033	rBV3	9601	9237	0.40%	0.037%
69	15.387	2040	2042	2045	rVB2	9273	9637	0.41%	0.038%
70	15.446	2051	2052	2057	rVB3	7965	8198	0.35%	0.033%

71	15.746	2102	2103	2107	rVB2	6355	5919	0.25%	0.024%
72	15.981	2136	2143	2153	rBV	1376844	2068153	88.52%	8.239%
73	16.081	2154	2160	2167	rBV	303123	469640	20.10%	1.871%
74	16.468	2224	2226	2229	rBV2	5156	5414	0.23%	0.022%
75	16.498	2229	2231	2235	rBV2	7842	8703	0.37%	0.035%

76	16.556	2238	2241	2247	rBV7	9510	18996	0.81%	0.076%
----	--------	------	------	------	------	------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059546.D
 Acq On : 30 Oct 2023 12:57
 Operator : MA/JU
 Sample : PB156394BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK394

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

77	16.750	2272	2274	2277	rBV3	5307	5735	0.25%	0.023%
78	17.185	2345	2348	2351	rVB3	7399	8156	0.35%	0.032%
79	17.285	2361	2365	2368	rVB3	9872	14305	0.61%	0.057%
80	17.391	2382	2383	2385	rBV	13817	7292	0.31%	0.029%
81	17.420	2385	2388	2394	rVB6	8355	13664	0.58%	0.054%
82	17.538	2407	2408	2411	rBV3	8377	5710	0.24%	0.023%
83	17.743	2436	2443	2451	rBV	909495	1361174	58.26%	5.423%
84	17.843	2454	2460	2468	rVB2	1539869	2336431	100.00%	9.308%
85	17.902	2468	2470	2471	rBV2	5896	5391	0.23%	0.021%
86	18.084	2500	2501	2503	rBV2	7306	5211	0.22%	0.021%
87	18.149	2511	2512	2515	rVB3	8090	5661	0.24%	0.023%
88	18.225	2524	2525	2528	rVB3	10349	5388	0.23%	0.021%
89	18.478	2566	2568	2570	rVB3	12145	6952	0.30%	0.028%
90	18.607	2589	2590	2593	rBV3	8247	7667	0.33%	0.031%
91	18.777	2617	2619	2626	rBV8	7396	20327	0.87%	0.081%
92	18.948	2646	2648	2651	rBV4	10939	16065	0.69%	0.064%
93	19.159	2683	2684	2685	rBV	11025	5572	0.24%	0.022%
94	19.676	2770	2772	2776	rVB5	22288	23063	0.99%	0.092%
95	19.741	2781	2783	2788	rVB4	21274	31072	1.33%	0.124%
96	19.858	2801	2803	2805	rBV3	13555	12441	0.53%	0.050%
97	20.117	2841	2847	2855	rVB	1571075	2302058	98.53%	9.171%
98	22.085	3176	3182	3191	rVB2	682645	1267591	54.25%	5.050%
99	25.452	3744	3755	3769	rVB3	616298	1971716	84.39%	7.855%
100	25.693	3788	3796	3809	rVB3	360151	1116894	47.80%	4.450%




Sum of corrected areas: 25100985

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
Data File : BG059546.D
Acq On : 30 Oct 2023 12:57
Operator : MA/JU
Sample : PB156394BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK394

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

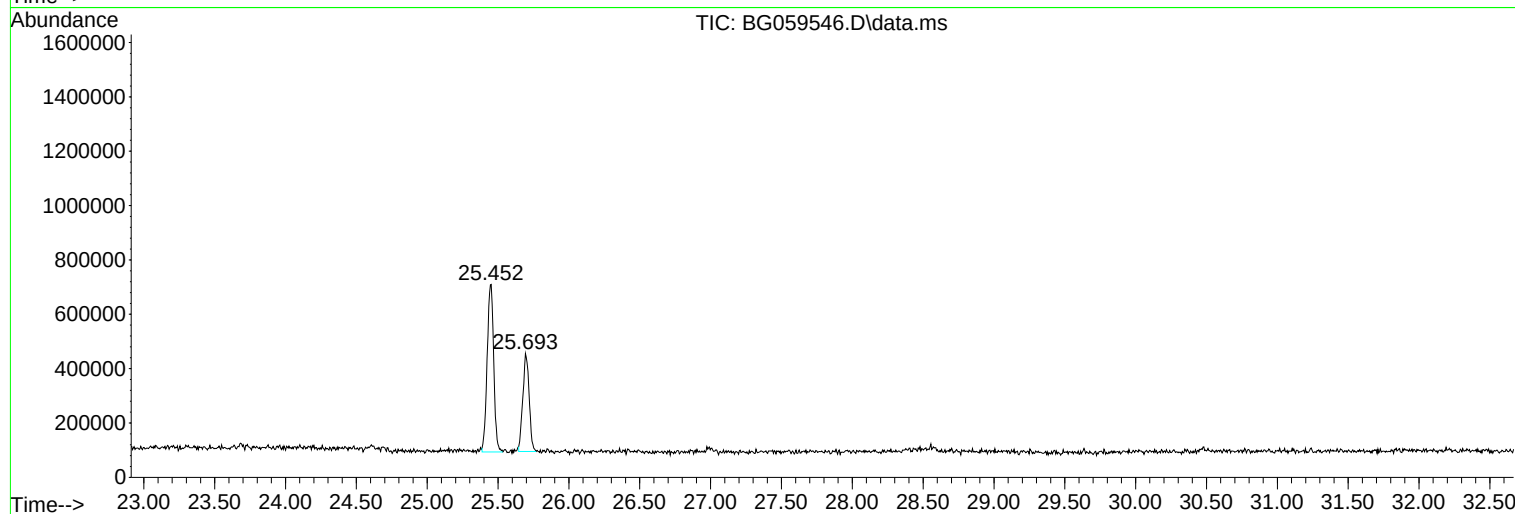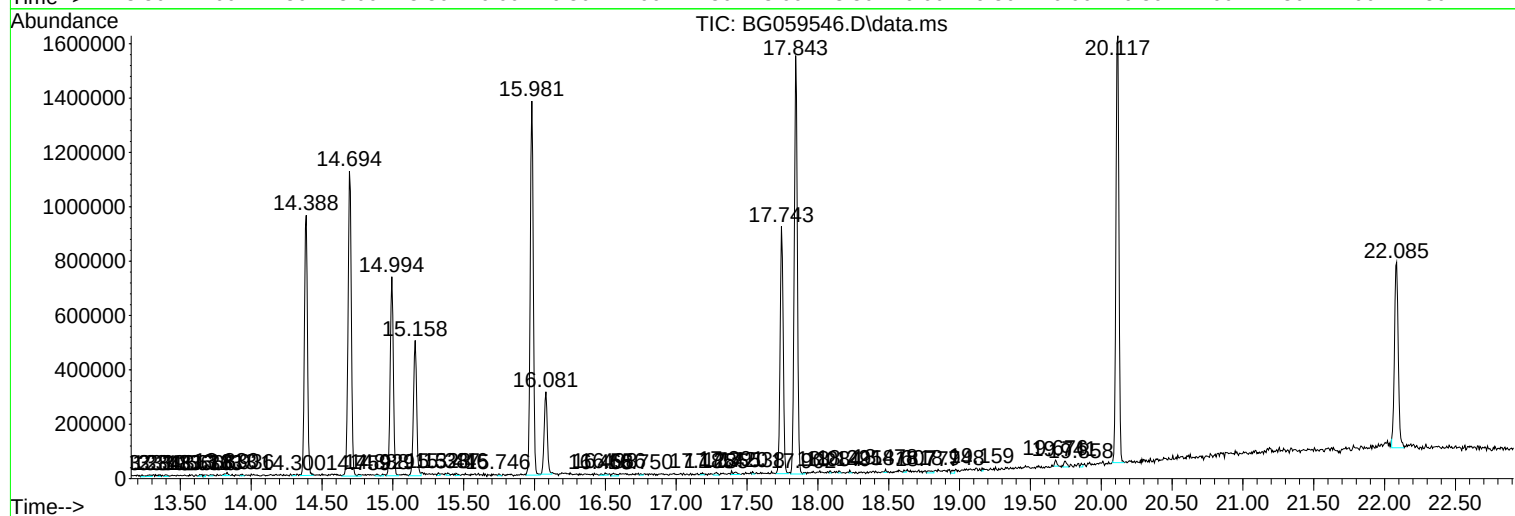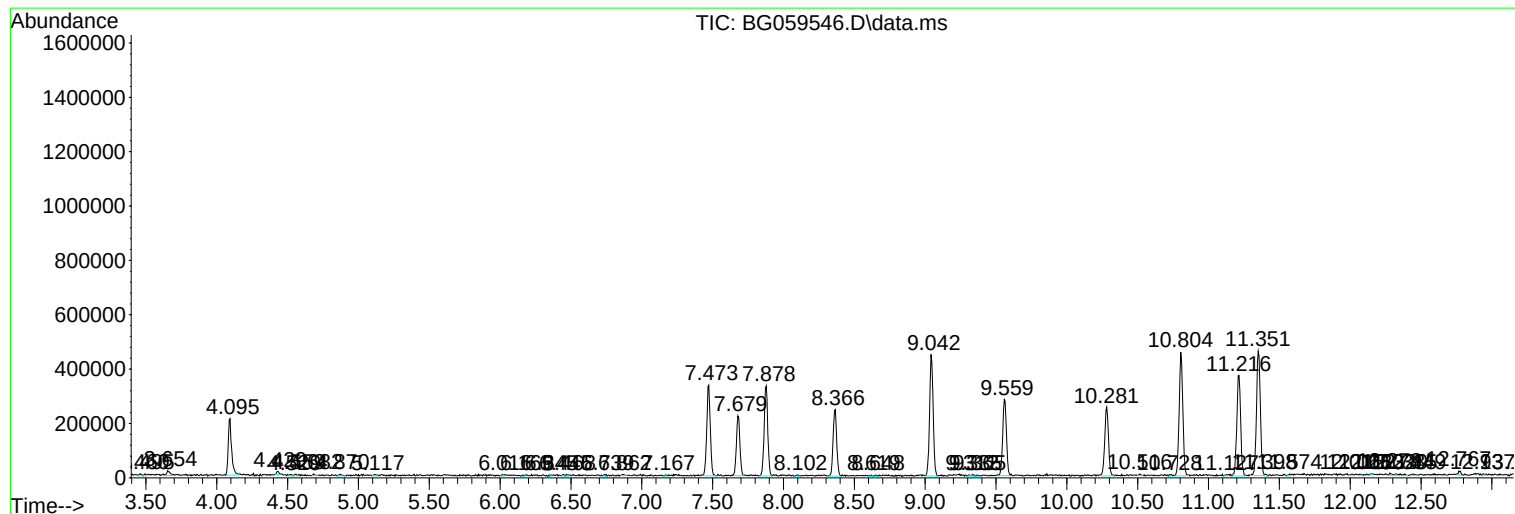

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
Data File : BG059546.D
Acq On : 30 Oct 2023 12:57
Operator : MA/JU
Sample : PB156394BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK394

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
Data File : BG059546.D
Acq On : 30 Oct 2023 12:57
Operator : MA/JU
Sample : PB156394BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK394

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------