

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059550.D
 Acq On : 30 Oct 2023 18:08
 Operator : MA/JU
 Sample : PB156396BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK396

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059550.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.547	23	27	31	rBV5	8960	12298	0.46%	0.045%
2	3.652	43	45	48	rBV2	23106	23853	0.89%	0.088%
3	3.782	66	67	69	rBV2	10173	7636	0.29%	0.028%
4	3.846	77	78	81	rBV2	5906	5913	0.22%	0.022%
5	3.887	83	85	86	rBV2	7728	5566	0.21%	0.021%
6	3.981	96	101	102	rBV4	8117	10034	0.38%	0.037%
7	4.081	114	118	129	rVB2	203628	373280	13.97%	1.377%
8	4.416	171	175	176	rVV3	6356	8974	0.34%	0.033%
9	4.428	176	177	182	rVB	11726	15943	0.60%	0.059%
10	5.233	313	314	317	rBV	5134	5295	0.20%	0.020%
11	5.809	409	412	413	rBV	5426	5844	0.22%	0.022%
12	6.414	512	515	517	rVB	5672	5588	0.21%	0.021%
13	7.360	674	676	679	rBV3	3760	5209	0.19%	0.019%
14	7.465	686	694	702	rVB2	306378	549582	20.56%	2.027%
15	7.524	702	704	708	rBV	4676	5521	0.21%	0.020%
16	7.677	724	730	737	rBV	218426	359693	13.46%	1.326%
17	7.871	756	763	773	rVB2	322274	564717	21.13%	2.082%
18	8.141	806	809	812	rBV	4911	7044	0.26%	0.026%
19	8.194	817	818	825	rVB	4753	8519	0.32%	0.031%
20	8.359	839	846	853	rVB	237756	419050	15.68%	1.545%
21	8.494	866	869	871	rVB	5024	6321	0.24%	0.023%
22	8.605	882	888	891	rVB	5628	10250	0.38%	0.038%
23	8.652	891	896	898	rBV	4648	6736	0.25%	0.025%
24	8.699	901	904	906	rVB	6036	5122	0.19%	0.019%
25	8.729	906	909	911	rBV2	5669	6187	0.23%	0.023%
26	8.811	921	923	925	rBV2	5853	5671	0.21%	0.021%
27	8.964	948	949	954	rBV2	6233	6493	0.24%	0.024%
28	9.040	954	962	972	rVV2	432358	725406	27.14%	2.675%
29	9.205	985	990	991	rBV2	5161	6372	0.24%	0.023%
30	9.287	1002	1004	1009	rVB2	3215	5158	0.19%	0.019%
31	9.357	1013	1016	1018	rBV	6249	5863	0.22%	0.022%
32	9.440	1026	1030	1032	rVB	4956	6162	0.23%	0.023%
33	9.557	1039	1050	1058	rBV2	279363	503902	18.85%	1.858%
34	9.704	1072	1075	1077	rBV2	6291	6807	0.25%	0.025%
35	9.786	1088	1089	1093	rBV	5660	6079	0.23%	0.022%
36	10.057	1130	1135	1136	rBV	6700	10705	0.40%	0.039%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059550.D
 Acq On : 30 Oct 2023 18:08
 Operator : MA/JU
 Sample : PB156396BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK396

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

37	10.280	1164	1173	1180	rVV	237606	440025	16.46%	1.623%
38	10.339	1180	1183	1186	rVB	5054	5533	0.21%	0.020%
39	10.585	1223	1225	1228	rBV	6587	6845	0.26%	0.025%
40	10.715	1245	1247	1251	rVB	6208	7407	0.28%	0.027%

41	10.803	1254	1262	1269	rVB	423786	763011	28.55%	2.814%
42	11.208	1322	1331	1338	rBV	353448	630826	23.60%	2.326%
43	11.349	1344	1355	1362	rBV2	432711	817372	30.58%	3.014%
44	11.661	1404	1408	1412	rVV	2370	5686	0.21%	0.021%
45	11.984	1460	1463	1465	rBV	6965	6530	0.24%	0.024%

46	12.113	1483	1485	1490	rVB2	5805	9061	0.34%	0.033%
47	12.189	1497	1498	1504	rVB2	7717	12685	0.47%	0.047%
48	12.248	1504	1508	1509	rBV2	7125	8726	0.33%	0.032%
49	12.324	1520	1521	1526	rVB3	4282	6413	0.24%	0.024%
50	12.512	1550	1553	1556	rVB	7300	8572	0.32%	0.032%

51	12.571	1559	1563	1566	rVB	5177	7039	0.26%	0.026%
52	12.665	1575	1579	1580	rBV	4824	6649	0.25%	0.025%
53	12.771	1593	1597	1601	rVB2	10350	16643	0.62%	0.061%
54	13.188	1666	1668	1671	rBV2	4899	5677	0.21%	0.021%
55	13.317	1687	1690	1693	rBV2	6756	8493	0.32%	0.031%

56	13.458	1708	1714	1717	rBV	2635	5909	0.22%	0.022%
57	13.641	1742	1745	1748	rBV	5282	8423	0.32%	0.031%
58	14.022	1806	1810	1811	rBV	5081	5187	0.19%	0.019%
59	14.387	1865	1872	1879	rBV	1045056	1372705	51.36%	5.062%
60	14.475	1884	1887	1889	rVV	5814	7213	0.27%	0.027%

61	14.516	1892	1894	1895	rVB2	9635	6279	0.23%	0.023%
62	14.569	1901	1903	1905	rVB2	7392	6412	0.24%	0.024%
63	14.604	1905	1909	1911	rVB2	7054	10931	0.41%	0.040%
64	14.628	1911	1913	1916	rBV	11392	13096	0.49%	0.048%
65	14.692	1917	1924	1931	rVB2	1283805	2000215	74.84%	7.376%

66	14.792	1940	1941	1944	rVB2	8117	7163	0.27%	0.026%
67	14.986	1967	1974	1983	rVB	777022	1255267	46.97%	4.629%
68	15.051	1983	1985	1987	rBV3	6439	6438	0.24%	0.024%
69	15.151	1996	2002	2012	rBV	557614	906544	33.92%	3.343%
70	15.480	2056	2058	2062	rBV2	6836	8732	0.33%	0.032%

71	15.550	2067	2070	2072	rVB2	10547	10109	0.38%	0.037%
72	15.574	2072	2074	2075	rBV2	7651	5904	0.22%	0.022%
73	15.832	2116	2118	2122	rVB2	5256	6085	0.23%	0.022%
74	15.903	2126	2130	2133	rBV4	13614	21833	0.82%	0.081%
75	15.979	2136	2143	2149	rBV	1468057	2256214	84.42%	8.320%

76	16.079	2153	2160	2168	rBV	325731	533146	19.95%	1.966%
----	--------	------	------	------	-----	--------	--------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059550.D
 Acq On : 30 Oct 2023 18:08
 Operator : MA/JU
 Sample : PB156396BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK396

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

77	16.202	2179	2181	2184	rBV4	9709	11601	0.43%	0.043%
78	16.408	2214	2216	2218	rBV	6991	7334	0.27%	0.027%
79	16.602	2247	2249	2250	rBV2	8008	6601	0.25%	0.024%
80	16.854	2290	2292	2295	rVB3	6357	5448	0.20%	0.020%
81	17.095	2331	2333	2335	rBV3	7440	8450	0.32%	0.031%
82	17.166	2344	2345	2347	rBV2	7473	5788	0.22%	0.021%
83	17.183	2347	2348	2351	rVB	13995	8096	0.30%	0.030%
84	17.213	2351	2353	2354	rBV	8028	7658	0.29%	0.028%
85	17.277	2362	2364	2366	rBV2	5603	5490	0.21%	0.020%
86	17.407	2383	2386	2388	rBV3	9842	11931	0.45%	0.044%
87	17.542	2407	2409	2413	rVB5	7504	6376	0.24%	0.024%
88	17.742	2436	2443	2451	rVB	965446	1481424	55.43%	5.463%
89	17.842	2453	2460	2468	rBV	1698133	2562062	95.86%	9.448%
90	18.335	2541	2544	2548	rBV6	9668	11697	0.44%	0.043%
91	18.641	2594	2596	2600	rVB5	9420	7614	0.28%	0.028%
92	18.729	2609	2611	2613	rBV3	7965	5028	0.19%	0.019%
93	18.805	2622	2624	2626	rVB2	7116	5746	0.21%	0.021%
94	19.404	2724	2726	2729	rBV3	11190	15800	0.59%	0.058%
95	19.434	2729	2731	2733	rVV2	10994	6691	0.25%	0.025%
96	19.745	2781	2784	2787	rVB	28159	35334	1.32%	0.130%
97	20.109	2840	2846	2853	rBV	1831899	2672579	100.00%	9.856%
98	22.078	3175	3181	3189	rVB	775226	1381613	51.70%	5.095%
99	25.438	3743	3753	3764	rVB2	800459	2502415	93.63%	9.228%
100	25.685	3787	3795	3806	rVB	459122	1394873	52.19%	5.144%




Sum of corrected areas: 27117440

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
Data File : BG059550.D
Acq On : 30 Oct 2023 18:08
Operator : MA/JU
Sample : PB156396BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK396

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

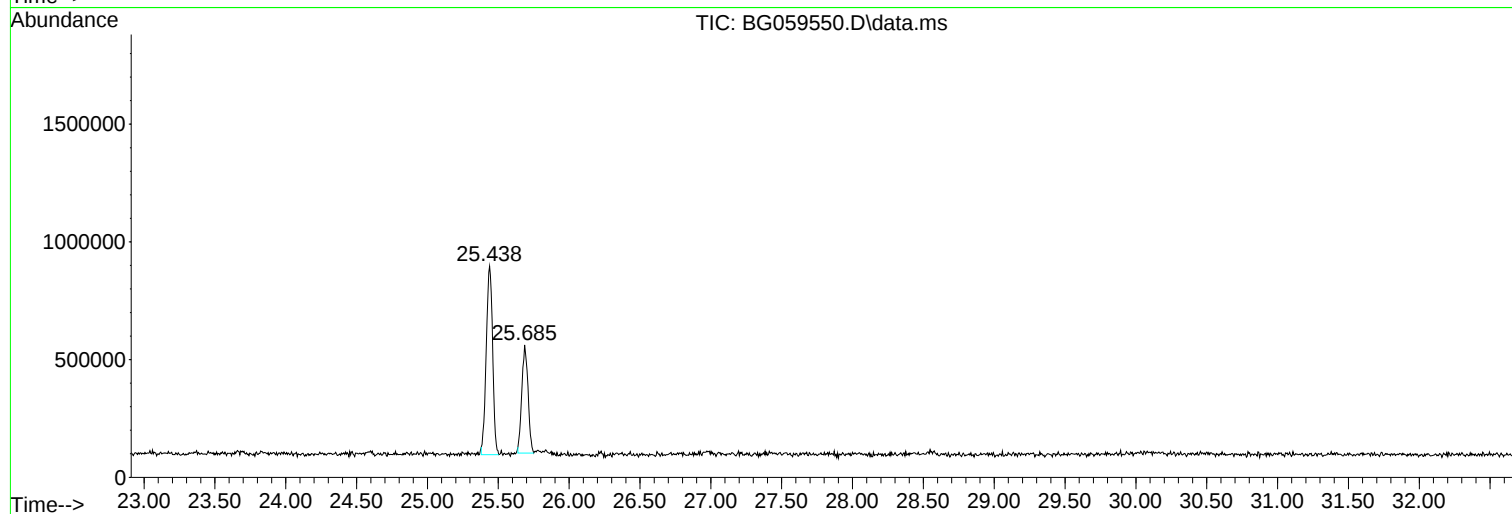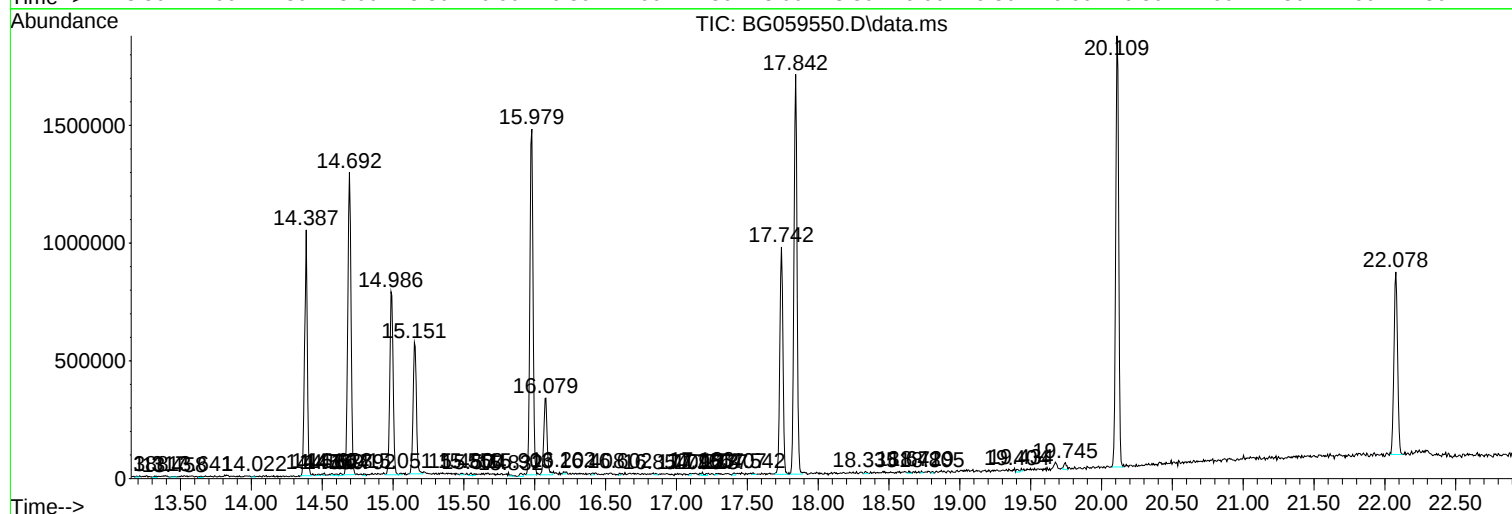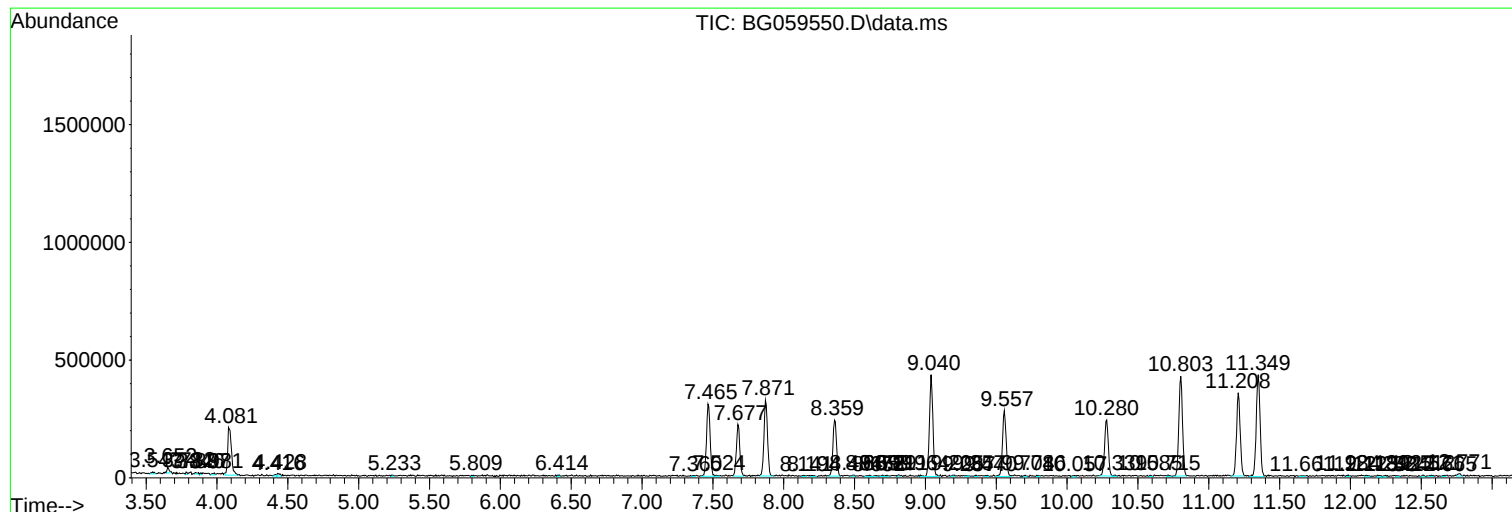

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
Data File : BG059550.D
Acq On : 30 Oct 2023 18:08
Operator : MA/JU
Sample : PB156396BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK396

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
Data File : BG059550.D
Acq On : 30 Oct 2023 18:08
Operator : MA/JU
Sample : PB156396BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK396

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc