

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059551.D
 Acq On : 30 Oct 2023 18:48
 Operator : MA/JU
 Sample : PB156398BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK398

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059551.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.612	36	38	40	rVV3	4902	5556	0.20%	0.021%
2	3.659	42	46	51	rVV	19462	32421	1.18%	0.123%
3	3.882	80	84	86	rBV	4926	8534	0.31%	0.032%
4	3.929	90	92	93	rBV	6183	5159	0.19%	0.019%
5	4.088	114	119	129	rBV	191303	329561	12.04%	1.246%
6	4.329	157	160	163	rVB2	8740	8635	0.32%	0.033%
7	4.429	173	177	180	rBV	12579	13032	0.48%	0.049%
8	4.682	216	220	224	rVB	6494	7490	0.27%	0.028%
9	4.729	224	228	230	rBV4	5967	7388	0.27%	0.028%
10	4.993	270	273	275	rBV	4703	5484	0.20%	0.021%
11	5.216	307	311	315	rVV2	5780	8495	0.31%	0.032%
12	5.251	315	317	322	rVB	7753	11964	0.44%	0.045%
13	5.539	364	366	371	rBV3	6405	7917	0.29%	0.030%
14	5.862	418	421	423	rVB	5787	5210	0.19%	0.020%
15	6.021	445	448	451	rVB	4957	7467	0.27%	0.028%
16	6.127	462	466	470	rVB2	9243	9117	0.33%	0.034%
17	6.338	499	502	504	rVB2	6174	5786	0.21%	0.022%
18	6.397	510	512	515	rVV	5483	5611	0.20%	0.021%
19	6.562	538	540	543	rVB	7050	8987	0.33%	0.034%
20	6.603	543	547	550	rBV	6136	9727	0.36%	0.037%
21	6.732	567	569	572	rVB2	5394	5595	0.20%	0.021%
22	6.861	588	591	592	rBV2	4748	5370	0.20%	0.020%
23	6.897	595	597	600	rBV	7200	9023	0.33%	0.034%
24	7.126	632	636	638	rBV	6044	5614	0.21%	0.021%
25	7.155	638	641	644	rVB	6554	7097	0.26%	0.027%
26	7.190	644	647	649	rBV2	6049	6269	0.23%	0.024%
27	7.466	685	694	701	rBV	342482	589421	21.53%	2.228%
28	7.607	714	718	719	rBV	4789	5772	0.21%	0.022%
29	7.678	724	730	737	rVV	220000	379362	13.85%	1.434%
30	7.872	757	763	773	rVV	342029	607892	22.20%	2.298%
31	8.360	839	846	854	rVB2	230896	413042	15.08%	1.561%
32	8.530	873	875	879	rVB2	6665	7718	0.28%	0.029%
33	8.565	879	881	885	rBV	5819	5812	0.21%	0.022%
34	8.777	914	917	920	rBV	5824	5922	0.22%	0.022%
35	8.941	942	945	947	rVB2	6749	5529	0.20%	0.021%
36	9.041	955	962	970	rBV2	444019	772549	28.21%	2.920%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059551.D
 Acq On : 30 Oct 2023 18:48
 Operator : MA/JU
 Sample : PB156398BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK398

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

37	9.394	1017	1022	1024	rBV2	4604	8759	0.32%	0.033%
38	9.558	1043	1050	1057	rBV	285890	514988	18.81%	1.946%
39	9.770	1083	1086	1089	rBV2	4432	6423	0.23%	0.024%
40	9.940	1112	1115	1118	rVB	4182	6466	0.24%	0.024%

41	10.152	1149	1151	1154	rBV	5150	6574	0.24%	0.025%
42	10.275	1165	1172	1181	rVB2	245316	461392	16.85%	1.744%
43	10.498	1207	1210	1211	rBV2	7317	5855	0.21%	0.022%
44	10.804	1253	1262	1270	rBV	425748	795235	29.04%	3.006%
45	10.939	1284	1285	1288	rBV	7051	6439	0.24%	0.024%

46	11.145	1317	1320	1322	rBV	4429	5624	0.21%	0.021%
47	11.209	1324	1331	1339	rVB	329283	597144	21.81%	2.257%
48	11.350	1346	1355	1364	rVB	425521	788207	28.79%	2.979%
49	11.456	1370	1373	1374	rBV	5511	5633	0.21%	0.021%
50	12.431	1535	1539	1540	rBV2	6293	6322	0.23%	0.024%

51	12.572	1558	1563	1565	rVV2	7101	8329	0.30%	0.031%
52	12.766	1591	1596	1601	rVV3	11814	21051	0.77%	0.080%
53	13.089	1649	1651	1654	rBV	6022	6901	0.25%	0.026%
54	13.266	1676	1681	1685	rVB4	8320	12384	0.45%	0.047%
55	13.430	1705	1709	1711	rBV2	3565	6044	0.22%	0.023%

56	13.694	1751	1754	1758	rVB4	5377	8609	0.31%	0.033%
57	13.830	1770	1777	1781	rBV5	18402	35949	1.31%	0.136%
58	13.929	1790	1794	1795	rBV2	4826	5480	0.20%	0.021%
59	13.976	1801	1802	1807	rVB3	5919	5589	0.20%	0.021%
60	14.382	1864	1871	1877	rBV	1019855	1457646	53.23%	5.509%

61	14.464	1883	1885	1887	rVB	8223	5973	0.22%	0.023%
62	14.494	1887	1890	1891	rBV	5820	6925	0.25%	0.026%
63	14.687	1917	1923	1931	rVB2	1072189	1723792	62.95%	6.515%
64	14.740	1931	1932	1934	rVB	8915	5559	0.20%	0.021%
65	14.987	1966	1974	1983	rVB	608565	1001584	36.58%	3.786%

66	15.152	1995	2002	2008	rBV	496699	802078	29.29%	3.032%
67	15.199	2008	2010	2016	rVV5	16000	25649	0.94%	0.097%
68	15.263	2019	2021	2023	rBV3	6214	5859	0.21%	0.022%
69	15.298	2025	2027	2029	rBV3	7059	5190	0.19%	0.020%
70	15.463	2051	2055	2056	rBV3	8668	8500	0.31%	0.032%

71	15.663	2087	2089	2091	rVB2	8655	7564	0.28%	0.029%
72	15.833	2116	2118	2120	rBV3	10168	8079	0.30%	0.031%
73	15.880	2124	2126	2129	rBV	6450	7240	0.26%	0.027%
74	15.974	2135	2142	2151	rVB	1341066	2021362	73.82%	7.640%
75	16.074	2153	2159	2166	rBV2	337952	510261	18.64%	1.929%

76	16.215	2179	2183	2186	rVB6	9029	14401	0.53%	0.054%
----	--------	------	------	------	------	------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059551.D
 Acq On : 30 Oct 2023 18:48
 Operator : MA/JU
 Sample : PB156398BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK398

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

77	16.444	2216	2222	2223	rBV4	7134	8272	0.30%	0.031%
78	16.562	2238	2242	2243	rVV4	9217	10016	0.37%	0.038%
79	16.603	2246	2249	2252	rVB3	6083	7917	0.29%	0.030%
80	16.650	2255	2257	2260	rVB3	6625	6133	0.22%	0.023%
81	16.685	2260	2263	2265	rBV2	5549	5894	0.22%	0.022%
82	16.808	2282	2284	2286	rVB2	6850	5778	0.21%	0.022%
83	16.826	2286	2287	2290	rBV3	8492	8123	0.30%	0.031%
84	17.249	2357	2359	2361	rBV	10466	12574	0.46%	0.048%
85	17.737	2435	2442	2452	rVB	899975	1390862	50.80%	5.257%
86	17.837	2452	2459	2466	rBV	1638102	2580510	94.24%	9.753%
87	18.001	2484	2487	2490	rBV4	7538	8767	0.32%	0.033%
88	18.072	2497	2499	2501	rBV3	8969	8168	0.30%	0.031%
89	18.283	2532	2535	2538	rBV3	8144	9503	0.35%	0.036%
90	18.360	2546	2548	2551	rVB5	10574	9527	0.35%	0.036%
91	18.706	2605	2607	2610	rBV4	8974	9427	0.34%	0.036%
92	19.306	2707	2709	2711	rBV3	10956	7848	0.29%	0.030%
93	19.423	2728	2729	2732	rBV3	9569	6329	0.23%	0.024%
94	19.664	2768	2770	2771	rBV2	25306	20895	0.76%	0.079%
95	20.052	2834	2836	2837	rBV2	13310	8365	0.31%	0.032%
96	20.110	2840	2846	2852	rVB	1890937	2738143	100.00%	10.349%
97	22.073	3175	3180	3188	rVB	744325	1383639	50.53%	5.230%
98	25.434	3742	3752	3763	rVB3	840016	2582104	94.30%	9.759%
99	25.686	3786	3795	3805	rVB	430673	1332393	48.66%	5.036%
100	28.988	4355	4357	4359	rBV3	27183	18299	0.67%	0.069%




Sum of corrected areas: 26458073

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
Data File : BG059551.D
Acq On : 30 Oct 2023 18:48
Operator : MA/JU
Sample : PB156398BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK398

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

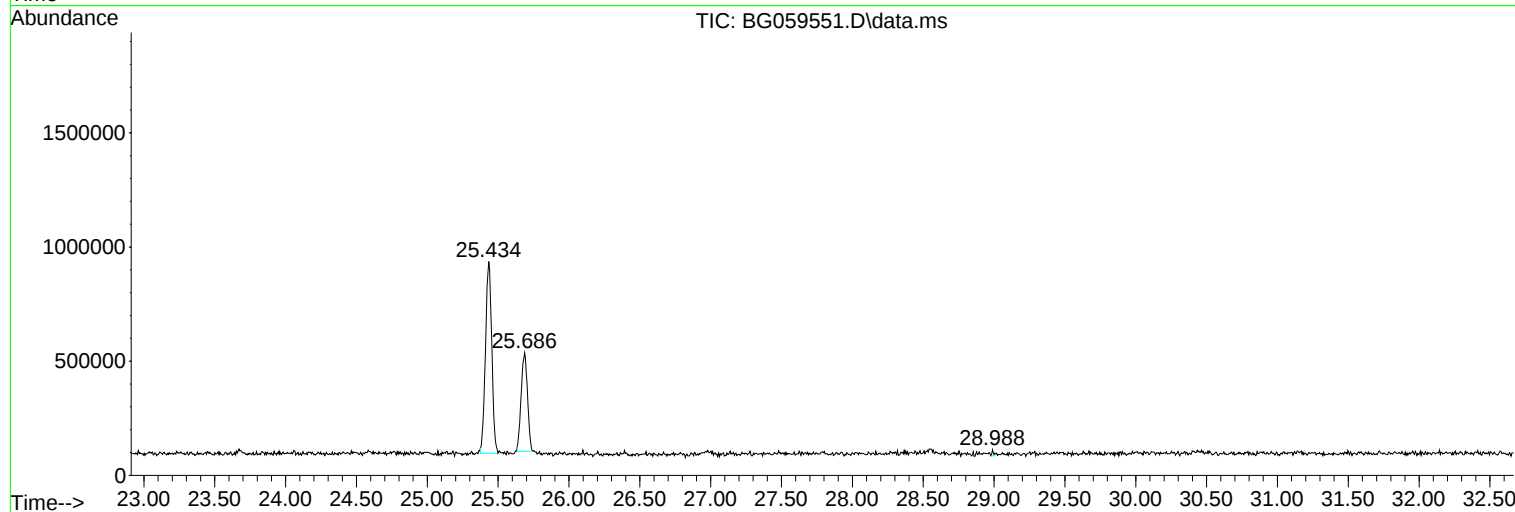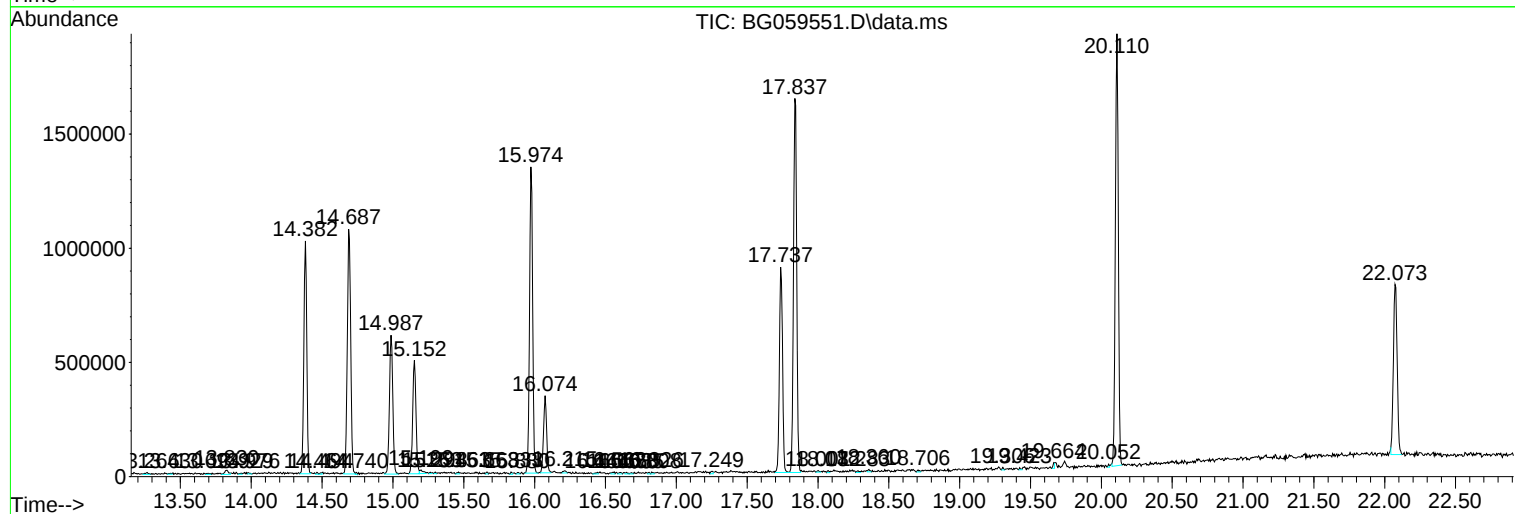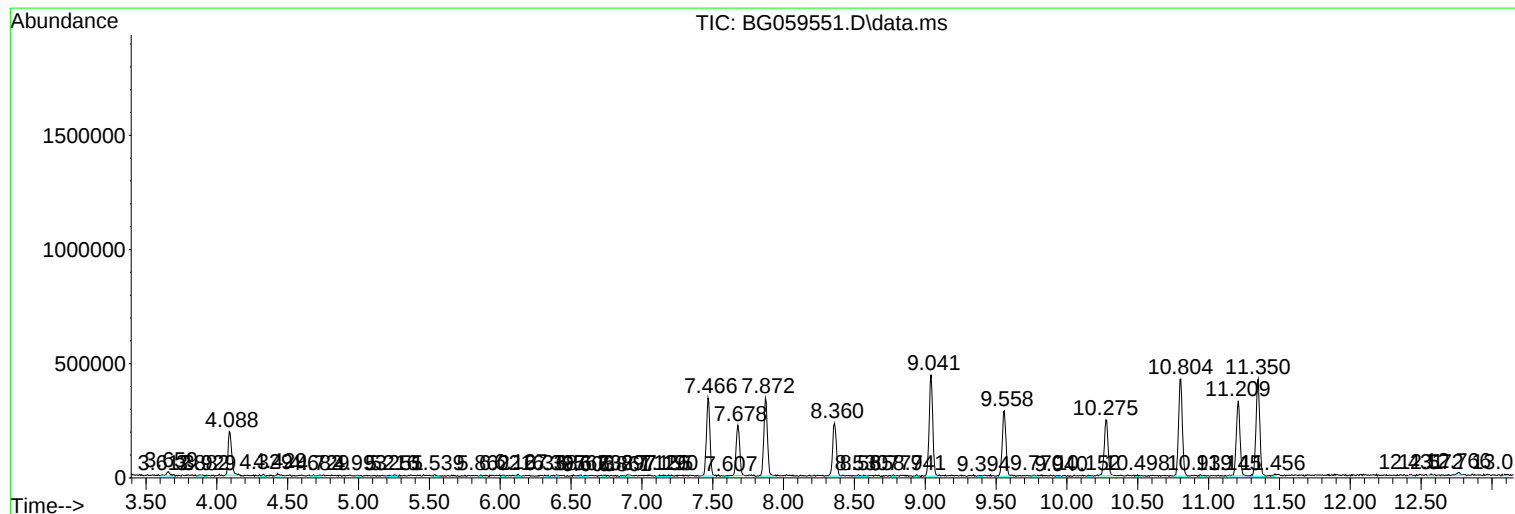

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
Data File : BG059551.D
Acq On : 30 Oct 2023 18:48
Operator : MA/JU
Sample : PB156398BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK398

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
Data File : BG059551.D
Acq On : 30 Oct 2023 18:48
Operator : MA/JU
Sample : PB156398BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK398

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc