

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059552.D
 Acq On : 30 Oct 2023 19:29
 Operator : MA/JU
 Sample : 04925-13DL 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GCCX9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059552.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.712	224	225	230	rBV	5122	6477	0.44%	0.090%
2	5.370	332	337	338	rBV3	5034	6831	0.47%	0.095%
3	5.969	436	439	441	rBV	4516	5362	0.37%	0.074%
4	6.022	446	448	451	rVB2	4985	4153	0.28%	0.058%
5	6.157	470	471	475	rBV2	3518	4062	0.28%	0.056%
6	6.357	503	505	507	rBV	5319	4092	0.28%	0.057%
7	6.627	548	551	556	rBV2	3819	6364	0.43%	0.088%
8	6.892	594	596	599	rVB	6371	5578	0.38%	0.077%
9	6.950	603	606	608	rBV	3612	4243	0.29%	0.059%
10	7.356	672	675	678	rBV	4580	3976	0.27%	0.055%
11	7.467	688	694	700	rBV2	39895	71497	4.88%	0.991%
12	7.679	725	730	735	rBV3	25613	47795	3.26%	0.663%
13	7.873	758	763	768	rBV2	36999	73032	4.99%	1.012%
14	7.949	774	776	779	rBV	3907	4918	0.34%	0.068%
15	8.125	804	806	807	rBV	5373	4605	0.31%	0.064%
16	8.219	818	822	824	rVB	4252	4638	0.32%	0.064%
17	8.361	838	846	853	rBV	201456	352008	24.03%	4.879%
18	8.490	864	868	870	rBV	3914	5002	0.34%	0.069%
19	8.572	879	882	884	rBV	3598	4227	0.29%	0.059%
20	8.707	903	905	907	rVB	7446	5238	0.36%	0.073%
21	8.825	921	925	927	rBV	5198	5491	0.37%	0.076%
22	9.042	957	962	967	rVB5	41843	72689	4.96%	1.008%
23	9.201	984	989	995	rBV2	21510	39079	2.67%	0.542%
24	9.301	1005	1006	1011	rVB2	5781	6288	0.43%	0.087%
25	9.348	1011	1014	1016	rBV2	3801	4736	0.32%	0.066%
26	9.500	1037	1040	1042	rVB	6550	7458	0.51%	0.103%
27	9.553	1042	1049	1054	rBV3	39116	78357	5.35%	1.086%
28	9.747	1078	1082	1085	rBV	4106	6969	0.48%	0.097%
29	9.947	1113	1116	1119	rBV	6016	7222	0.49%	0.100%
30	10.176	1153	1155	1157	rBV	6053	4338	0.30%	0.060%
31	10.282	1164	1173	1177	rBV2	36815	68189	4.66%	0.945%
32	10.341	1179	1183	1185	rBV	8103	9280	0.63%	0.129%
33	10.393	1190	1192	1193	rVB	7021	4455	0.30%	0.062%
34	10.511	1210	1212	1215	rBV	4198	4247	0.29%	0.059%
35	10.611	1227	1229	1230	rBV	5283	4133	0.28%	0.057%
36	10.805	1256	1262	1269	rBV2	51363	101464	6.93%	1.406%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
 Data File : BG059552.D
 Acq On : 30 Oct 2023 19:29
 Operator : MA/JU
 Sample : 04925-13DL 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GCCX9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

37	11.028	1298	1300	1301	rBV2	4978	3893	0.27%	0.054%
38	11.134	1316	1318	1321	rBV	4657	5341	0.36%	0.074%
39	11.210	1324	1331	1338	rVV	336536	598777	40.88%	8.300%
40	11.504	1378	1381	1382	rBV	5936	6407	0.44%	0.089%
41	11.539	1386	1387	1391	rBV4	5774	6376	0.44%	0.088%
42	11.663	1406	1408	1410	rBV4	5120	5840	0.40%	0.081%
43	12.097	1480	1482	1484	rBV2	5171	4799	0.33%	0.067%
44	12.274	1510	1512	1513	rBV2	5835	4461	0.30%	0.062%
45	12.321	1518	1520	1521	rBV2	7726	5600	0.38%	0.078%
46	12.432	1537	1539	1542	rVB	7096	4829	0.33%	0.067%
47	12.679	1578	1581	1582	rBV2	7837	7013	0.48%	0.097%
48	13.167	1662	1664	1666	rBV2	8144	8625	0.59%	0.120%
49	13.255	1677	1679	1680	rVB2	8390	4159	0.28%	0.058%
50	13.672	1746	1750	1751	rBV2	6217	7773	0.53%	0.108%
51	13.813	1772	1774	1781	rVB7	11720	17113	1.17%	0.237%
52	14.001	1804	1806	1809	rBV2	5505	5299	0.36%	0.073%
53	14.312	1857	1859	1862	rBV3	10459	12055	0.82%	0.167%
54	14.377	1865	1870	1876	rVB	120319	187917	12.83%	2.605%
55	14.471	1884	1886	1887	rBV2	7317	3868	0.26%	0.054%
56	14.688	1918	1923	1929	rVB2	144161	227342	15.52%	3.151%
57	14.988	1968	1974	1981	rVB	572780	883826	60.35%	12.251%
58	15.147	1998	2001	2007	rVB4	38025	57908	3.95%	0.803%
59	15.975	2138	2142	2148	rVB2	177609	266310	18.18%	3.692%
60	17.356	2371	2377	2383	rBV	954026	1464572	100.00%	20.302%
61	17.738	2437	2442	2448	rBV	711615	1052643	71.87%	14.592%
62	17.838	2455	2459	2464	rVB2	193325	268325	18.32%	3.719%
63	22.074	3176	3180	3187	rVB2	605459	1044510	71.32%	14.479%




Sum of corrected areas: 7214074

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
Data File : BG059552.D
Acq On : 30 Oct 2023 19:29
Operator : MA/JU
Sample : 04925-13DL 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCCX9DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

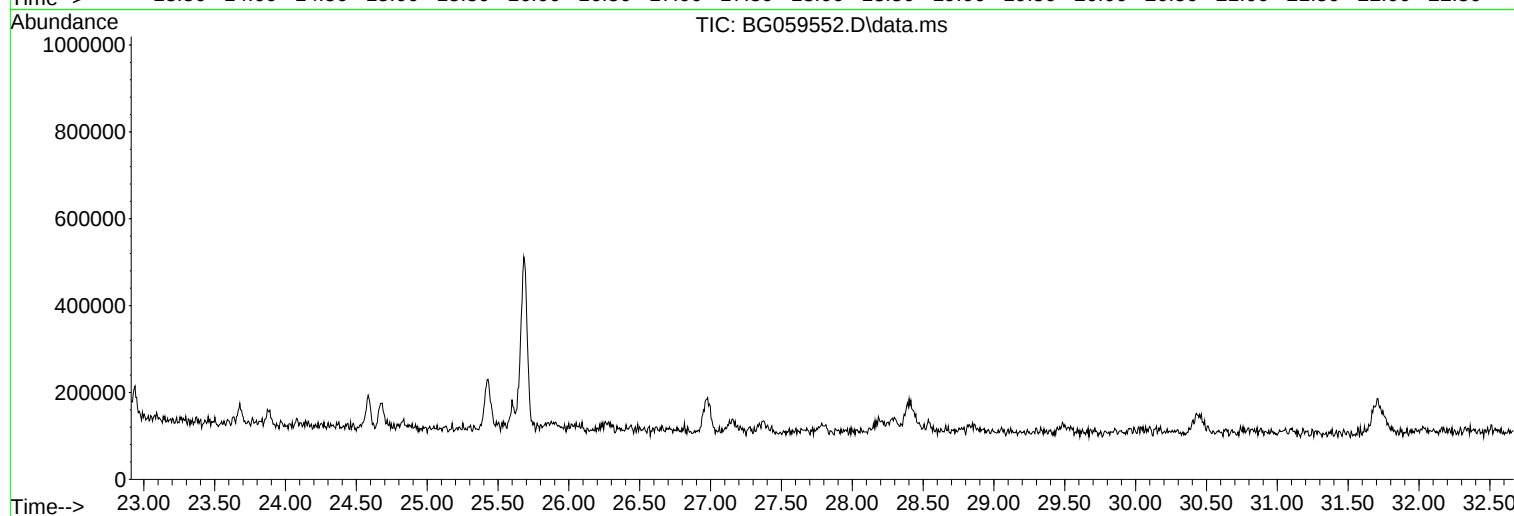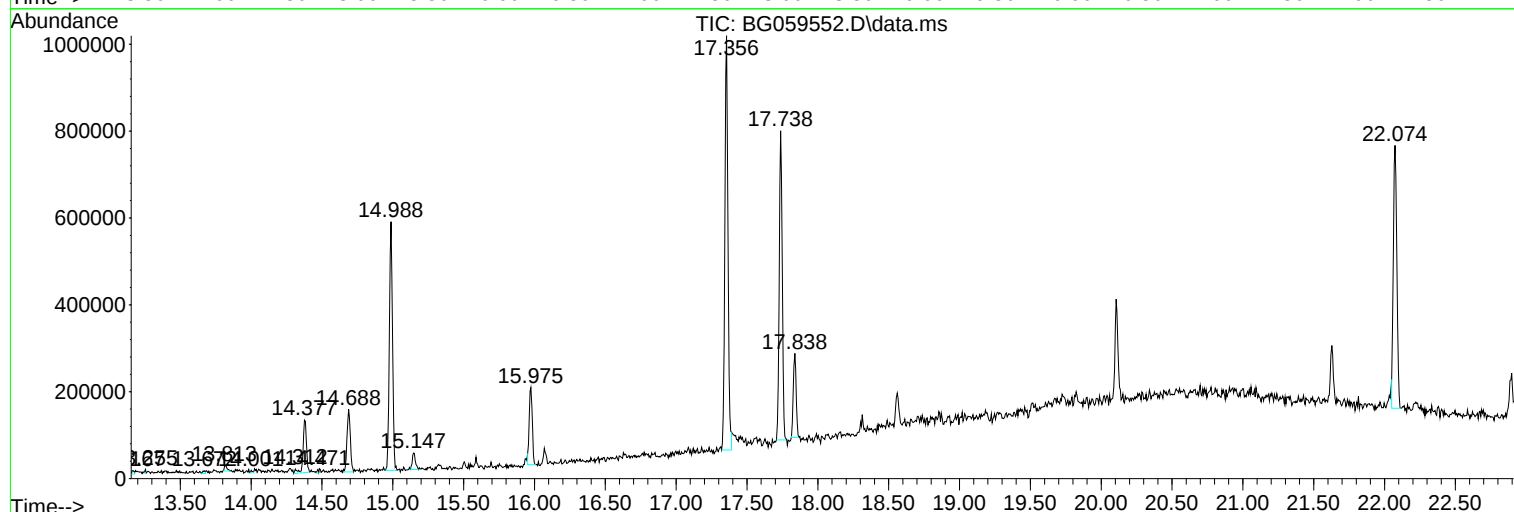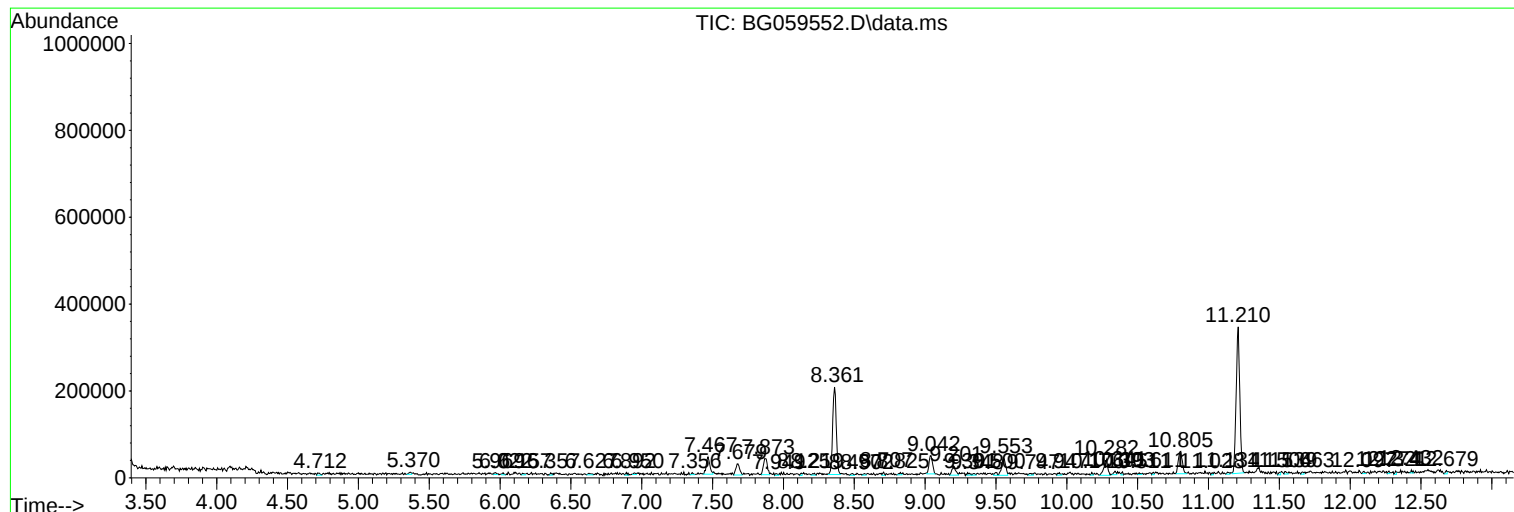

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
Data File : BG059552.D
Acq On : 30 Oct 2023 19:29
Operator : MA/JU
Sample : 04925-13DL 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCCX9DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103023\
Data File : BG059552.D
Acq On : 30 Oct 2023 19:29
Operator : MA/JU
Sample : 04925-13DL 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCCX9DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc