
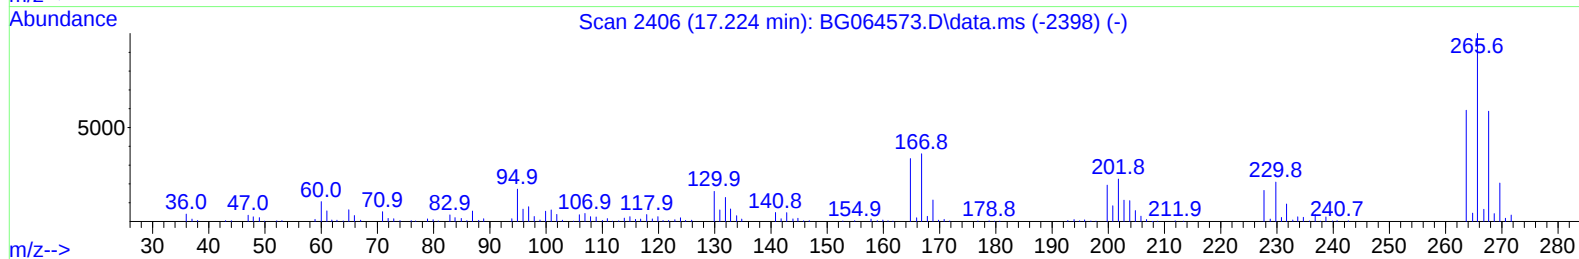
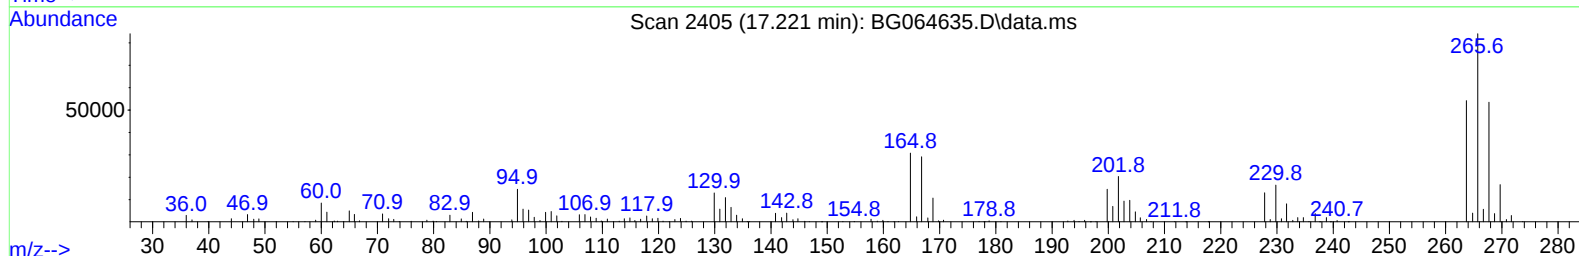


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103025\
Data File : BG064635.D
Acq On : 30 Oct 2025 10:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 30 11:34:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 16:40:26 2025
Response via : Initial Calibration

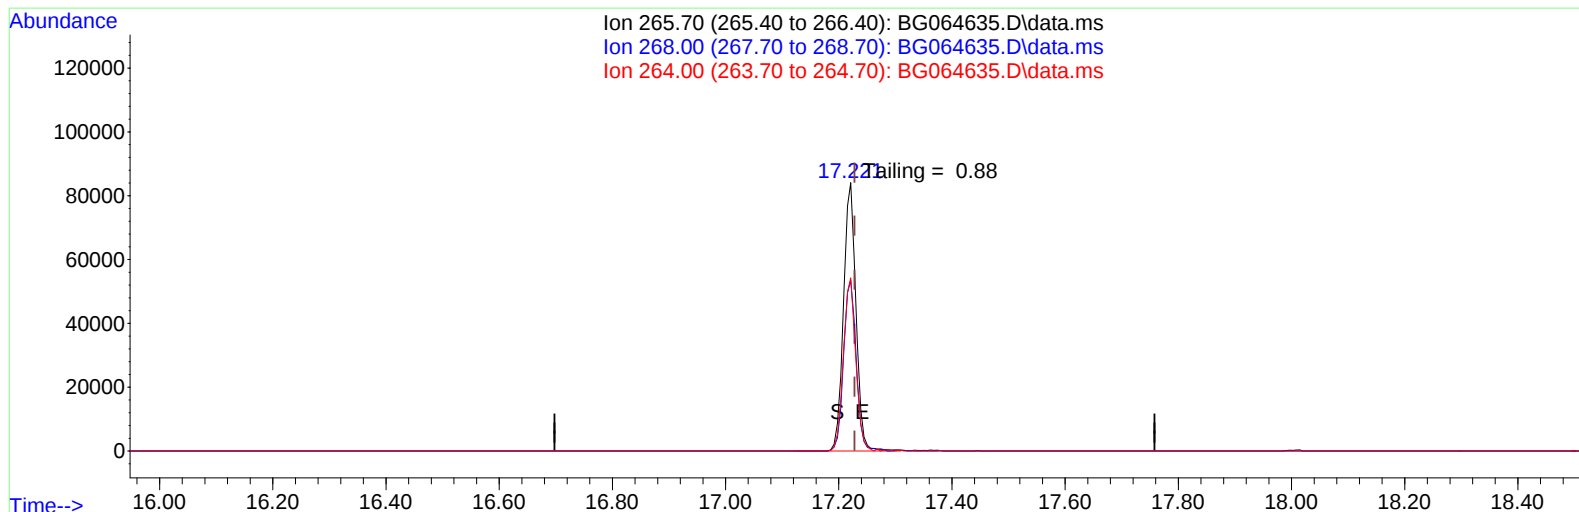

TIC: BG064635.D\data.ms

(70) Pentachlorophenol (C)




17.221min (-0.007) 25561.00 ng

response 128648

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	68.13
264.00	59.10	64.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103025\
Data File : BG064635.D
Acq On : 30 Oct 2025 10:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 30 11:34:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 16:40:26 2025
Response via : Initial Calibration

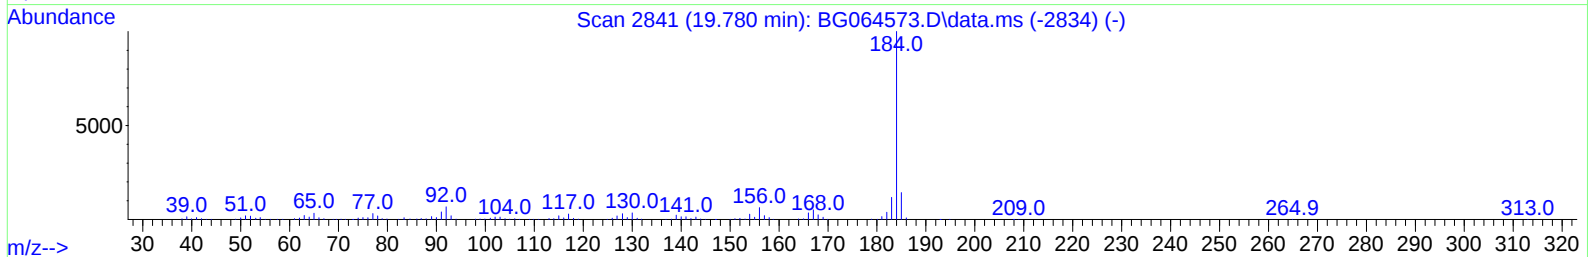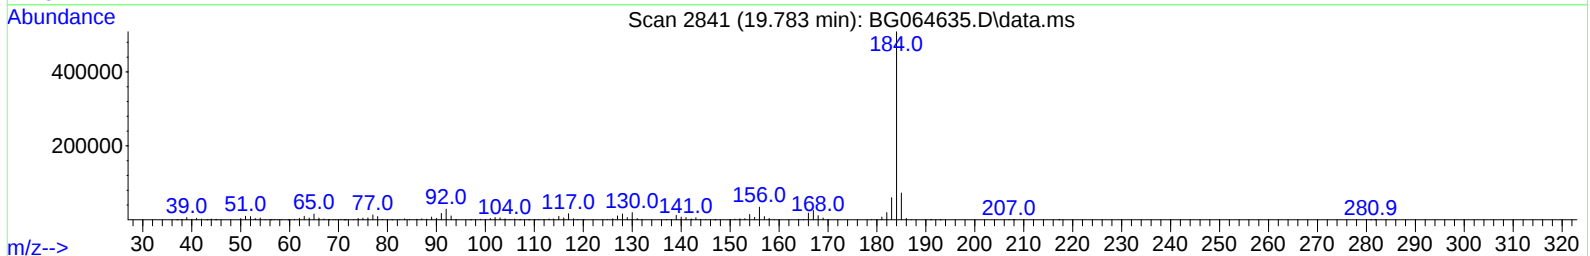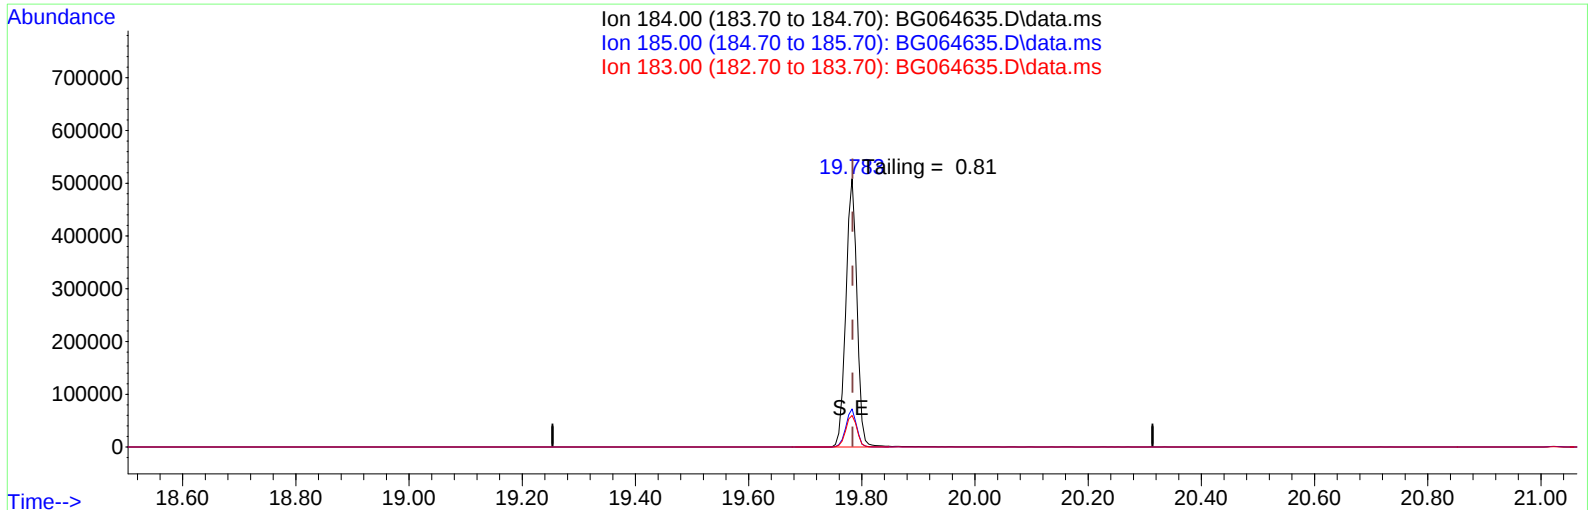

TIC: BG064635.D\data.ms

(77) Benzidine

19.783min (-0.001) 0.00 ng

response 690984

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.22
183.00	11.80	11.74
0.00	0.00	0.00