
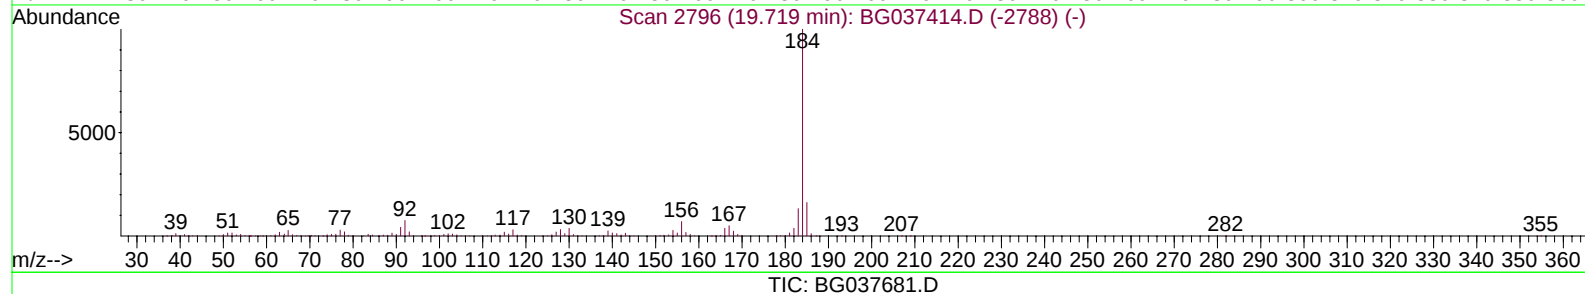
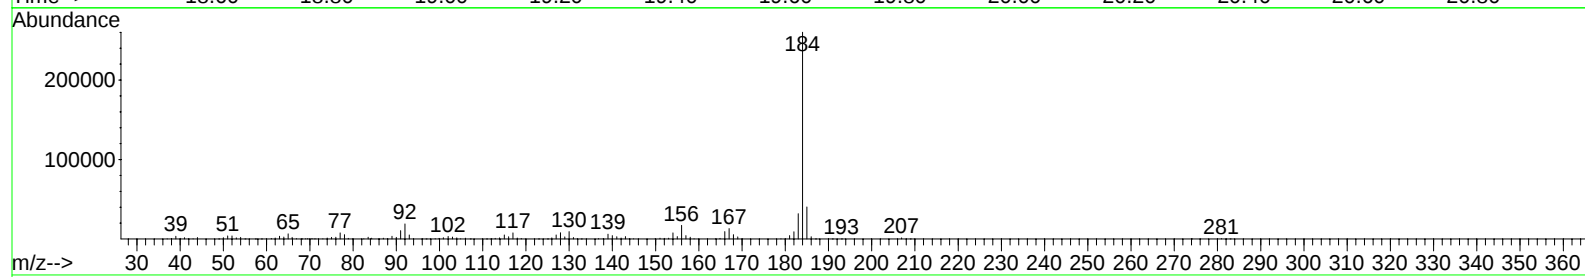


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG103118\
Data File : BG037681.D
Acq On : 31 Oct 2018 13:02
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 01 10:25:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

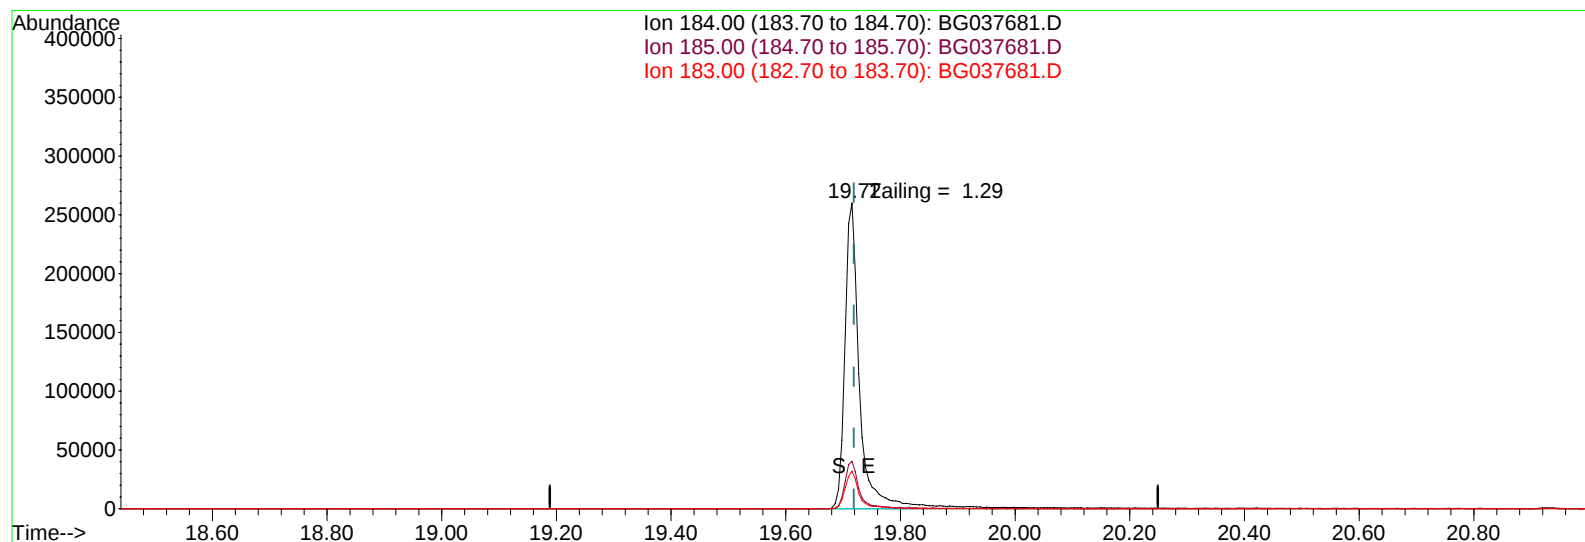

(77) Benzidine


19.715min (-0.003) 0.00ng

response 463277

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.55
183.00	12.70	12.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG103118\
Data File : BG037681.D
Acq On : 31 Oct 2018 13:02
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 01 10:25:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

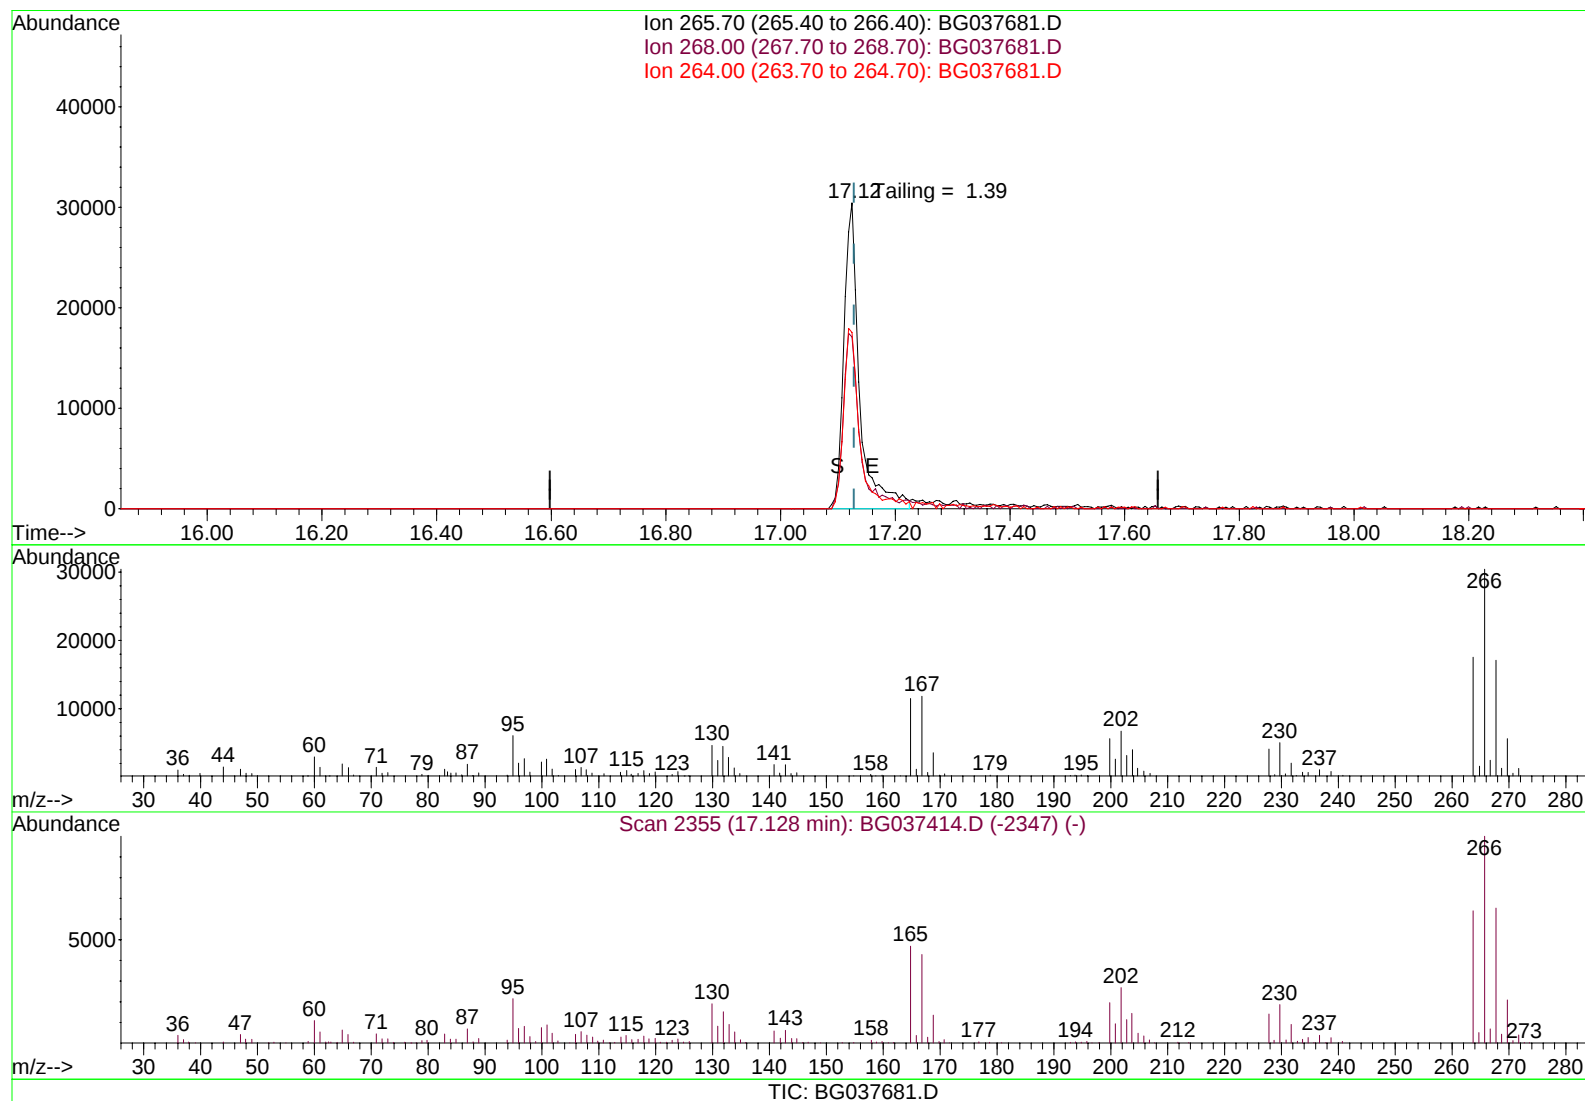

(70) Pentachlorophenol (C)

17.124min (-0.003) 33872.30ng

response 60168

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	60.48
264.00	73.60	57.65#
0.00	0.00	0.00