

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG103118\
 Data File : BG037716.D
 Acq On : 1 Nov 2018 13:15
 Operator : JU/SJ
 Sample : J5731-06
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 103018-SIDI-E-U-B

Quant Time: Nov 01 14:26:13 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 18 14:06:42 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	56269	20.00	ng	-0.01
21) Naphthalene-d8	10.92	136	246851	20.00	ng	0.00
39) Acenaphthene-d10	14.73	164	168762	20.00	ng	-0.01
64) Phenanthrene-d10	17.48	188	394062	20.00	ng	0.00
76) Chrysene-d12	21.76	240	353641	20.00	ng	-0.01
87) Perylene-d12	25.10	264	321861	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	145698	43.29	ng	0.00
7) Phenol-d6	7.24	99	135281	26.58	ng	-0.01
23) Nitrobenzene-d5	9.28	82	440951	100.07	ng	0.00
42) 2,4,6-Tribromophenol	16.22	330	160753	87.33	ng	0.00
45) 2-Fluorobiphenyl	13.35	172	1046901	93.54	ng	-0.01
79) Terphenyl-d14	20.08	244	1445801	87.36	ng	0.00
Target Compounds						
10) Phenol	7.27	94	19818	3.691	ng	Qvalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG103118\
Data File : BG037716.D
Acq On : 1 Nov 2018 13:15
Operator : JU/SJ
Sample : J5731-06
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
103018-SIDI-E-U-B

Quant Time: Nov 01 14:26:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

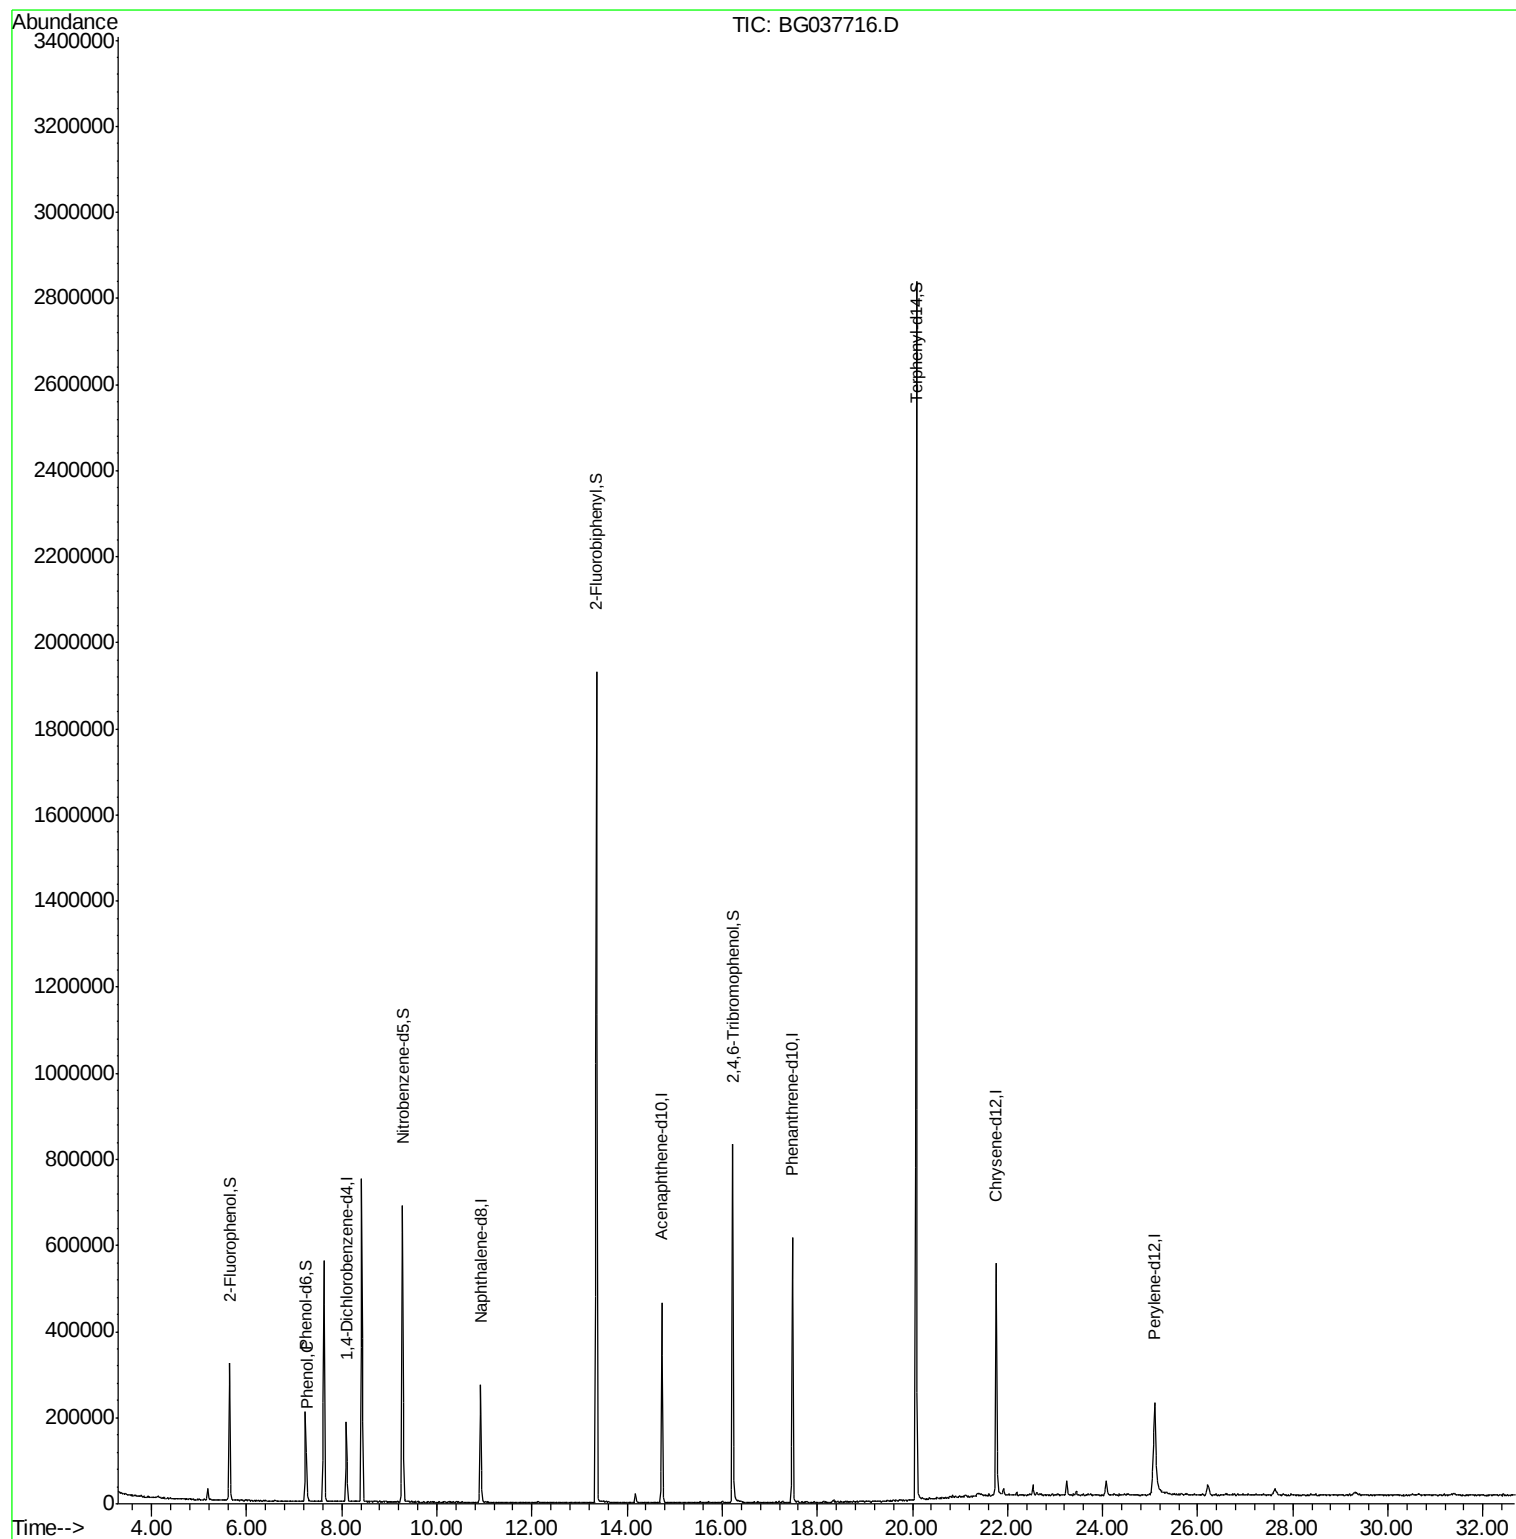







#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.10 min Scan# 818
 Delta R.T. -0.01 min
 Lab File: BG037716.D
 Acq: 1 Nov 2018 13:15

Instrument :
 BNA_G
 ClientSampleId :
 103018-SIDI-E-U-B

Tot Ion:152 Resp: 56269
 Ion Ratio Lower Upper
 152 100
 150 153.3 126.0 189.0
 115 56.0 45.5 68.3

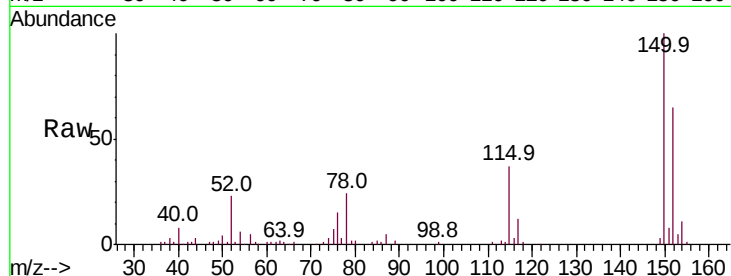


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

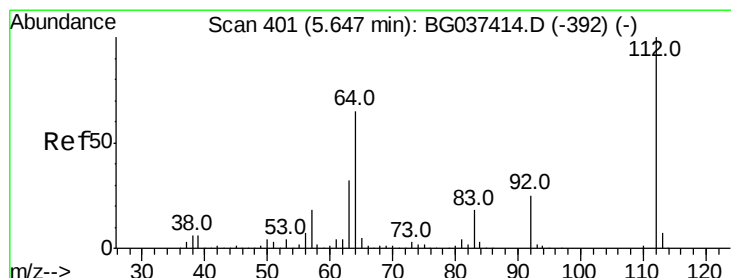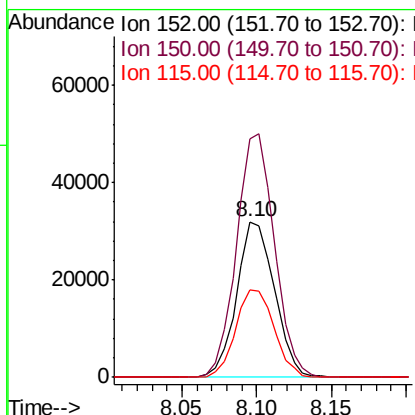
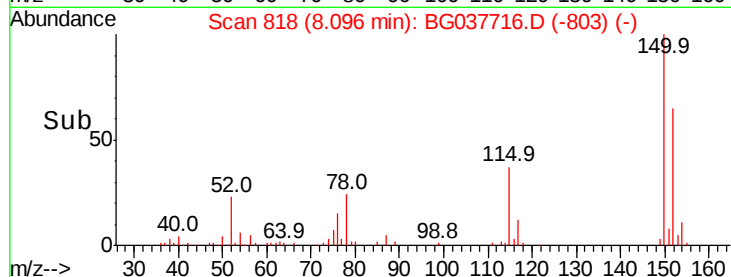



#5
 2-Fluorophenol
 Concen: 43.289 ng
 RT: 5.64 min Scan# 400
 Delta R.T. -0.01 min
 Lab File: BG037716.D
 Acq: 1 Nov 2018 13:15

Tgt Ion:112 Resp: 145698
 Ion Ratio Lower Upper
 112 100
 64 65.0 53.1 79.7
 63 31.0 27.3 40.9

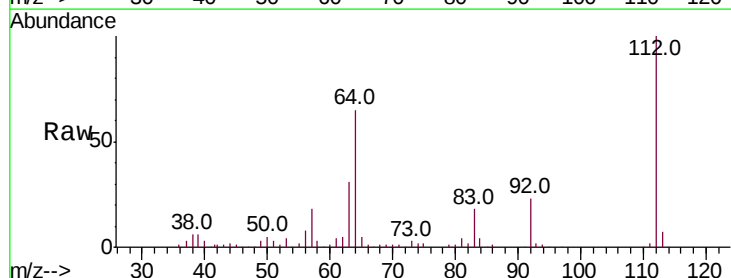

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BG
 Ion 63.00 (62.70 to 63.70): BG

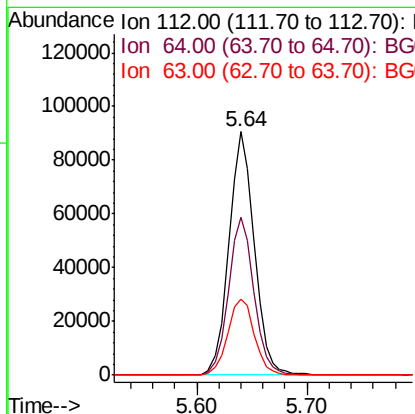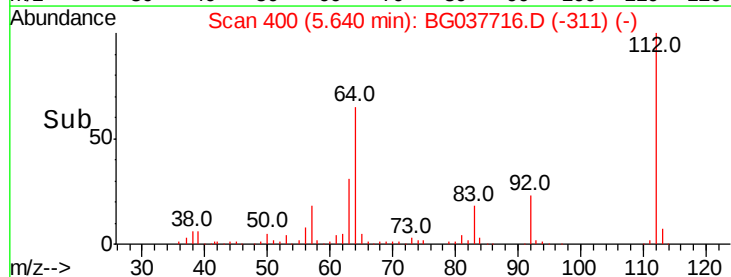

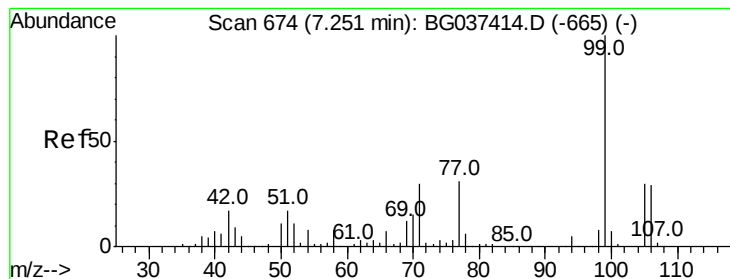

#7

Phenol-d6

Concen: 26.581 ng

RT: 7.24 min Scan# 672

Delta R.T. -0.01 min

Lab File: BG037716.D

Acq: 1 Nov 2018 13:15

Instrument :

BNA_G

ClientSampleId :

103018-SIDI-E-U-B


Tot Ion: 99 Resp: 135281

Ion Ratio Lower Upper




99 100

42 18.3 15.0 22.4

71 29.0 25.5 38.3

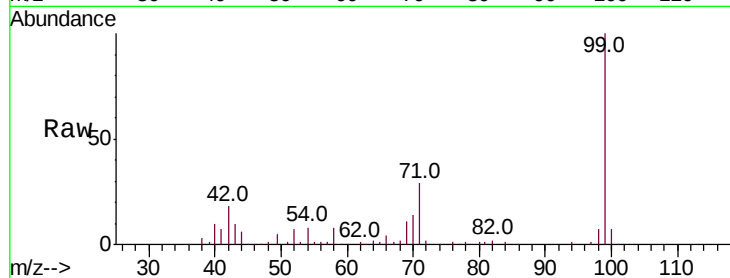

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

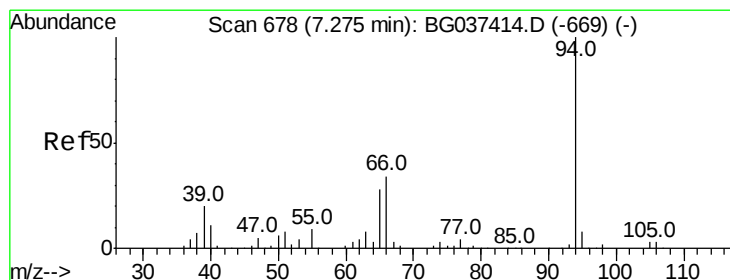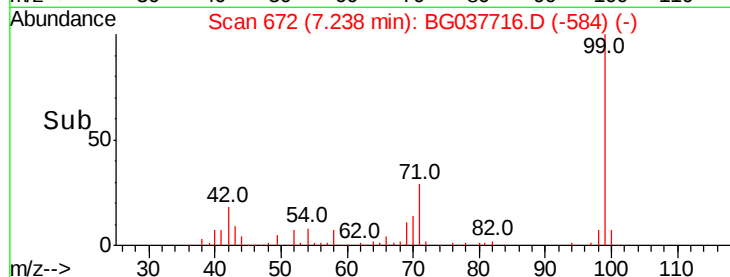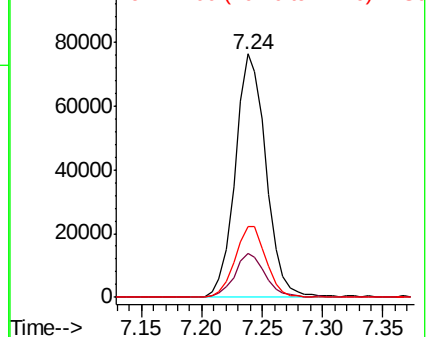

#10

Phenol

Concen: 3.691 ng

RT: 7.27 min Scan# 677

Delta R.T. -0.01 min

Lab File: BG037716.D

Acq: 1 Nov 2018 13:15


Tgt Ion: 94 Resp: 19818

Ion Ratio Lower Upper



94 100

65 27.1 9.7 49.7

66 37.8 15.9 55.9

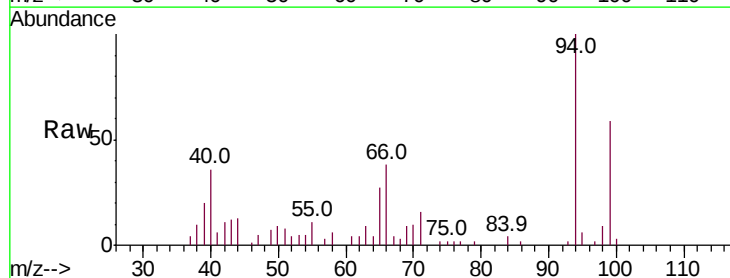

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

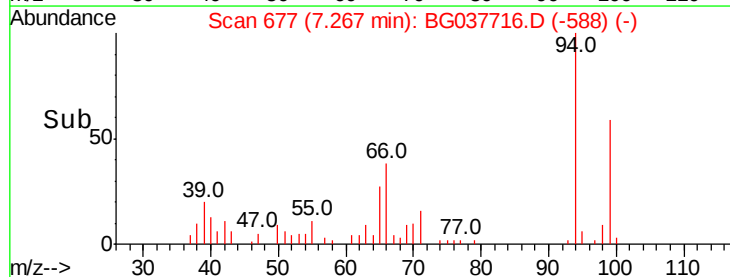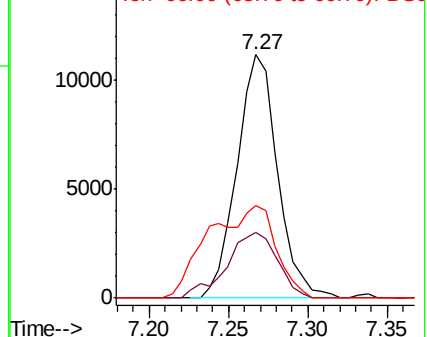







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.92 min Scan# 1299
Delta R.T. -0.01 min
Lab File: BG037716.D
Acq: 1 Nov 2018 13:15

Instrument :
BNA_G
ClientSampleId :
103018-SIDI-E-U-B

Tot Ion:136	Resp:	246851
Ion	Ratio	Lower Upper
136	100	
137	11.1	9.6 14.4
54	10.2	7.9 11.9
68	6.3	4.8 7.2

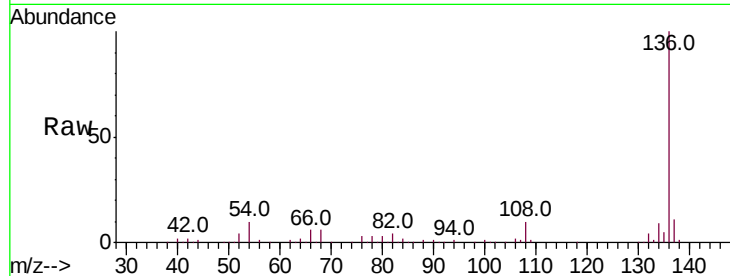


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

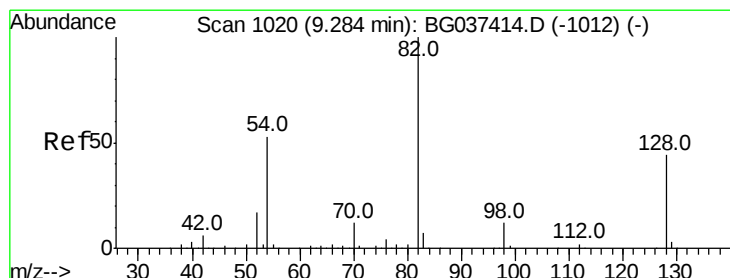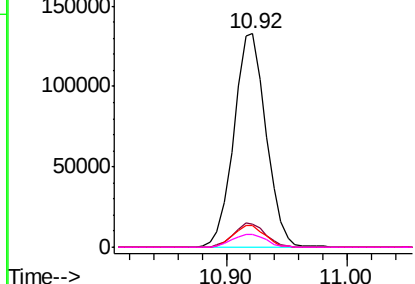
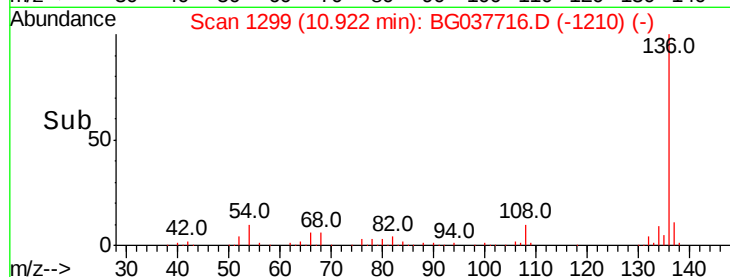



#23
Nitrobenzene-d5
Concen: 100.067 ng
RT: 9.28 min Scan# 1019
Delta R.T. -0.01 min
Lab File: BG037716.D
Acq: 1 Nov 2018 13:15

Tgt Ion: 82	Resp:	440951
Ion	Ratio	Lower Upper
82	100	
128	46.1	34.6 51.8
54	56.0	45.3 67.9

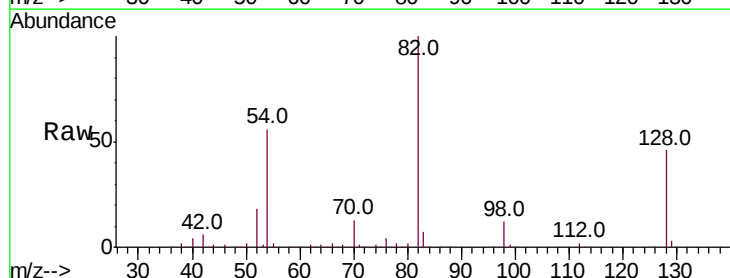

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

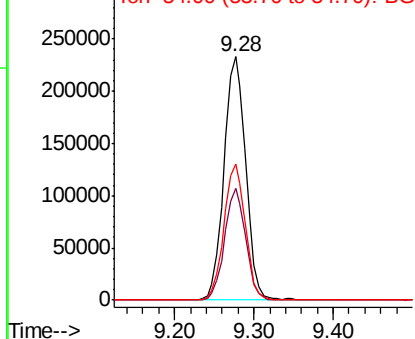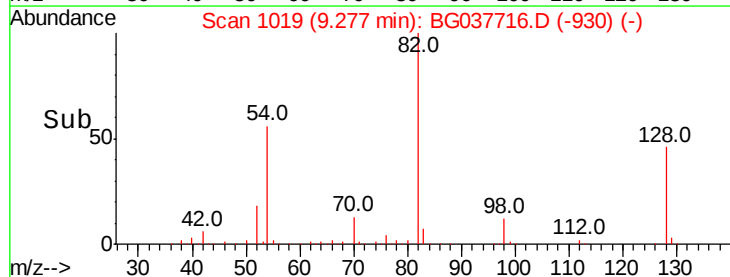

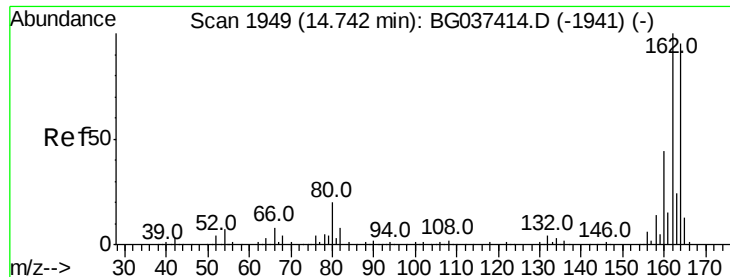

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.73 min Scan# 1947

Delta R.T. -0.01 min

Lab File: BG037716.D

Acq: 1 Nov 2018 13:15

Instrument :

BNA_G

ClientSampleId :

103018-SIDI-E-U-B


Tot Ion:164 Resp: 168762

Ion Ratio Lower Upper

164 100

162 103.2 81.3 121.9



160 44.3 36.3 54.5

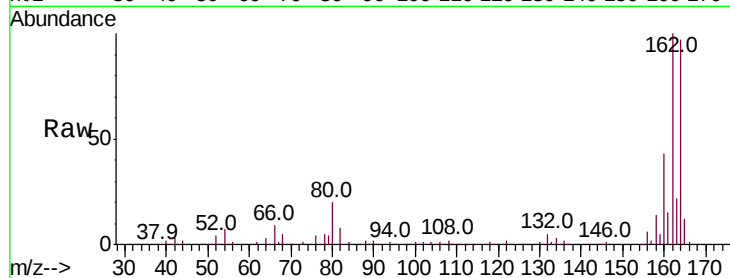

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

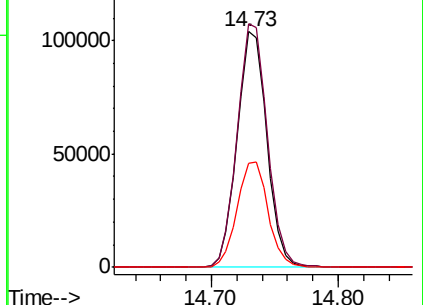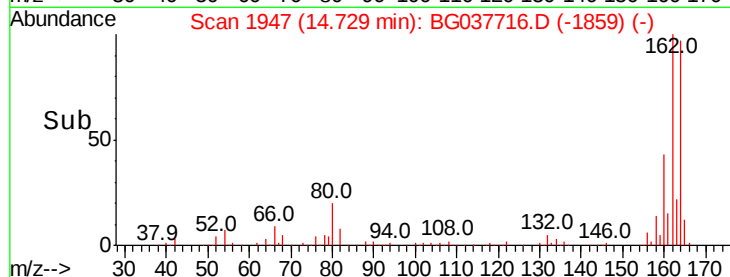

#42

2,4,6-Tribromophenol

Concen: 87.334 ng

RT: 16.22 min Scan# 2201

Delta R.T. -0.01 min

Lab File: BG037716.D

Acq: 1 Nov 2018 13:15


Tgt Ion:330 Resp: 160753

Ion Ratio Lower Upper

330 100

332 93.7 78.4 117.6



141 40.2 32.2 48.2

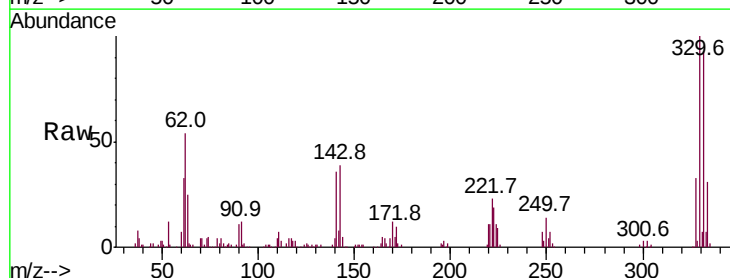

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



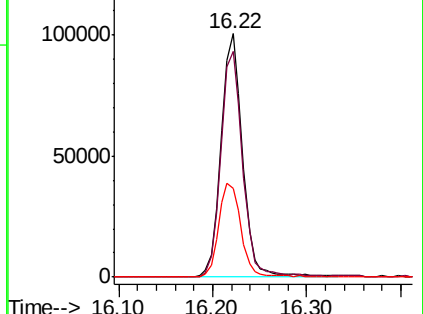
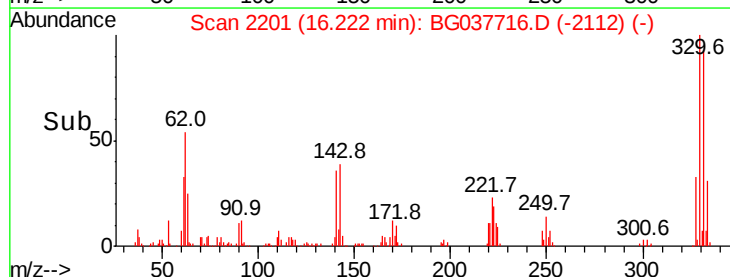




#45
2-Fluorobiphenyl
Concen: 93.544 ng
RT: 13.35 min Scan# 1713
Delta R.T. -0.01 min
Lab File: BG037716.D
Acq: 1 Nov 2018 13:15




Instrument :
BNA_G
ClientSampleId :
103018-SIDI-E-U-B


Tot Ion:172 Resp: 1046901
Ion Ratio Lower Upper
172 100
171 38.2 31.0 46.4
170 25.1 20.2 30.2

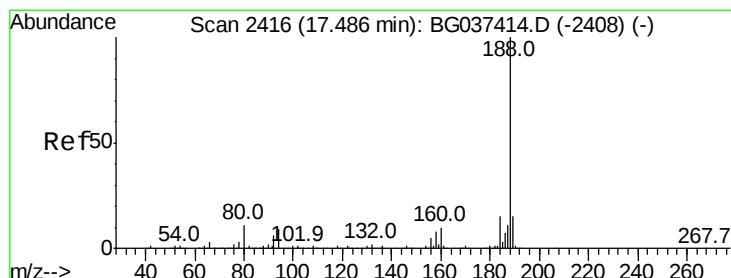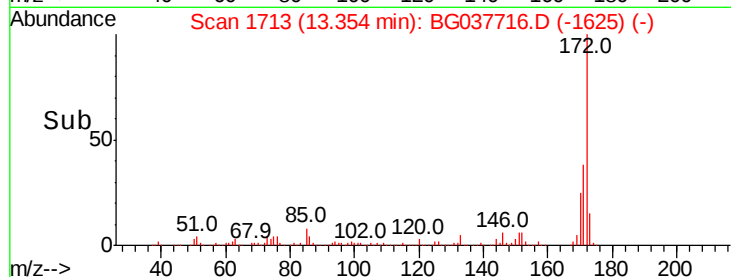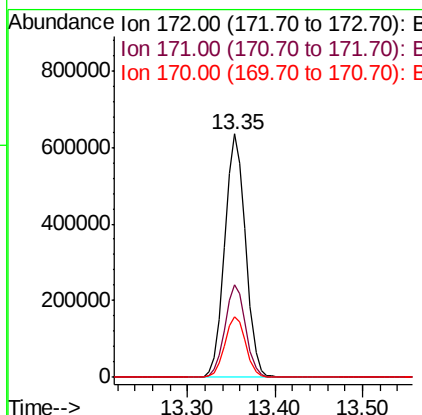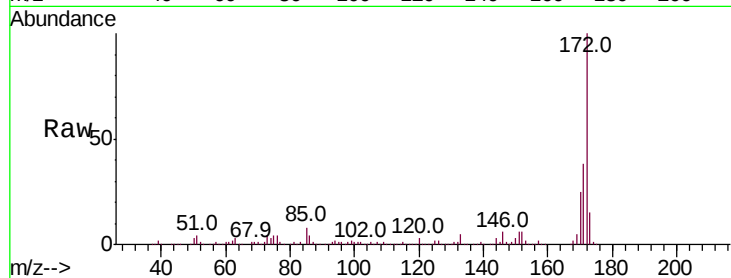

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.48 min Scan# 2415
Delta R.T. -0.01 min
Lab File: BG037716.D
Acq: 1 Nov 2018 13:15

Tgt Ion:188 Resp: 394062
Ion Ratio Lower Upper
188 100
94 9.4 7.2 10.8
80 10.6 7.7 11.5

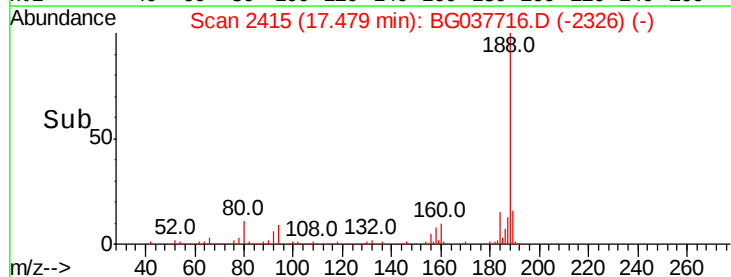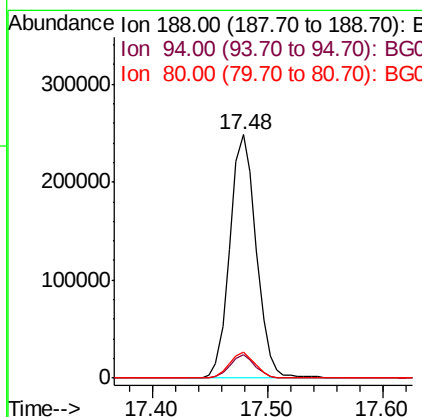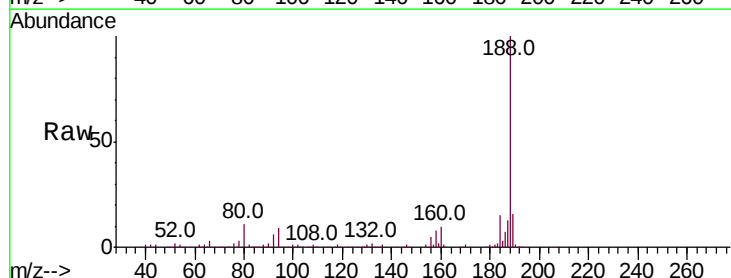

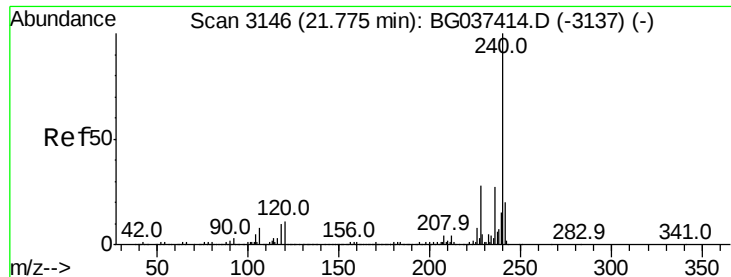

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.76 min Scan# 3144

Delta R.T. -0.01 min

Lab File: BG037716.D

Acq: 1 Nov 2018 13:15

Instrument :

BNA_G

ClientSampleId :

103018-SIDI-E-U-B


Tot Ion:240 Resp: 353641

Ion Ratio Lower Upper

240 100

120 11.1 8.1 12.1




236 27.9 21.4 32.0

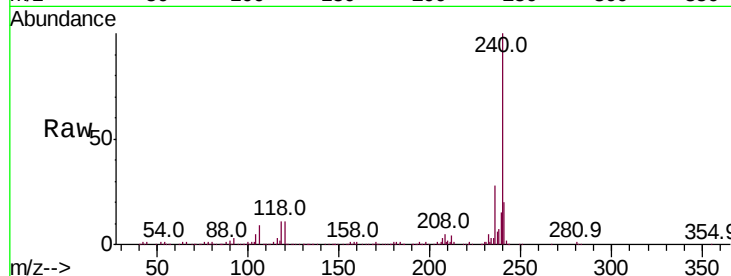

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

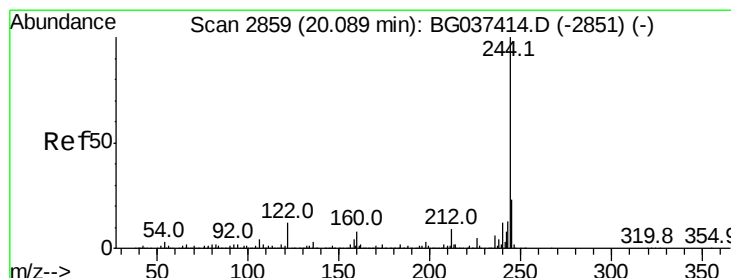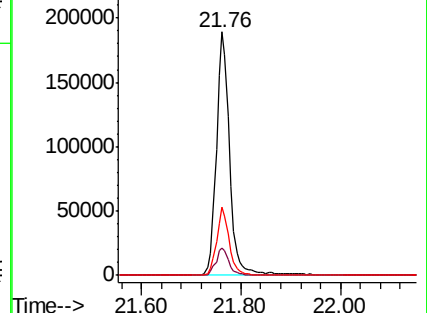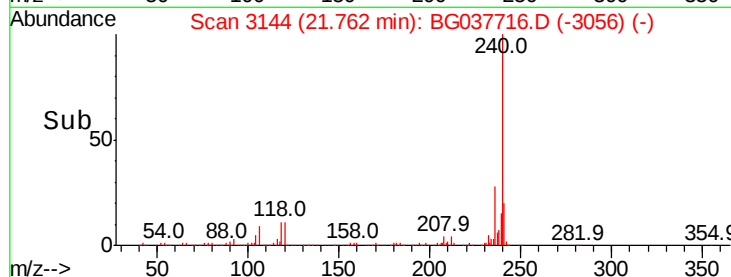

#79

Terphenyl-d14

Concen: 87.358 ng

RT: 20.08 min Scan# 2858

Delta R.T. -0.01 min

Lab File: BG037716.D

Acq: 1 Nov 2018 13:15


Tgt Ion:244 Resp: 1445801

Ion Ratio Lower Upper

244 100

212 8.3 6.5 9.7



122 11.4 9.0 13.4

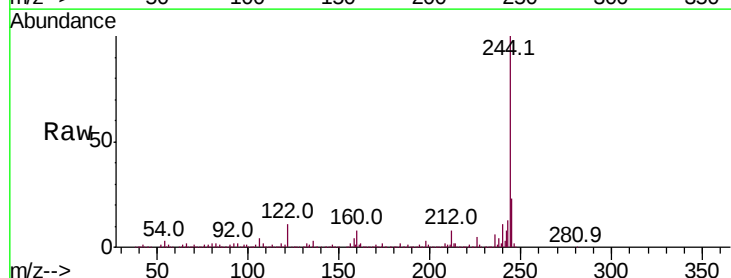


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

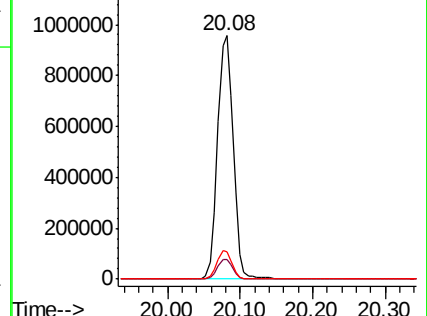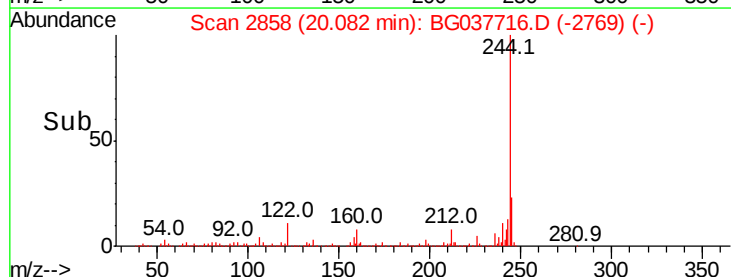


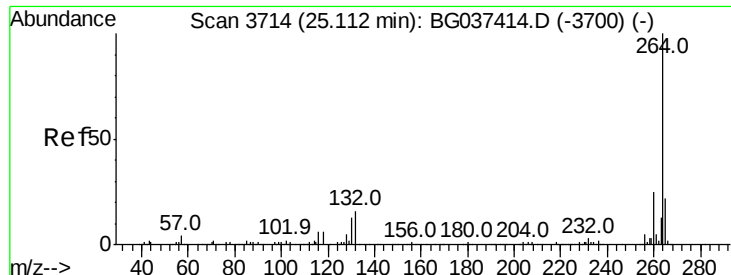

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 25.10 min Scan# 3712
 Delta R.T. -0.01 min
 Lab File: BG037716.D
 Acq: 1 Nov 2018 13:15

Instrument :
 BNA_G
 ClientSampleId :
 103018-SIDI-E-U-B

Tot Ion:264 Resp: 321861
 Ion Ratio Lower Upper
 264 100
 260 21.7 18.2 27.4
 265 23.0 17.9 26.9

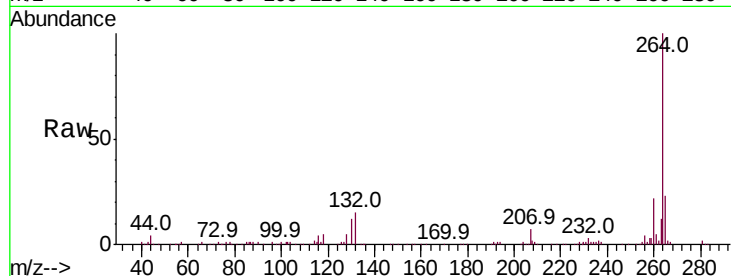

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

