


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103118\
 Data File : BG037681.D
 Acq On : 31 Oct 2018 13:02
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 18 14:06:42 2018

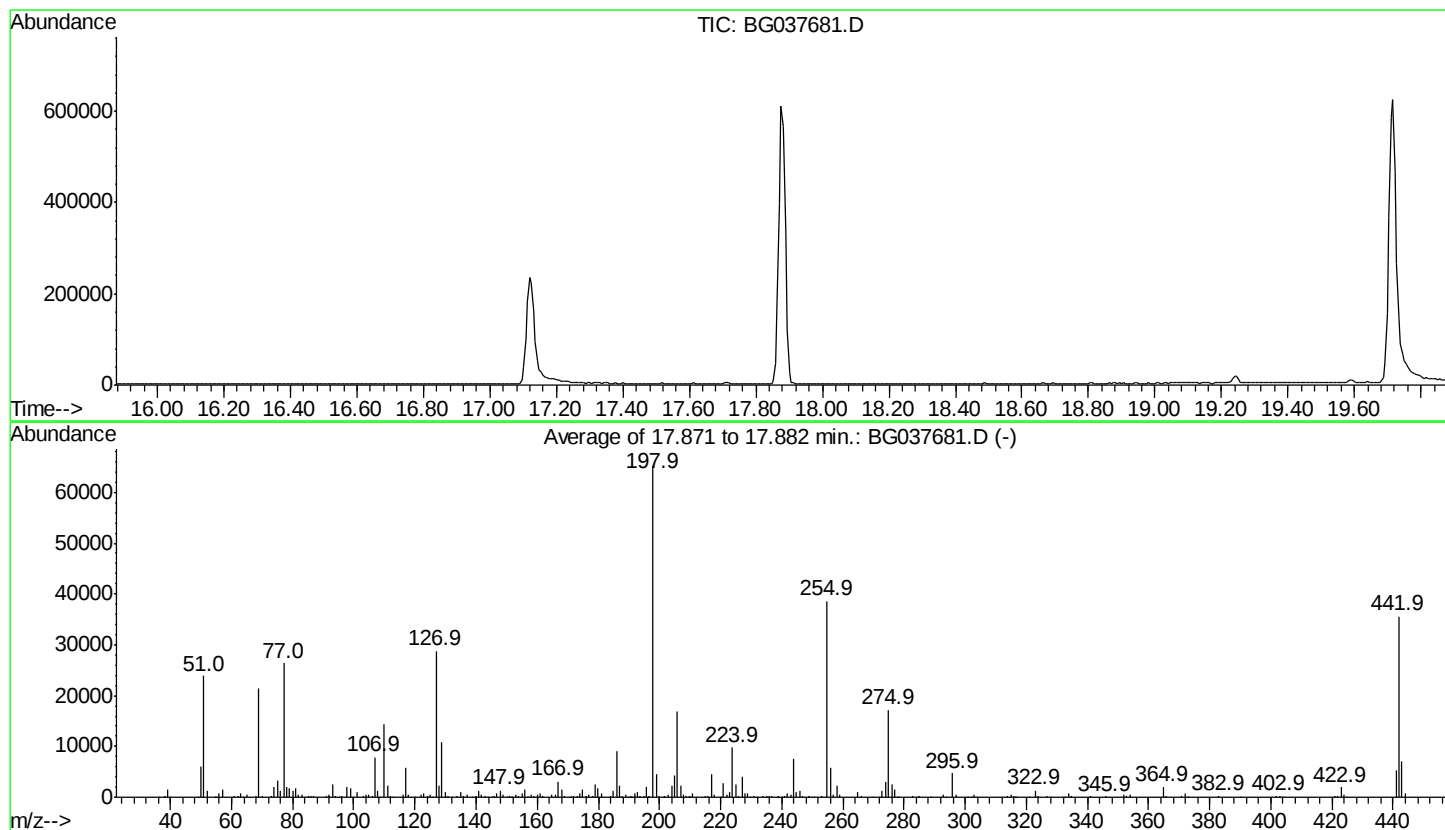

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	23880	PASS
68	69	0.00	2	1.5	313	PASS
69	198	0.00	100	32.8	21413	PASS
70	69	0.00	2	0.7	145	PASS
127	198	10	80	44.1	28757	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	65253	PASS
199	198	5	9	7.0	4541	PASS
275	198	10	60	26.4	17256	PASS
365	198	1	100	3.1	2019	PASS
441	198	0.01	100	8.2	5365	PASS
442	198	50	100	54.6	35640	PASS
443	442	15	24	19.9	7080	PASS