
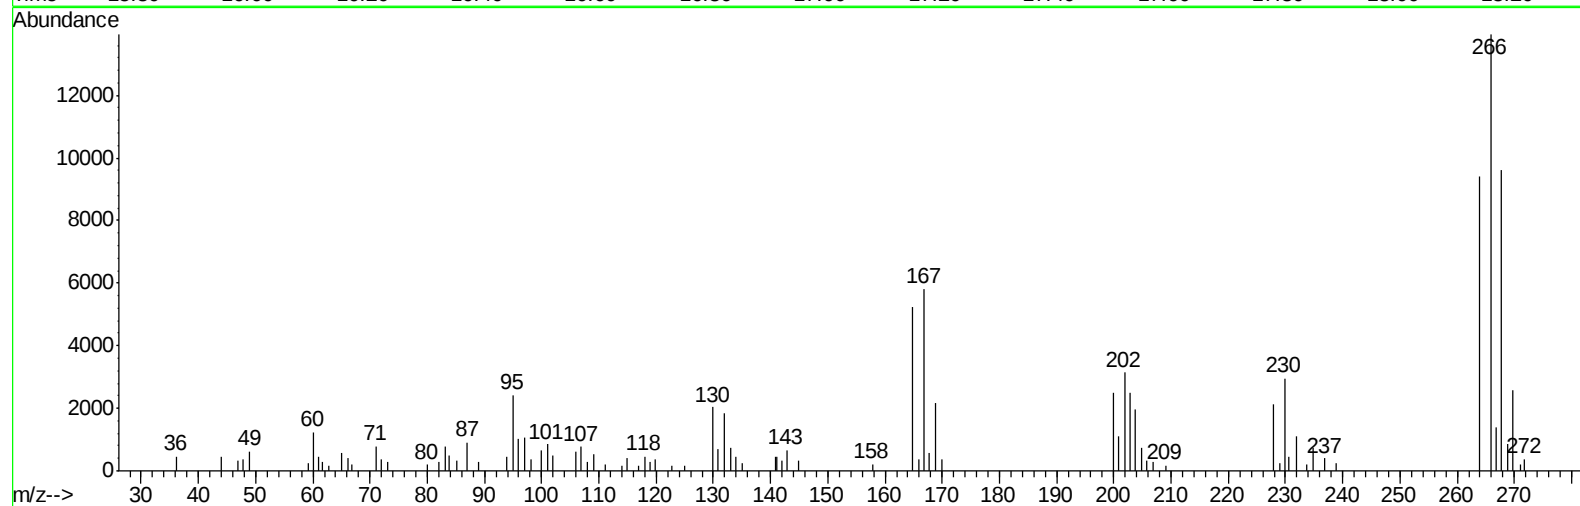


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG103119\
Data File : BG043453.D
Acq On : 1 Nov 2019 4:45
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 01 08:24:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 16:37:43 2019
Response via : Initial Calibration

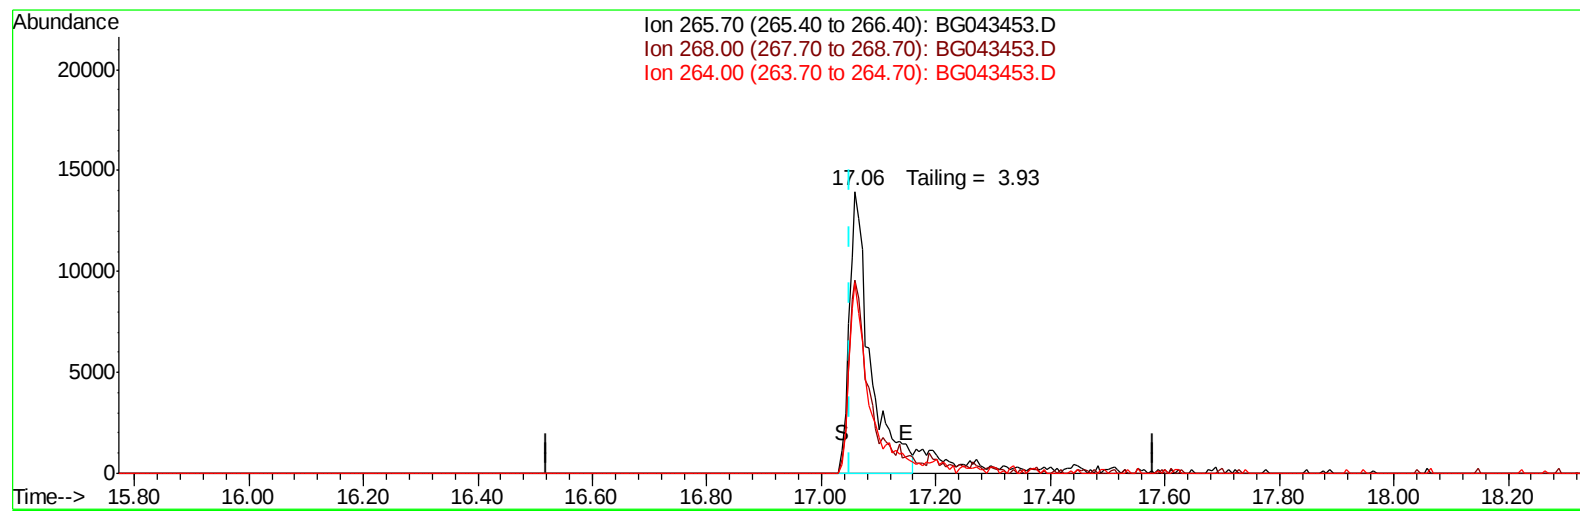

TIC: BG043453.D

(70) Pentachlorophenol (C)



17.059min (+0.009) 19296.91ng

response 35316

Ion	Exp%	Act%
265.70	100	100
268.00	58.90	68.83
264.00	63.00	67.51
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG103119\
Data File : BG043453.D
Acq On : 1 Nov 2019 4:45
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 01 08:24:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 16:37:43 2019
Response via : Initial Calibration

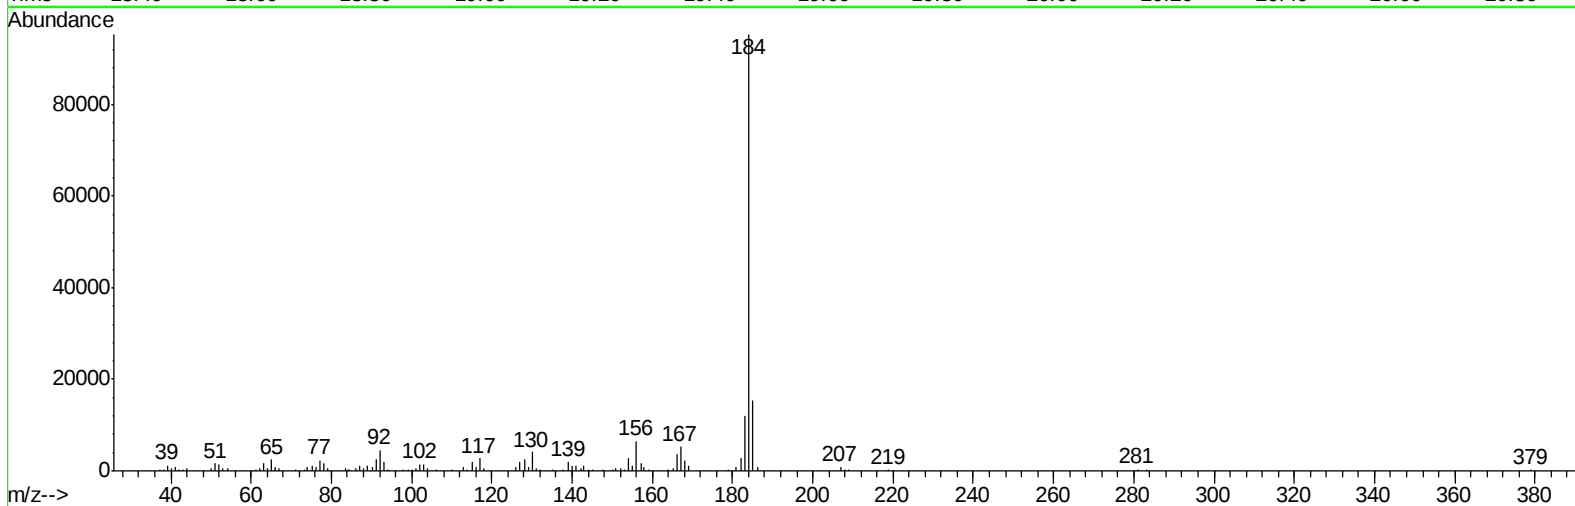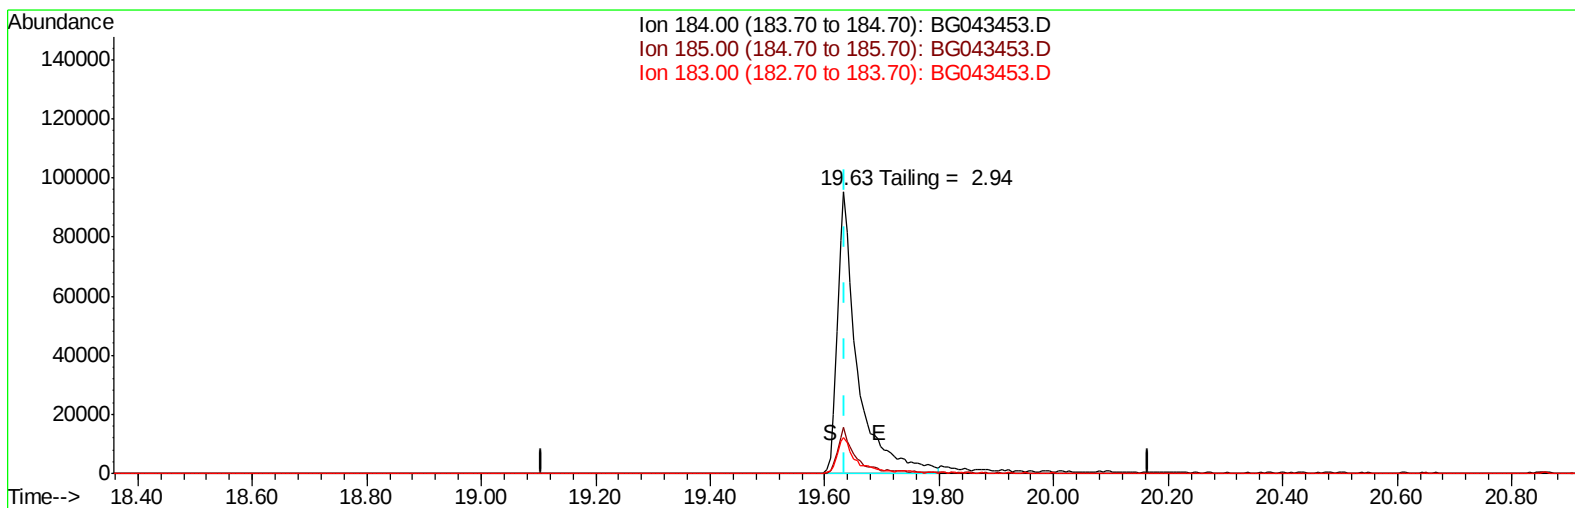

TIC: BG043453.D

(77) Benzidine

19.633min (-0.002) 210190.30ng

response 232658

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	16.17
183.00	13.30	12.72
0.00	0.00	0.00