




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
 Data File : BG059568.D
 Acq On : 31 Oct 2023 19:52
 Operator : MA/JU
 Sample : 04950-21MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A49M0MS

Manual IntegrationsAPPROVED

Quant Time: Nov 01 03:20:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/02/2023
 Supervised By :mohammad ahmed 11/02/2023

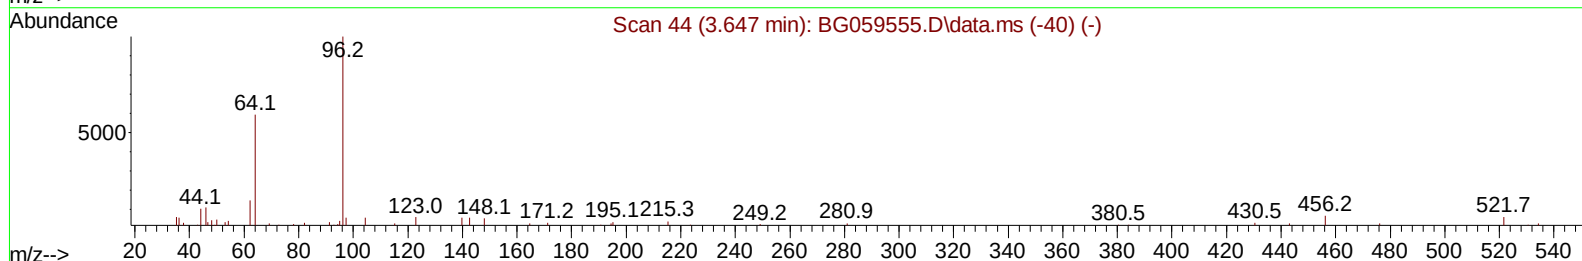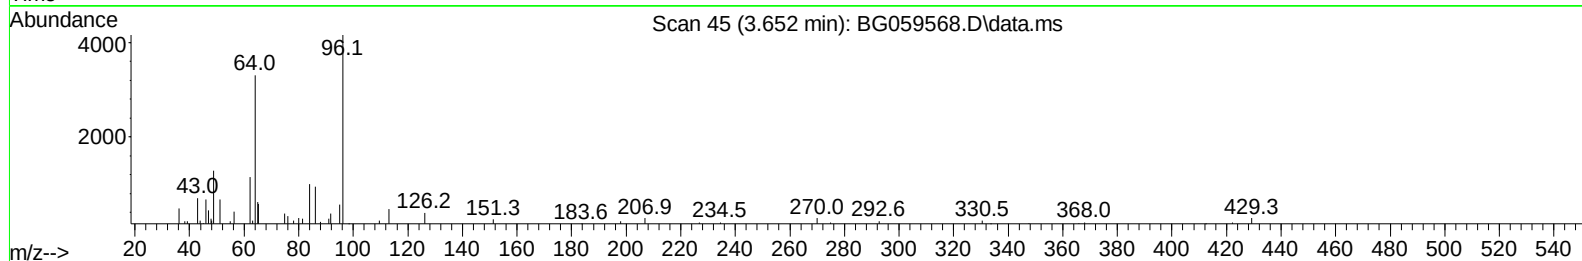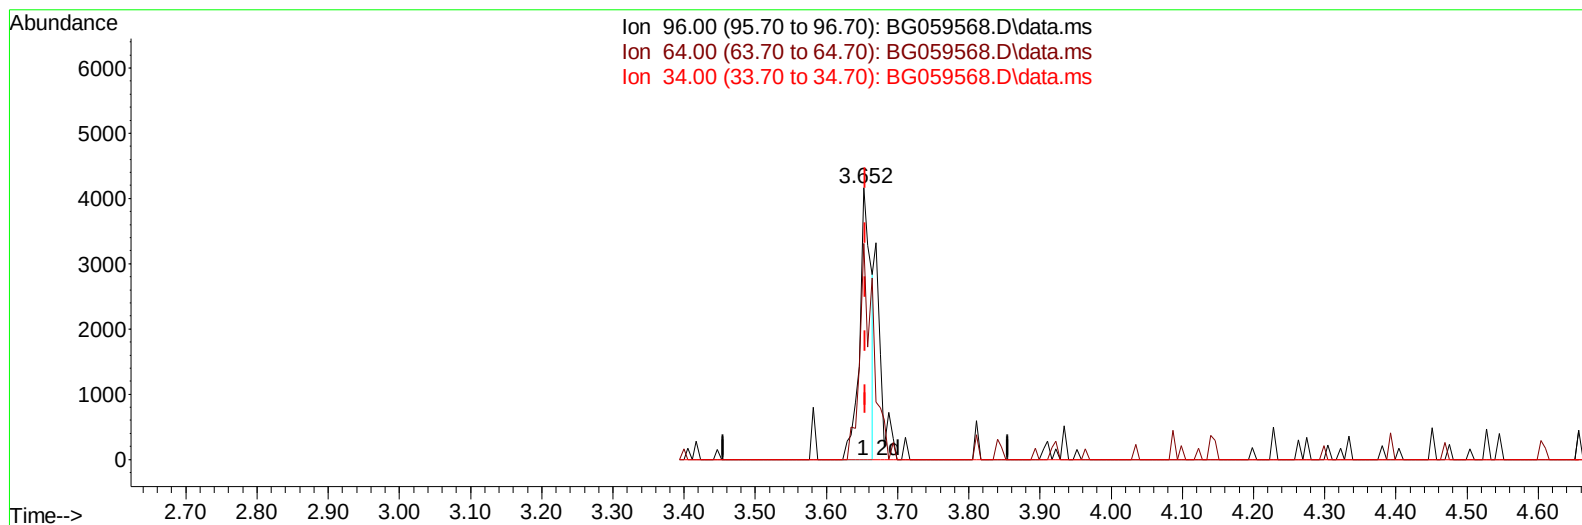

TIC: BG059568.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.652min (-0.003) 2.27 ng/uL

response 4666

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	52.90	79.60#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
 Data File : BG059568.D
 Acq On : 31 Oct 2023 19:52
 Operator : MA/JU
 Sample : 04950-21MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A49M0MS

Manual IntegrationsAPPROVED

Quant Time: Nov 01 03:20:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/02/2023
 Supervised By :mohammad ahmed 11/02/2023

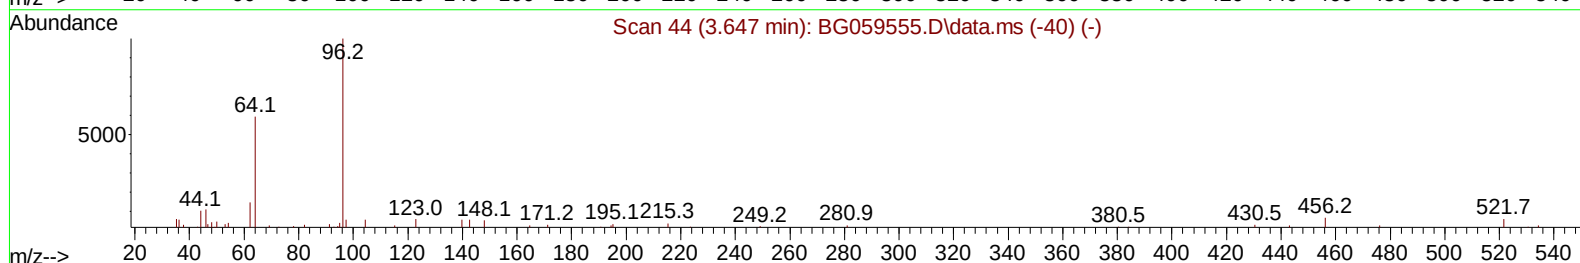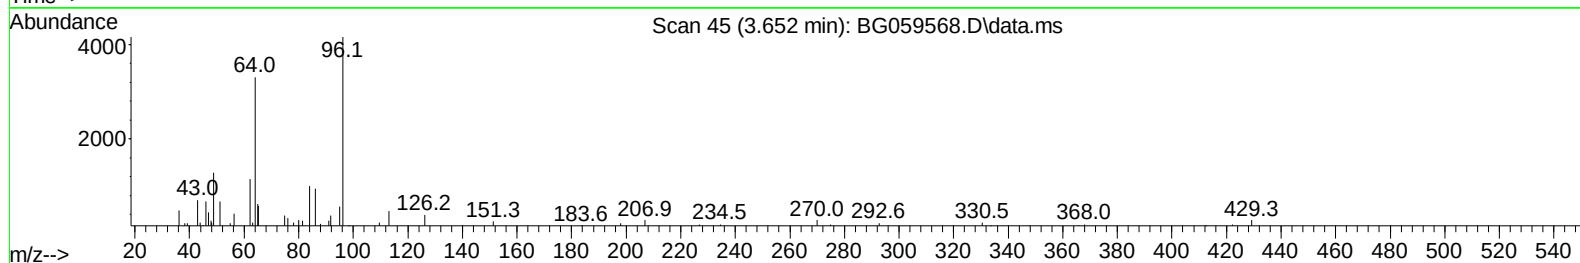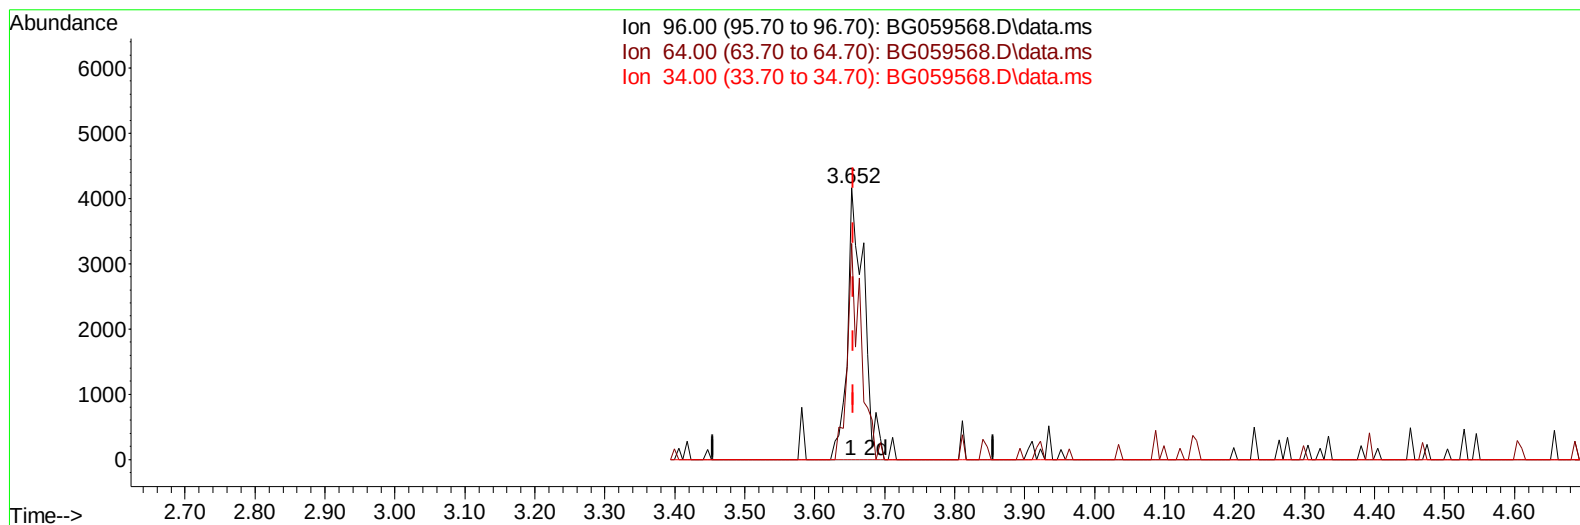

TIC: BG059568.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.652min (-0.003) 3.32 ng/uL m

response 6836

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	52.90	79.60#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
Data File : BG059568.D
Acq On : 31 Oct 2023 19:52
Operator : MA/JU
Sample : 04950-21MS
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A49M0MS

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/02/2023
Supervised By :mohammad ahmed 11/02/2023

Quant Time: Nov 01 03:20:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 28 03:56:42 2023
Response via : Initial Calibration

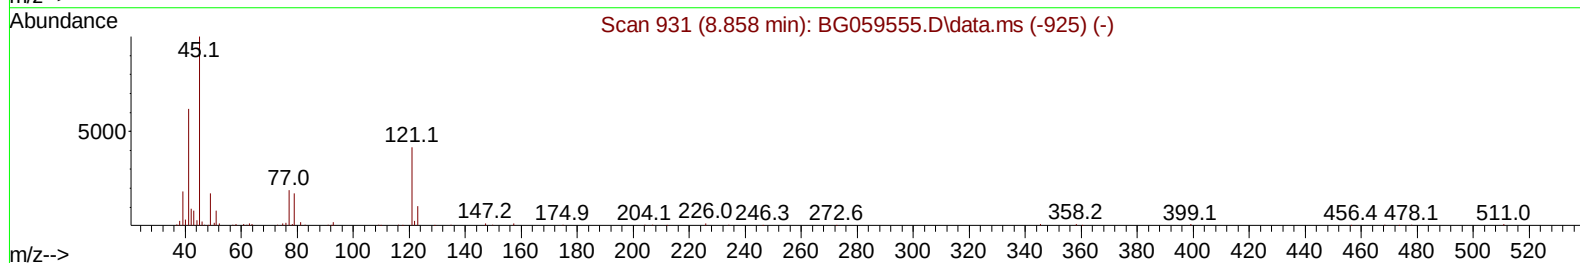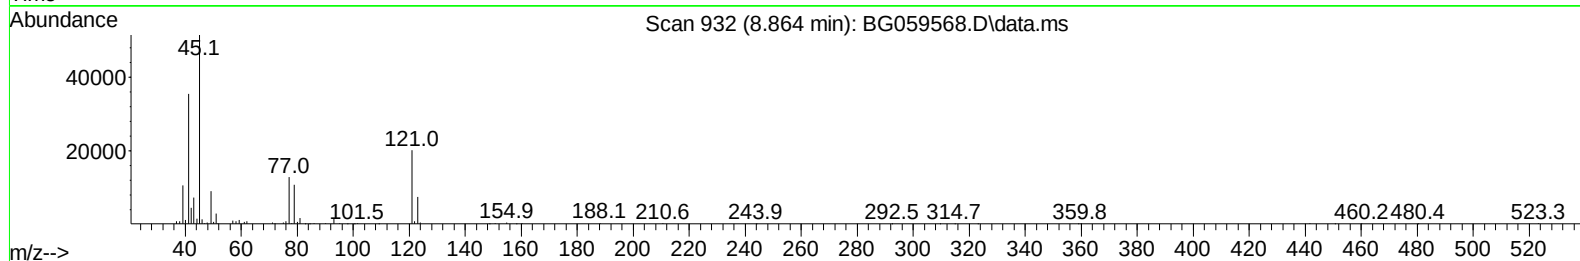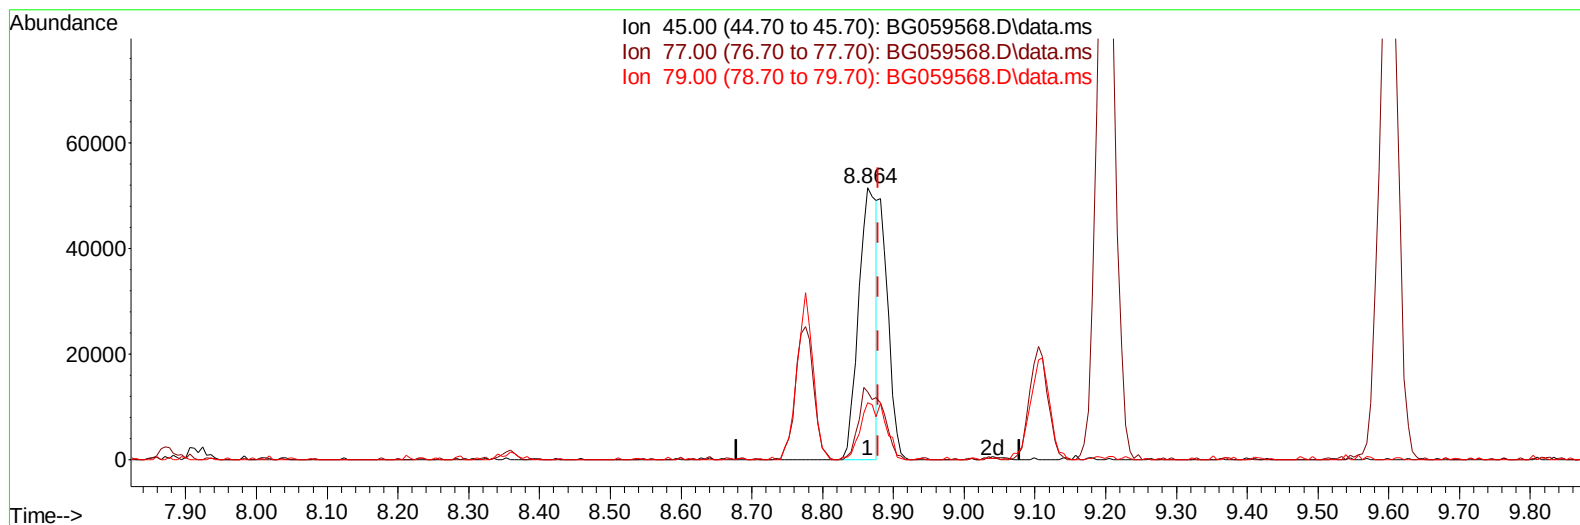

TIC: BG059568.D\data.ms

(14) 2,2'-oxybis(1-Chloropropane)

8.864min (-0.014) 17.66 ng/u1

response 90908

Ion	Exp%	Act%
45.00	100.00	100.00
77.00	18.80	24.90#
79.00	12.50	20.82#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
 Data File : BG059568.D
 Acq On : 31 Oct 2023 19:52
 Operator : MA/JU
 Sample : 04950-21MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A49M0MS

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/02/2023
 Supervised By :mohammad ahmed 11/02/2023

Quant Time: Nov 01 03:20:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

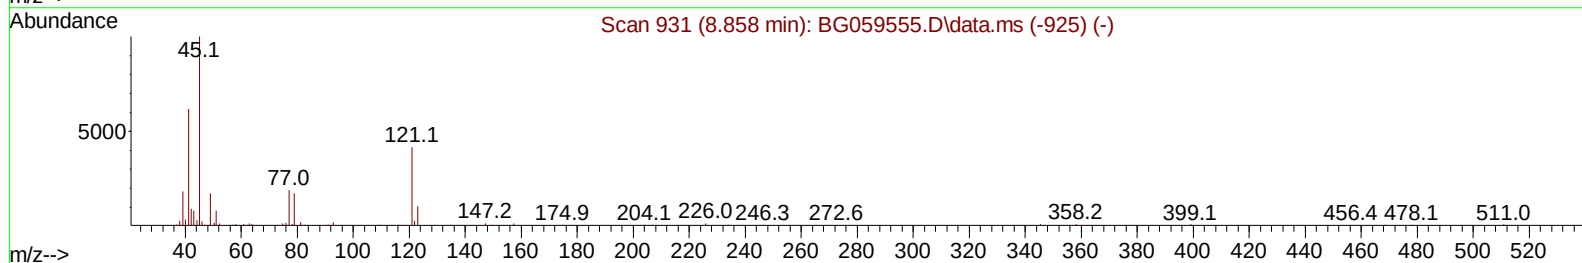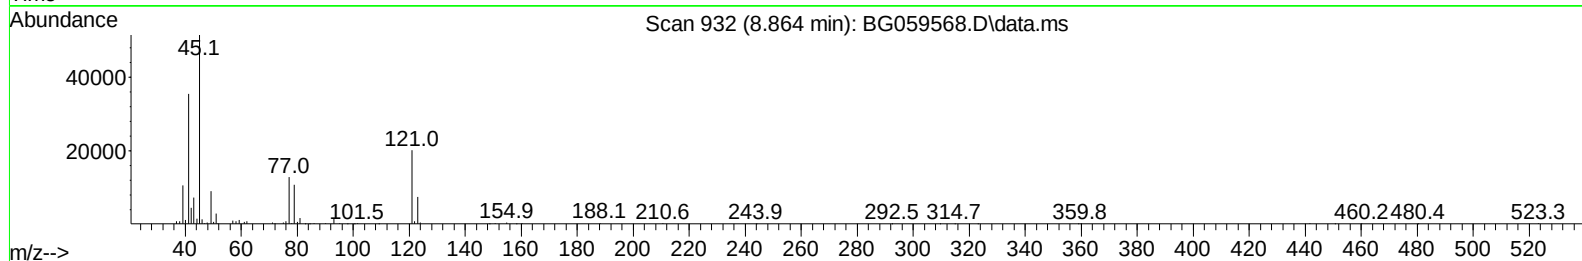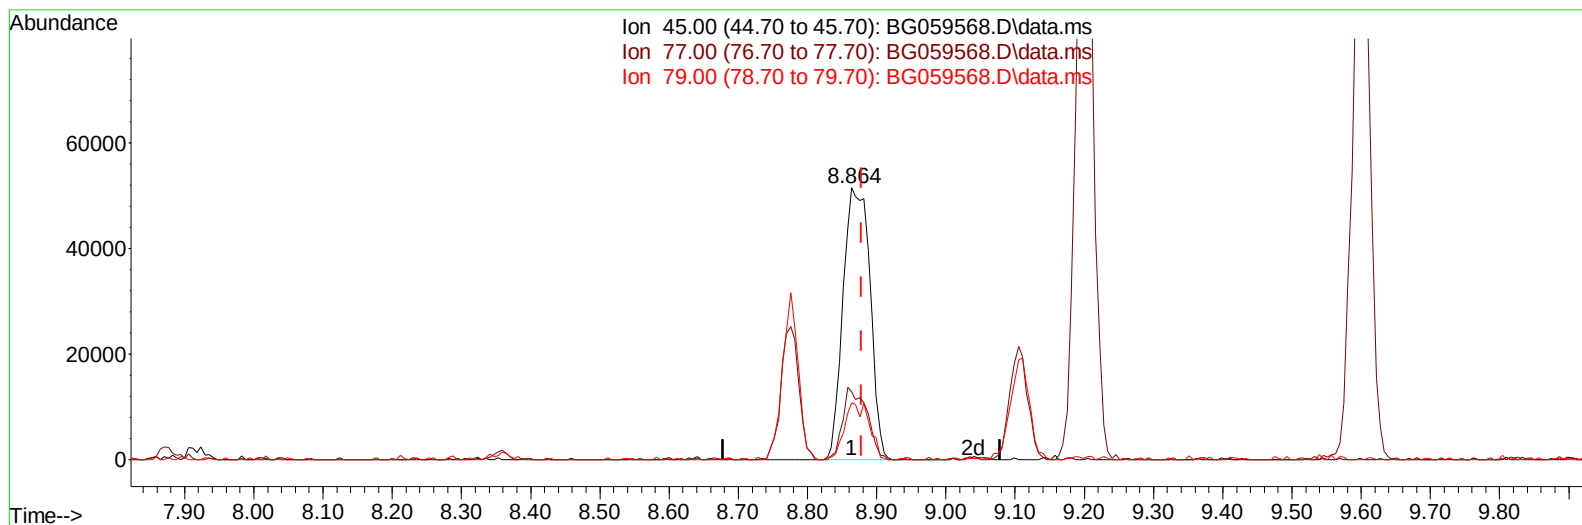

TIC: BG059568.D\data.ms

(14) 2,2'-oxybis(1-Chloropropane)

8.864min (-0.014) 26.88 ng/ul m

response 138338

Ion	Exp%	Act%
45.00	100.00	100.00
77.00	18.80	24.90#
79.00	12.50	20.82#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
 Data File : BG059568.D
 Acq On : 31 Oct 2023 19:52
 Operator : MA/JU
 Sample : 04950-21MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A49M0MS

Manual IntegrationsAPPROVED

Quant Time: Nov 01 03:20:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/02/2023
 Supervised By :mohammad ahmed 11/02/2023

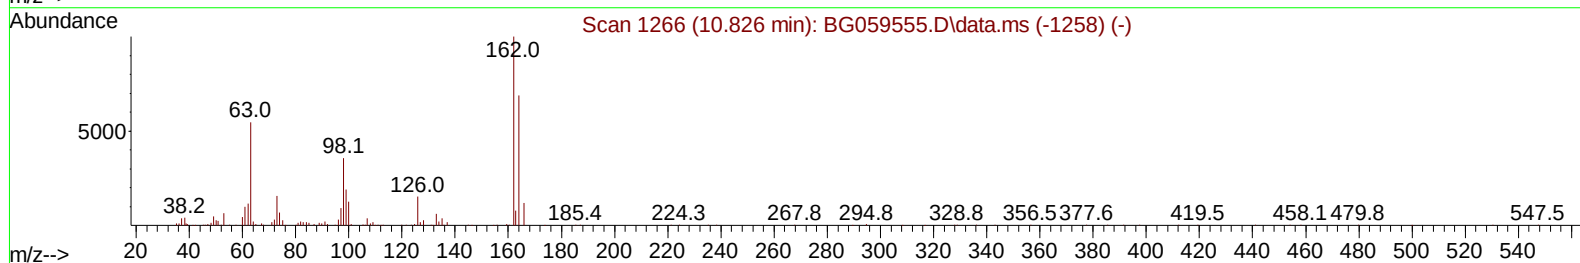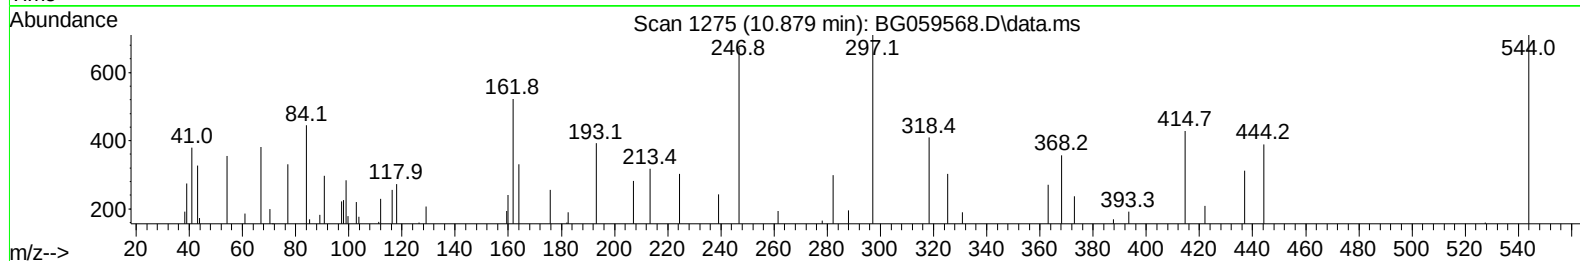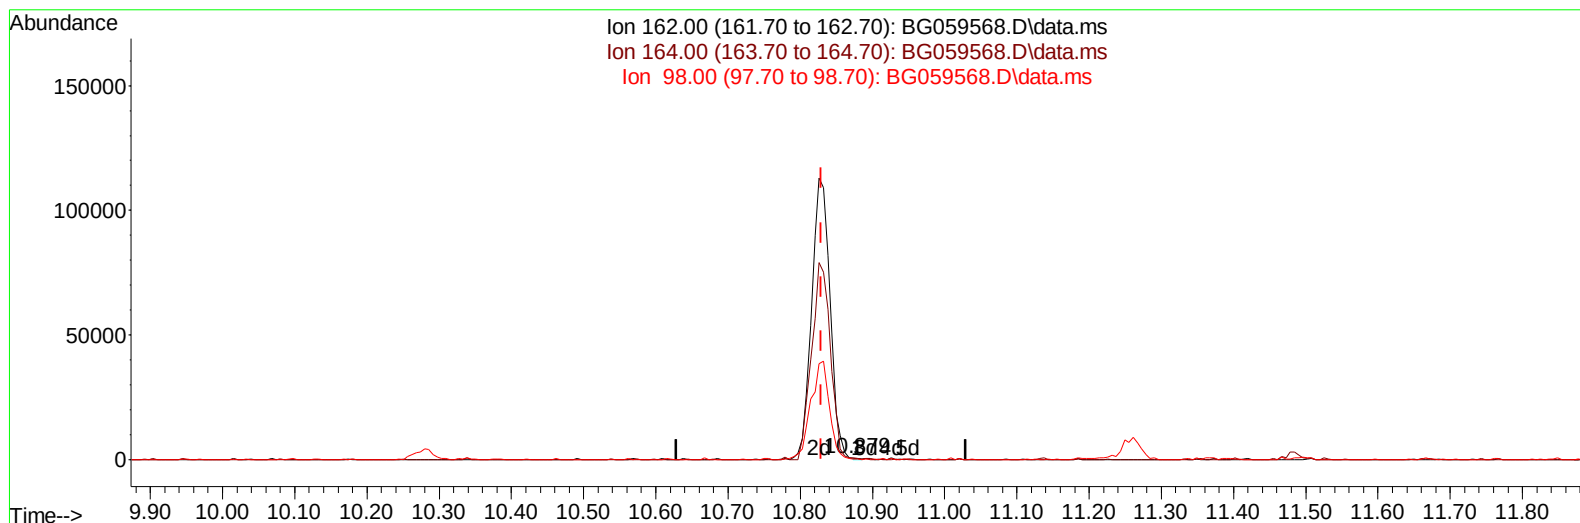

TIC: BG059568.D\data.ms

(29) 2,4-Dichlorophenol (C)

10.879min (+ 0.050) 0.04 ng/ul

response 261

Ion	Exp%	Act%
162.00	100.00	100.00
164.00	56.60	63.29
98.00	40.30	43.21
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
 Data File : BG059568.D
 Acq On : 31 Oct 2023 19:52
 Operator : MA/JU
 Sample : 04950-21MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A49M0MS

Manual IntegrationsAPPROVED

Quant Time: Nov 01 03:20:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/02/2023
 Supervised By :mohammad ahmed 11/02/2023

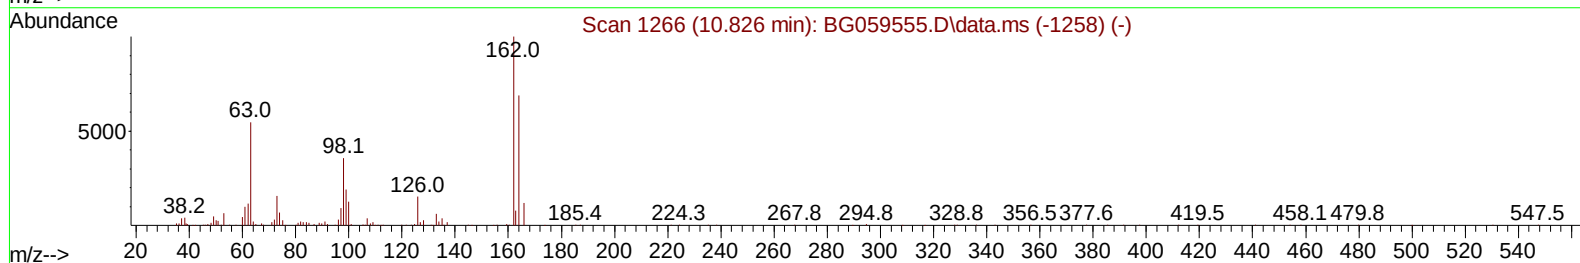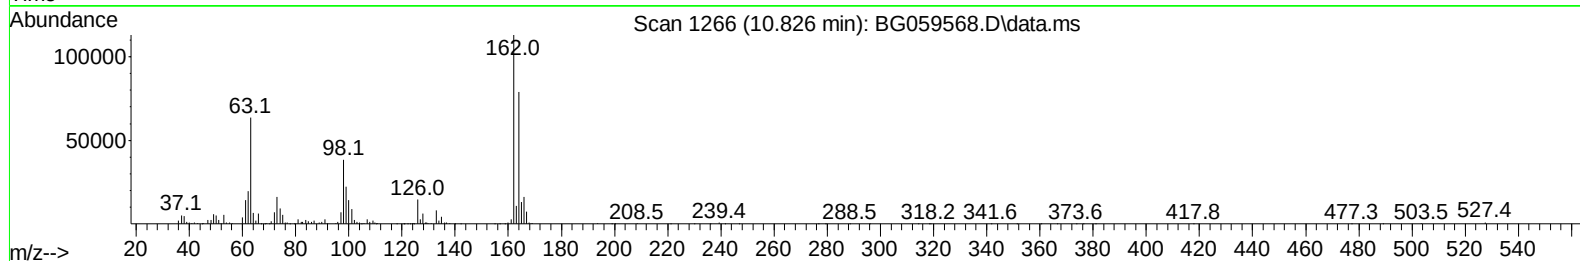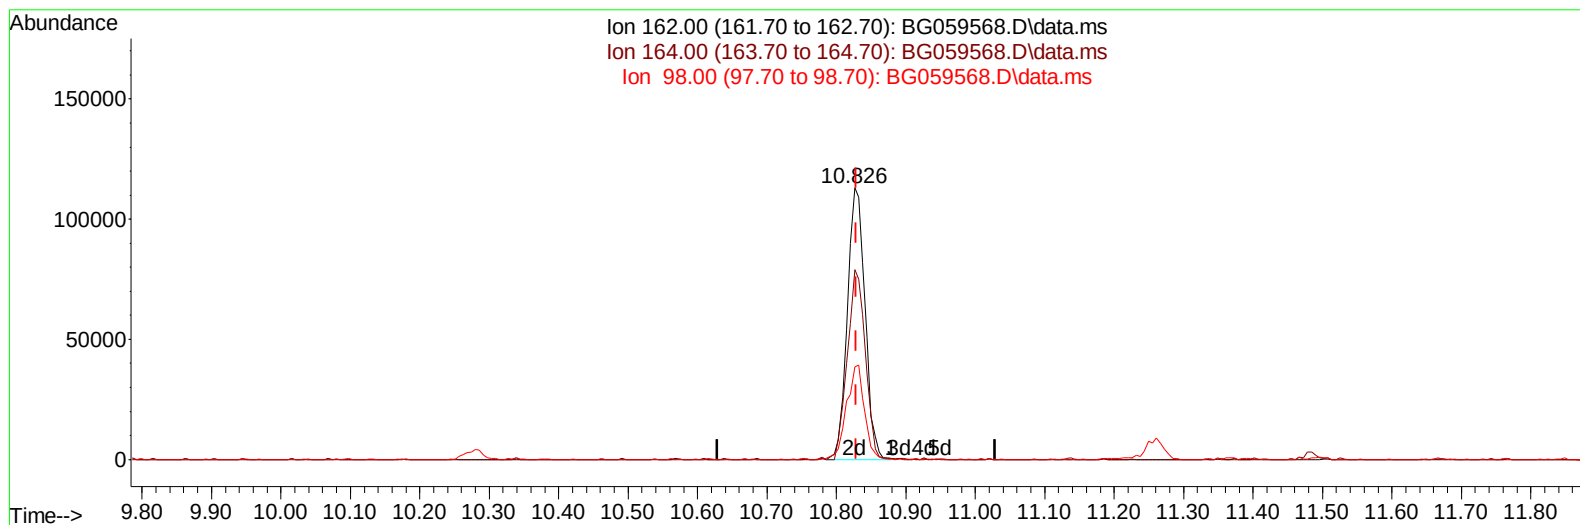

TIC: BG059568.D\data.ms

(29) 2,4-Dichlorophenol (C)

10.826min (-0.003) 29.14 ng/ul m

response 200301

Ion	Exp%	Act%
162.00	100.00	100.00
164.00	56.60	69.93#
98.00	40.30	34.02
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
 Data File : BG059568.D
 Acq On : 31 Oct 2023 19:52
 Operator : MA/JU
 Sample : 04950-21MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A49M0MS

Manual IntegrationsAPPROVED

Quant Time: Nov 01 03:20:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/02/2023
 Supervised By :mohammad ahmed 11/02/2023

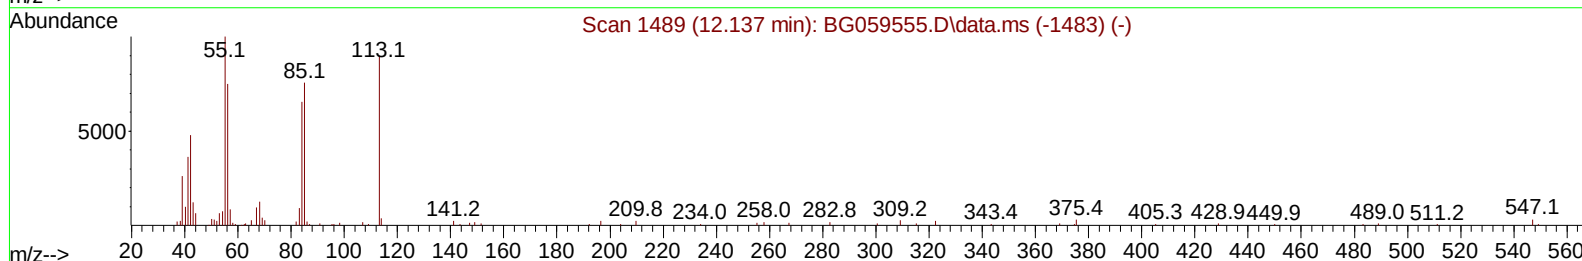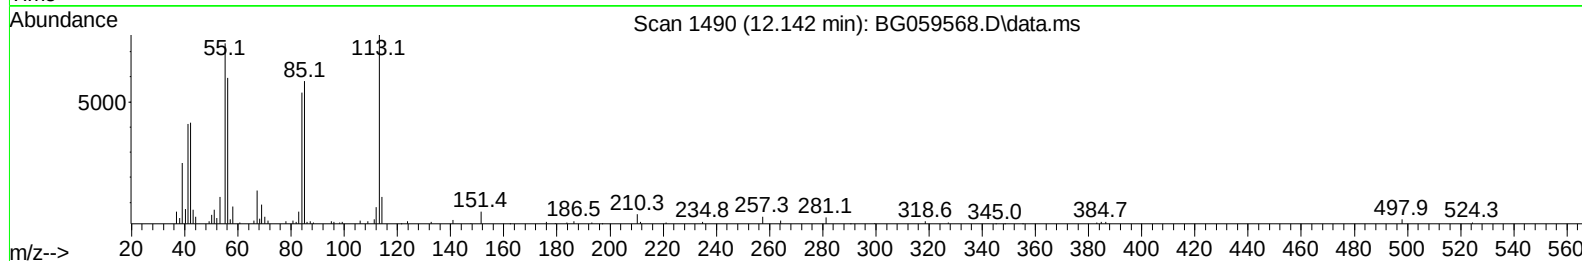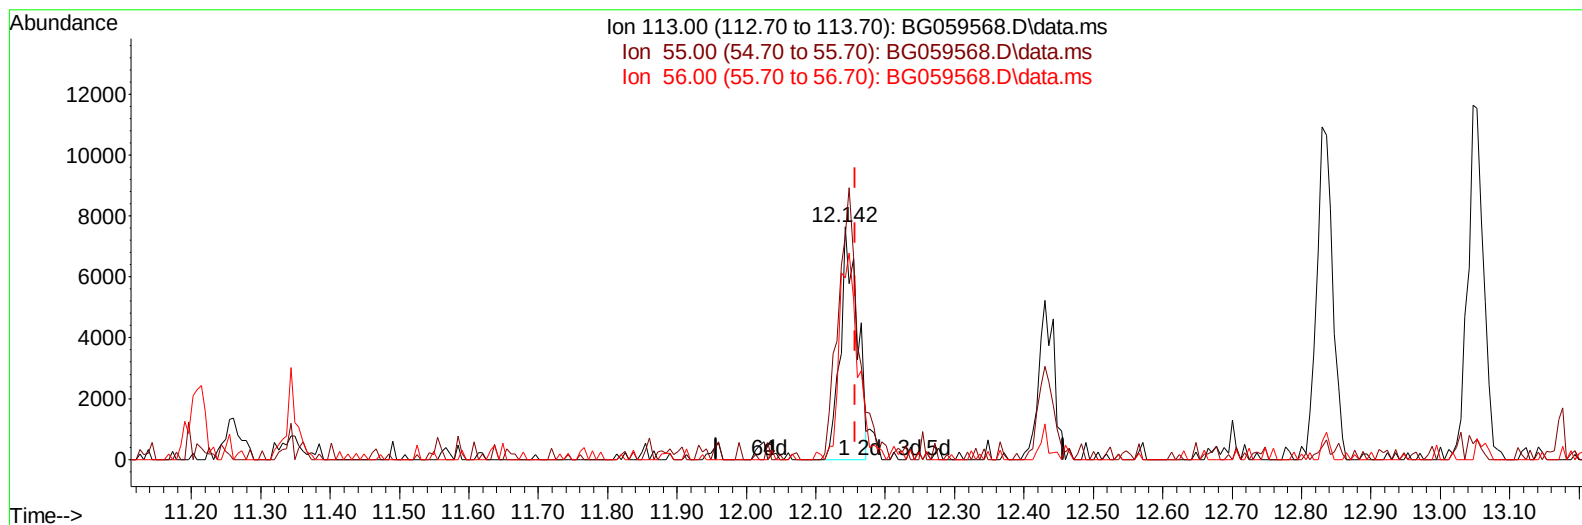

TIC: BG059568.D\data.ms

(34) Caprolactam

12.142min (-0.014) 5.14 ng/ul

response 12936

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	108.60	95.63
56.00	80.50	77.91
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
 Data File : BG059568.D
 Acq On : 31 Oct 2023 19:52
 Operator : MA/JU
 Sample : 04950-21MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A49M0MS

Manual IntegrationsAPPROVED

Quant Time: Nov 01 03:20:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/02/2023
 Supervised By :mohammad ahmed 11/02/2023

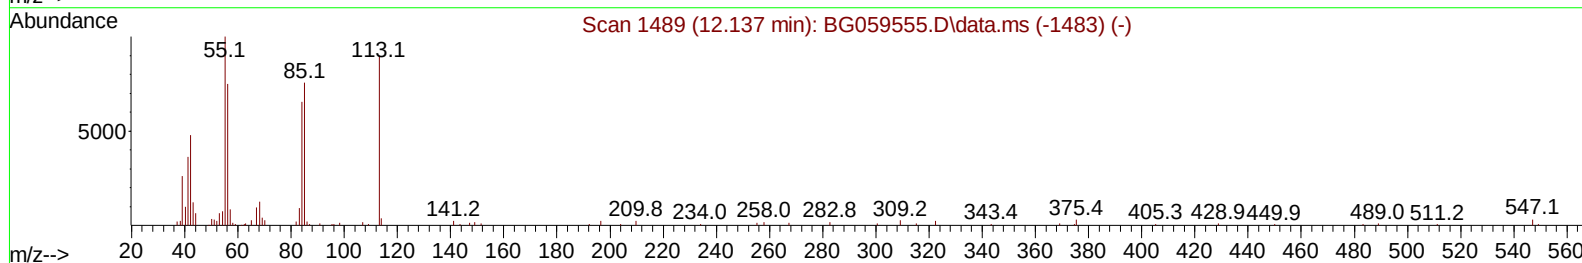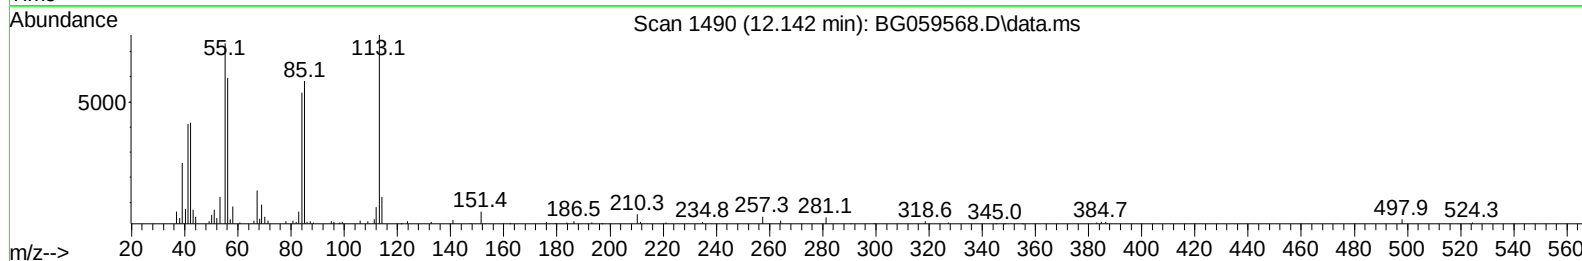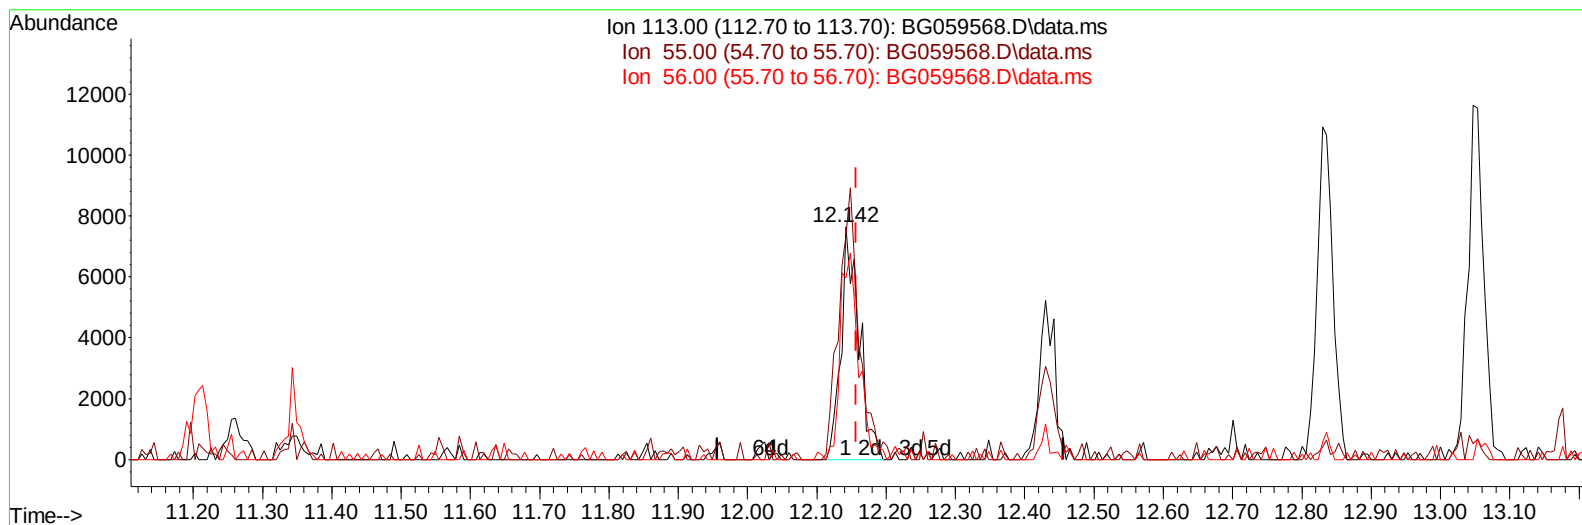

TIC: BG059568.D\data.ms

(34) Caprolactam

12.142min (-0.014) 5.48 ng/ul m

response 13769

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	108.60	95.63
56.00	80.50	77.91
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
 Data File : BG059568.D
 Acq On : 31 Oct 2023 19:52
 Operator : MA/JU
 Sample : 04950-21MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A49M0MS

Manual IntegrationsAPPROVED

Quant Time: Nov 01 03:20:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/02/2023
 Supervised By :mohammad ahmed 11/02/2023

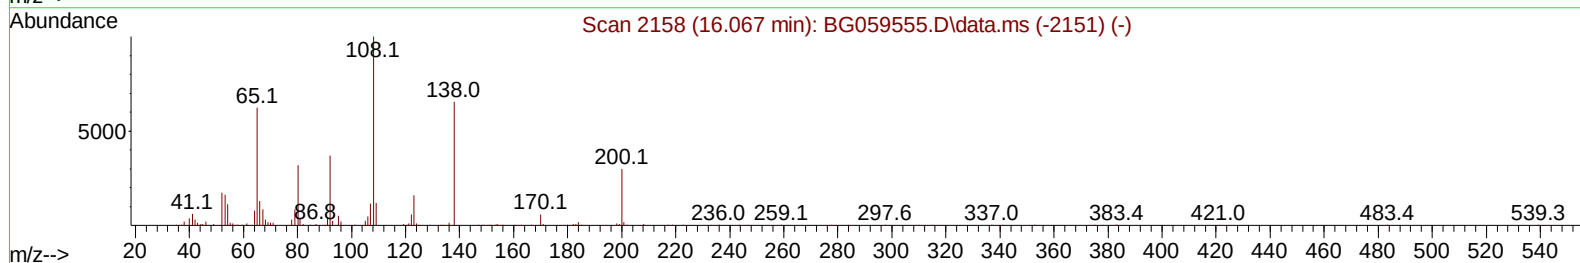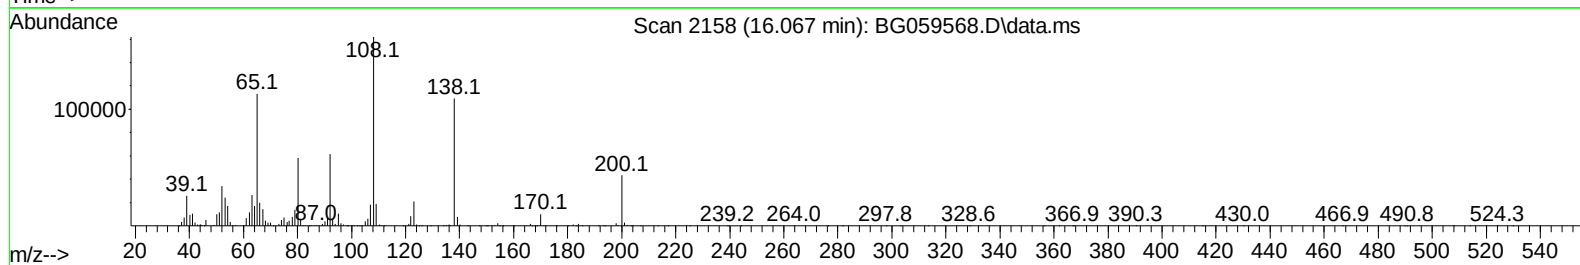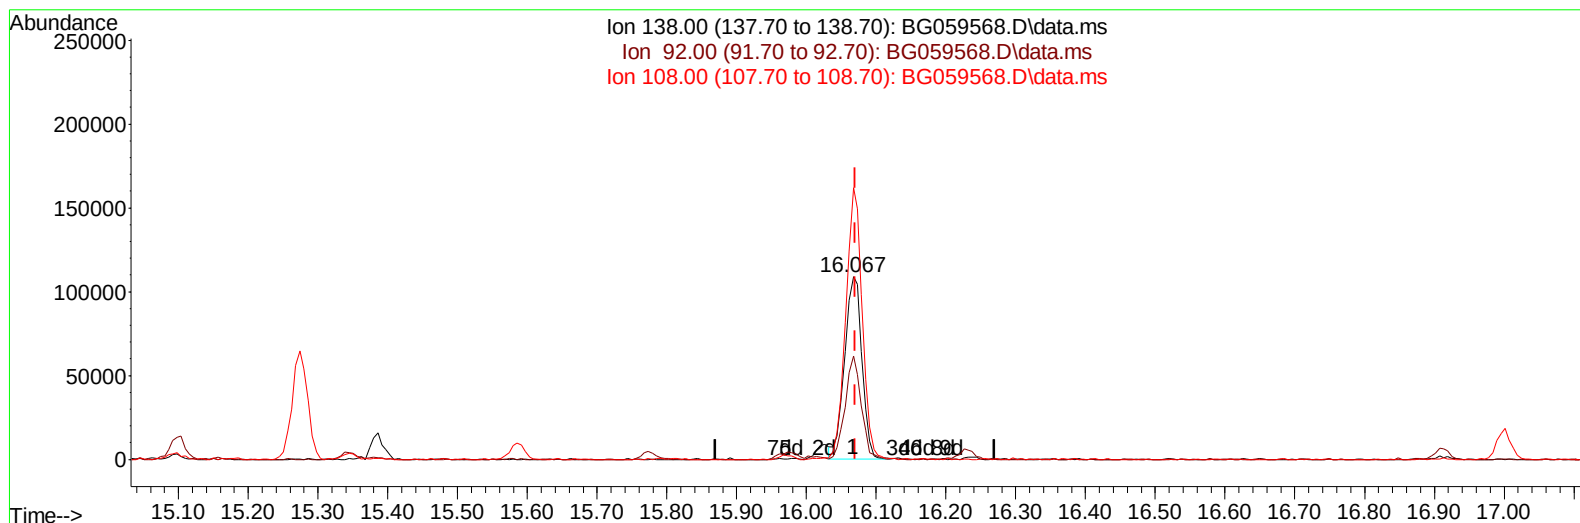

TIC: BG059568.D\data.ms

(63) 4-Nitroaniline

16.067min (-0.003) 40.00 ng/ul

response 187778

Ion	Exp%	Act%
138.00	100.00	100.00
92.00	62.30	56.65
108.00	126.10	148.38
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
 Data File : BG059568.D
 Acq On : 31 Oct 2023 19:52
 Operator : MA/JU
 Sample : 04950-21MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A49M0MS

Manual IntegrationsAPPROVED

Quant Time: Nov 01 03:20:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/02/2023
 Supervised By :mohammad ahmed 11/02/2023

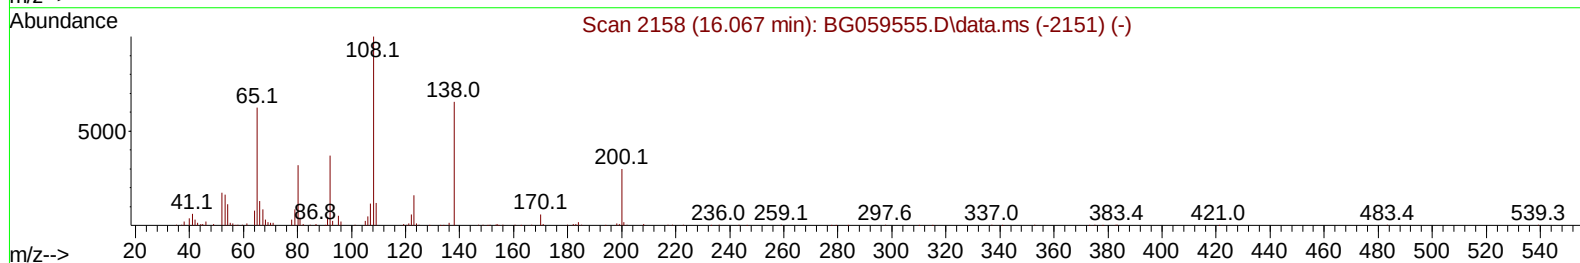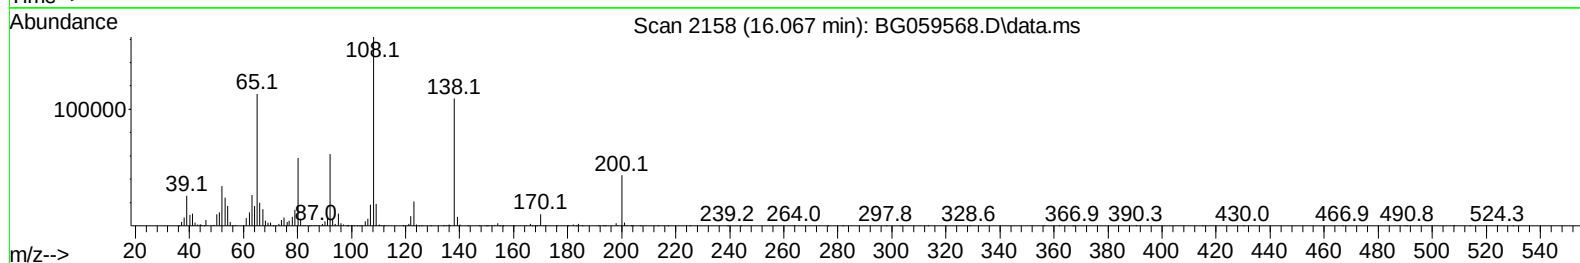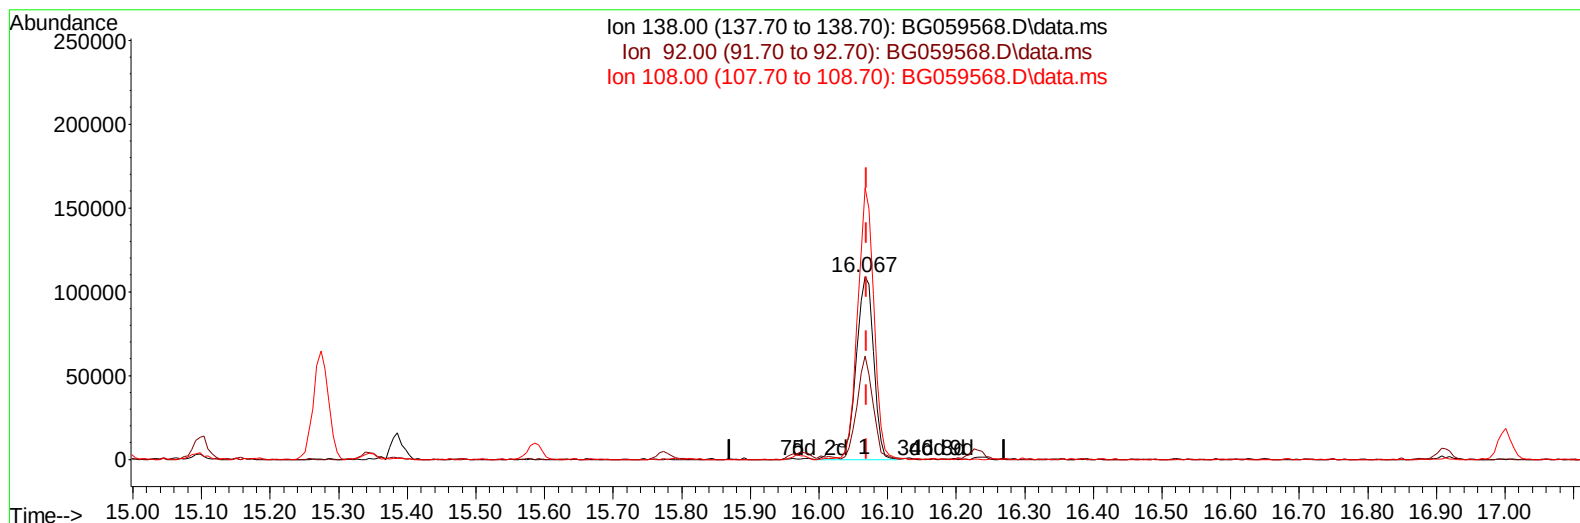

TIC: BG059568.D\data.ms

(63) 4-Nitroaniline

16.067min (-0.003) 42.82 ng/ul m

response 201025

Ion	Exp%	Act%
138.00	100.00	100.00
92.00	62.30	56.65
108.00	126.10	148.38
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
 Data File : BG059568.D
 Acq On : 31 Oct 2023 19:52
 Operator : MA/JU
 Sample : 04950-21MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A49M0MS

Manual IntegrationsAPPROVED

Quant Time: Nov 01 03:20:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/02/2023
 Supervised By :mohammad ahmed 11/02/2023

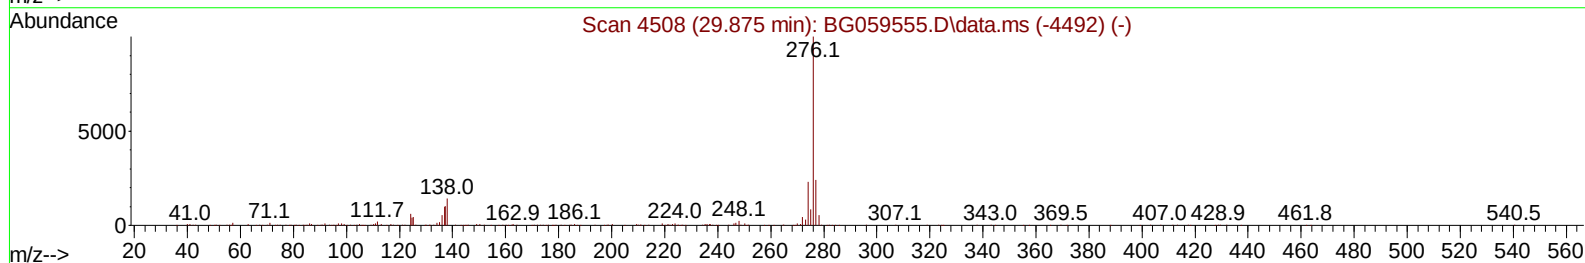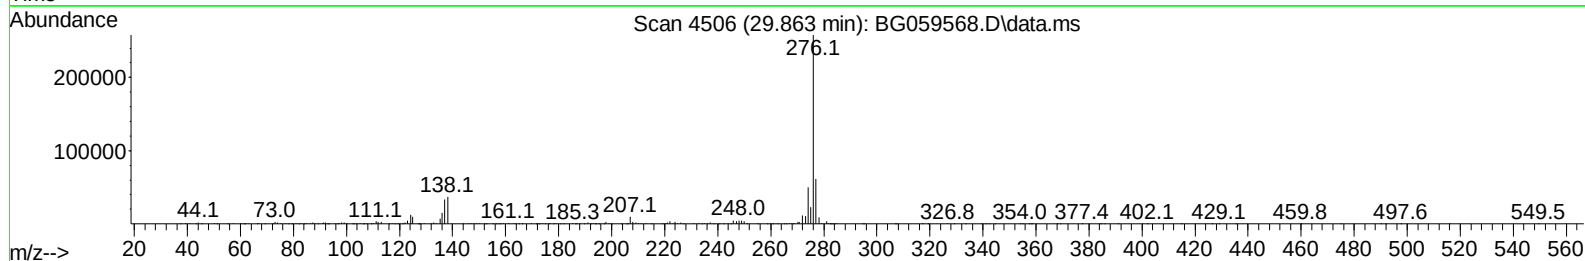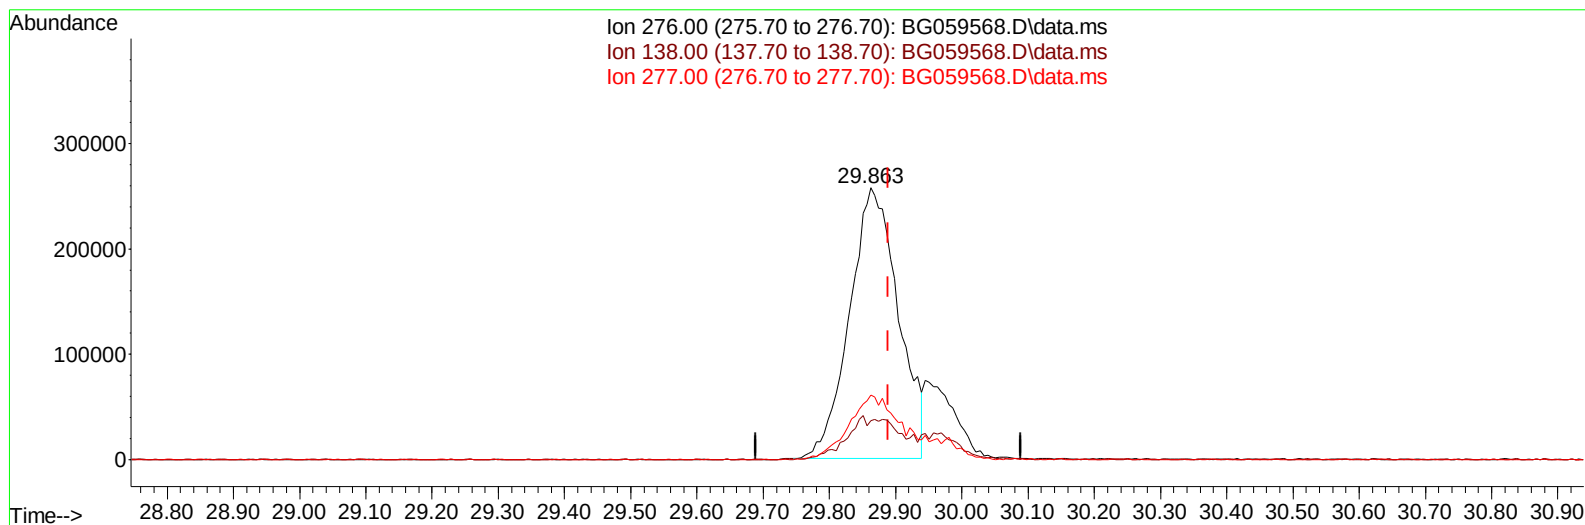

TIC: BG059568.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

29.863min (-0.026) 32.84 ng/ul

response 1317573

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	19.10	14.34#
277.00	20.50	23.64
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
Data File : BG059568.D
Acq On : 31 Oct 2023 19:52
Operator : MA/JU
Sample : 04950-21MS
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A49M0MS

Manual IntegrationsAPPROVED

Quant Time: Nov 01 03:20:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 28 03:56:42 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/02/2023
Supervised By :mohammad ahmed 11/02/2023

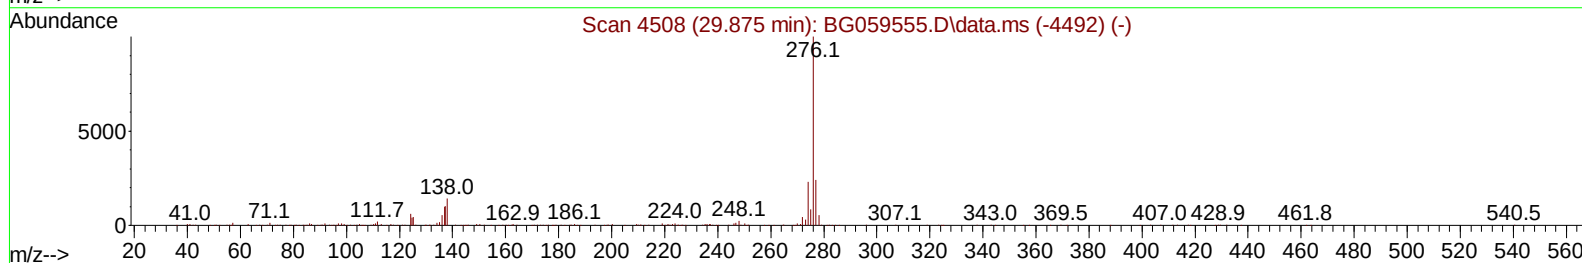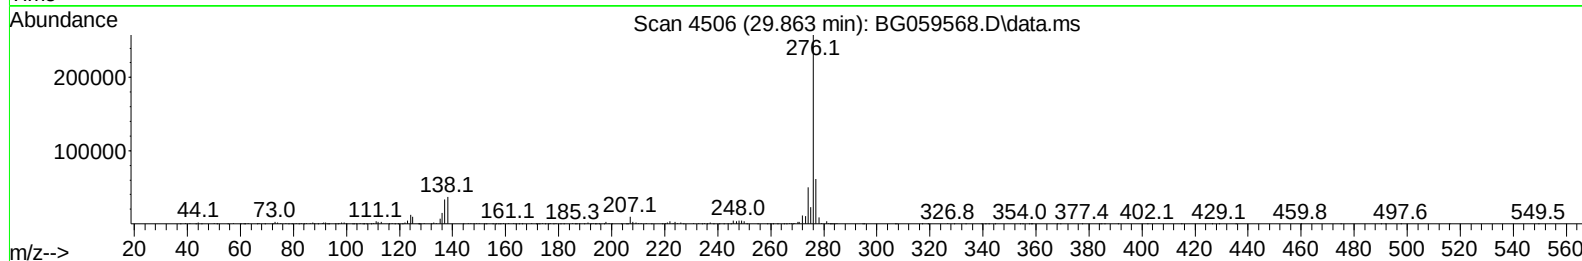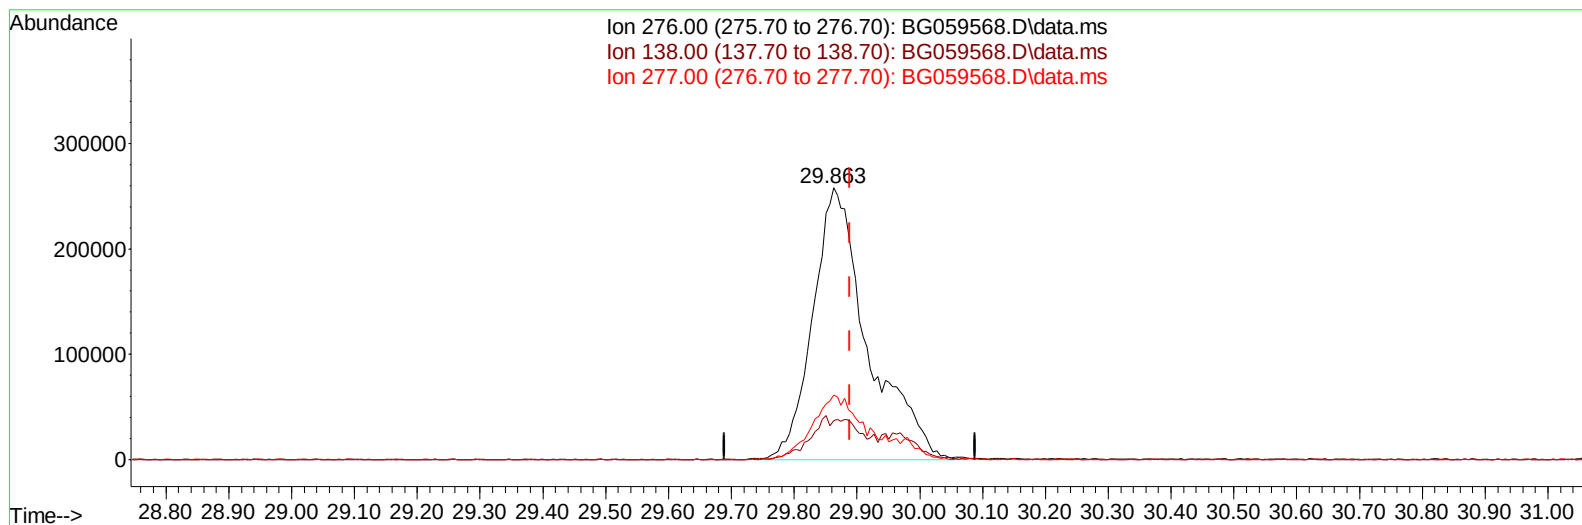

TIC: BG059568.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

29.863min (-0.026) 38.98 ng/ul m

response 1564061

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	19.10	14.34#
277.00	20.50	23.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
 Data File : BG059568.D
 Acq On : 31 Oct 2023 19:52
 Operator : MA/JU
 Sample : 04950-21MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A49M0MS

Manual IntegrationsAPPROVED

Quant Time: Nov 01 04:17:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/02/2023
 Supervised By :mohammad ahmed 11/02/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.359	152	76989	20.000	ng/ul	0.00
20) Naphthalene-d8	11.208	136	441801	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.986	164	262839	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.736	188	552447	20.000	ng/ul	0.00
79) Chrysene-d12	22.078	240	436472	20.000	ng/ul	0.00
88) Perylene-d12	25.679	264	462065	20.000	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.652	96	6836m	3.322	ng/uL	0.00
4) Pyridine-d5	4.093	84	42308	7.358	ng/ul	0.00
7) Phenol-d5	7.471	99	44485	5.623	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.677	67	99692	27.434	ng/ul	0.00
11) 2-Chlorophenol-d4	7.871	132	134712	20.988	ng/ul	0.00
15) 4-Methylphenol-d8	9.040	113	80501	12.825	ng/ul	0.00
21) Nitrobenzene-d5	9.551	128	88648	28.220	ng/ul	0.00
24) 2-Nitrophenol-d4	10.274	143	98573	30.566	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.803	165	201212	28.319	ng/ul	0.00
31) 4-Chloroaniline-d4	11.343	131	254381	21.749	ng/ul	0.00
46) Dimethylphthalate-d6	14.381	166	760126	31.921	ng/ul	0.00
49) Acenaphthylene-d8	14.692	160	844623	30.224	ng/ul	0.00
54) 4-Nitrophenol-d4	15.151	143	30189	7.393	ng/ul	0.00
60) Fluorene-d10	15.973	176	645247	31.707	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.079	200	120840	46.189	ng/ul	0.00
73) Anthracene-d10	17.836	188	983164	32.849	ng/ul	0.00
81) Pyrene-d10	20.109	212	1027030	33.853	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.427	264	982907	36.124	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.693	88	10562	4.586	ng/ul#	96
5) Pyridine	4.111	79	46277	8.159	ng/ul#	85
6) Benzaldehyde	7.501	77	110981	31.144	ng/ul	89
8) Phenol	7.495	94	49114	6.585	ng/ul#	93
10) Bis(2-Chloroethyl)ether	7.771	93	159947	29.243	ng/ul	97
12) 2-Chlorophenol	7.906	128	138683	21.795	ng/ul	98
13) 2-Methylphenol	8.776	108	110796	17.820	ng/ul	99
14) 2,2'-oxybis(1-Chloropr...	8.864	45	138338m	26.877	ng/ul	
16) Acetophenone	9.205	105	309309	31.262	ng/ul	89
17) N-Nitroso-di-n-propyla...	9.163	70	135607	29.088	ng/ul#	93
18) 4-Methylphenol	9.105	108	99460	15.034	ng/ul	82
19) Hexachloroethane	9.451	117	63302	25.048	ng/ul	90
22) Nitrobenzene	9.598	77	193830	28.587	ng/ul	96
23) Isophorone	10.109	82	404148	23.669	ng/ul#	88
25) 2-Nitrophenol	10.309	139	130175	37.533	ng/ul#	80
26) 2,4-Dimethylphenol	10.333	107	200038	21.928	ng/ul	89
27) Bis(2-Chloroethoxy)met...	10.591	93	288745	30.370	ng/ul	99
29) 2,4-Dichlorophenol	10.826	162	200301m	29.139	ng/ul	
30) Naphthalene	11.261	128	814206	29.568	ng/ul	98
32) 4-Chloroaniline	11.373	127	258176	23.238	ng/ul	88
33) Hexachlorobutadiene	11.490	225	120853	29.306	ng/ul	99
34) Caprolactam	12.142	113	13769m	5.475	ng/ul	
35) 4-Chloro-3-methylphenol	12.430	107	240849	29.365	ng/ul	87

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
 Data File : BG059568.D
 Acq On : 31 Oct 2023 19:52
 Operator : MA/JU
 Sample : 04950-21MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A49M0MS

Manual IntegrationsAPPROVED

Quant Time: Nov 01 04:17:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 28 03:56:42 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/02/2023
 Supervised By :mohammad ahmed 11/02/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
36) 2-Methylnaphthalene	12.836	142	581997	30.722	ng/ul	92
37) 1-Methylnaphthalene	13.053	142	584249	30.963	ng/ul#	95
39) 1,2,4,5-Tetrachloroben...	13.176	216	255237	33.668	ng/ul	99
40) Hexachlorocyclopentadiene	13.129	237	120462	27.259	ng/ul	95
41) 2,4,6-Trichlorophenol	13.411	196	189176	36.038	ng/ul	93
42) 2,4,5-Trichlorophenol	13.482	196	204759	36.029	ng/ul	95
43) 1,1'-Biphenyl	13.823	154	782610	32.914	ng/ul	97
44) 2-Chloronaphthalene	13.876	162	598930	32.409	ng/ul#	94
45) 2-Nitroaniline	14.087	65	173524	50.464	ng/ul	96
47) Dimethylphthalate	14.428	163	823748	35.014	ng/ul#	95
48) 2,6-Dinitrotoluene	14.569	165	165143	46.533	ng/ul#	73
50) Acenaphthylene	14.716	152	1053198	32.710	ng/ul	98
51) 3-Nitroaniline	14.904	138	173238	39.162	ng/ul#	78
52) Acenaphthene	15.051	153	693923	33.062	ng/ul	97
53) 2,4-Dinitrophenol	15.098	184	85958	42.628	ng/ul#	73
55) 4-Nitrophenol	15.162	109	38290	8.508	ng/ul	94
56) Dibenzofuran	15.386	168	949237	34.885	ng/ul	97
57) 2,4-Dinitrotoluene	15.344	165	242618	48.601	ng/ul#	90
58) 2,3,4,6-Tetrachlorophenol	15.585	232	177831	39.868	ng/ul#	91
59) Diethylphthalate	15.773	149	935276	36.443	ng/ul	97
61) Fluorene	16.032	166	802200	34.150	ng/ul	94
62) 4-Chlorophenyl-phenyle...	16.014	204	368966	36.753	ng/ul	98
63) 4-Nitroaniline	16.067	138	201025m	42.821	ng/ul	
66) 4,6-Dinitro-2-methylph...	16.091	198	130356	47.277	ng/ul#	67
67) N-Nitrosodiphenylamine	16.232	169	706211	37.412	ng/ul	98
68) 4-Bromophenyl-phenylether	16.913	248	214597	38.819	ng/ul	86
69) Hexachlorobenzene	17.001	284	242202	37.909	ng/ul	96
70) Atrazine	17.166	200	193355	33.056	ng/ul	93
71) Pentachlorophenol	17.354	266	153762	42.127	ng/ul	94
72) Phenanthrene	17.783	178	1320365	36.764	ng/ul	98
74) Anthracene	17.871	178	1288194	35.524	ng/ul	97
75) 1,2,3,4-Tetrachloroben...	13.782	216	253371	34.440	ng/uL	97
76) Pentachlorobenzene	15.274	250	253985	36.382	ng/uL	98
77) Carbazole	18.147	167	1199877	38.517	ng/ul	96
78) Di-n-butylphthalate	18.658	149	1543623	36.064	ng/ul	99
80) Fluoranthene	19.775	202	1394913	37.719	ng/ul#	97
82) Pyrene	20.139	202	1419173	36.944	ng/ul#	95
83) Butylbenzylphthalate	21.003	149	684247	39.441	ng/ul	95
84) 3,3'-Dichlorobenzidine	21.960	252	281780	24.826	ng/ul	93
85) Benzo(a)anthracene	22.054	228	1304203	36.310	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.896	149	986371	38.104	ng/ul	97
87) Chrysene	22.125	228	1208998	36.184	ng/ul	95
89) Di-n-octyl phthalate	23.247	149	1687687	41.718	ng/ul	100
90) Benzo(b)fluoranthene	24.516	252	1303535	38.919	ng/ul#	96
91) Benzo(k)fluoranthene	24.592	252	1328170	39.699	ng/ul#	97
93) Benzo(a)pyrene	25.509	252	1236540	39.061	ng/ul	96
94) Indeno(1,2,3-cd)pyrene	29.863	276	1564061m	38.980	ng/ul	
95) Dibenzo(a,h)anthracene	29.968	278	1301489	39.273	ng/ul	97
96) Benzo(g,h,i)perylene	31.208	276	1259676	38.358	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :

BNA_G

ClientSampleId :

A49M0MS

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/02/2023

Supervised By :mohammad ahmed 11/02/2023

