

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
 Data File : BG059556.D
 Acq On : 31 Oct 2023 10:10
 Operator : MA/JU
 Sample : PB156466BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK466

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059556.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.659	40	46	50	rBV2	15352	25670	0.90%	0.087%
2	3.782	64	67	69	rVB2	5424	6021	0.21%	0.020%
3	4.088	114	119	130	rVB	221317	379282	13.35%	1.287%
4	4.429	172	177	180	rBV3	12321	22140	0.78%	0.075%
5	4.487	184	187	190	rBV	5080	6420	0.23%	0.022%
6	4.816	241	243	246	rBV	5417	5918	0.21%	0.020%
7	4.904	256	258	263	rVB2	5448	7247	0.26%	0.025%
8	5.092	287	290	292	rVV2	6213	7039	0.25%	0.024%
9	5.110	292	293	298	rVB3	5438	6365	0.22%	0.022%
10	5.316	324	328	330	rVB	5428	6603	0.23%	0.022%
11	5.433	344	348	353	rVB2	3458	5720	0.20%	0.019%
12	5.492	353	358	361	rBV2	4920	6956	0.24%	0.024%
13	5.580	368	373	374	rBV2	5862	6592	0.23%	0.022%
14	5.633	380	382	386	rVB2	4825	6082	0.21%	0.021%
15	6.080	456	458	463	rVB2	5693	6249	0.22%	0.021%
16	6.373	506	508	512	rBV2	5117	6083	0.21%	0.021%
17	6.444	517	520	523	rVB2	4589	5956	0.21%	0.020%
18	7.031	619	620	625	rVB2	6593	6334	0.22%	0.021%
19	7.108	631	633	637	rVV	5198	5971	0.21%	0.020%
20	7.384	674	680	681	rBV	7003	11075	0.39%	0.038%
21	7.466	686	694	700	rVV	422714	718067	25.28%	2.436%
22	7.678	723	730	740	rVB	228757	395780	13.94%	1.343%
23	7.872	754	763	771	rVB	337014	600141	21.13%	2.036%
24	8.353	837	845	852	rBV	258593	458546	16.15%	1.556%
25	8.653	893	896	902	rVB	4794	8877	0.31%	0.030%
26	8.718	905	907	911	rBV	4142	5783	0.20%	0.020%
27	9.041	955	962	969	rBV	439914	780690	27.49%	2.649%
28	9.258	996	999	1003	rVV	4210	5988	0.21%	0.020%
29	9.376	1014	1019	1021	rBV	3665	6896	0.24%	0.023%
30	9.552	1041	1049	1058	rVV	396696	675336	23.78%	2.291%
31	9.740	1079	1081	1086	rBV2	4376	7339	0.26%	0.025%
32	9.963	1116	1119	1120	rBV2	6684	5636	0.20%	0.019%
33	10.010	1126	1127	1131	rBV	5971	6054	0.21%	0.021%
34	10.069	1133	1137	1140	rBV2	9281	14034	0.49%	0.048%
35	10.163	1151	1153	1155	rVB2	9511	8014	0.28%	0.027%
36	10.192	1155	1158	1160	rBV3	7480	10716	0.38%	0.036%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
 Data File : BG059556.D
 Acq On : 31 Oct 2023 10:10
 Operator : MA/JU
 Sample : PB156466BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK466

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

37	10.275	1164	1172	1182	rVB2	345330	633329	22.30%	2.149%
38	10.798	1251	1261	1271	rBV	568765	1072351	37.76%	3.638%
39	10.956	1285	1288	1289	rBV	8299	7049	0.25%	0.024%
40	11.209	1324	1331	1339	rVB	473026	903750	31.82%	3.066%
41	11.344	1344	1354	1362	rBV	570930	1039809	36.61%	3.528%
42	11.520	1381	1384	1386	rVV2	6667	7272	0.26%	0.025%
43	11.550	1386	1389	1392	rVV2	7519	7601	0.27%	0.026%
44	11.591	1392	1396	1397	rVB	8675	10562	0.37%	0.036%
45	11.614	1397	1400	1402	rBV	8256	10179	0.36%	0.035%
46	11.708	1412	1416	1417	rBV2	7892	7734	0.27%	0.026%
47	11.749	1422	1423	1427	rVB	6532	7902	0.28%	0.027%
48	11.790	1427	1430	1432	rBV	5504	7042	0.25%	0.024%
49	11.967	1457	1460	1461	rVV3	5434	6201	0.22%	0.021%
50	12.178	1491	1496	1499	rBV	5739	8934	0.31%	0.030%
51	12.243	1505	1507	1508	rBV	8002	6554	0.23%	0.022%
52	12.302	1514	1517	1519	rVV2	7158	6773	0.24%	0.023%
53	12.378	1529	1530	1534	rBV2	6159	5933	0.21%	0.020%
54	12.472	1544	1546	1550	rBV2	5951	8930	0.31%	0.030%
55	12.519	1552	1554	1556	rVB	7390	7122	0.25%	0.024%
56	12.760	1591	1595	1600	rVB2	16720	33068	1.16%	0.112%
57	12.813	1603	1604	1606	rVB	8906	6073	0.21%	0.021%
58	13.024	1639	1640	1643	rBV	8560	5677	0.20%	0.019%
59	13.289	1683	1685	1689	rVB	5288	5745	0.20%	0.019%
60	13.818	1772	1775	1778	rVV4	16986	22596	0.80%	0.077%
61	13.876	1782	1785	1787	rBV4	7001	9835	0.35%	0.033%
62	13.953	1797	1798	1801	rVB2	9028	6356	0.22%	0.022%
63	13.988	1801	1804	1805	rBV	8219	6322	0.22%	0.021%
64	14.288	1852	1855	1856	rVB2	8518	6460	0.23%	0.022%
65	14.305	1856	1858	1860	rBV3	7796	7693	0.27%	0.026%
66	14.382	1864	1871	1878	rVB	1085493	1576804	55.52%	5.350%
67	14.687	1916	1923	1930	rVV	1180722	1901509	66.95%	6.451%
68	14.852	1949	1951	1953	rBV3	6409	6745	0.24%	0.023%
69	14.893	1955	1958	1961	rVV3	5740	6939	0.24%	0.024%
70	14.987	1967	1974	1983	rVB2	768352	1224068	43.10%	4.153%
71	15.057	1983	1986	1988	rBV2	9398	13412	0.47%	0.046%
72	15.151	1995	2002	2010	rBV	523076	853924	30.07%	2.897%
73	15.210	2010	2012	2015	rVB4	7025	6989	0.25%	0.024%
74	15.909	2129	2131	2135	rBV3	5044	7321	0.26%	0.025%
75	15.974	2135	2142	2149	rVV	1525135	2281546	80.33%	7.741%
76	16.074	2153	2159	2166	rVB2	347438	524854	18.48%	1.781%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
 Data File : BG059556.D
 Acq On : 31 Oct 2023 10:10
 Operator : MA/JU
 Sample : PB156466BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK466

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

77	16.467	2224	2226	2228	rBV2	5586	6326	0.22%	0.021%
78	16.602	2245	2249	2250	rVV3	6070	6588	0.23%	0.022%
79	16.679	2260	2262	2266	rVB5	8242	7920	0.28%	0.027%
80	17.214	2350	2353	2354	rBV2	6320	6124	0.22%	0.021%
81	17.355	2374	2377	2378	rBV2	7137	7741	0.27%	0.026%
82	17.578	2412	2415	2416	rBV3	10404	8915	0.31%	0.030%
83	17.736	2435	2442	2450	rVV	1030656	1554870	54.75%	5.275%
84	17.836	2453	2459	2467	rVB2	1686993	2544295	89.58%	8.632%
85	18.277	2530	2534	2539	rVB5	9227	14379	0.51%	0.049%
86	18.348	2544	2546	2547	rBV	13350	10499	0.37%	0.036%
87	18.565	2579	2583	2588	rBV6	8270	16495	0.58%	0.056%
88	18.618	2591	2592	2596	rBV3	12399	15035	0.53%	0.051%
89	18.735	2610	2612	2615	rBV4	7013	7018	0.25%	0.024%
90	18.882	2635	2637	2638	rBV2	8613	6281	0.22%	0.021%
91	18.935	2644	2646	2648	rBV3	8884	8094	0.28%	0.027%
92	19.170	2684	2686	2688	rBV2	9646	5975	0.21%	0.020%
93	19.258	2699	2701	2704	rVB4	15193	14162	0.50%	0.048%
94	19.288	2704	2706	2708	rBV3	8879	9650	0.34%	0.033%
95	20.040	2833	2834	2835	rBV	12748	5952	0.21%	0.020%
96	20.110	2839	2846	2852	rBV	1928390	2840131	100.00%	9.636%
97	22.073	3174	3180	3188	rVB2	870170	1522425	53.60%	5.165%
98	23.336	3393	3395	3396	rBV2	27071	18032	0.63%	0.061%
99	25.433	3742	3752	3762	rVB2	901829	2703220	95.18%	9.171%
100	25.686	3785	3795	3806	rVB	519753	1608502	56.63%	5.457%




Sum of corrected areas: 29475212

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
Data File : BG059556.D
Acq On : 31 Oct 2023 10:10
Operator : MA/JU
Sample : PB156466BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK466

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

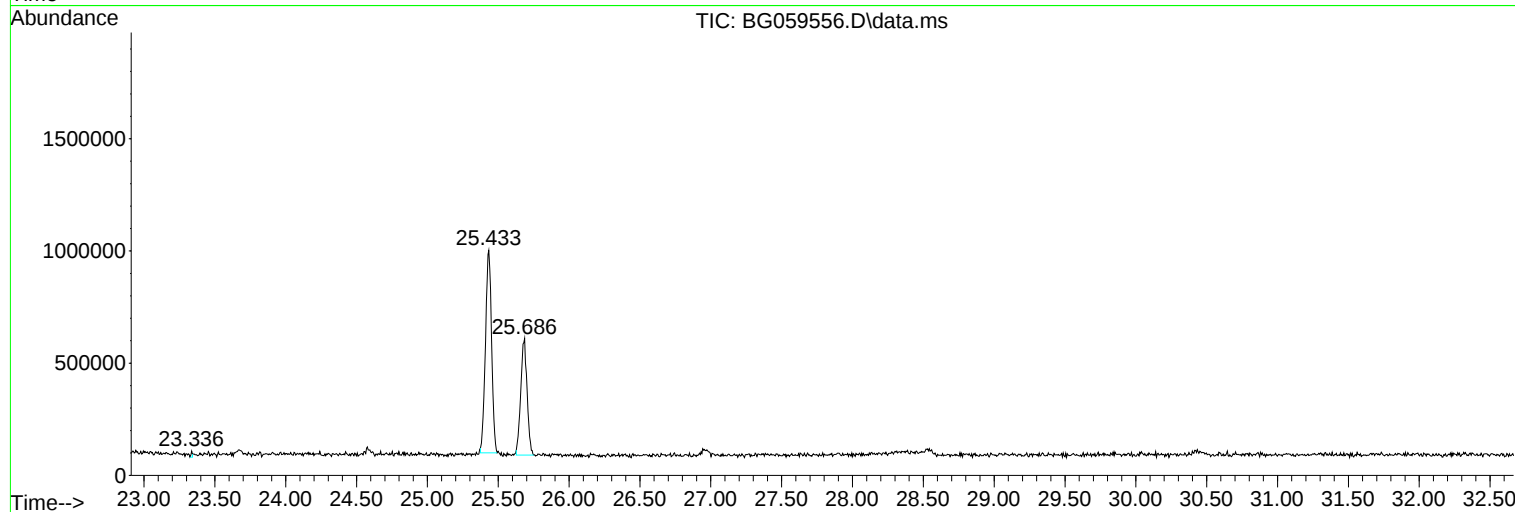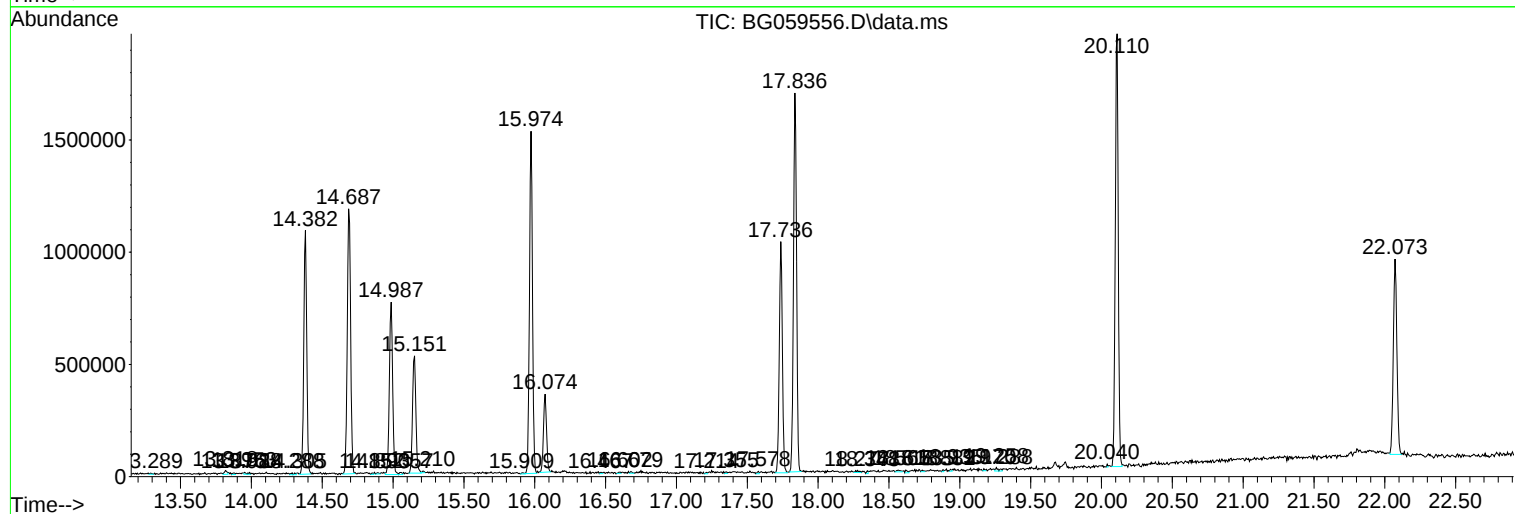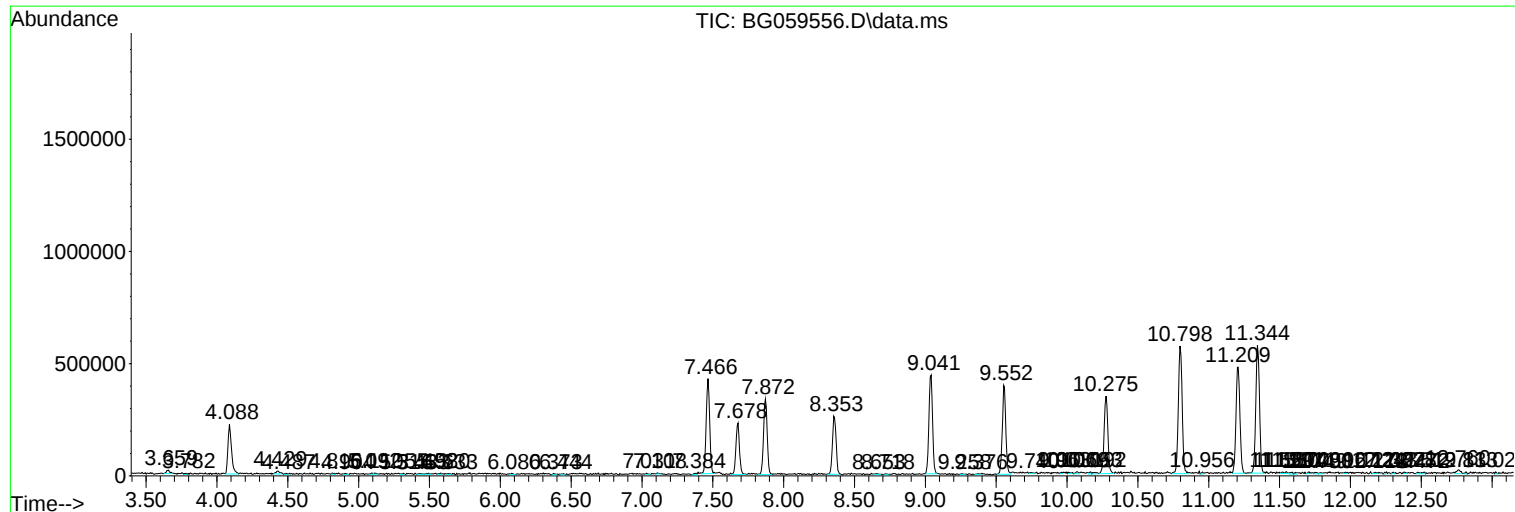

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
Data File : BG059556.D
Acq On : 31 Oct 2023 10:10
Operator : MA/JU
Sample : PB156466BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK466

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
Data File : BG059556.D
Acq On : 31 Oct 2023 10:10
Operator : MA/JU
Sample : PB156466BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK466

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------