

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
 Data File : BG059561.D
 Acq On : 31 Oct 2023 14:04
 Operator : MA/JU
 Sample : PB156470BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK470

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059561.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.441	7	9	12	rVB2	6084	5998	0.26%	0.024%
2	3.470	12	14	16	rBV3	4960	4975	0.21%	0.020%
3	3.553	25	28	31	rBV4	3174	4825	0.21%	0.019%
4	3.658	42	46	49	rVB2	16570	22823	0.98%	0.090%
5	3.876	80	83	87	rBV3	4154	5964	0.26%	0.023%
6	4.087	114	119	127	rBV	238276	383413	16.46%	1.505%
7	4.293	151	154	158	rBV2	5508	7942	0.34%	0.031%
8	4.434	172	178	180	rBV3	9766	13975	0.60%	0.055%
9	4.722	226	227	231	rBV2	3957	5105	0.22%	0.020%
10	4.939	262	264	267	rVB	5206	4857	0.21%	0.019%
11	4.986	267	272	274	rBV2	5127	8052	0.35%	0.032%
12	5.274	318	321	324	rVB2	5385	5040	0.22%	0.020%
13	5.304	324	326	329	rBV2	4531	6108	0.26%	0.024%
14	5.586	372	374	376	rVB2	5542	4530	0.19%	0.018%
15	5.644	382	384	387	rBV	5088	4677	0.20%	0.018%
16	5.685	389	391	393	rBV	5663	5581	0.24%	0.022%
17	5.920	428	431	433	rVV	6317	6662	0.29%	0.026%
18	6.232	480	484	485	rBV2	4472	6184	0.27%	0.024%
19	6.972	607	610	613	rBV2	3708	4303	0.18%	0.017%
20	7.037	619	621	624	rVB	5680	4527	0.19%	0.018%
21	7.383	679	680	683	rBV	5939	6023	0.26%	0.024%
22	7.466	687	694	701	rVV2	371451	621596	26.68%	2.439%
23	7.677	724	730	737	rVB	237663	417197	17.91%	1.637%
24	7.730	737	739	742	rBV2	6010	6509	0.28%	0.026%
25	7.871	757	763	769	rBV	381713	616599	26.47%	2.420%
26	7.989	782	783	786	rVB	4876	4763	0.20%	0.019%
27	8.359	839	846	855	rBV	258848	446222	19.15%	1.751%
28	8.852	926	930	934	rVB	5862	10830	0.46%	0.042%
29	9.040	954	962	971	rBV	491250	859645	36.90%	3.373%
30	9.246	995	997	999	rBV	6747	5988	0.26%	0.023%
31	9.275	1000	1002	1006	rVB2	5113	4770	0.20%	0.019%
32	9.551	1040	1049	1058	rVV	318296	597280	25.64%	2.344%
33	9.645	1061	1065	1066	rVB	4294	4411	0.19%	0.017%
34	9.657	1066	1067	1070	rBV2	5472	5464	0.23%	0.021%
35	10.274	1165	1172	1178	rBV2	290855	526080	22.58%	2.064%
36	10.433	1197	1199	1202	rVB2	4368	4753	0.20%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
 Data File : BG059561.D
 Acq On : 31 Oct 2023 14:04
 Operator : MA/JU
 Sample : PB156470BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK470

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

37	10.497	1208	1210	1215	rVB2	4986	7510	0.32%	0.029%
38	10.668	1237	1239	1241	rBV	3976	4952	0.21%	0.019%
39	10.797	1254	1261	1270	rVV	504476	900781	38.67%	3.535%
40	11.208	1322	1331	1338	rBV	387143	716672	30.76%	2.812%

41	11.343	1346	1354	1362	rBV	469901	884872	37.98%	3.472%
42	11.467	1372	1375	1376	rBV	4622	4434	0.19%	0.017%
43	11.549	1388	1389	1395	rBV	3478	5976	0.26%	0.023%
44	11.931	1453	1454	1459	rVV2	6439	6175	0.27%	0.024%
45	11.978	1459	1462	1465	rVB2	9416	9554	0.41%	0.037%

46	12.107	1481	1484	1487	rBV	4198	5884	0.25%	0.023%
47	12.513	1551	1553	1556	rBV2	5086	5067	0.22%	0.020%
48	12.636	1573	1574	1577	rBV	5381	5117	0.22%	0.020%
49	12.754	1592	1594	1599	rVB2	12183	18594	0.80%	0.073%
50	12.842	1607	1609	1612	rVB	7612	5190	0.22%	0.020%

51	12.942	1622	1626	1630	rBV	3215	6757	0.29%	0.027%
52	13.265	1679	1681	1684	rVB2	4800	4926	0.21%	0.019%
53	13.394	1701	1703	1705	rBV	7560	6389	0.27%	0.025%
54	13.541	1725	1728	1729	rBV	6076	7134	0.31%	0.028%
55	13.823	1770	1776	1780	rBV4	15048	29323	1.26%	0.115%

56	14.076	1814	1819	1821	rVB	4684	4500	0.19%	0.018%
57	14.381	1863	1871	1877	rVV	997250	1449083	62.20%	5.686%
58	14.616	1908	1911	1912	rBV	3741	4431	0.19%	0.017%
59	14.687	1916	1923	1930	rVV	1094397	1742536	74.80%	6.838%
60	14.787	1938	1940	1941	rBV	6462	4319	0.19%	0.017%

61	14.839	1944	1949	1952	rBV2	4184	7767	0.33%	0.030%
62	14.986	1967	1974	1981	rVB2	656322	1023152	43.92%	4.015%
63	15.069	1986	1988	1993	rVB	7220	9982	0.43%	0.039%
64	15.151	1993	2002	2011	rBV	459258	779428	33.46%	3.059%
65	15.697	2094	2095	2097	rBV2	7366	5472	0.23%	0.021%

66	15.909	2129	2131	2134	rBV	5443	5812	0.25%	0.023%
67	15.973	2134	2142	2150	rVV	1332350	2075244	89.08%	8.144%
68	16.073	2153	2159	2167	rBV	340339	507334	21.78%	1.991%
69	16.208	2180	2182	2183	rVV	7794	6536	0.28%	0.026%
70	16.220	2183	2184	2187	rVB3	10661	4655	0.20%	0.018%

71	16.643	2253	2256	2257	rBV2	6597	4931	0.21%	0.019%
72	16.678	2260	2262	2265	rBV2	3905	5688	0.24%	0.022%
73	16.725	2267	2270	2271	rBV2	4384	4452	0.19%	0.017%
74	16.849	2288	2291	2293	rVB2	5367	4494	0.19%	0.018%
75	16.890	2293	2298	2299	rBV3	5560	6781	0.29%	0.027%

76	16.931	2302	2305	2308	rBV3	4364	6362	0.27%	0.025%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
 Data File : BG059561.D
 Acq On : 31 Oct 2023 14:04
 Operator : MA/JU
 Sample : PB156470BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK470

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

77	17.248	2358	2359	2361	rBV2	8864	4746	0.20%	0.019%
78	17.383	2379	2382	2383	rBV	4622	4347	0.19%	0.017%
79	17.466	2394	2396	2398	rBV	9058	6965	0.30%	0.027%
80	17.736	2436	2442	2449	rBV	828934	1252508	53.76%	4.915%
81	17.836	2452	2459	2466	rVV2	1491291	2232734	95.84%	8.762%
82	18.030	2489	2492	2494	rVB4	5268	6036	0.26%	0.024%
83	18.071	2497	2499	2502	rBV	5309	7278	0.31%	0.029%
84	18.406	2553	2556	2558	rBV3	5555	5412	0.23%	0.021%
85	18.494	2570	2571	2574	rBV2	5973	4502	0.19%	0.018%
86	18.553	2579	2581	2584	rVV3	6449	8233	0.35%	0.032%
87	18.582	2584	2586	2587	rVV2	7865	4716	0.20%	0.019%
88	18.617	2590	2592	2594	rVV	8237	7271	0.31%	0.029%
89	18.752	2613	2615	2618	rVB3	7832	5202	0.22%	0.020%
90	18.782	2618	2620	2624	rBV3	4240	6106	0.26%	0.024%
91	18.870	2632	2635	2637	rBV4	5733	5878	0.25%	0.023%
92	18.952	2645	2649	2651	rBV5	6250	8666	0.37%	0.034%
93	19.040	2663	2664	2668	rVB3	7909	8122	0.35%	0.032%
94	19.158	2682	2684	2686	rVB3	8732	6845	0.29%	0.027%
95	19.234	2695	2697	2699	rBV2	9308	9509	0.41%	0.037%
96	19.669	2768	2771	2775	rVB4	20858	29808	1.28%	0.117%
97	20.110	2839	2846	2852	rBV	1579745	2329656	100.00%	9.142%
98	22.072	3173	3180	3189	rVB2	647369	1194376	51.27%	4.687%
99	25.427	3741	3751	3762	rVB2	721940	2185972	93.83%	8.578%
100	25.680	3784	3794	3804	rVB2	383458	1196259	51.35%	4.694%




Sum of corrected areas: 25483084

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
Data File : BG059561.D
Acq On : 31 Oct 2023 14:04
Operator : MA/JU
Sample : PB156470BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK470

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

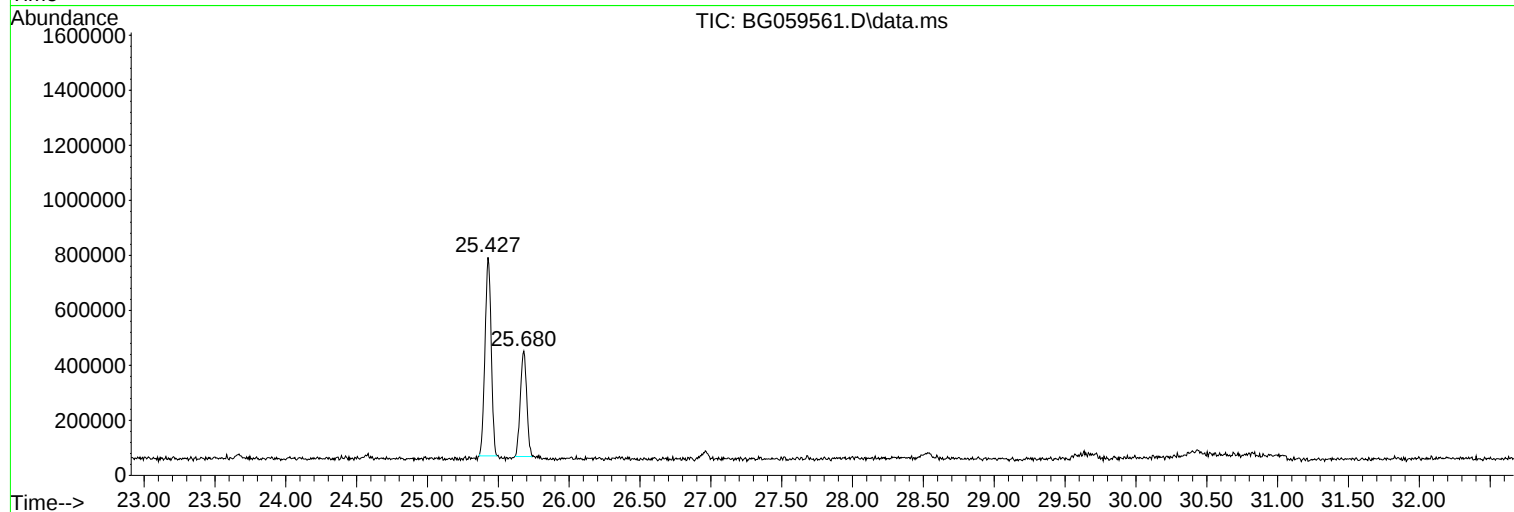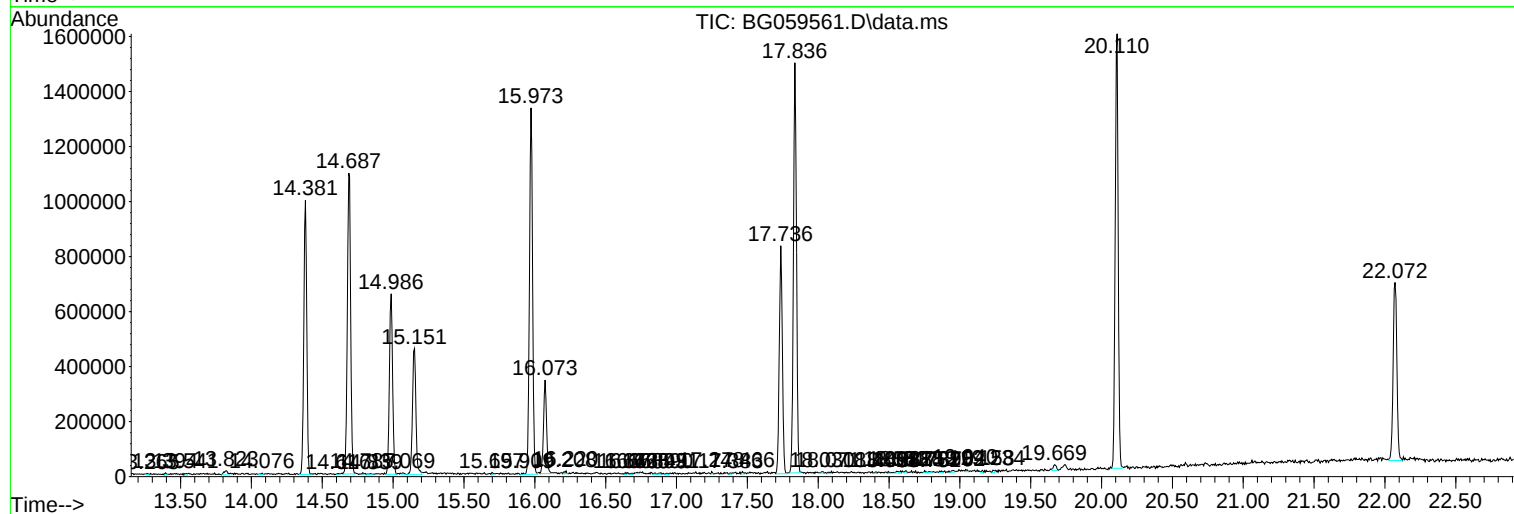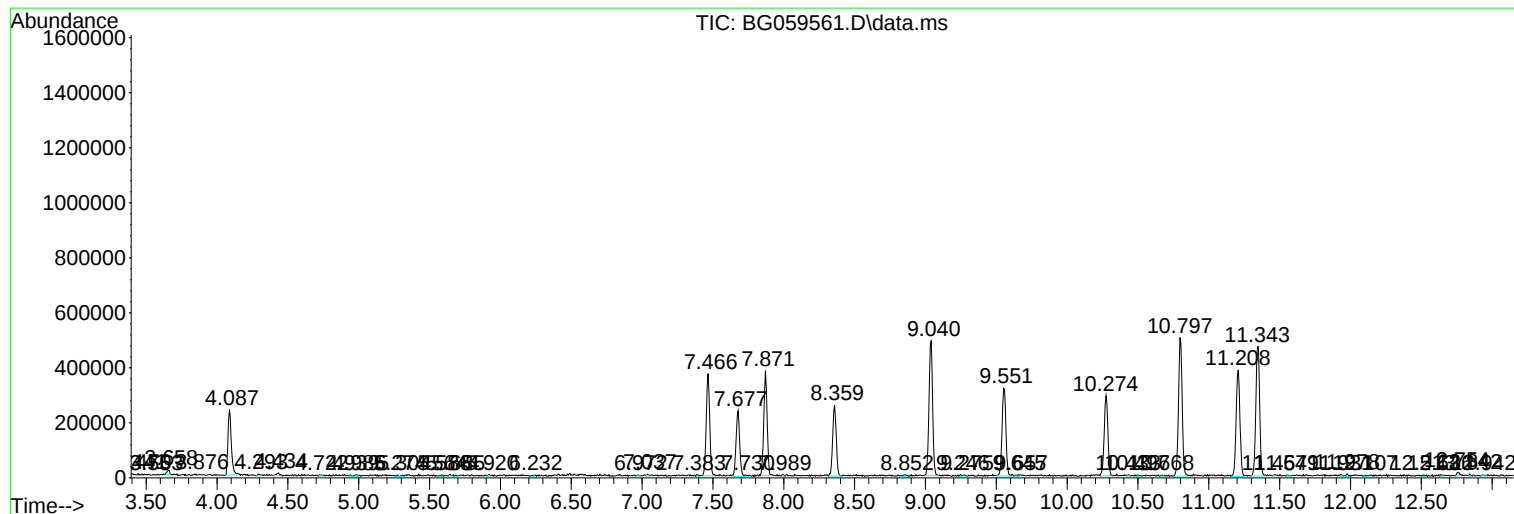

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
Data File : BG059561.D
Acq On : 31 Oct 2023 14:04
Operator : MA/JU
Sample : PB156470BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK470

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103123\
Data File : BG059561.D
Acq On : 31 Oct 2023 14:04
Operator : MA/JU
Sample : PB156470BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK470

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc