
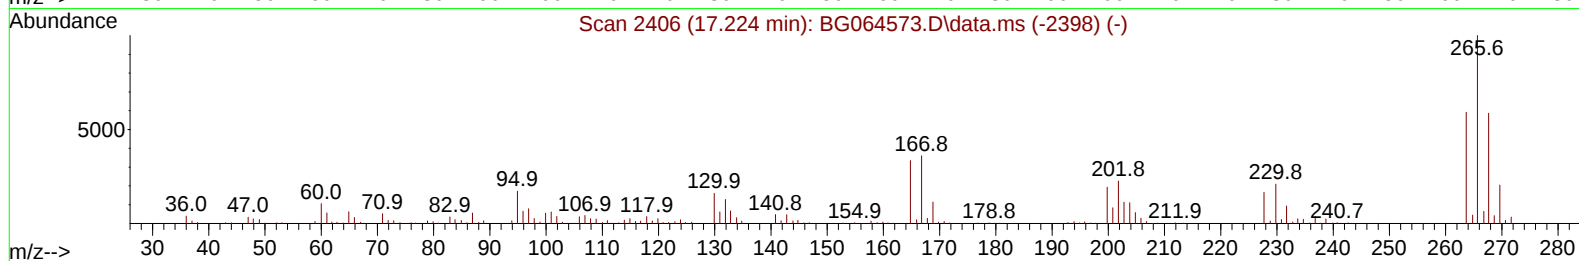
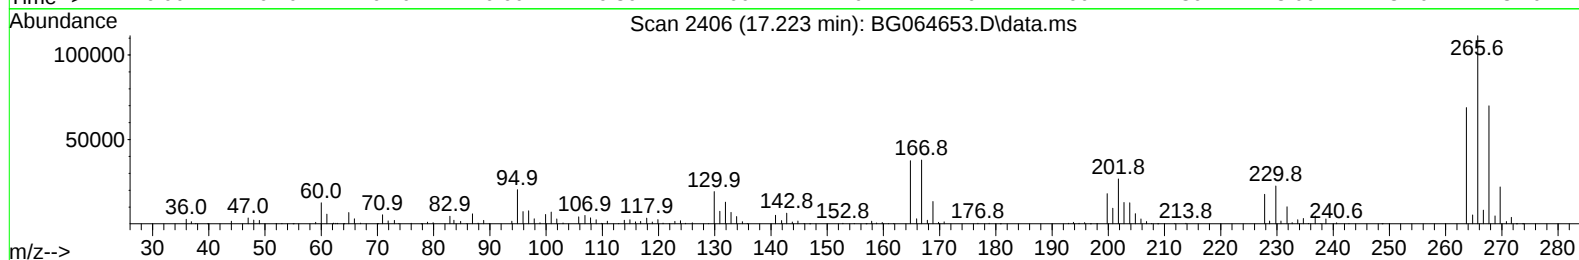


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103125\
Data File : BG064653.D
Acq On : 31 Oct 2025 12:42
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 31 13:23:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 16:40:26 2025
Response via : Initial Calibration

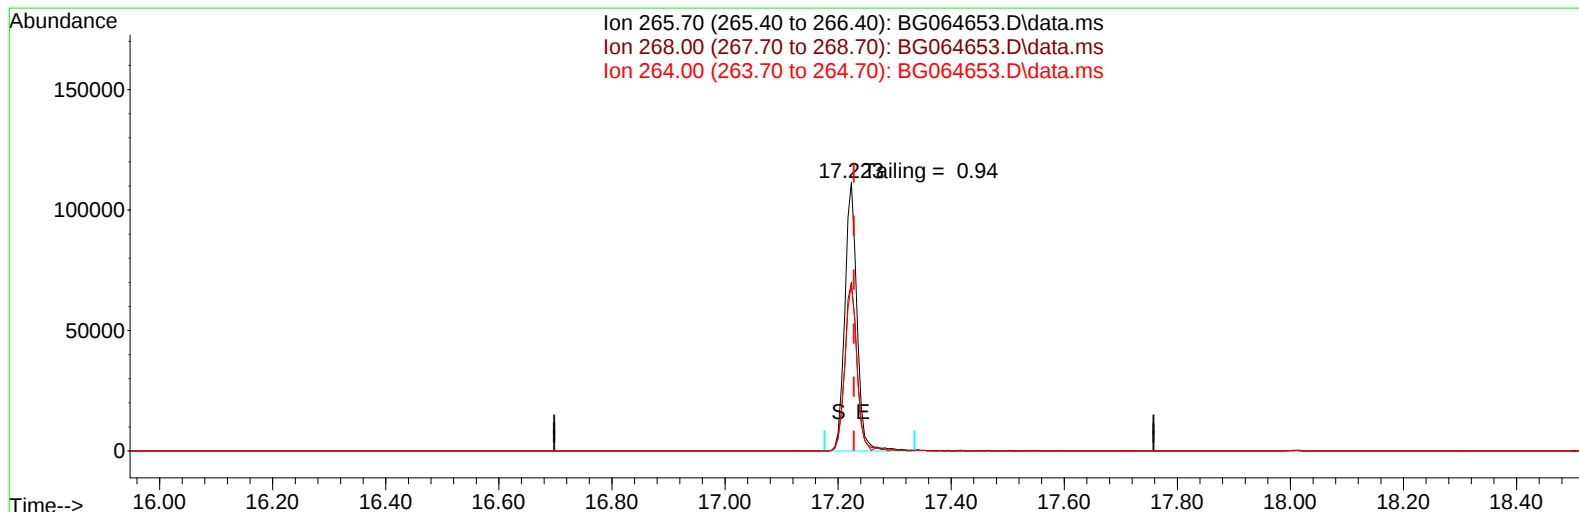

TIC: BG064653.D\data.ms

(70) Pentachlorophenol (C)




17.223min (-0.004) 30324.08 ng m

response 166681

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	62.76
264.00	59.10	61.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103125\
Data File : BG064653.D
Acq On : 31 Oct 2025 12:42
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 31 13:23:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 16:40:26 2025
Response via : Initial Calibration

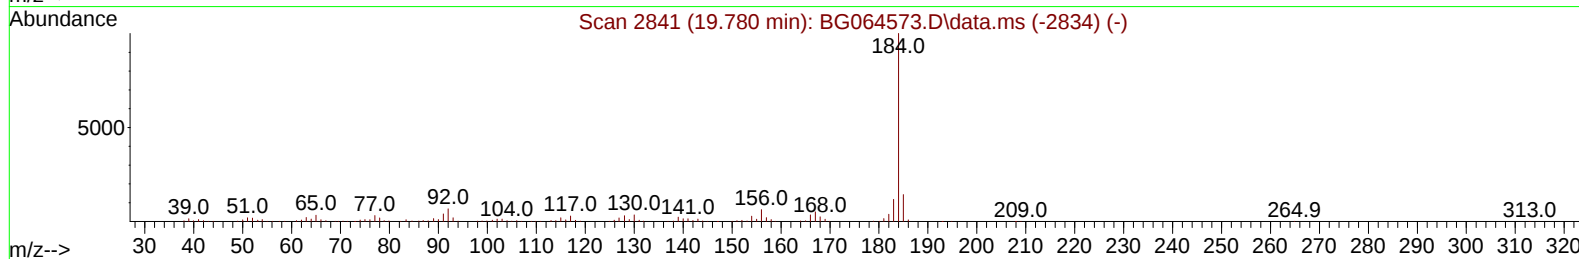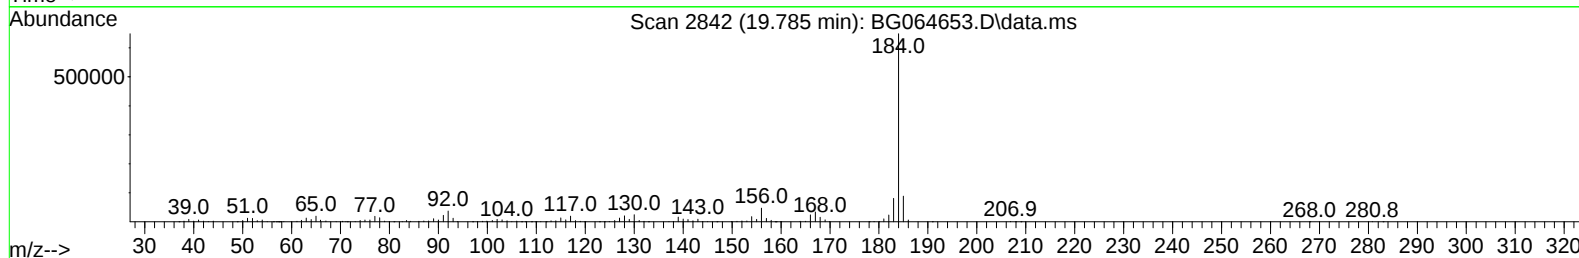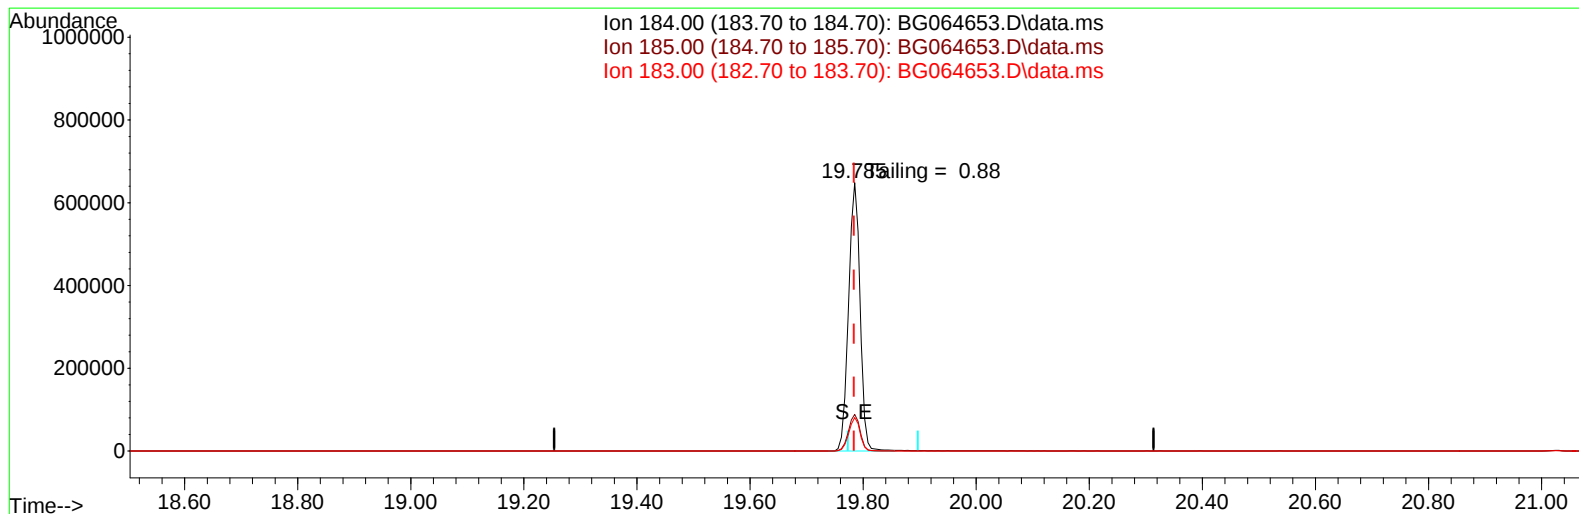

TIC: BG064653.D\data.ms

(77) Benzidine**19.785min (+ 0.002) 516456.63 ng****response 740529**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.67
183.00	11.80	12.49
0.00	0.00	0.00