

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103125\
 Data File : BG064667.D
 Acq On : 31 Oct 2025 22:22
 Operator : RC/JU
 Sample : Q3503-03 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 323

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG064667.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	14	19	29	rBV5	12034	33608	4.61%	0.625%
2	3.288	29	34	41	rVV	56571	90388	12.41%	1.680%
3	5.749	447	453	461	rBV	56171	86336	11.85%	1.605%
4	7.353	720	726	732	rBV	56581	98471	13.52%	1.831%
5	8.223	866	874	881	rBV	150957	258469	35.48%	4.805%
6	9.380	1065	1071	1077	rVB2	39420	66783	9.17%	1.242%
7	11.043	1345	1354	1362	rBV	209211	385462	52.92%	7.166%
8	12.447	1589	1593	1597	rBV6	5344	8811	1.21%	0.164%
9	12.776	1643	1649	1651	rBV6	6030	11696	1.61%	0.217%
10	12.935	1672	1676	1681	rBV5	10369	16152	2.22%	0.300%
11	13.076	1696	1700	1705	rVB7	6239	10529	1.45%	0.196%
12	13.241	1725	1728	1732	rVB5	9150	12879	1.77%	0.239%
13	13.388	1751	1753	1758	rVB5	13630	16411	2.25%	0.305%
14	13.470	1761	1767	1775	rBV	124531	200181	27.48%	3.722%
15	13.564	1778	1783	1787	rBV7	9471	16915	2.32%	0.314%
16	13.646	1787	1797	1798	rBV8	22768	44448	6.10%	0.826%
17	13.752	1811	1815	1817	rBV5	7487	12604	1.73%	0.234%
18	13.793	1817	1822	1826	rVB6	18560	28989	3.98%	0.539%
19	13.846	1828	1831	1834	rBV5	12116	16957	2.33%	0.315%
20	14.128	1873	1879	1883	rBV9	27960	60107	8.25%	1.117%
21	14.281	1900	1905	1909	rBV	71864	124609	17.11%	2.317%
22	14.604	1953	1960	1965	rBV9	43774	120820	16.59%	2.246%
23	14.686	1970	1974	1979	rVB3	95822	153381	21.06%	2.852%
24	14.733	1980	1982	1983	rBV2	20729	15593	2.14%	0.290%
25	14.839	1991	2000	2008	rBV	358695	712383	97.80%	13.244%
26	15.567	2121	2124	2129	rVB5	40421	56927	7.82%	1.058%
27	15.638	2133	2136	2140	rVV2	65601	88445	12.14%	1.644%
28	16.566	2291	2294	2300	rVB	119738	151844	20.85%	2.823%
29	17.389	2431	2434	2444	rVB	160065	274692	37.71%	5.107%
30	17.583	2462	2467	2473	rVB	372414	582711	80.00%	10.834%
31	20.168	2904	2907	2912	rVB	197495	244614	33.58%	4.548%
32	21.854	3189	3194	3203	rVB2	410064	728428	100.00%	13.543%
33	25.203	3756	3764	3773	rVB	225447	648068	88.97%	12.049%



Sum of corrected areas: 5378711

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103125\
Data File : BG064667.D
Acq On : 31 Oct 2025 22:22
Operator : RC/JU
Sample : Q3503-03 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
323

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

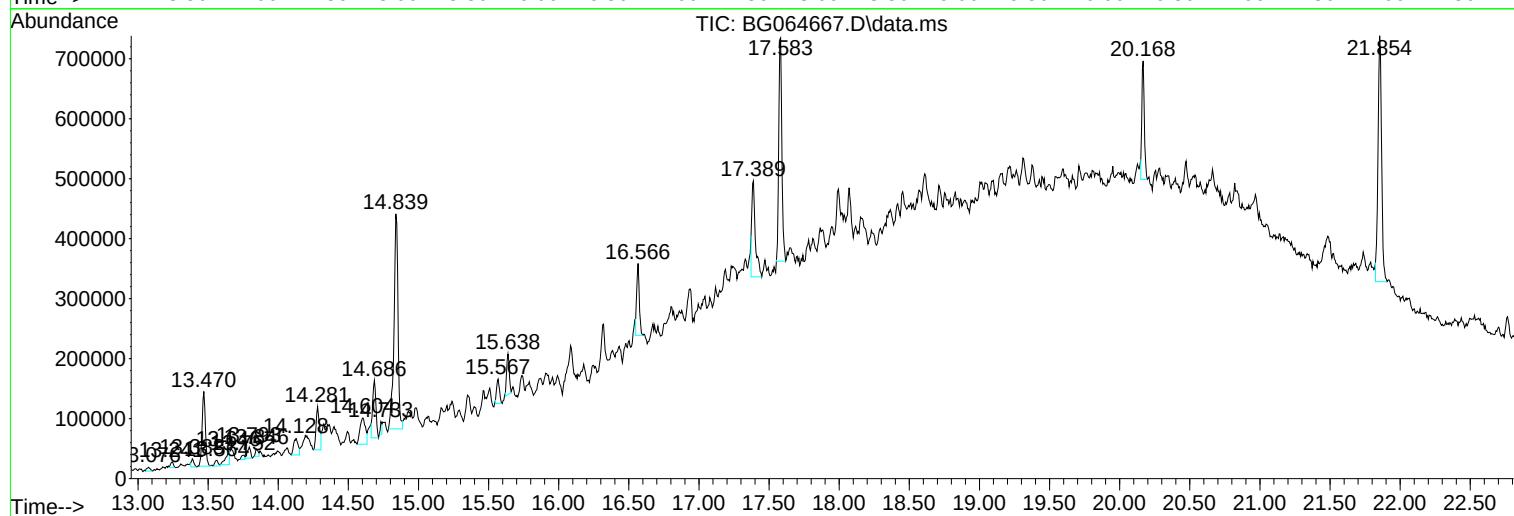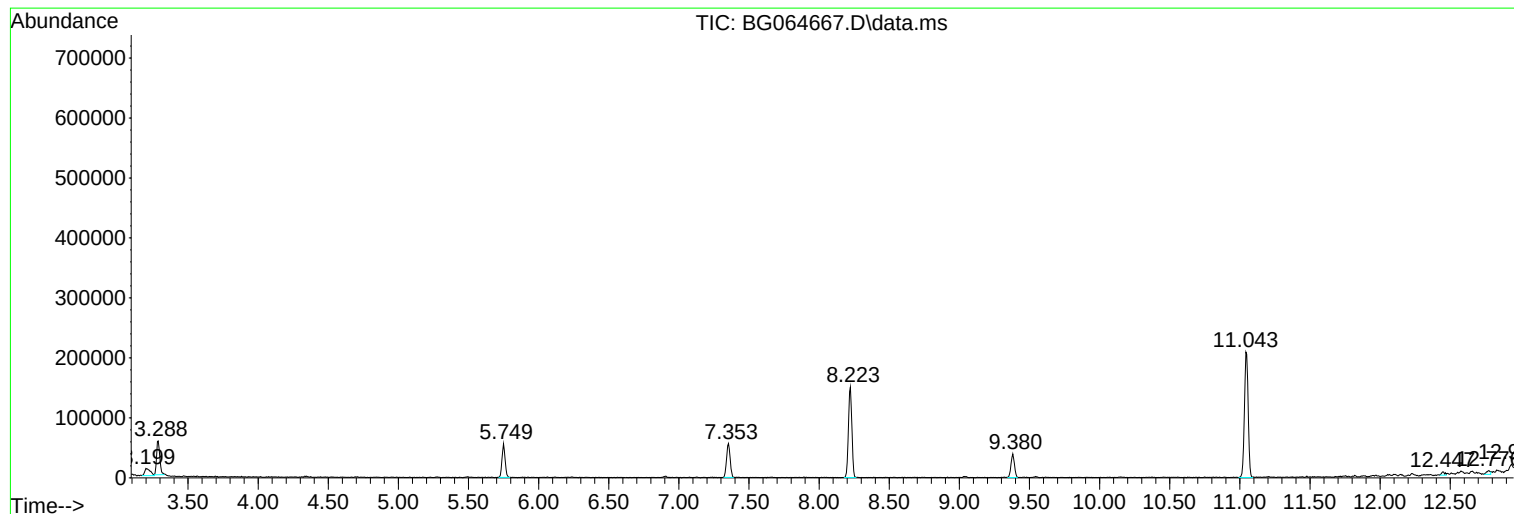

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103125\
Data File : BG064667.D
Acq On : 31 Oct 2025 22:22
Operator : RC/JU
Sample : Q3503-03 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
323

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103125\
Data File : BG064667.D
Acq On : 31 Oct 2025 22:22
Operator : RC/JU
Sample : Q3503-03 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
323

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------