
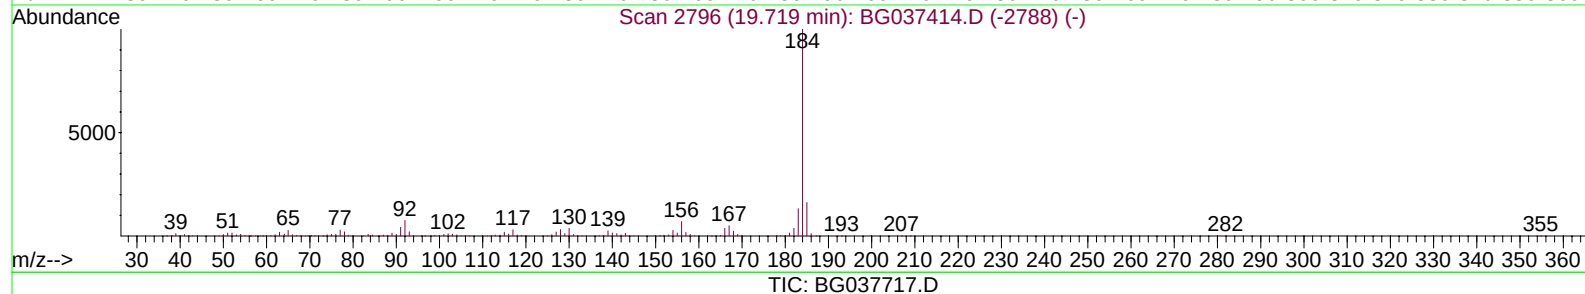
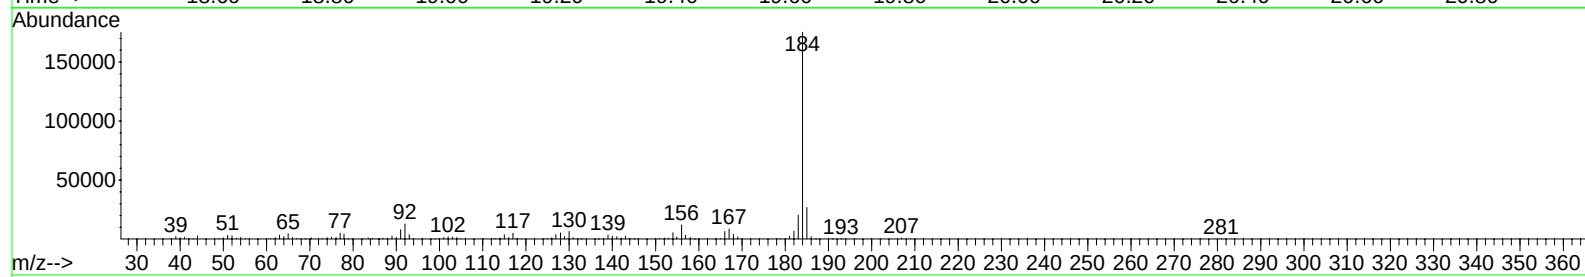


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110118\
Data File : BG037717.D
Acq On : 1 Nov 2018 13:55
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 10:10:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

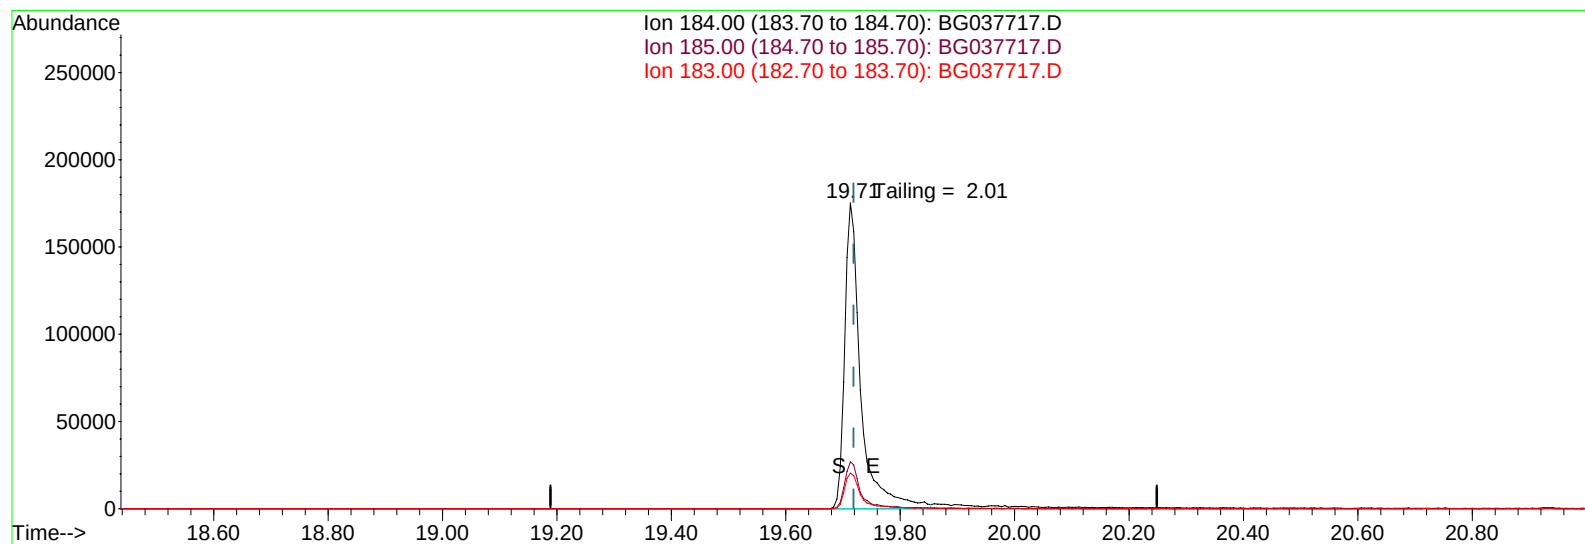

TIC: BG037717.D

(77) Benzidine




19.713min (-0.006) 142727.28ng

response 344570

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.35
183.00	12.70	11.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110118\
Data File : BG037717.D
Acq On : 1 Nov 2018 13:55
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 10:10:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

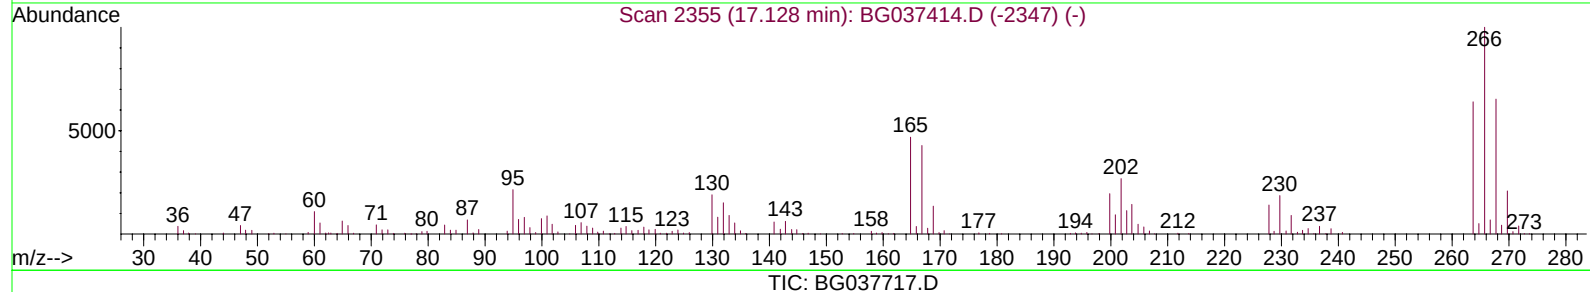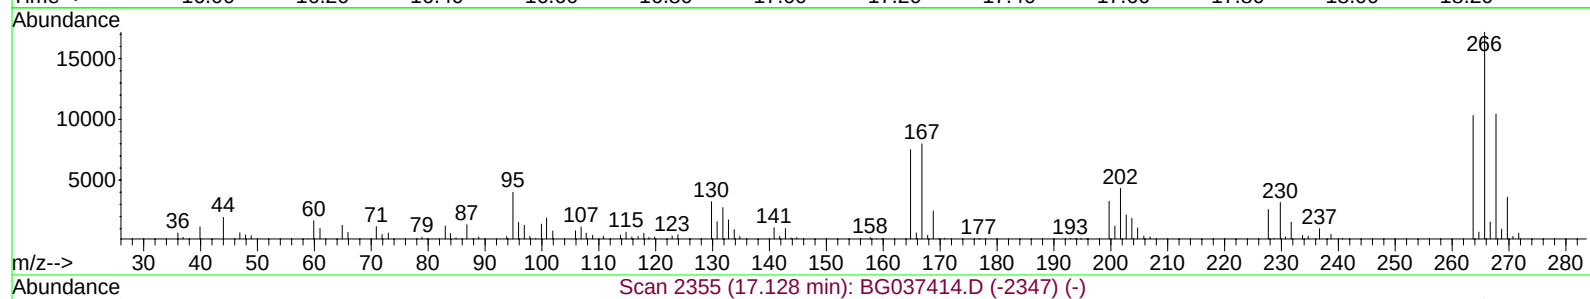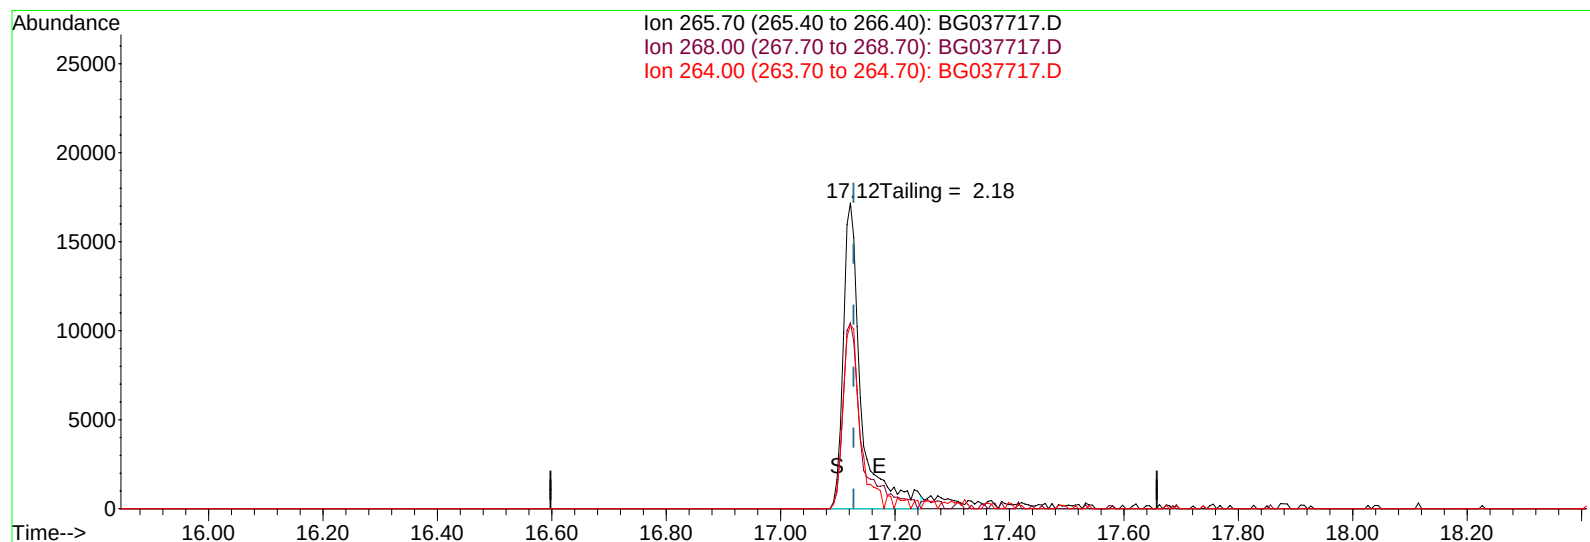

(70) Pentachlorophenol (C)

17.122min (-0.006) 31949.81ng

response 35562

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	66.39
264.00	73.60	64.29
0.00	0.00	0.00