
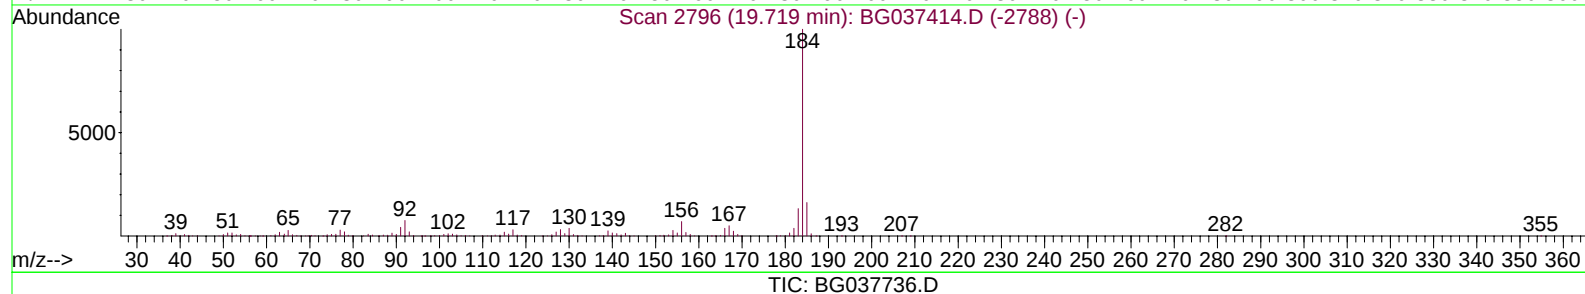
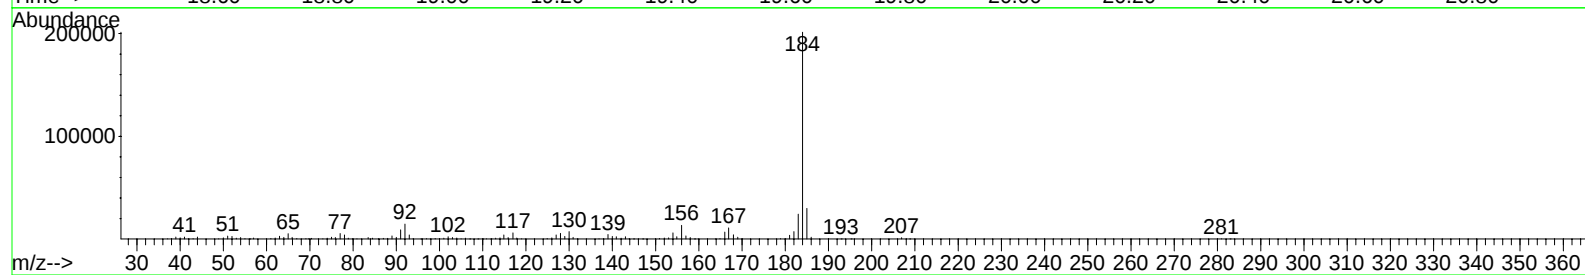


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110118\
Data File : BG037736.D
Acq On : 2 Nov 2018 2:20
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 10:14:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

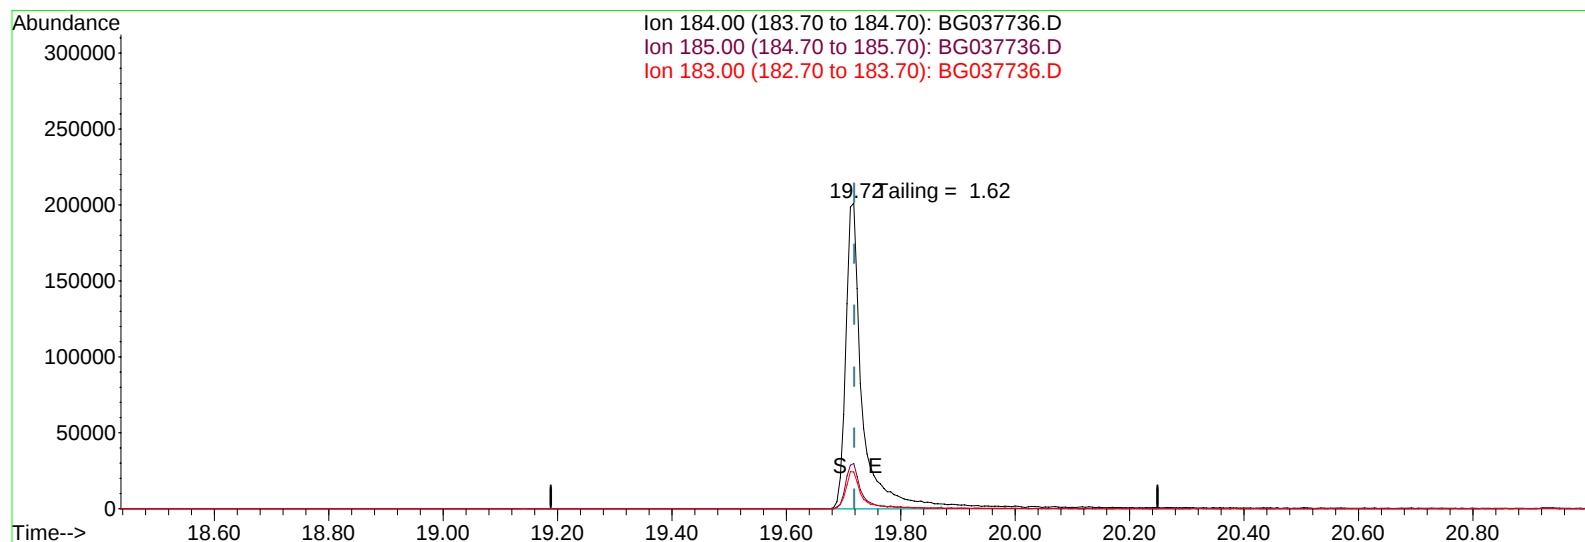

(77) Benzidine


19.718min (-0.001) 200948.96ng

response 416800

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.82
183.00	12.70	12.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110118\
Data File : BG037736.D
Acq On : 2 Nov 2018 2:20
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 10:14:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

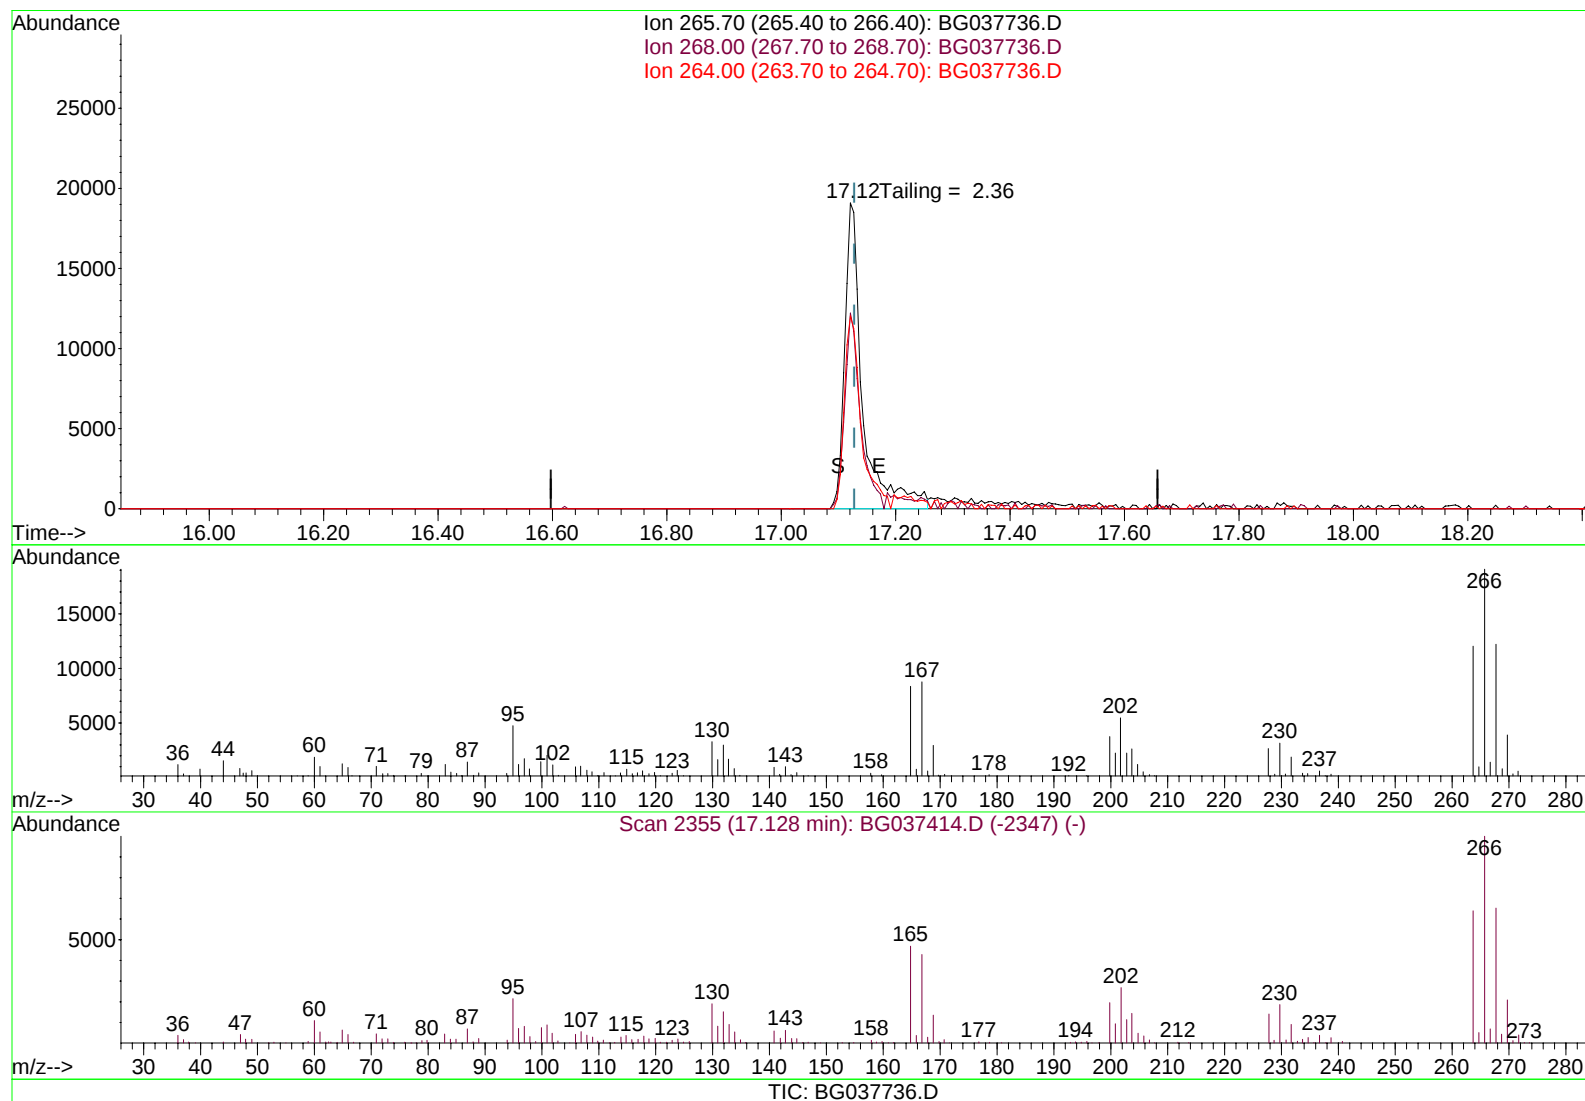

(70) Pentachlorophenol (C)

17.121min (-0.007) 14158.29ng

response 38534

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	63.99
264.00	73.60	68.24
0.00	0.00	0.00