


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG110118\
 Data File : BG037717.D
 Acq On : 1 Nov 2018 13:55
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 18 14:06:42 2018

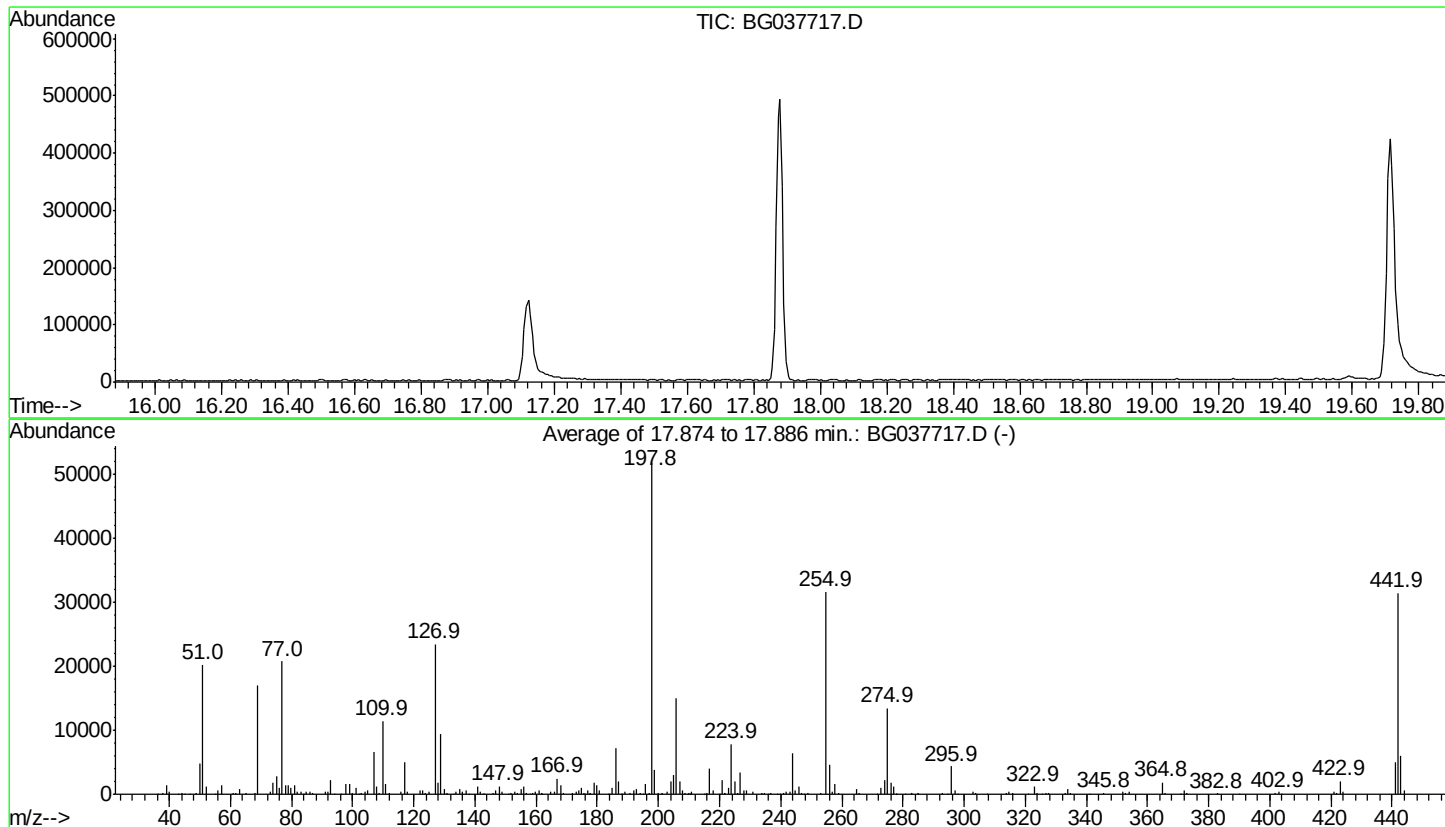

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	20238	PASS
68	69	0.00	2	1.1	191	PASS
69	198	0.00	100	33.0	17125	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.2	23456	PASS
197	198	0.00	2	0.4	214	PASS
198	198	100	100	100.0	51869	PASS
199	198	5	9	7.3	3803	PASS
275	198	10	60	26.0	13508	PASS
365	198	1	100	3.5	1816	PASS
441	198	0.01	100	9.7	5035	PASS
442	198	50	100	60.7	31480	PASS
443	442	15	24	19.1	6017	PASS