
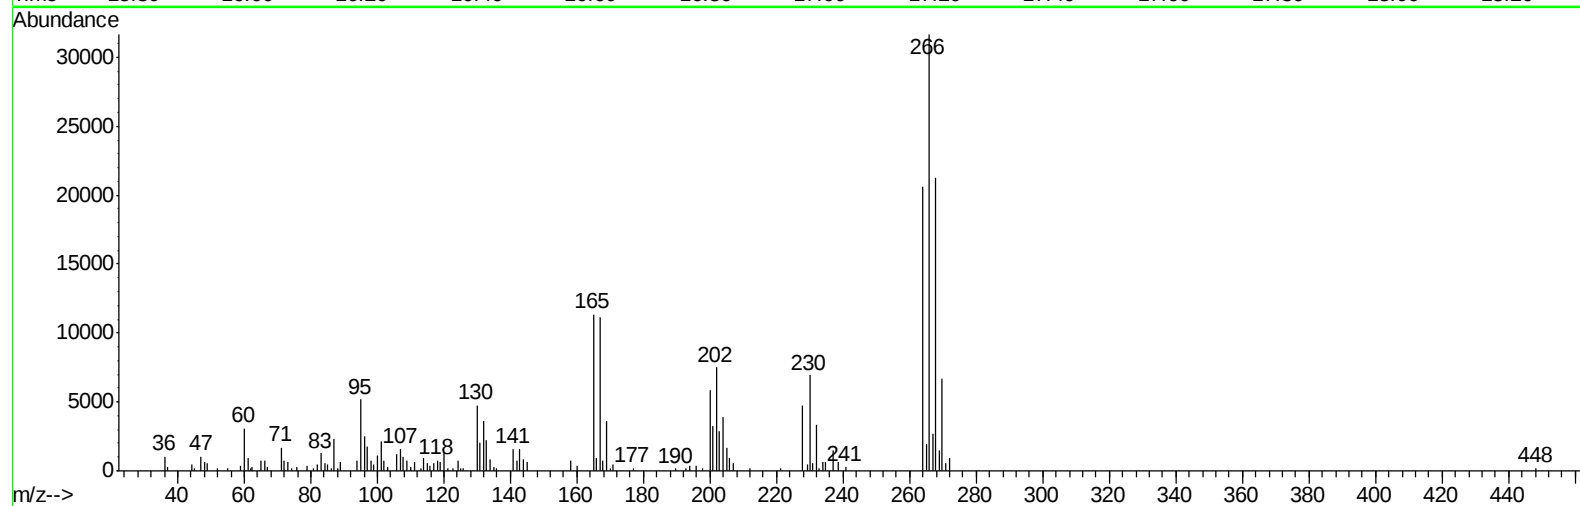


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110119\
Data File : BG043460.D
Acq On : 1 Nov 2019 11:32
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 05:42:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 16:37:43 2019
Response via : Initial Calibration

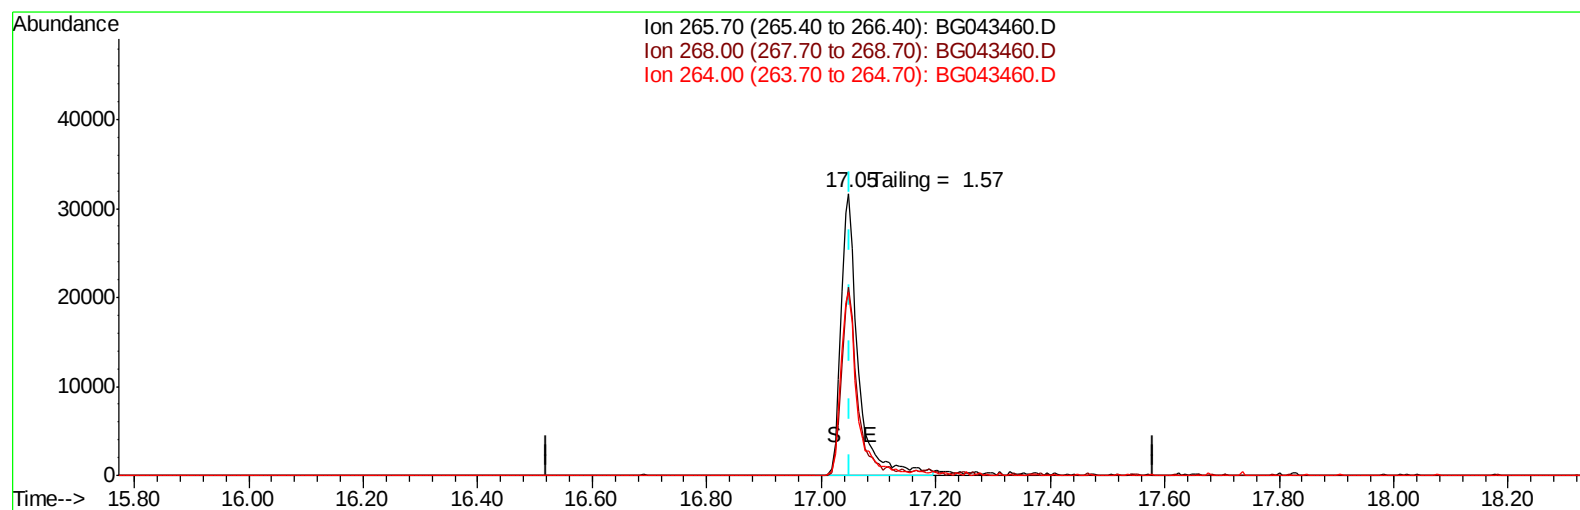

TIC: BG043460.D

(70) Pentachlorophenol (C)



17.048min (-0.002) 146336.80ng

response 64894

Ion	Exp%	Act%
265.70	100	100
268.00	58.90	67.05
264.00	63.00	65.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110119\
 Data File : BG043460.D
 Acq On : 1 Nov 2019 11:32
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 05:42:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 21 16:37:43 2019
 Response via : Initial Calibration

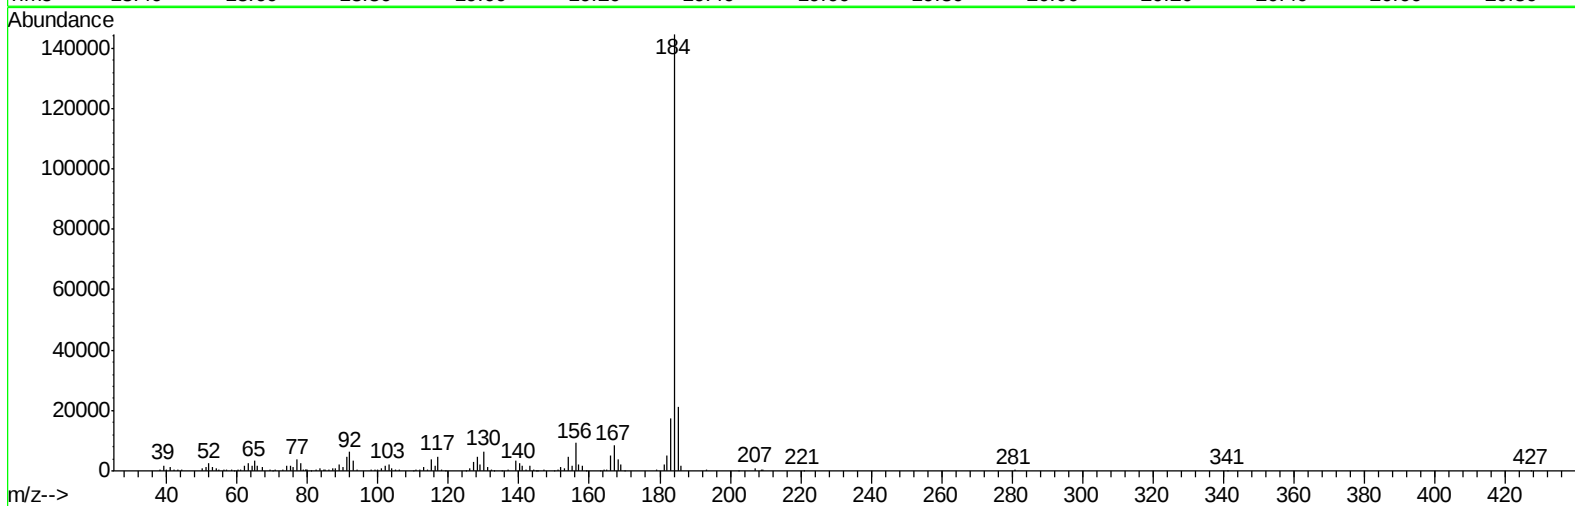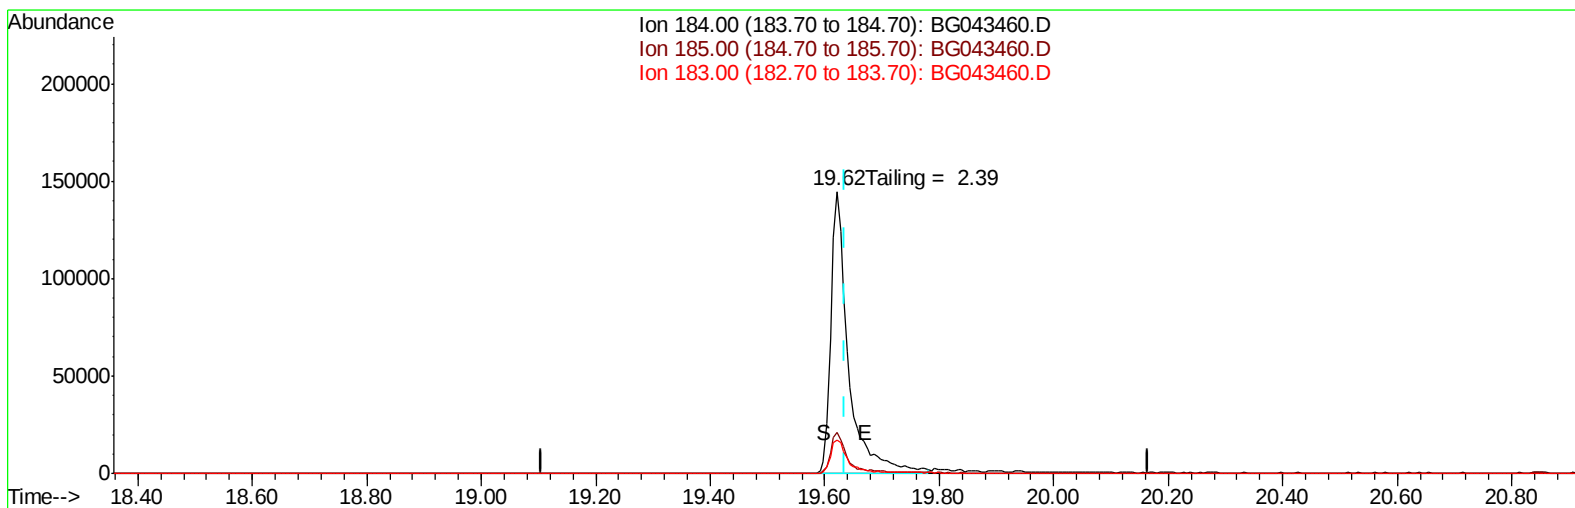

TIC: BG043460.D

(77) Benzidine

19.621min (-0.014) 0.00ng

response 307110

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.71
183.00	13.30	12.05
0.00	0.00	0.00