


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110119\
 Data File : BG043460.D
 Acq On : 1 Nov 2019 11:32
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 21 16:37:43 2019

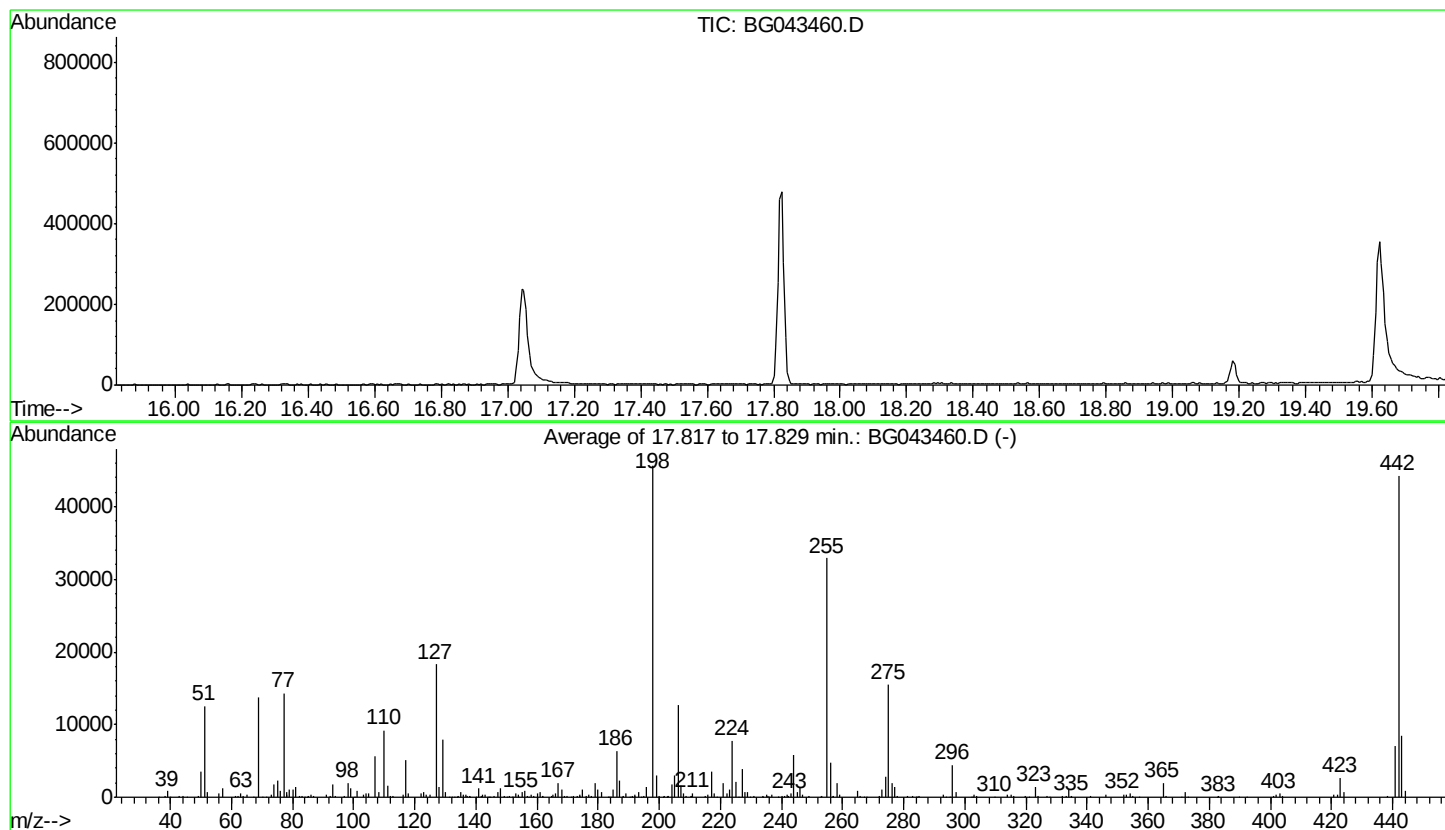

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.6	12579	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.1	13728	PASS
70	69	0.00	2	0.4	61	PASS
127	198	10	80	40.0	18274	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45640	PASS
199	198	5	9	6.8	3083	PASS
275	198	10	60	33.8	15445	PASS
365	198	1	100	4.4	2014	PASS
441	198	0.01	100	15.4	7024	PASS
442	198	50	100	96.9	44245	PASS
443	442	15	24	19.1	8451	PASS