

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110123\
 Data File : BG059574.D
 Acq On : 1 Nov 2023 11:16
 Operator : MA/JU
 Sample : PB156564BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK564

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059574.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.659	40	46	51	rBV	26081	40280	1.53%	0.134%
2	3.911	85	89	92	rBV2	6531	7179	0.27%	0.024%
3	3.941	92	94	98	rVB4	6202	9242	0.35%	0.031%
4	4.094	115	120	133	rBV	289748	536297	20.36%	1.780%
5	4.428	175	177	181	rVB	7733	9504	0.36%	0.032%
6	4.570	198	201	204	rBV	6683	6010	0.23%	0.020%
7	5.727	395	398	399	rBV	6215	6440	0.24%	0.021%
8	5.774	401	406	408	rVV	6556	10016	0.38%	0.033%
9	6.103	460	462	468	rVB	6059	9173	0.35%	0.030%
10	6.332	497	501	504	rBV2	4003	5845	0.22%	0.019%
11	7.108	627	633	636	rVB2	6223	7812	0.30%	0.026%
12	7.237	649	655	657	rBV4	5834	9986	0.38%	0.033%
13	7.266	657	660	662	rVB4	5570	5647	0.21%	0.019%
14	7.466	687	694	703	rBV	416991	735520	27.93%	2.441%
15	7.678	721	730	738	rVB	306452	516097	19.60%	1.713%
16	7.872	756	763	771	rVB	434171	775877	29.46%	2.575%
17	8.201	817	819	824	rVB	5438	8438	0.32%	0.028%
18	8.236	824	825	828	rBV	5909	6227	0.24%	0.021%
19	8.359	839	846	854	rVB2	322894	569343	21.62%	1.889%
20	8.441	858	860	862	rBV2	7524	5874	0.22%	0.019%
21	8.935	940	944	949	rVB	4625	7924	0.30%	0.026%
22	8.988	949	953	954	rBV2	7879	8832	0.34%	0.029%
23	9.041	954	962	971	rBV2	583447	1047594	39.78%	3.476%
24	9.252	994	998	1001	rVB	4842	6179	0.23%	0.021%
25	9.287	1001	1004	1006	rBV	4942	5756	0.22%	0.019%
26	9.423	1026	1027	1030	rBV	7463	7821	0.30%	0.026%
27	9.558	1042	1050	1058	rBV	416038	732863	27.83%	2.432%
28	9.904	1108	1109	1115	rVB	4476	6114	0.23%	0.020%
29	10.010	1125	1127	1130	rBV	5264	6716	0.26%	0.022%
30	10.275	1165	1172	1182	rVB	371940	676562	25.69%	2.245%
31	10.445	1197	1201	1204	rBV	5309	6522	0.25%	0.022%
32	10.797	1254	1261	1271	rVB	575101	1049698	39.86%	3.483%
33	11.209	1323	1331	1338	rVB	460688	849985	32.28%	2.821%
34	11.344	1345	1354	1364	rBV	585148	1107262	42.05%	3.674%
35	11.896	1444	1448	1451	rVB2	3567	6027	0.23%	0.020%
36	12.137	1487	1489	1496	rVB	4486	7993	0.30%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110123\
 Data File : BG059574.D
 Acq On : 1 Nov 2023 11:16
 Operator : MA/JU
 Sample : PB156564BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK564

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

37	12.760	1592	1595	1596	rBV2	10110	11523	0.44%	0.038%
38	12.836	1605	1608	1611	rBV2	5381	7398	0.28%	0.025%
39	12.889	1614	1617	1618	rBV2	6070	6351	0.24%	0.021%
40	12.971	1627	1631	1632	rBV	5912	6843	0.26%	0.023%

41	13.060	1645	1646	1650	rBV	4546	5651	0.21%	0.019%
42	13.095	1650	1652	1654	rBV2	4703	5452	0.21%	0.018%
43	13.436	1708	1710	1712	rBV	6662	5613	0.21%	0.019%
44	13.741	1760	1762	1765	rBV	4859	6112	0.23%	0.020%
45	13.817	1773	1775	1779	rBV3	12996	16599	0.63%	0.055%

46	13.959	1796	1799	1804	rVB2	5305	8488	0.32%	0.028%
47	14.082	1818	1820	1825	rVB	6649	8289	0.31%	0.028%
48	14.382	1864	1871	1877	rBV	1136150	1654603	62.83%	5.491%
49	14.434	1877	1880	1882	rVB	6753	6850	0.26%	0.023%
50	14.687	1916	1923	1931	rBV	1297019	2058998	78.19%	6.833%

51	14.987	1968	1974	1982	rVB	756394	1197371	45.47%	3.973%
52	15.075	1986	1989	1992	rVB	5352	7131	0.27%	0.024%
53	15.151	1992	2002	2019	rBV	566038	921340	34.99%	3.057%
54	15.527	2064	2066	2069	rVB2	6219	7219	0.27%	0.024%
55	15.580	2072	2075	2076	rVV	6043	6613	0.25%	0.022%

56	15.715	2096	2098	2101	rVB	5169	6207	0.24%	0.021%
57	15.974	2134	2142	2149	rBV	1594785	2356312	89.48%	7.819%
58	16.074	2153	2159	2165	rBV	414457	605087	22.98%	2.008%
59	16.215	2177	2183	2186	rBV3	10554	15850	0.60%	0.053%
60	16.244	2186	2188	2191	rVB	5117	5726	0.22%	0.019%

61	16.597	2246	2248	2249	rBV2	7294	6065	0.23%	0.020%
62	16.796	2281	2282	2287	rVB3	6304	6680	0.25%	0.022%
63	16.849	2289	2291	2295	rVV2	5963	5490	0.21%	0.018%
64	16.996	2311	2316	2319	rBV2	4959	8348	0.32%	0.028%
65	17.037	2319	2323	2325	rVV3	5478	6316	0.24%	0.021%

66	17.261	2357	2361	2363	rBV3	5090	5504	0.21%	0.018%
67	17.402	2383	2385	2389	rVB3	5779	7038	0.27%	0.023%
68	17.501	2398	2402	2403	rBV3	4802	6067	0.23%	0.020%
69	17.736	2435	2442	2452	rBV	918038	1394827	52.97%	4.629%
70	17.836	2452	2459	2466	rBV2	1684766	2544815	96.63%	8.445%

71	17.954	2477	2479	2483	rBV4	4726	8374	0.32%	0.028%
72	18.177	2514	2517	2519	rVB3	6660	5539	0.21%	0.018%
73	18.389	2549	2553	2555	rVB	6815	10159	0.39%	0.034%
74	18.424	2555	2559	2560	rBV2	6247	7007	0.27%	0.023%
75	18.441	2560	2562	2566	rVV4	4730	8328	0.32%	0.028%

76	19.070	2667	2669	2672	rBV3	8758	9701	0.37%	0.032%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110123\
 Data File : BG059574.D
 Acq On : 1 Nov 2023 11:16
 Operator : MA/JU
 Sample : PB156564BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK564

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

77	19.105	2672	2675	2676	rBV2	8761	7937	0.30%	0.026%
78	19.252	2698	2700	2704	rBV4	5873	6959	0.26%	0.023%
79	19.417	2725	2728	2729	rBV3	6820	5553	0.21%	0.018%
80	19.640	2764	2766	2767	rBV2	9690	9257	0.35%	0.031%
81	19.669	2767	2771	2775	rVV6	24286	41374	1.57%	0.137%
82	19.734	2780	2782	2787	rVV3	24432	35562	1.35%	0.118%
83	19.816	2794	2796	2798	rBV2	8299	9708	0.37%	0.032%
84	19.963	2818	2821	2824	rBV4	16111	22212	0.84%	0.074%
85	19.993	2824	2826	2828	rVB2	9211	6026	0.23%	0.020%
86	20.110	2838	2846	2852	rBV	1793756	2633477	100.00%	8.739%
87	20.280	2873	2875	2877	rVB4	14063	9689	0.37%	0.032%
88	21.385	3061	3063	3065	rBV3	17153	13152	0.50%	0.044%
89	21.773	3127	3129	3131	rBV3	14935	13989	0.53%	0.046%
90	22.073	3173	3180	3186	rBV2	753153	1301585	49.42%	4.319%
91	23.389	3402	3404	3405	rVB2	13654	6262	0.24%	0.021%
92	23.588	3436	3438	3447	rVB7	38904	68076	2.59%	0.226%
93	24.722	3625	3631	3639	rVB10	51593	132189	5.02%	0.439%
94	25.433	3741	3752	3763	rVB2	829326	2525744	95.91%	8.382%
95	25.680	3784	3794	3806	rVB2	423247	1431645	54.36%	4.751%
96	28.453	4264	4266	4267	rBV2	17975	10520	0.40%	0.035%
97	28.906	4342	4343	4347	rBV4	18888	15591	0.59%	0.052%
98	29.687	4474	4476	4478	rVB3	16016	9776	0.37%	0.032%
99	31.973	4863	4865	4867	rBV2	15459	15324	0.58%	0.051%
100	32.360	4929	4931	4932	rBV2	14245	9877	0.38%	0.033%




Sum of corrected areas: 30134023

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110123\
Data File : BG059574.D
Acq On : 1 Nov 2023 11:16
Operator : MA/JU
Sample : PB156564BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK564

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

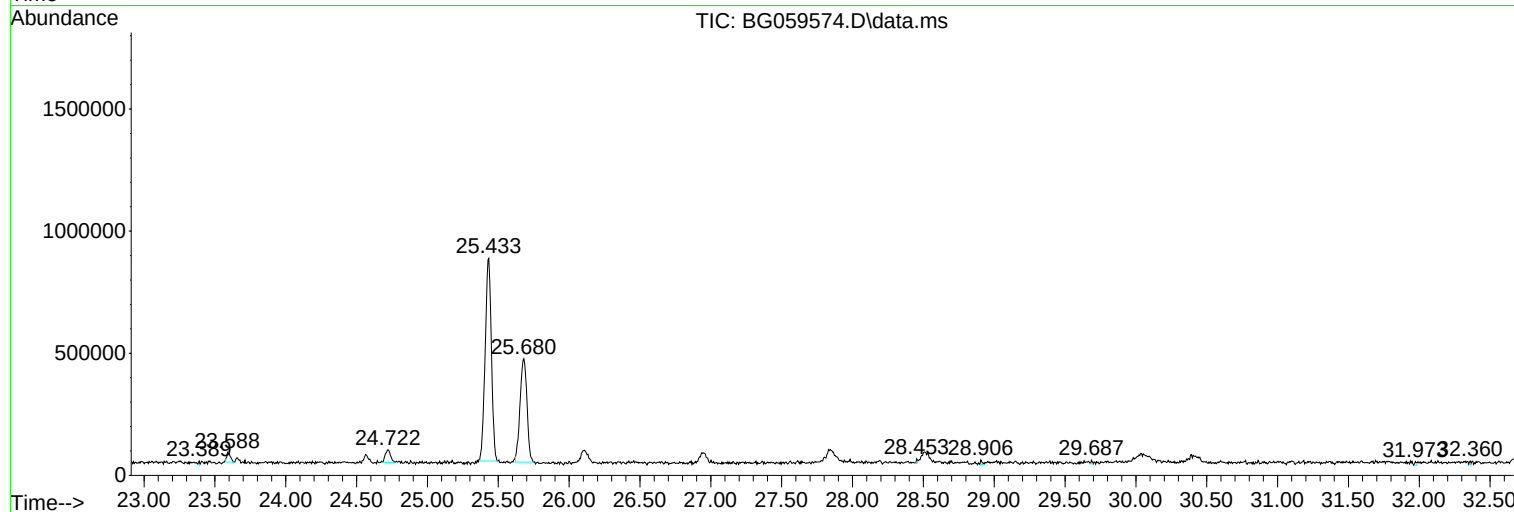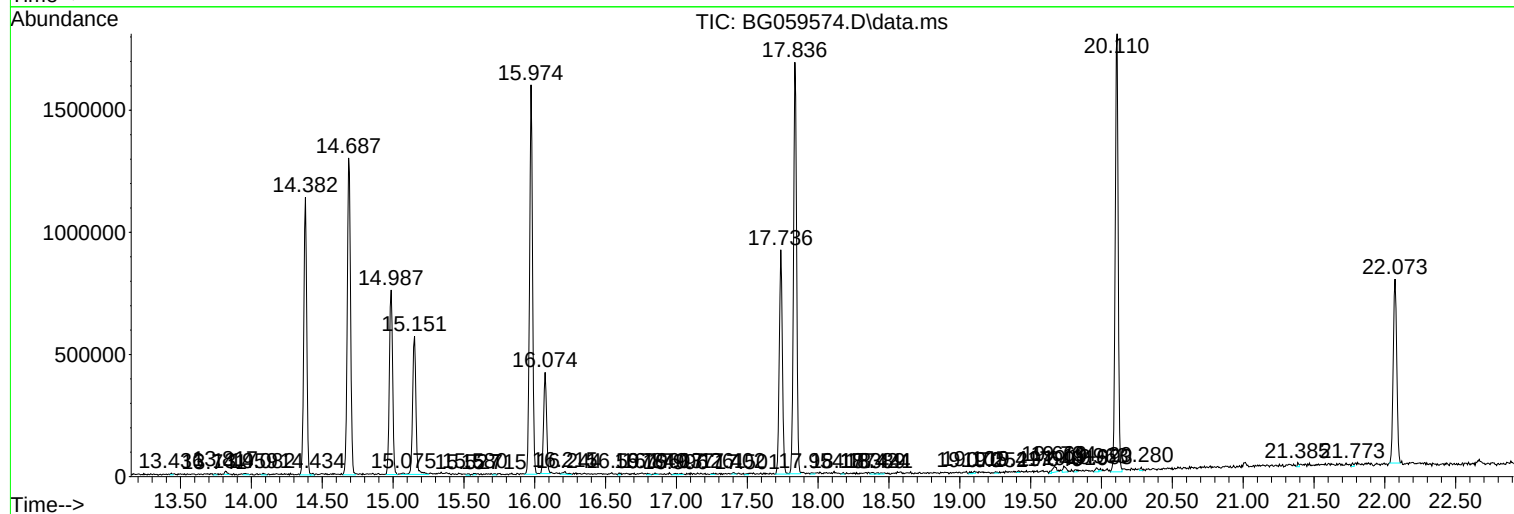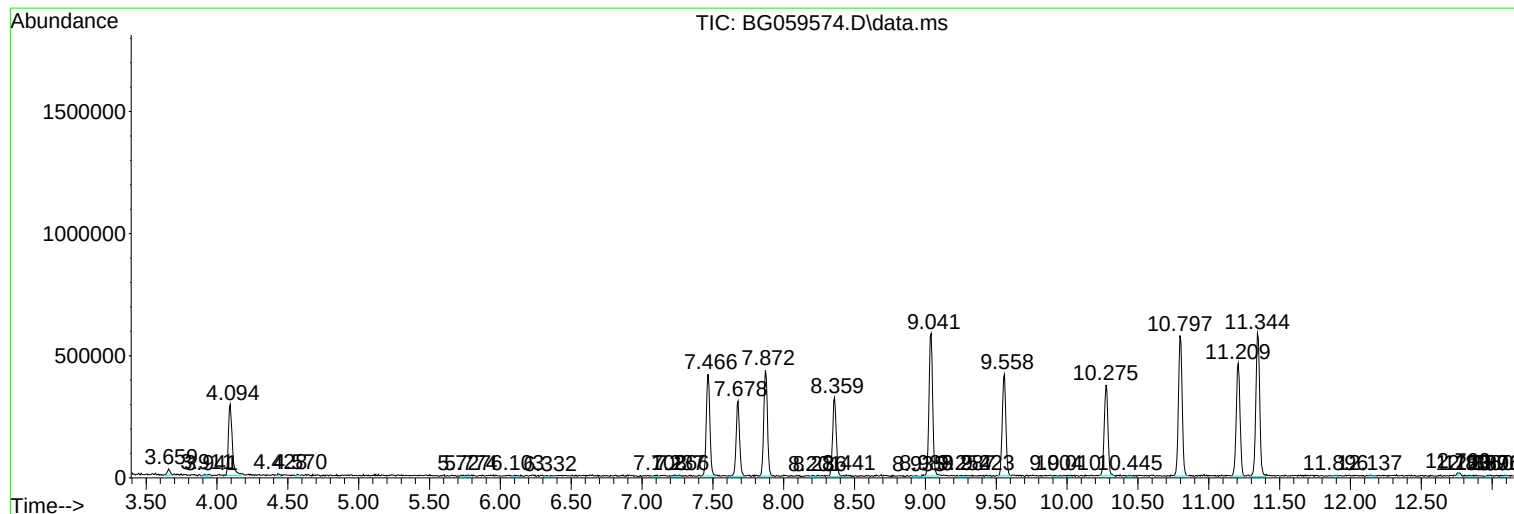

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110123\
Data File : BG059574.D
Acq On : 1 Nov 2023 11:16
Operator : MA/JU
Sample : PB156564BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK564

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110123\
Data File : BG059574.D
Acq On : 1 Nov 2023 11:16
Operator : MA/JU
Sample : PB156564BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK564

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc