

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110123\
 Data File : BG059584.D
 Acq On : 1 Nov 2023 19:24
 Operator : MA/JU
 Sample : PB156511BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK511

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059584.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.629	37	41	42	rBV4	5255	6098	0.19%	0.019%
2	3.653	42	45	49	rVB4	18057	23737	0.74%	0.074%
3	3.794	67	69	72	rVB2	6870	6554	0.20%	0.020%
4	4.088	114	119	131	rVV	212863	374039	11.70%	1.163%
5	4.176	133	134	138	rVB4	8212	6432	0.20%	0.020%
6	4.405	170	173	174	rBV2	7915	6157	0.19%	0.019%
7	4.428	174	177	185	rVV3	14549	23947	0.75%	0.074%
8	4.511	189	191	194	rVB	7753	6385	0.20%	0.020%
9	4.552	194	198	200	rBV2	4582	7113	0.22%	0.022%
10	4.887	253	255	257	rBV	7184	6085	0.19%	0.019%
11	5.850	415	419	423	rBV4	5254	10153	0.32%	0.032%
12	5.933	429	433	438	rBV3	4768	9044	0.28%	0.028%
13	6.027	445	449	452	rBV2	4545	5793	0.18%	0.018%
14	6.520	531	533	538	rBV	6018	6231	0.19%	0.019%
15	6.679	557	560	561	rBV	6893	7064	0.22%	0.022%
16	6.691	561	562	566	rVV2	10171	14089	0.44%	0.044%
17	6.738	568	570	573	rVV2	8995	11308	0.35%	0.035%
18	6.779	575	577	580	rVB2	5343	6051	0.19%	0.019%
19	7.466	687	694	703	rBV2	376134	664944	20.80%	2.068%
20	7.672	723	729	739	rBV	255107	439759	13.75%	1.368%
21	7.871	755	763	772	rBV	387095	696226	21.77%	2.165%
22	7.971	777	780	784	rVB	6549	7959	0.25%	0.025%
23	8.359	840	846	853	rVB	286300	482556	15.09%	1.501%
24	8.565	878	881	883	rBV3	6150	9268	0.29%	0.029%
25	9.035	953	961	969	rBV	522151	922302	28.85%	2.869%
26	9.552	1041	1049	1057	rVV	339236	634107	19.83%	1.972%
27	10.116	1143	1145	1148	rBV2	5697	5644	0.18%	0.018%
28	10.275	1164	1172	1180	rBV	451330	805318	25.19%	2.505%
29	10.680	1239	1241	1244	rBV2	7602	7758	0.24%	0.024%
30	10.721	1246	1248	1250	rBV2	6588	5965	0.19%	0.019%
31	10.797	1252	1261	1268	rBV	714407	1302639	40.74%	4.051%
32	10.933	1281	1284	1287	rVB	7721	10475	0.33%	0.033%
33	10.962	1287	1289	1293	rBV	8168	9250	0.29%	0.029%
34	11.150	1320	1321	1323	rVB	9610	5637	0.18%	0.018%
35	11.203	1323	1330	1339	rBV	578260	1061323	33.19%	3.301%
36	11.344	1346	1354	1364	rBV	731921	1309691	40.96%	4.073%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110123\
 Data File : BG059584.D
 Acq On : 1 Nov 2023 19:24
 Operator : MA/JU
 Sample : PB156511BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK511

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

37	11.438	1368	1370	1373	rVB	6159	6306	0.20%	0.020%
38	11.508	1379	1382	1385	rBV2	5317	7430	0.23%	0.023%
39	11.649	1405	1406	1409	rVB2	9132	8032	0.25%	0.025%
40	11.679	1409	1411	1415	rBV	6781	10066	0.31%	0.031%

41	11.738	1419	1421	1422	rVB2	10523	6141	0.19%	0.019%
42	11.761	1424	1425	1427	rVV	10283	7029	0.22%	0.022%
43	11.779	1427	1428	1432	rVB2	10720	7636	0.24%	0.024%
44	11.908	1448	1450	1452	rVB	7385	5965	0.19%	0.019%
45	12.161	1491	1493	1497	rBV2	5716	6251	0.20%	0.019%

46	12.284	1512	1514	1516	rBV	11627	6829	0.21%	0.021%
47	12.319	1516	1520	1521	rVB	9968	10993	0.34%	0.034%
48	12.337	1521	1523	1526	rBV	8084	12119	0.38%	0.038%
49	12.396	1531	1533	1536	rVB4	7352	8498	0.27%	0.026%
50	12.537	1555	1557	1561	rVB	8935	7965	0.25%	0.025%

51	12.589	1564	1566	1568	rBV2	11363	11085	0.35%	0.034%
52	12.736	1589	1591	1592	rBV2	9881	7068	0.22%	0.022%
53	12.760	1592	1595	1599	rVV3	19859	27927	0.87%	0.087%
54	12.807	1602	1603	1607	rVB2	9973	6112	0.19%	0.019%
55	13.077	1647	1649	1651	rBV	7627	8015	0.25%	0.025%

56	13.406	1703	1705	1709	rBV3	9414	11790	0.37%	0.037%
57	13.477	1716	1717	1720	rVB	8400	5689	0.18%	0.018%
58	13.506	1720	1722	1725	rVB	6346	5881	0.18%	0.018%
59	13.641	1743	1745	1748	rBV2	6660	6754	0.21%	0.021%
60	13.812	1768	1774	1778	rBV5	15494	31007	0.97%	0.096%

61	13.859	1781	1782	1785	rVB3	8634	6063	0.19%	0.019%
62	14.070	1816	1818	1820	rVB3	6733	5651	0.18%	0.018%
63	14.099	1820	1823	1824	rBV	6774	6393	0.20%	0.020%
64	14.376	1864	1870	1876	rVB	1298602	1904499	59.56%	5.923%
65	14.687	1916	1923	1931	rBV	1481522	2358263	73.76%	7.335%

66	14.740	1931	1932	1936	rVB3	10019	7207	0.23%	0.022%
67	14.769	1936	1937	1940	rBV	6765	7776	0.24%	0.024%
68	14.822	1944	1946	1947	rBV	7452	5914	0.18%	0.018%
69	14.875	1953	1955	1958	rVB2	8057	5989	0.19%	0.019%
70	14.928	1961	1964	1966	rBV	5890	7864	0.25%	0.024%

71	14.987	1967	1974	1982	rVB	885094	1434628	44.87%	4.462%
72	15.045	1982	1984	1986	rBV2	6767	7737	0.24%	0.024%
73	15.151	1994	2002	2008	rBV	729061	1116752	34.93%	3.473%
74	15.674	2088	2091	2093	rVB	9833	9288	0.29%	0.029%
75	15.698	2093	2095	2099	rBV2	9525	11260	0.35%	0.035%

76	15.768	2104	2107	2109	rVB	9201	11215	0.35%	0.035%
----	--------	------	------	------	-----	------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110123\
 Data File : BG059584.D
 Acq On : 1 Nov 2023 19:24
 Operator : MA/JU
 Sample : PB156511BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK511

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

77	15.974	2135	2142	2150	rVB	1826482	2806098	87.76%	8.728%
78	16.074	2152	2159	2165	rBV	458611	696223	21.77%	2.165%
79	16.373	2208	2210	2213	rBV3	6758	8082	0.25%	0.025%
80	16.444	2221	2222	2224	rBV2	8519	6722	0.21%	0.021%
81	16.503	2230	2232	2233	rBV2	7244	5901	0.18%	0.018%
82	16.544	2237	2239	2241	rBV3	9240	9696	0.30%	0.030%
83	16.626	2251	2253	2256	rVB2	9068	11190	0.35%	0.035%
84	16.655	2256	2258	2259	rBV2	10396	7391	0.23%	0.023%
85	16.708	2266	2267	2270	rBV3	10083	9231	0.29%	0.029%
86	16.749	2272	2274	2277	rVB3	10529	7508	0.23%	0.023%
87	16.896	2296	2299	2304	rBV4	6950	12216	0.38%	0.038%
88	17.090	2330	2332	2334	rVB	11424	9379	0.29%	0.029%
89	17.108	2334	2335	2336	rBV	12333	5810	0.18%	0.018%
90	17.196	2348	2350	2352	rBV3	9507	6922	0.22%	0.022%
91	17.313	2369	2370	2372	rBV2	8722	6262	0.20%	0.019%
92	17.736	2435	2442	2451	rVB	1159365	1777844	55.60%	5.529%
93	17.836	2451	2459	2468	rBV2	2078879	3197410	100.00%	9.945%
94	18.283	2534	2535	2538	rBV2	9279	6080	0.19%	0.019%
95	18.324	2540	2542	2545	rBV4	9463	8089	0.25%	0.025%
96	18.465	2564	2566	2567	rBV2	11504	7504	0.23%	0.023%
97	18.976	2651	2653	2655	rBV3	16159	9590	0.30%	0.030%
98	20.110	2840	2846	2852	rVB	2134040	3090329	96.65%	9.612%
99	22.072	3174	3180	3188	rVB2	864420	1552417	48.55%	4.828%
100	25.427	3742	3751	3767	rVB3	905754	2838067	88.76%	8.827%




Sum of corrected areas: 32152149

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110123\
Data File : BG059584.D
Acq On : 1 Nov 2023 19:24
Operator : MA/JU
Sample : PB156511BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK511

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

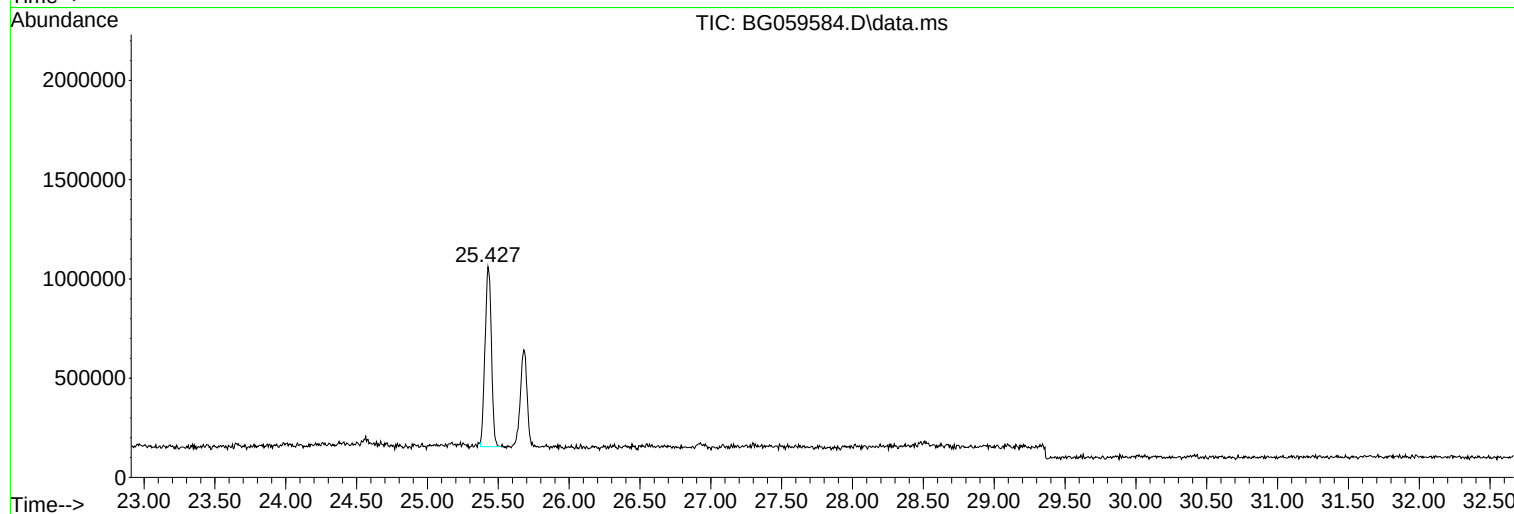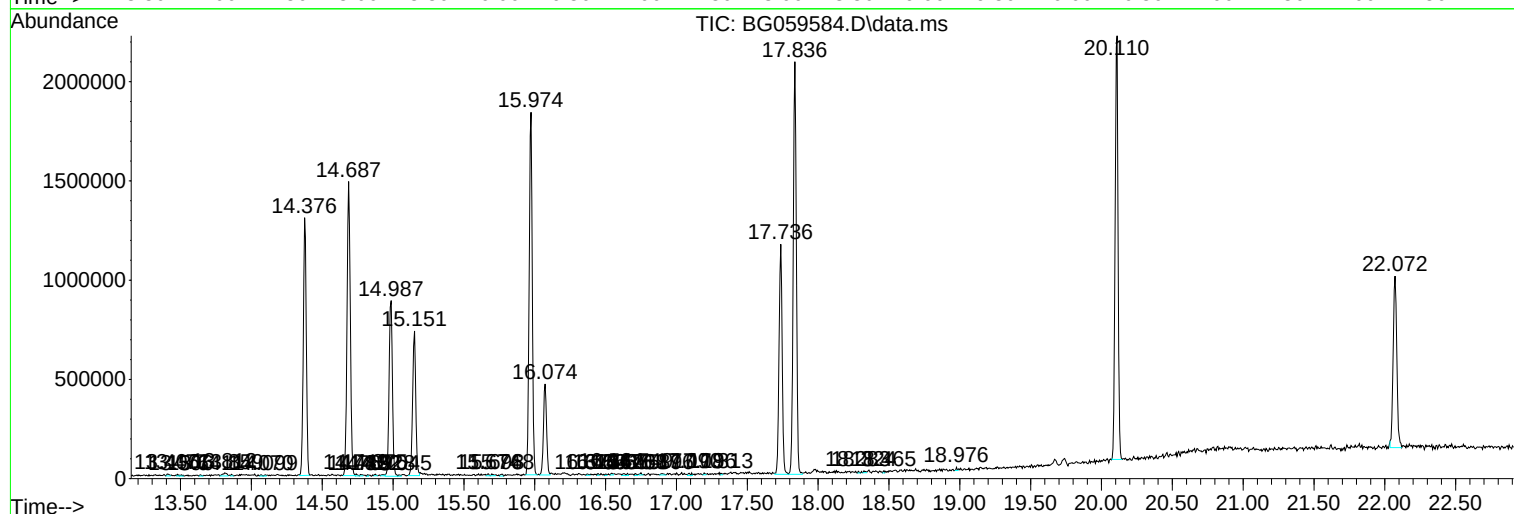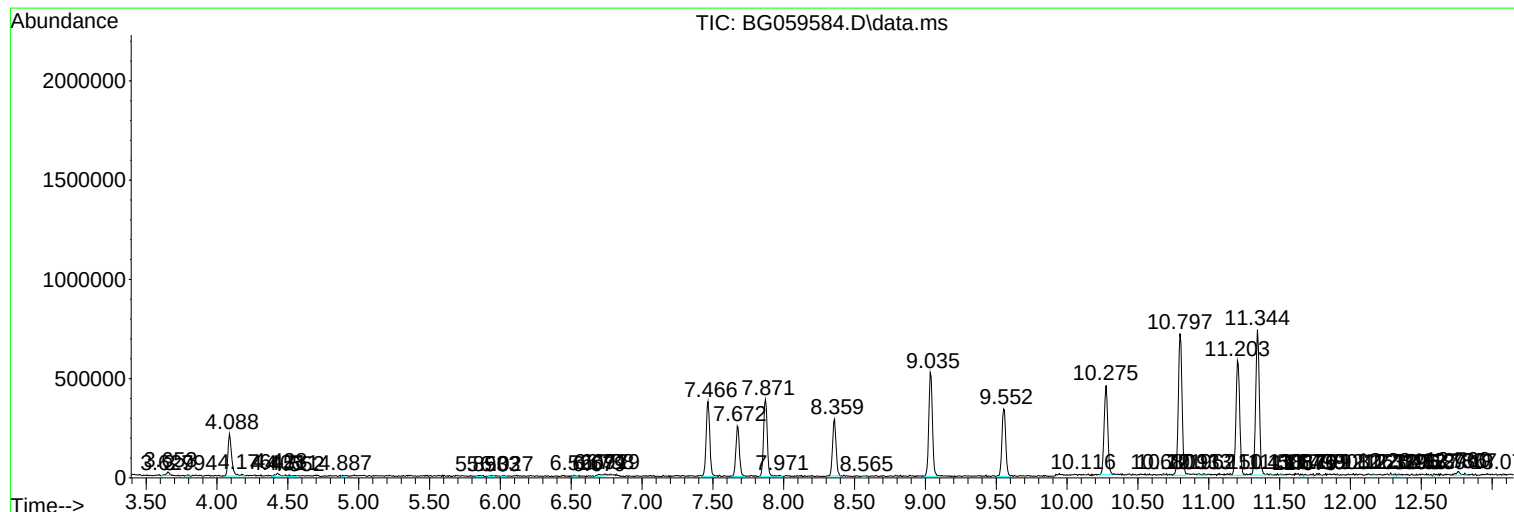

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110123\
Data File : BG059584.D
Acq On : 1 Nov 2023 19:24
Operator : MA/JU
Sample : PB156511BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK511

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110123\
Data File : BG059584.D
Acq On : 1 Nov 2023 19:24
Operator : MA/JU
Sample : PB156511BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK511

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------