

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG110218\
 Data File : BG037770.D
 Acq On : 3 Nov 2018 1:14
 Operator : JU/SJ
 Sample : J5803-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Nov 03 02:31:42 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 18 14:06:42 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	57020	20.00	ng	0.00
21) Naphthalene-d8	10.92	136	260871	20.00	ng	0.00
39) Acenaphthene-d10	14.74	164	172542	20.00	ng	0.00
64) Phenanthrene-d10	17.48	188	368992	20.00	ng	0.00
76) Chrysene-d12	21.76	240	332566	20.00	ng	-0.01
87) Perylene-d12	25.10	264	317994	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	515302	151.09	ng	0.00
7) Phenol-d6	7.25	99	778604	150.97	ng	0.00
23) Nitrobenzene-d5	9.28	82	465574	99.98	ng	0.00
42) 2,4,6-Tribromophenol	16.22	330	282308	150.01	ng	0.00
45) 2-Fluorobiphenyl	13.36	172	1025745	89.65	ng	-0.01
79) Terphenyl-d14	20.08	244	1268641	81.51	ng	0.00
Target Compounds						
10) Phenol	7.27	94	50309	9.246	ng	93
19) n-Nitroso-di-n-propylamine	9.28	70	59082	16.637	ng	# 73
50) Dimethylphthalate	14.18	163	161946	12.132	ng	99
57) 2,4-Dinitrotoluene	14.73	165	22595	5.829	ng	# 25
65) 4,6-Dinitro-2-methylphenol	16.22	198	932	8.904	ng	77
67) 4-Bromophenyl-phenylether	16.22	248	20733	5.117	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG110218\
Data File : BG037770.D
Acq On : 3 Nov 2018 1:14
Operator : JU/SJ
Sample : J5803-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Nov 03 02:31:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

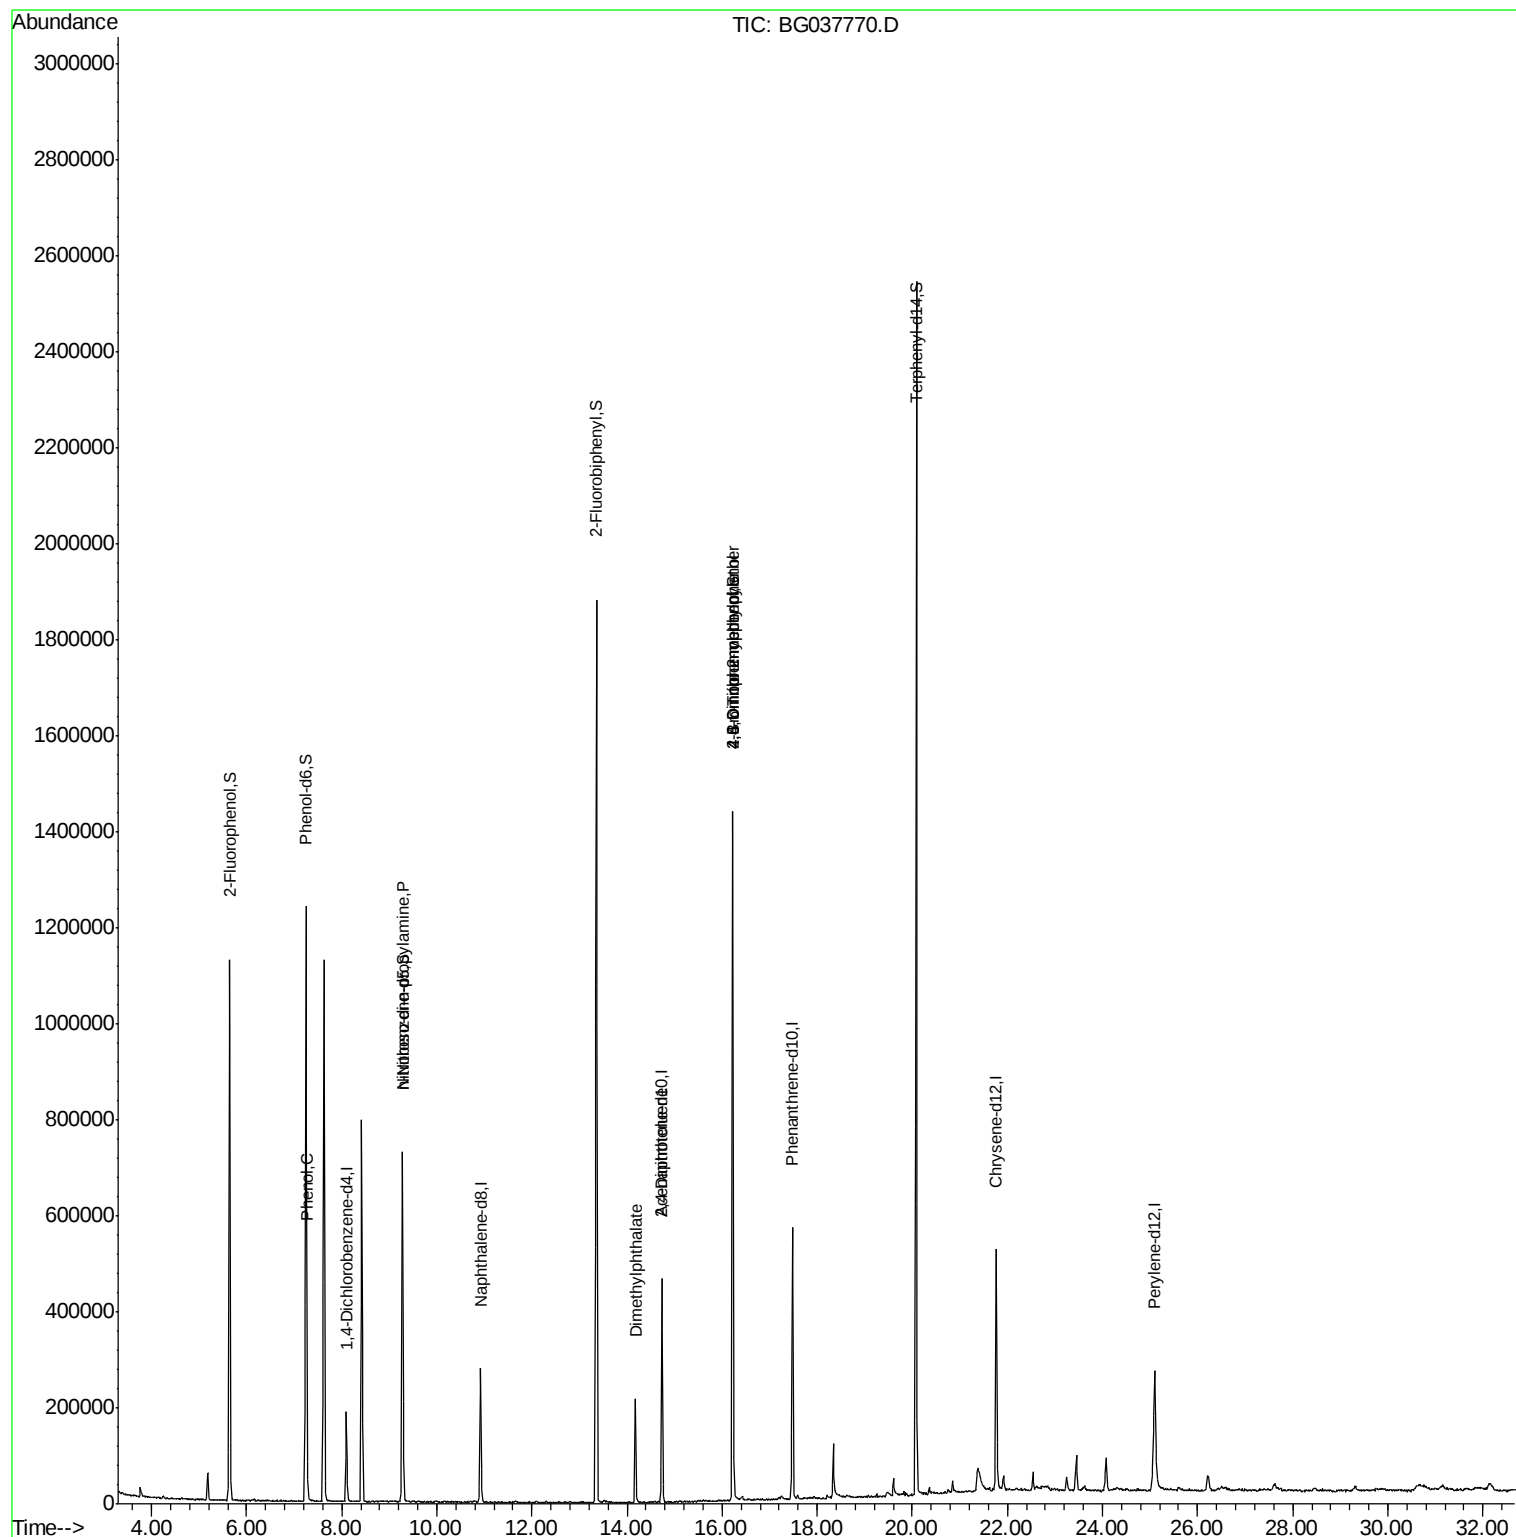




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.10 min Scan# 819
Delta R.T. -0.01 min
Lab File: BG037770.D
Acq: 3 Nov 2018 1:14

Instrument :
BNA_G
ClientSampleId :

Tot Ion:152 Resp: 57020
Ion Ratio Lower Upper
152 100
150 149.7 126.0 189.0
115 55.8 45.5 68.3

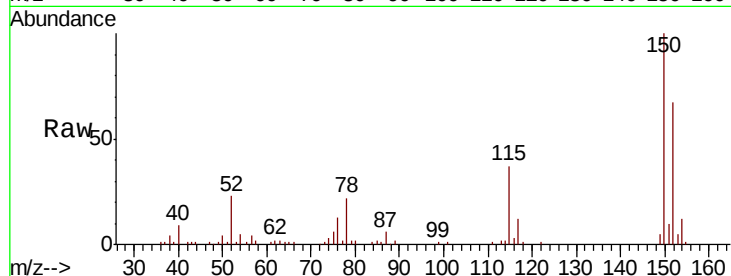


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

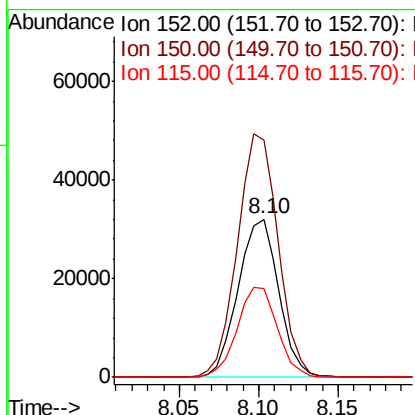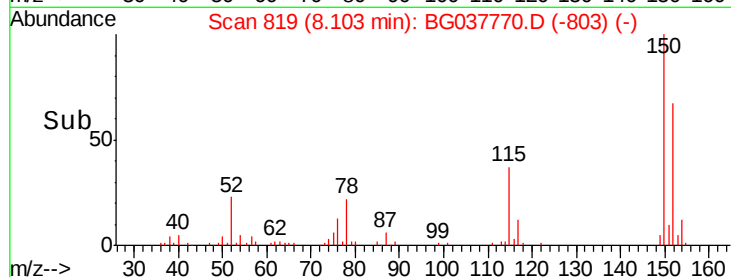



#5

2-Fluorophenol
Concen: 151.089 ng
RT: 5.64 min Scan# 400
Delta R.T. -0.01 min
Lab File: BG037770.D
Acq: 3 Nov 2018 1:14

Tgt Ion:112 Resp: 515302
Ion Ratio Lower Upper
112 100
64 66.7 53.1 79.7
63 34.2 27.3 40.9



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

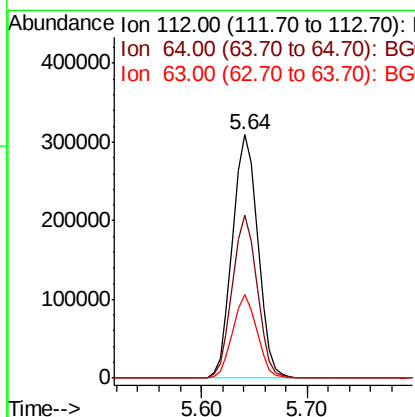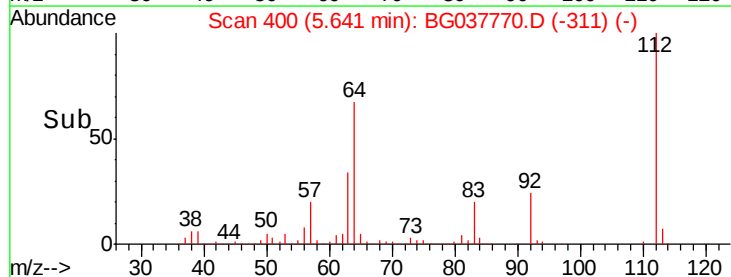



#7

Phenol-d6

Concen: 150.973 ng

RT: 7.25 min Scan# 673

Delta R.T. -0.01 min

Lab File: BG037770.D

Acq: 3 Nov 2018 1:14

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 778604

Ion Ratio Lower Upper




99 100

42 18.5 15.0 22.4

71 31.9 25.5 38.3

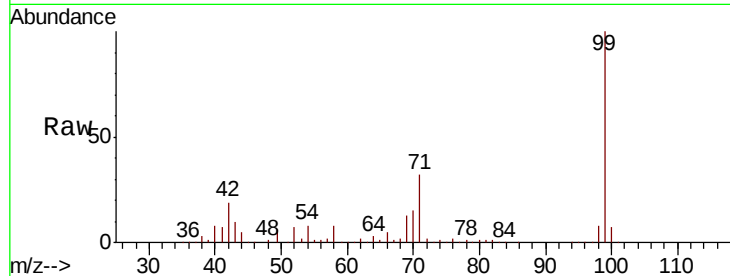

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

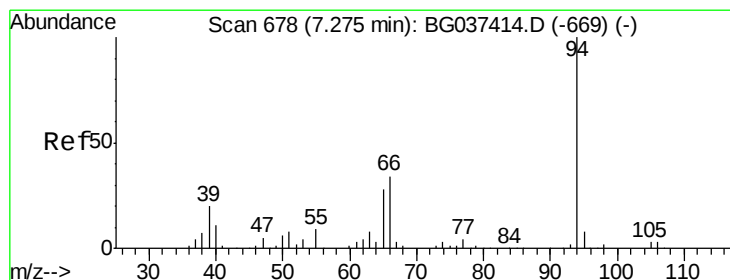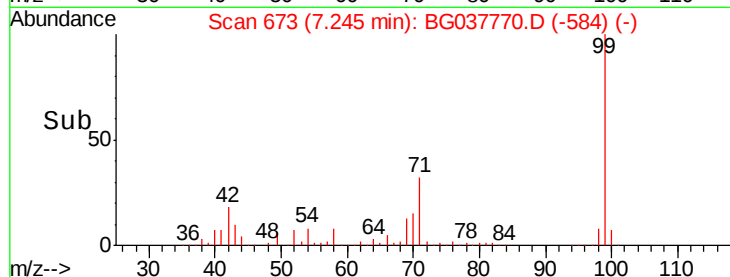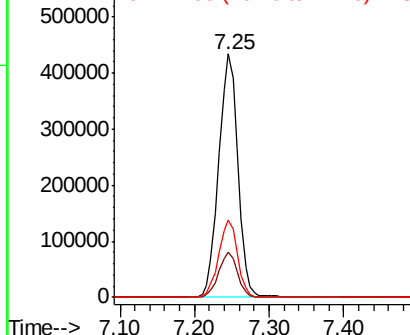

#10

Phenol

Concen: 9.246 ng

RT: 7.27 min Scan# 677

Delta R.T. -0.01 min

Lab File: BG037770.D

Acq: 3 Nov 2018 1:14


Tgt Ion: 94 Resp: 50309

Ion Ratio Lower Upper



94 100

65 30.8 9.7 49.7

66 42.5 15.9 55.9

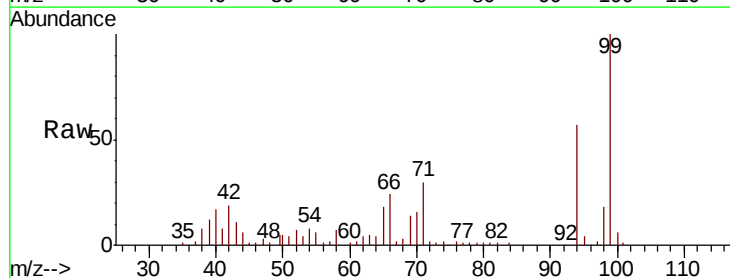

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC



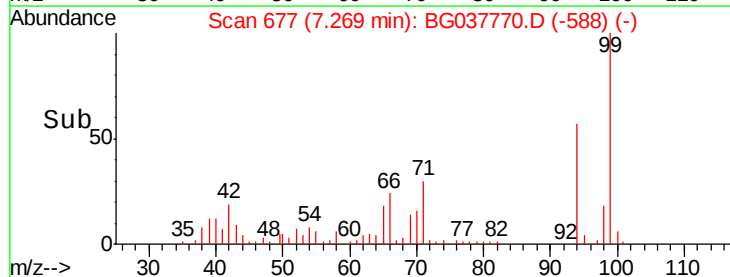
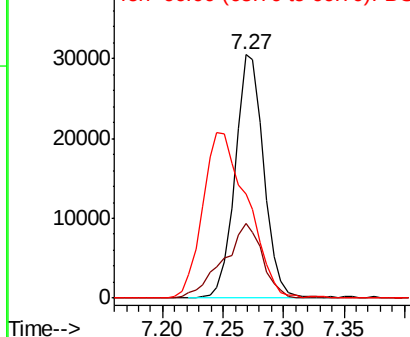




#19
n-Nitroso-di-n-propylamine
Concen: 16.637 ng
RT: 9.28 min Scan# 1019
Delta R.T. 0.36 min
Lab File: BG037770.D
Acq: 3 Nov 2018 1:14




Instrument :
BNA_G
ClientSampleId :

Tot Ion: 70 Resp: 59082
Ion Ratio Lower Upper
70 100
42 50.6 53.9 80.9#
101 0.0 8.2 12.2#
130 2.1 18.2 27.4#

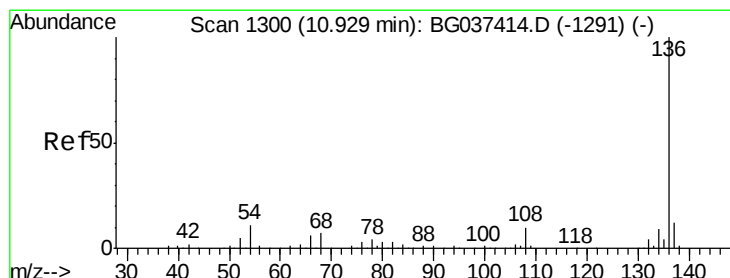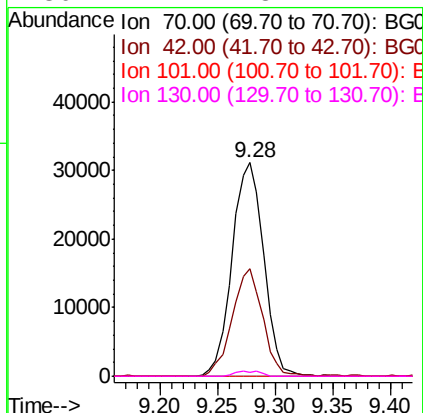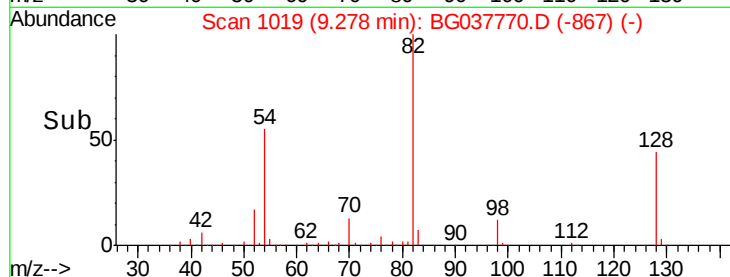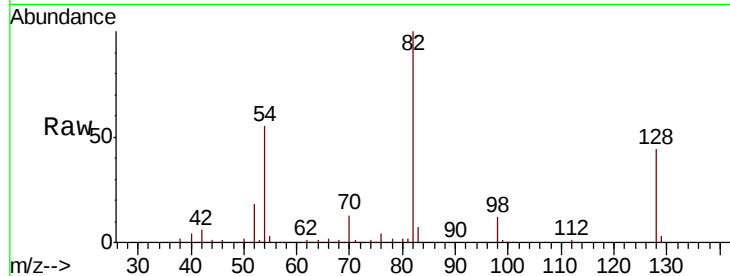

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.92 min Scan# 1299
Delta R.T. -0.01 min
Lab File: BG037770.D
Acq: 3 Nov 2018 1:14

Tgt Ion:136 Resp: 260871
Ion Ratio Lower Upper
136 100
137 11.7 9.6 14.4
54 9.3 7.9 11.9
68 6.3 4.8 7.2


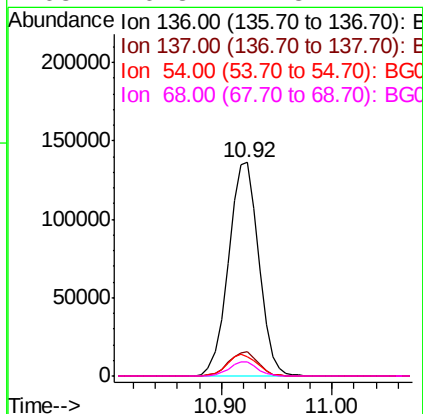
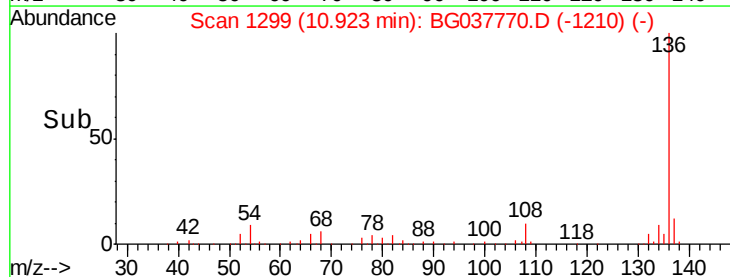
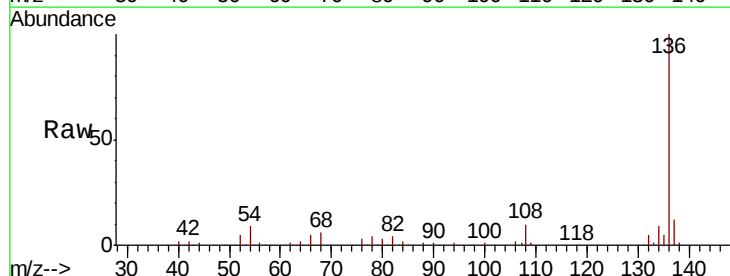




#23
Nitrobenzene-d5
Concen: 99.977 ng
RT: 9.28 min Scan# 1019
Delta R.T. -0.01 min
Lab File: BG037770.D
Acq: 3 Nov 2018 1:14




Instrument :
BNA_G
ClientSampleId :


Tot Ion: 82 Resp: 465574
Ion Ratio Lower Upper
82 100
128 44.3 34.6 51.8
54 54.9 45.3 67.9

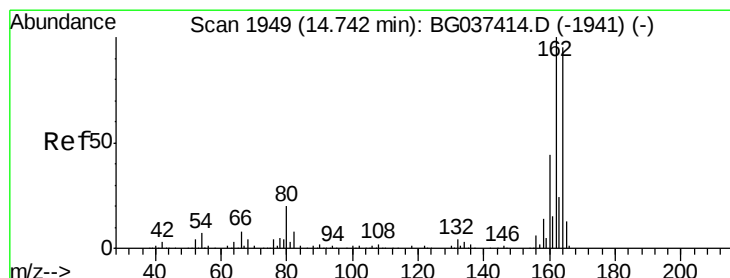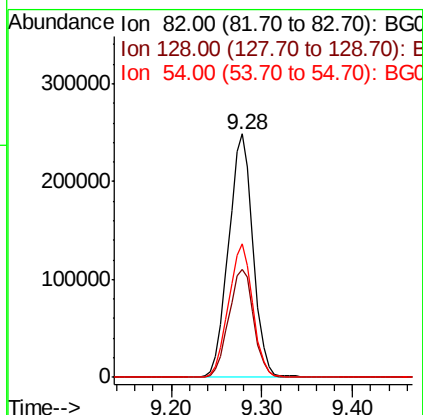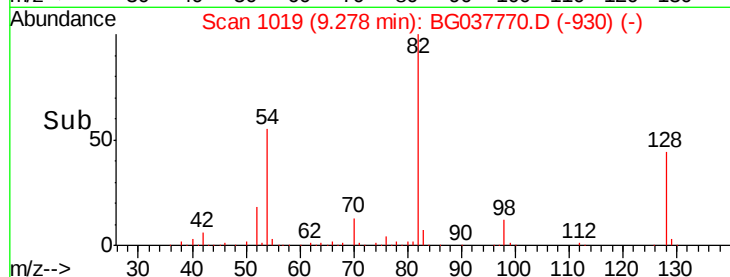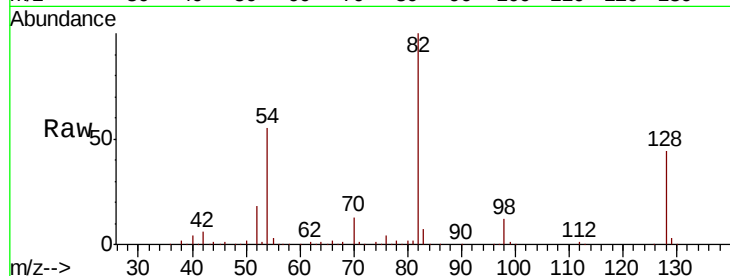

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.74 min Scan# 1948
Delta R.T. -0.01 min
Lab File: BG037770.D
Acq: 3 Nov 2018 1:14

Tgt Ion:164 Resp: 172542
Ion Ratio Lower Upper
164 100
162 102.0 81.3 121.9
160 45.2 36.3 54.5

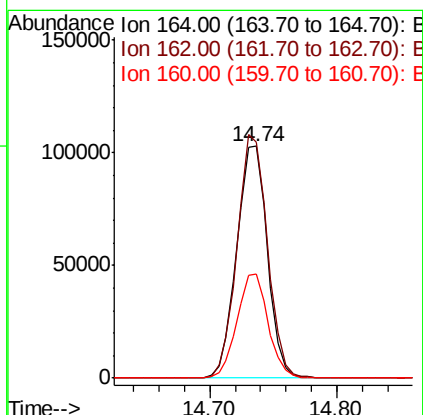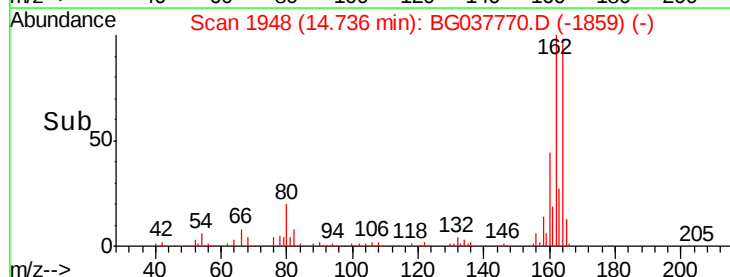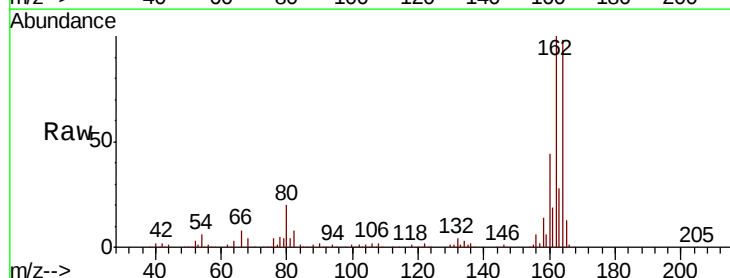

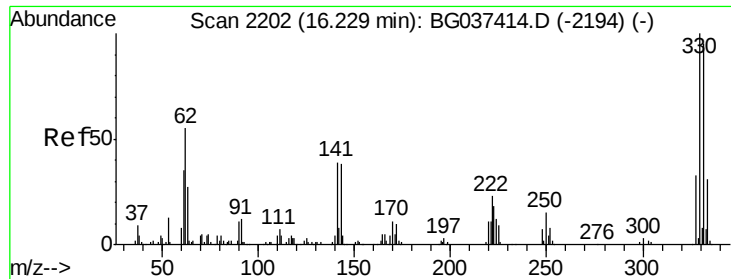

#42

2,4,6-Tribromophenol

Concen: 150.012 ng

RT: 16.22 min Scan# 2201

Delta R.T. -0.01 min

Lab File: BG037770.D

Acq: 3 Nov 2018 1:14

Instrument :

BNA_G

ClientSampleId :


Tot Ion:330 Resp: 282308

Ion Ratio Lower Upper

330 100

332 97.4 78.4 117.6




141 38.0 32.2 48.2



Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

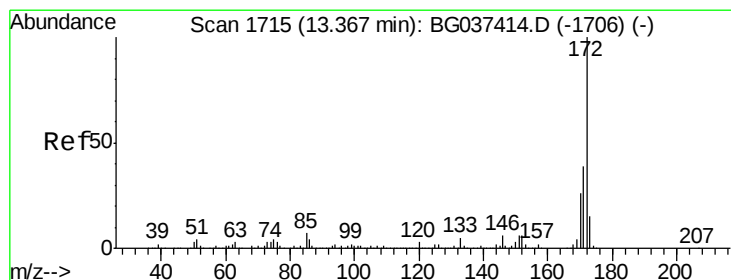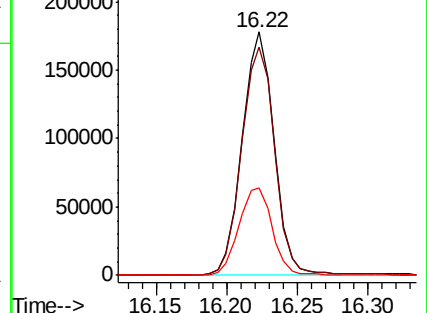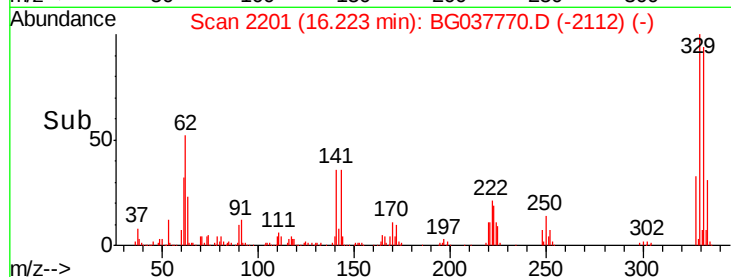

#45

2-Fluorobiphenyl

Concen: 89.646 ng

RT: 13.36 min Scan# 1713

Delta R.T. -0.01 min

Lab File: BG037770.D

Acq: 3 Nov 2018 1:14


Tgt Ion:172 Resp: 1025745

Ion Ratio Lower Upper

172 100

171 38.9 31.0 46.4



170 25.4 20.2 30.2




Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

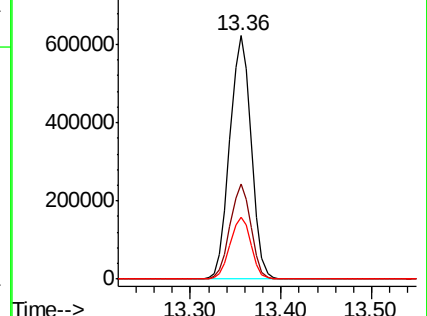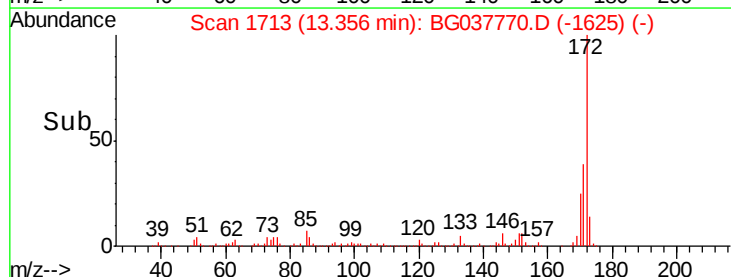

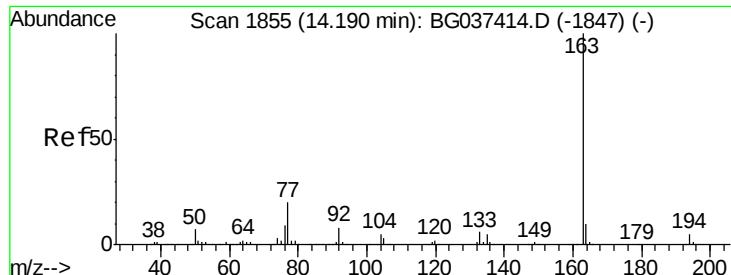

#50

Dimethylphthalate

Concen: 12.132 ng

RT: 14.18 min Scan# 1853

Delta R.T. -0.01 min

Lab File: BG037770.D

Acq: 3 Nov 2018 1:14

Instrument :

BNA_G

ClientSampled :


Tot Ion:163 Resp: 161946

Ion Ratio Lower Upper

163 100

194 4.3 3.5 5.3




164 10.3 8.5 12.7



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

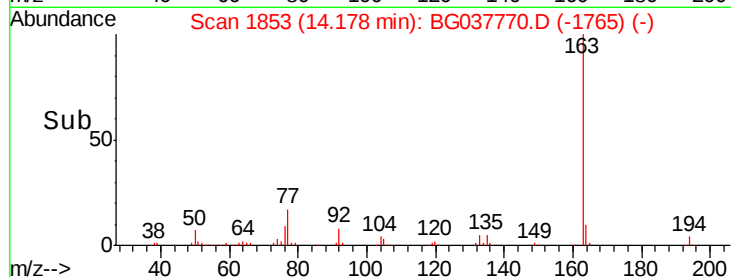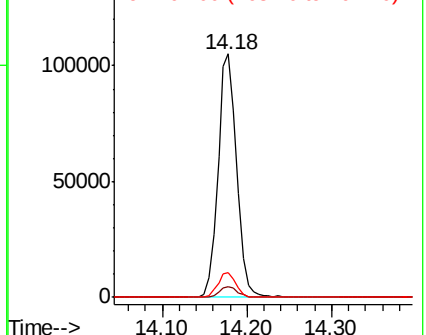

#57

2,4-Dinitrotoluene

Concen: 5.829 ng

RT: 14.73 min Scan# 1947

Delta R.T. -0.37 min

Lab File: BG037770.D

Acq: 3 Nov 2018 1:14

Tgt Ion:165 Resp: 22595


Ion Ratio Lower Upper

165 100

63 1.1 33.4 50.0#

89 1.3 57.2 85.8#

182 0.0 2.6 4.0#






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC

Ion 89.00 (88.70 to 89.70): BGC

Ion 182.00 (181.70 to 182.70): E

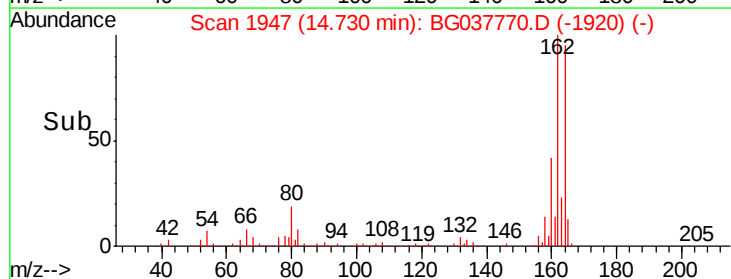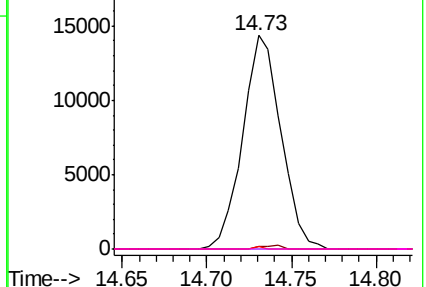

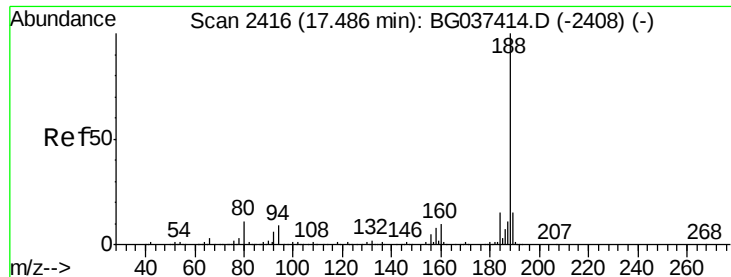

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.48 min Scan# 2415

Delta R.T. -0.01 min

Lab File: BG037770.D

Acq: 3 Nov 2018 1:14

Instrument :

BNA_G

ClientSampleId :


Tot Ion:188 Resp: 368992

Ion Ratio Lower Upper

188 100

94 8.9 7.2 10.8

80 10.2 7.7 11.5


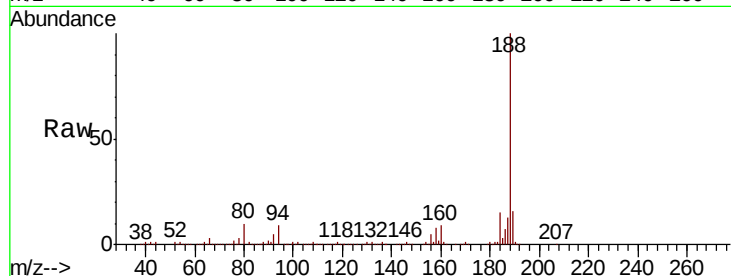


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

Time-->

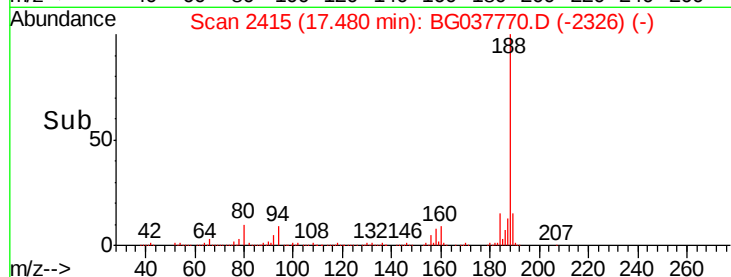

#65

4,6-Dinitro-2-methylphenol

Concen: 8.904 ng

RT: 16.22 min Scan# 2201

Delta R.T. 0.36 min

Lab File: BG037770.D

Acq: 3 Nov 2018 1:14


Tgt Ion:198 Resp: 932

Ion Ratio Lower Upper

198 100

51 24.3 22.7 62.7

105 29.3 19.7 59.7




Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BG

Ion 105.00 (104.70 to 105.70): E

Time-->

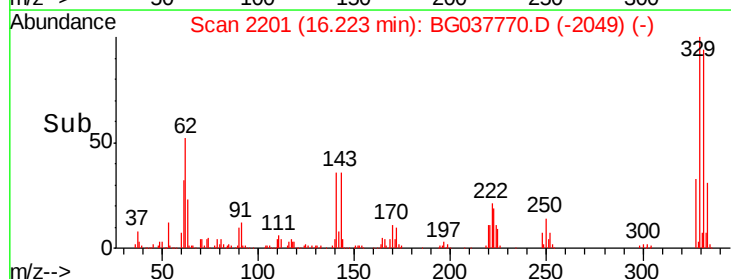







#67
4-Bromophenyl-phenylether
Concen: 5.117 ng
RT: 16.22 min Scan# 2201
Delta R.T. -0.45 min
Lab File: BG037770.D
Acq: 3 Nov 2018 1:14

Instrument :
BNA_G
ClientSampleId :

Tot Ion:248 Resp: 20733
Ion Ratio Lower Upper
248 100
250 191.2 77.0 115.6#
141 381.2 55.5 83.3#

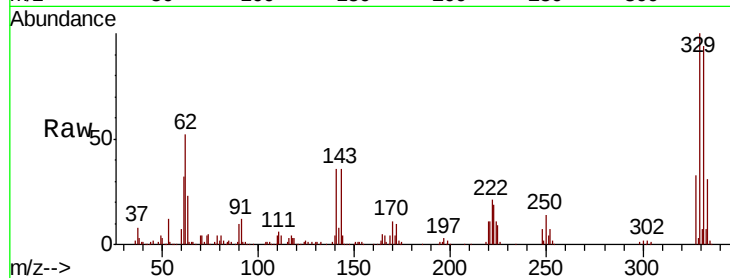


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

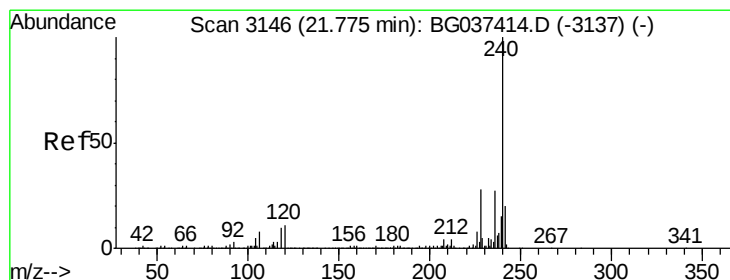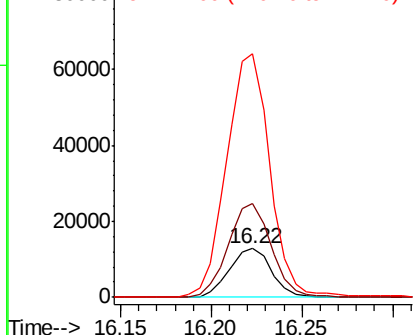
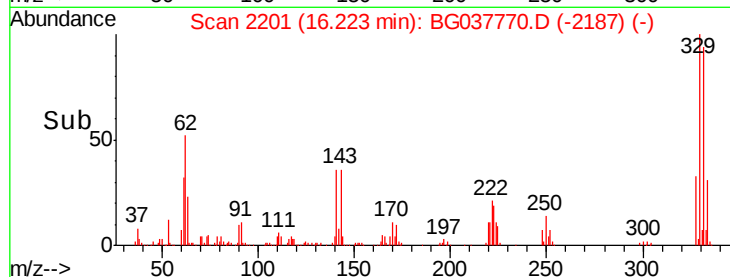


#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.76 min Scan# 3144
Delta R.T. -0.01 min
Lab File: BG037770.D
Acq: 3 Nov 2018 1:14

Tgt Ion:240 Resp: 332566
Ion Ratio Lower Upper
240 100
120 10.3 8.1 12.1
236 26.1 21.4 32.0

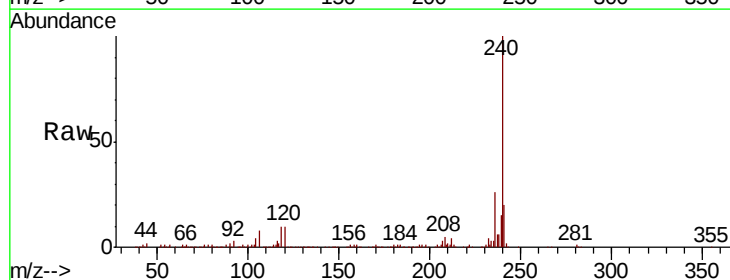

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

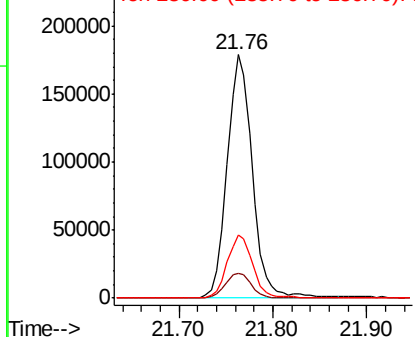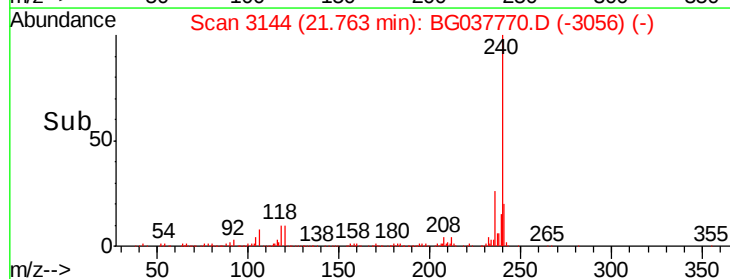



#79

Terphenyl-d14

Concen: 81.511 ng

RT: 20.08 min Scan# 2858

Delta R.T. -0.01 min

Lab File: BG037770.D

Acq: 3 Nov 2018 1:14


Instrument :

BNA_G

ClientSampleId :

Tot Ion:244 Resp: 1268641

Ion	Ratio	Lower	Upper
244	100		
212	8.5	6.5	9.7
122	10.3	9.0	13.4






Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

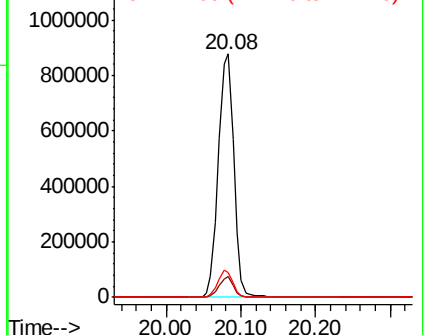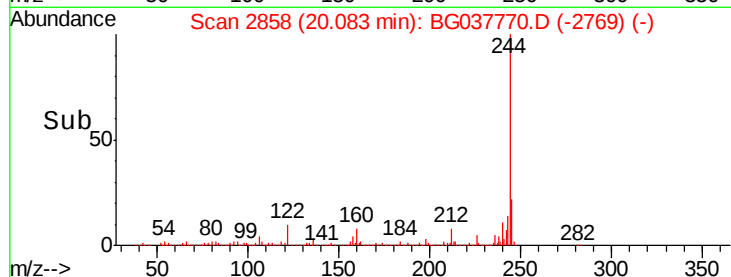

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.10 min Scan# 3712


Delta R.T. -0.01 min

Lab File: BG037770.D

Acq: 3 Nov 2018 1:14

Tgt Ion:264 Resp: 317994

Ion	Ratio	Lower	Upper
264	100		
260	23.6	18.2	27.4
265	21.8	17.9	26.9



Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

