
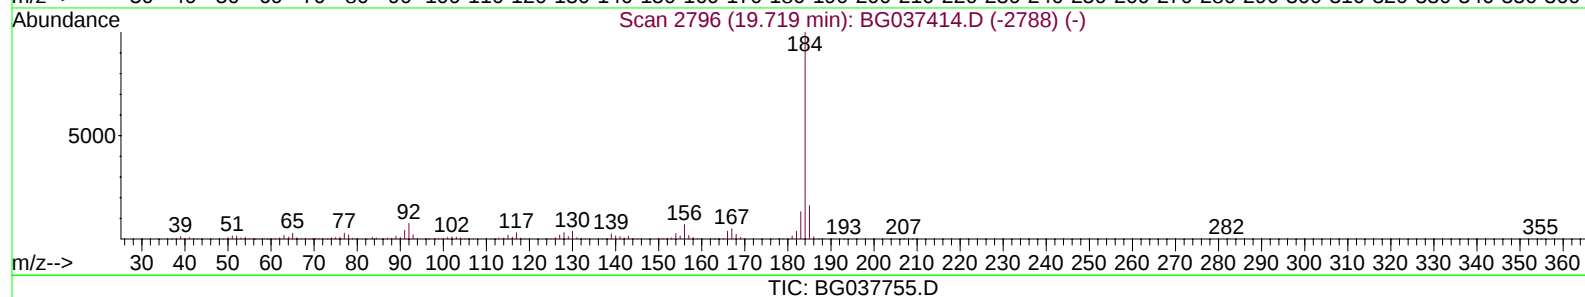
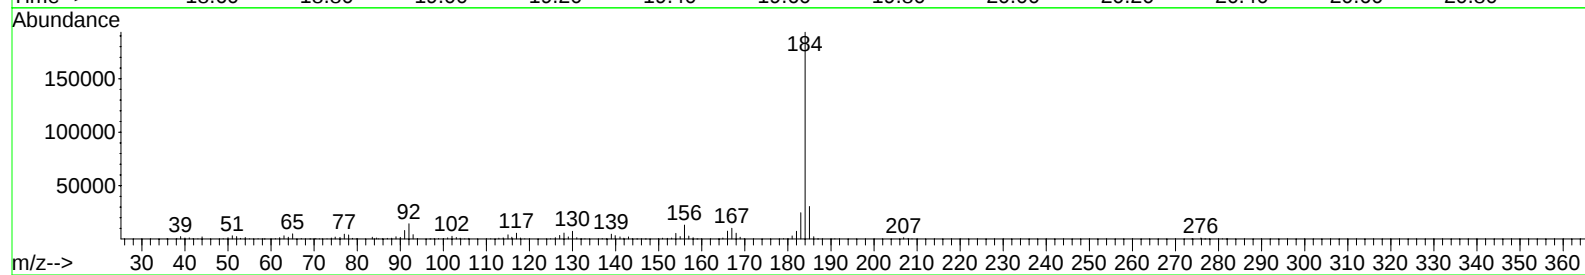


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110218\
Data File : BG037755.D
Acq On : 2 Nov 2018 15:23
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 06:34:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

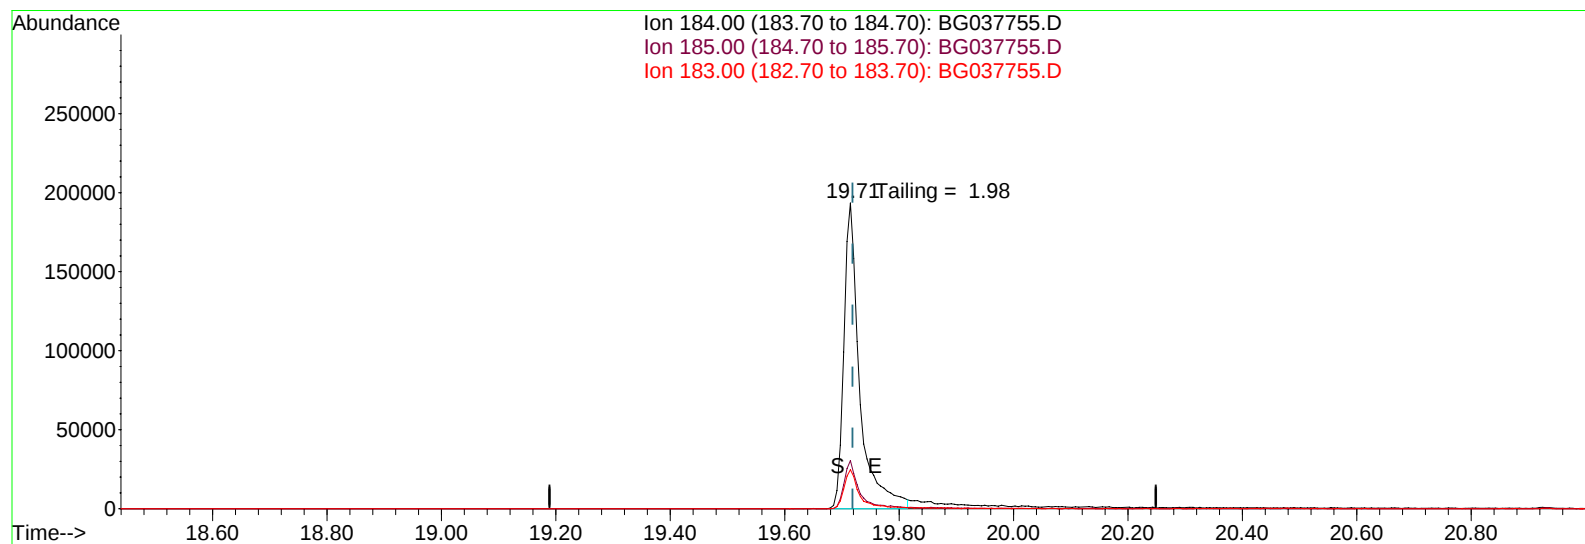

(77) Benzidine




19.715min (-0.004) 196632.52ng

response 401161

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.76
183.00	12.70	12.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110218\
Data File : BG037755.D
Acq On : 2 Nov 2018 15:23
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 06:34:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

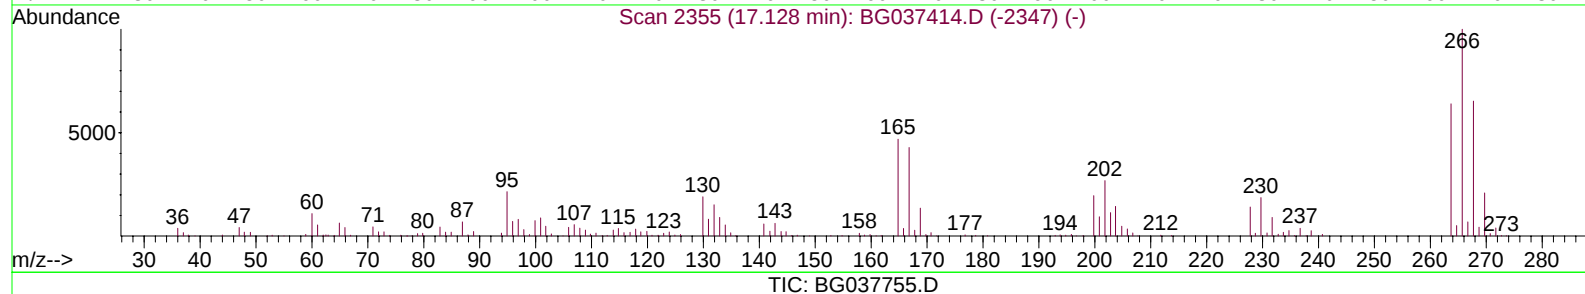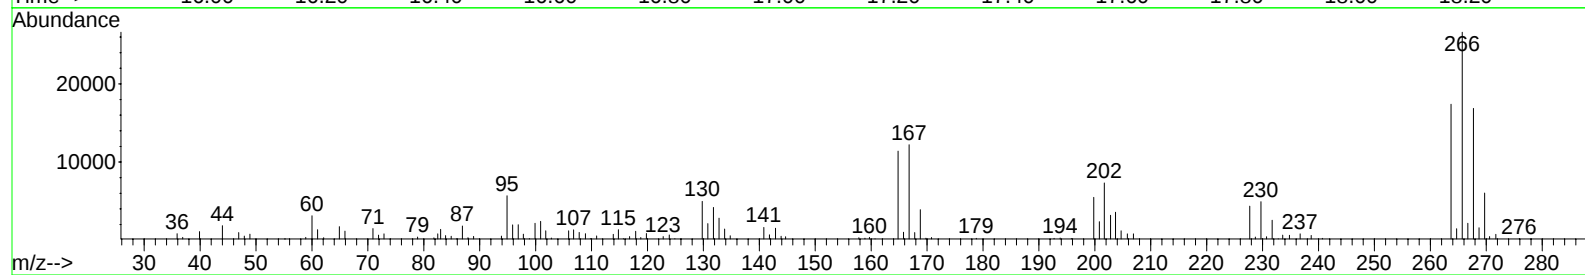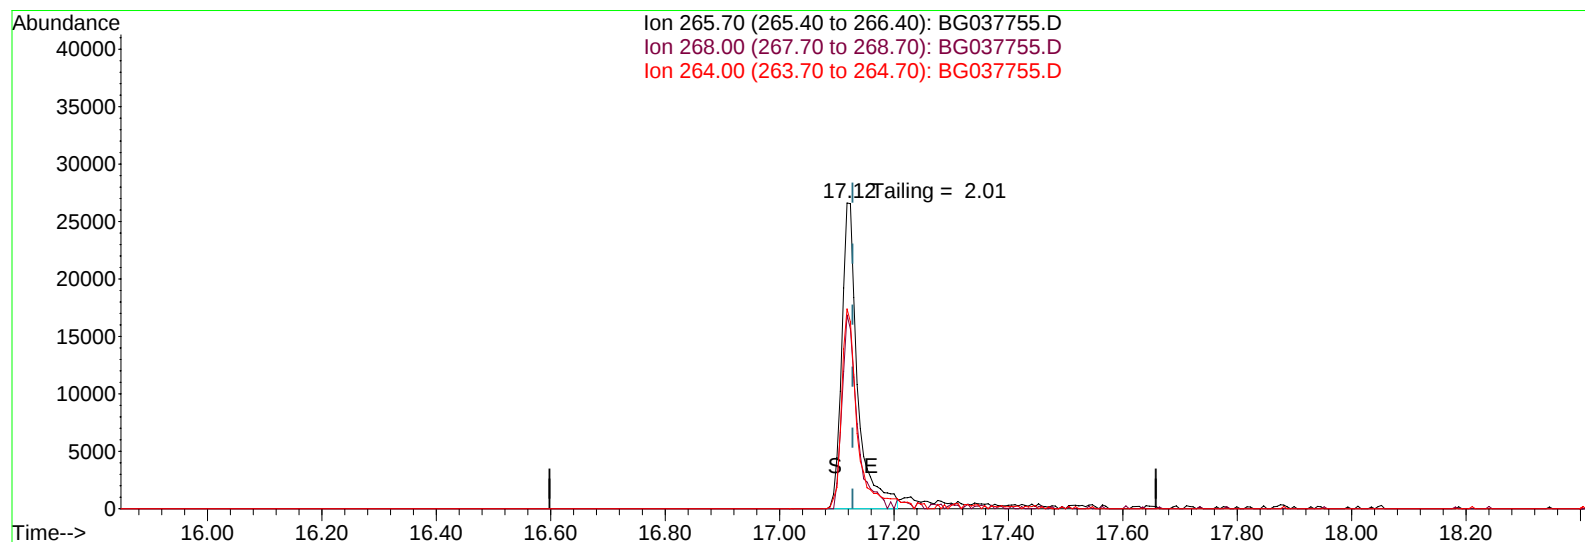

(70) Pentachlorophenol (C)

17.118min (-0.010) 108810.84ng

response 52261

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	69.33
264.00	73.60	70.81
0.00	0.00	0.00