
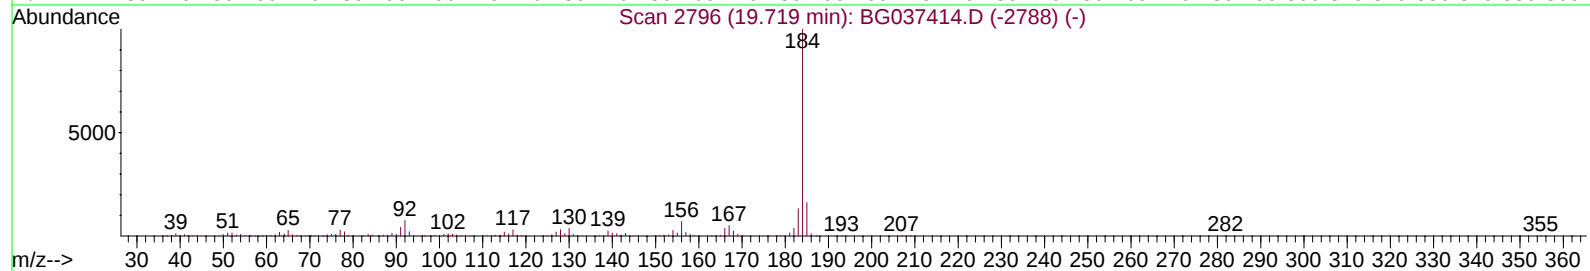
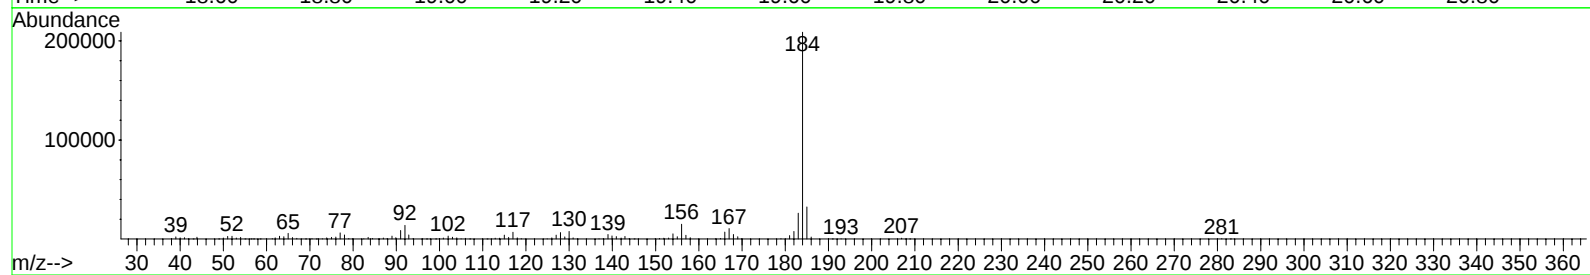


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110218\  
Data File : BG037774.D  
Acq On : 3 Nov 2018 3:51  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 06:36:39 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Oct 18 14:06:42 2018  
Response via : Initial Calibration

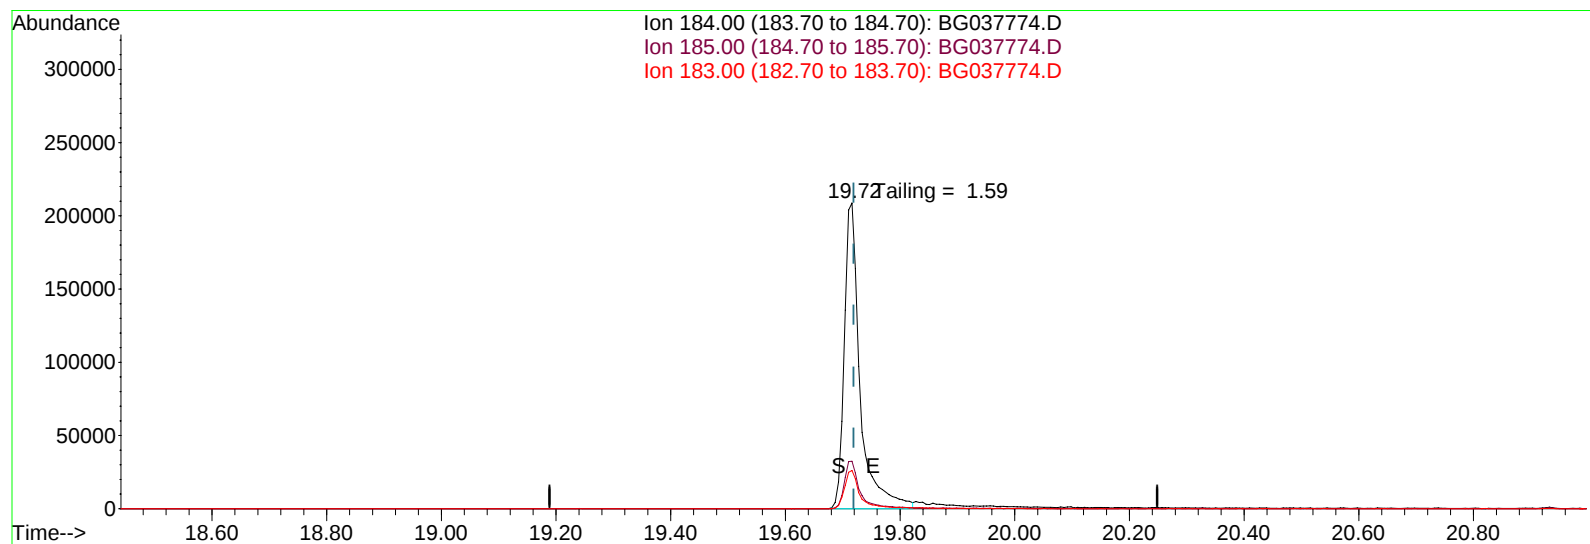

TIC: BG037774.D

(77) Benzidine




19.716min (-0.003) 155560.87ng

response 402000

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.70 | 15.53 |
| 183.00 | 12.70 | 12.50 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110218\  
Data File : BG037774.D  
Acq On : 3 Nov 2018 3:51  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 06:36:39 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Oct 18 14:06:42 2018  
Response via : Initial Calibration

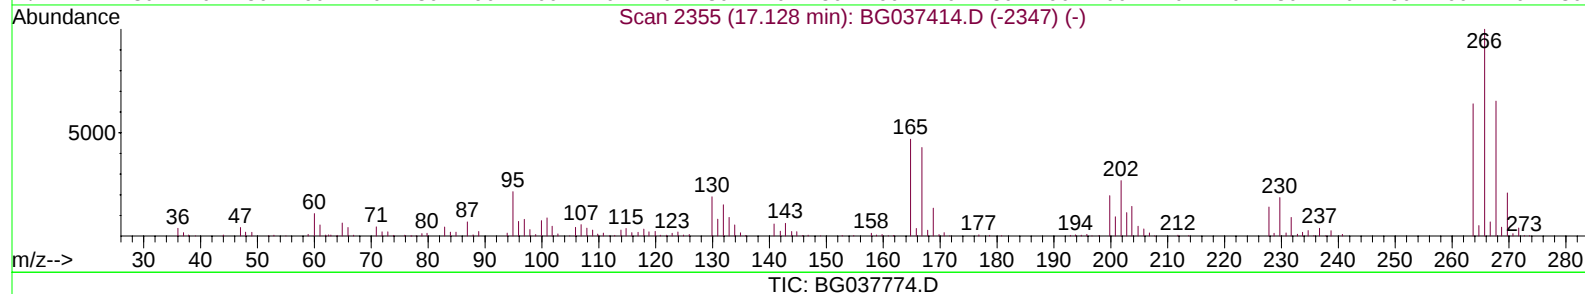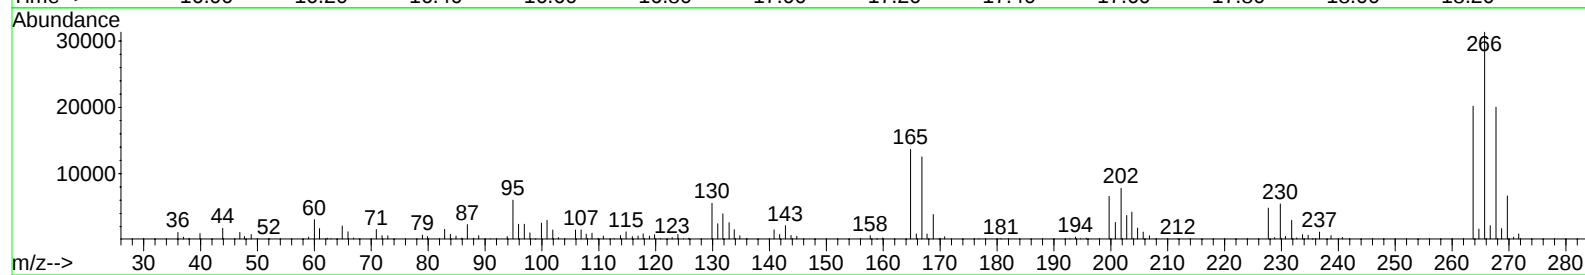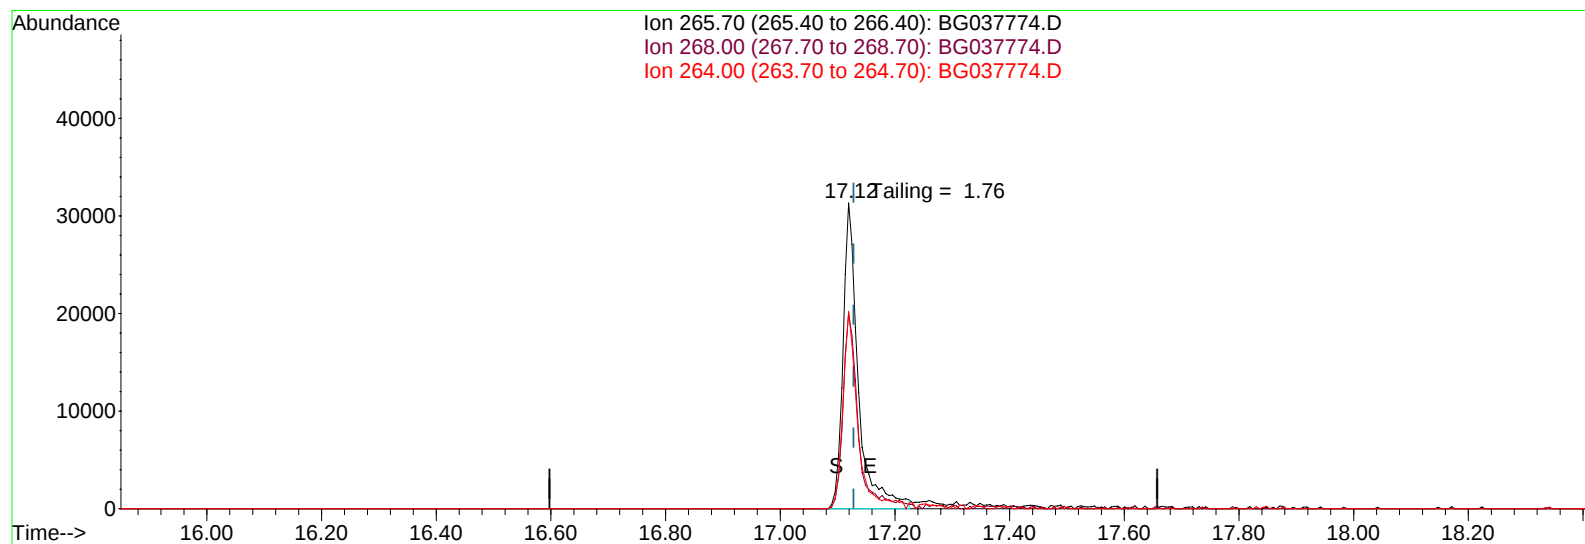

(70) Pentachlorophenol (C)

17.119min (-0.009) 136025.75ng

response 59110

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 68.80 | 69.44 |
| 264.00 | 73.60 | 69.66 |
| 0.00   | 0.00  | 0.00  |