


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110218\
 Data File : BG037755.D
 Acq On : 2 Nov 2018 15:23
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 18 14:06:42 2018

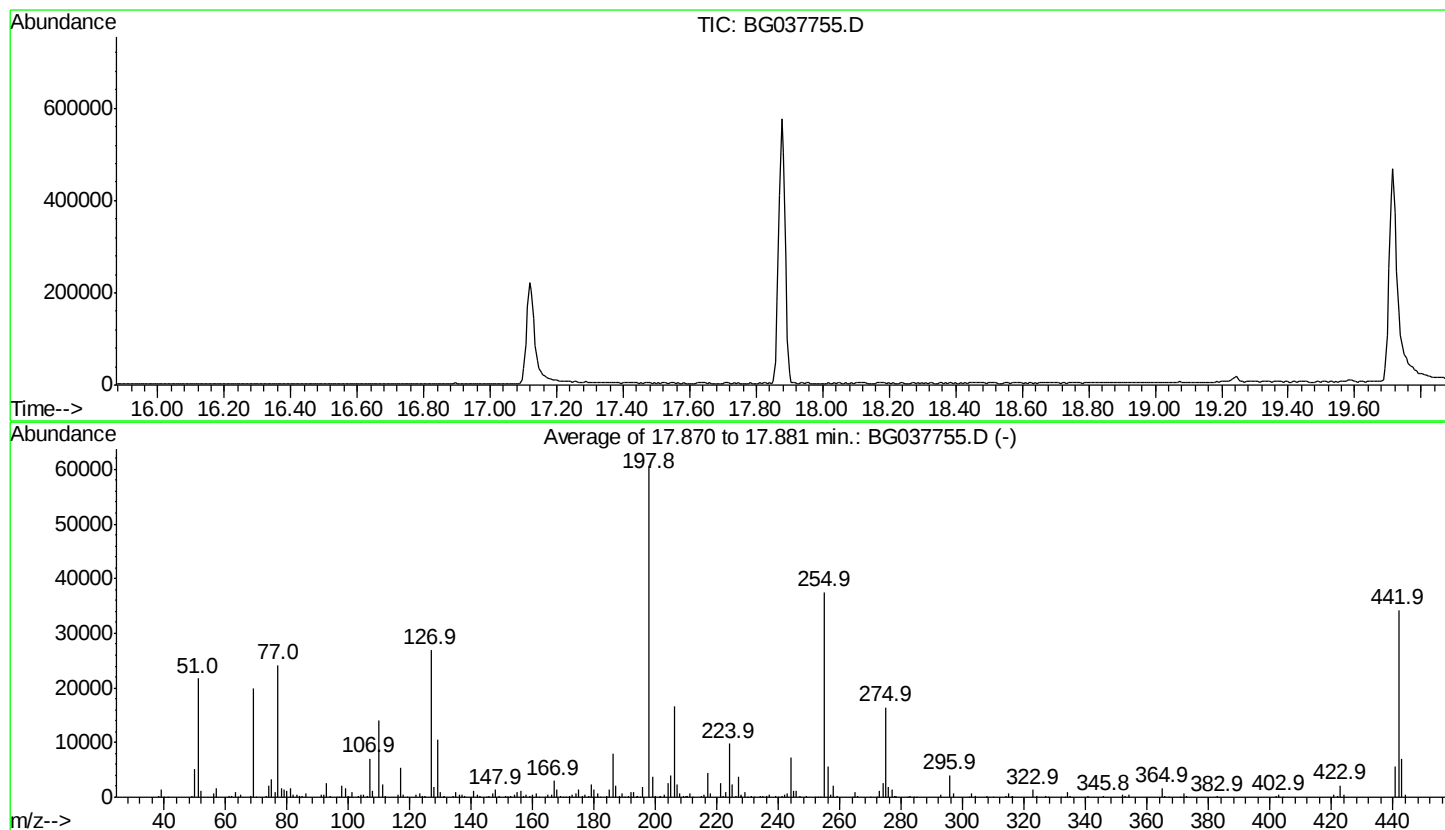

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	21706	PASS
68	69	0.00	2	0.9	172	PASS
69	198	0.00	100	32.8	19914	PASS
70	69	0.00	2	0.4	78	PASS
127	198	10	80	44.5	26986	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	60677	PASS
199	198	5	9	6.4	3860	PASS
275	198	10	60	27.1	16469	PASS
365	198	1	100	2.9	1764	PASS
441	198	0.01	100	9.2	5563	PASS
442	198	50	100	56.4	34208	PASS
443	442	15	24	20.6	7046	PASS