
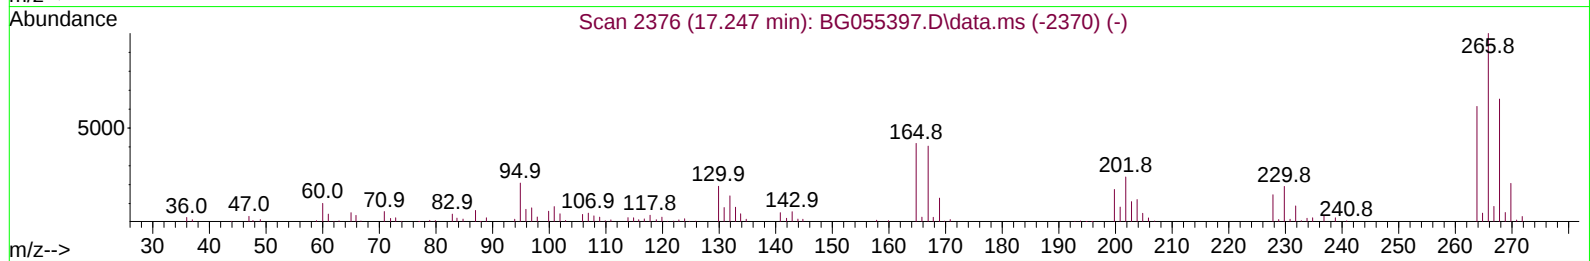
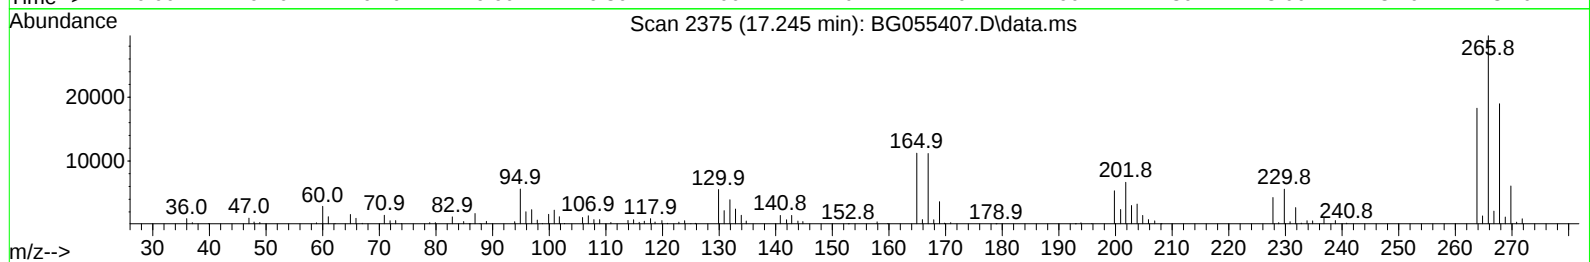


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110222\
Data File : BG055407.D
Acq On : 2 Nov 2022 9:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 09:07:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 02 05:05:12 2022
Response via : Initial Calibration

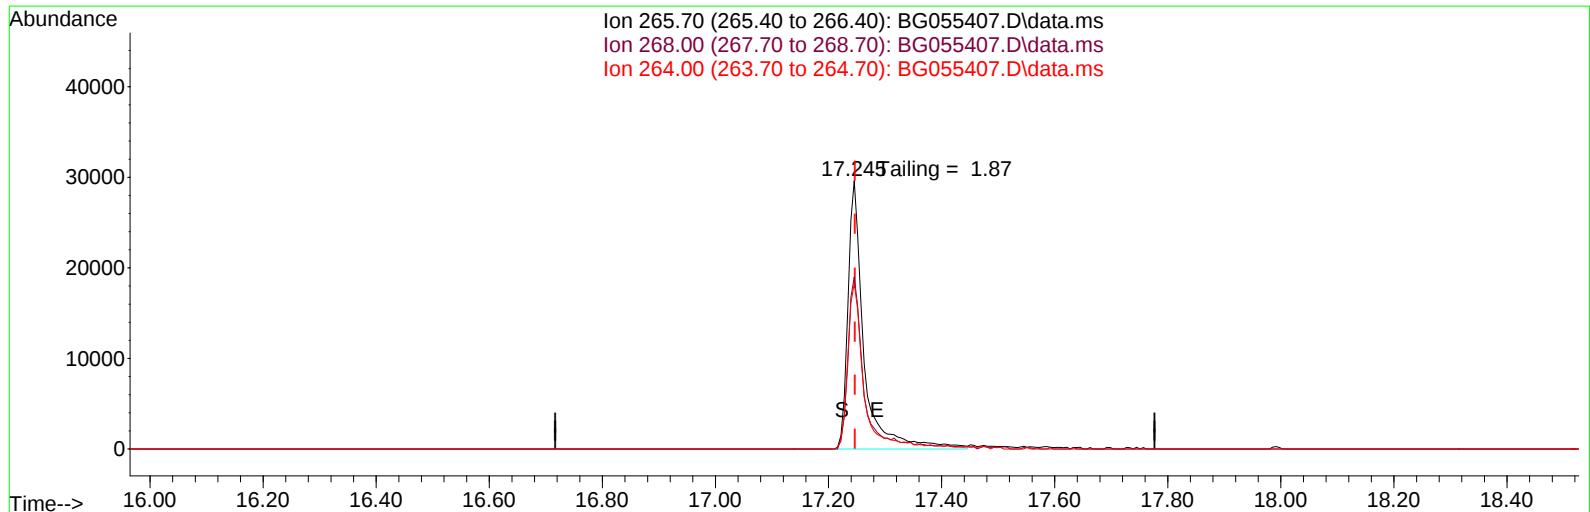

TIC: BG055407.D\data.ms

(70) Pentachlorophenol (C)




17.245min (-0.002) 37144.97 ng

response 58888

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.01
264.00	61.50	61.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110222\
Data File : BG055407.D
Acq On : 2 Nov 2022 9:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 09:07:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 02 05:05:12 2022
Response via : Initial Calibration

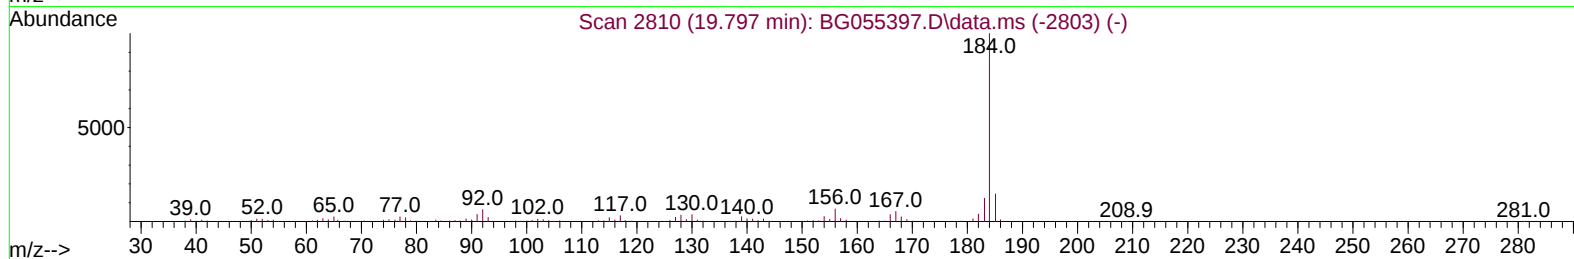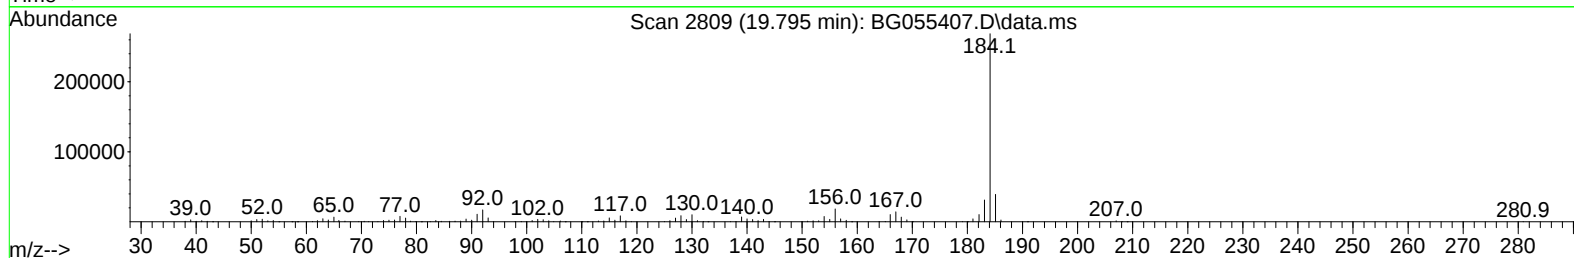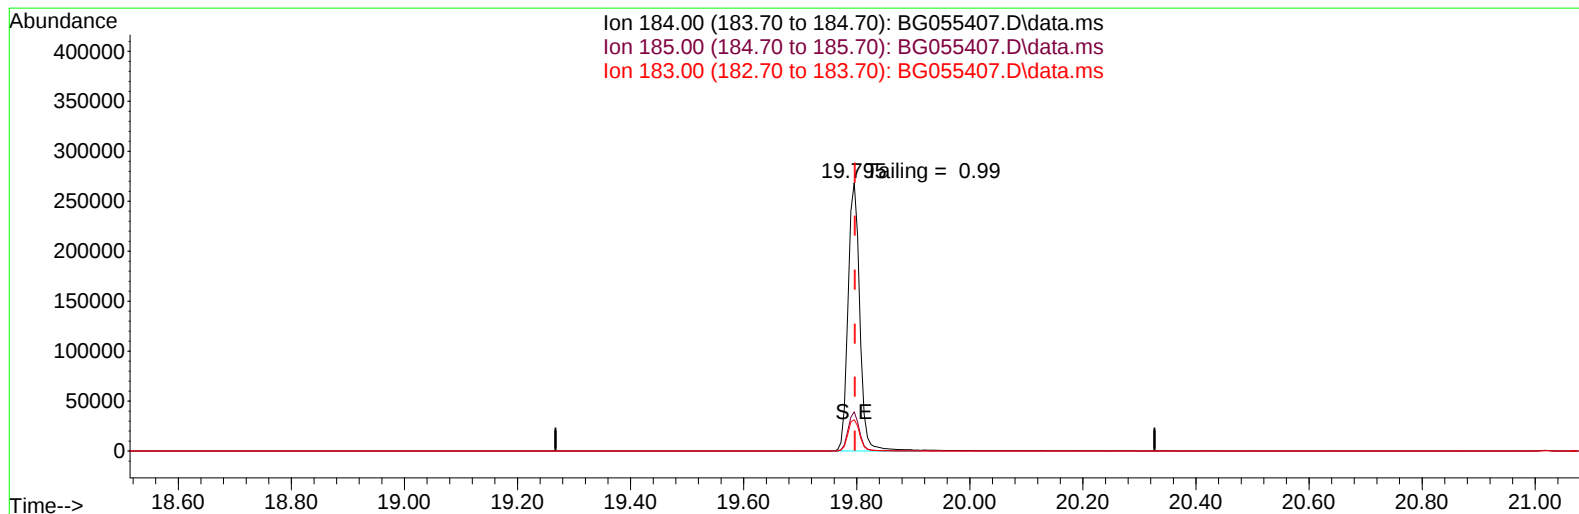

TIC: BG055407.D\data.ms

(77) Benzidine**19.795min (-0.002) 33811.28 ng****response 388568**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.63
183.00	12.30	11.66
0.00	0.00	0.00