
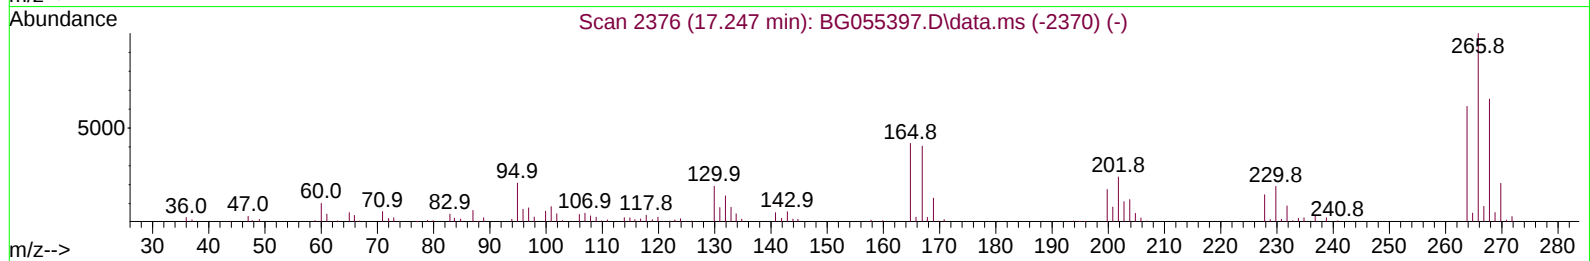
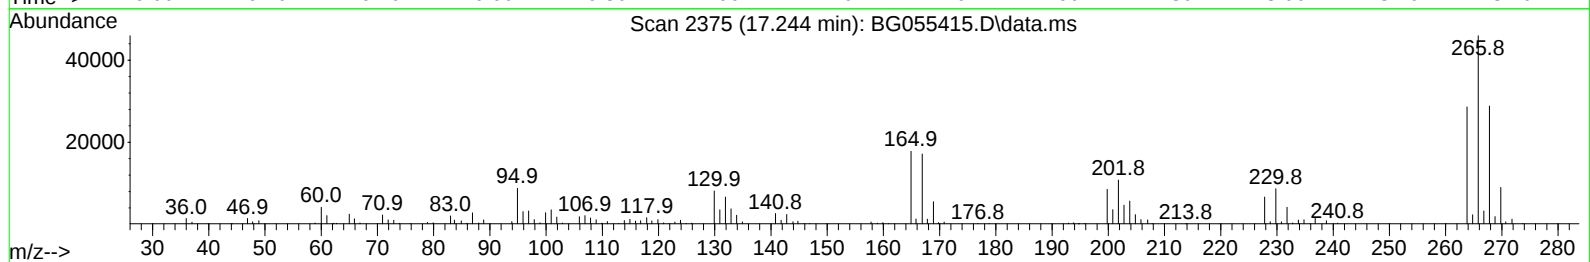


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110222\
Data File : BG055415.D
Acq On : 2 Nov 2022 14:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 09:09:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 02 05:05:12 2022
Response via : Initial Calibration

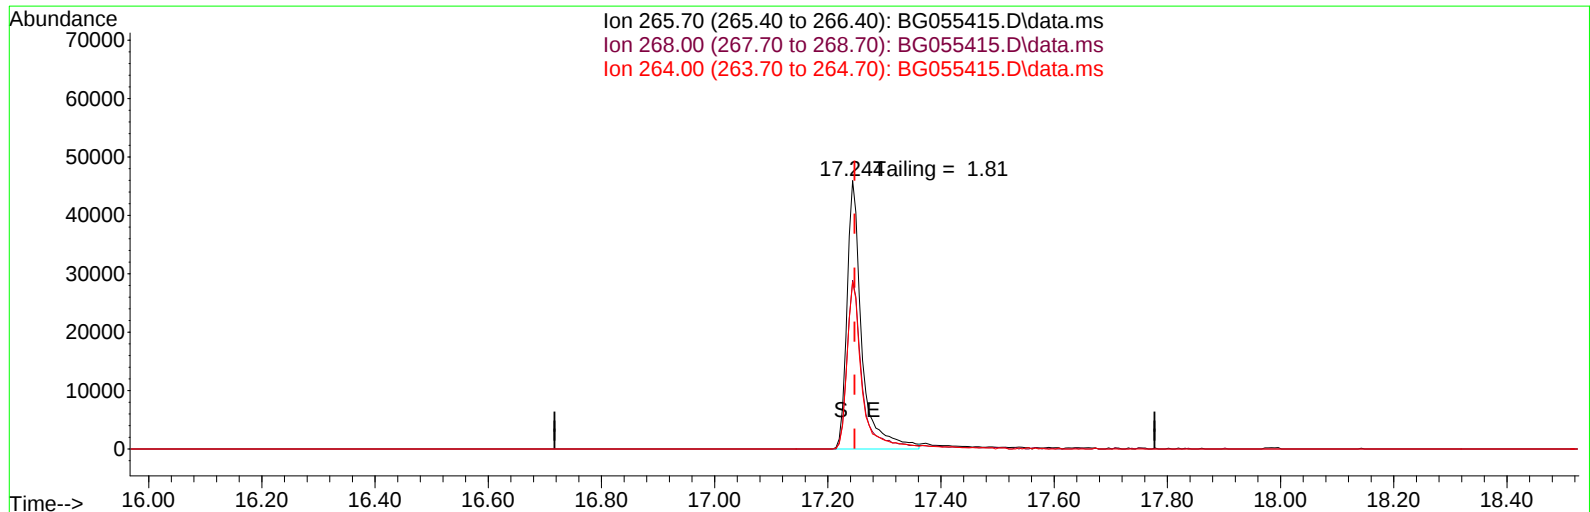

TIC: BG055415.D\data.ms

(70) Pentachlorophenol (C)




17.244min (-0.003) 31619.87 ng

response 84168

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	62.80
264.00	61.50	62.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110222\
Data File : BG055415.D
Acq On : 2 Nov 2022 14:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 09:09:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 02 05:05:12 2022
Response via : Initial Calibration

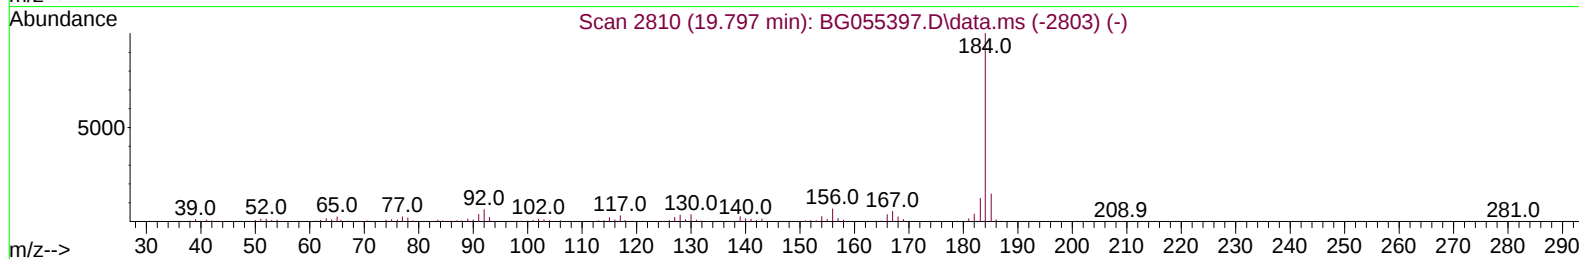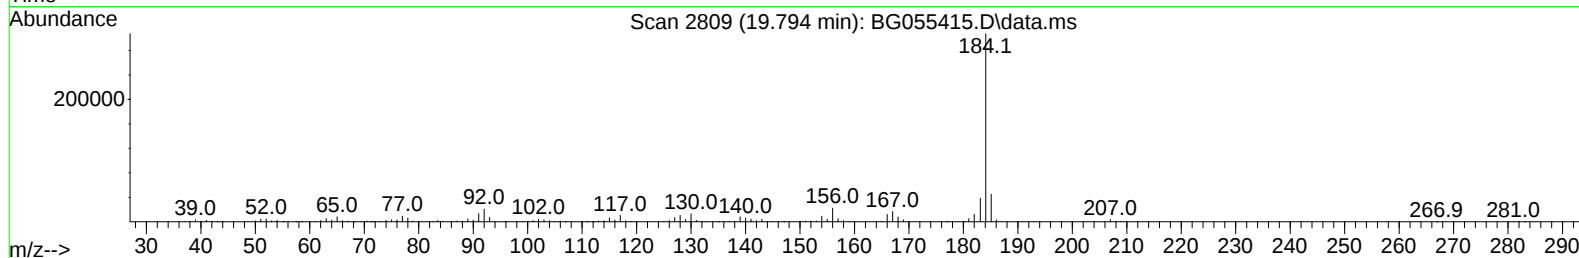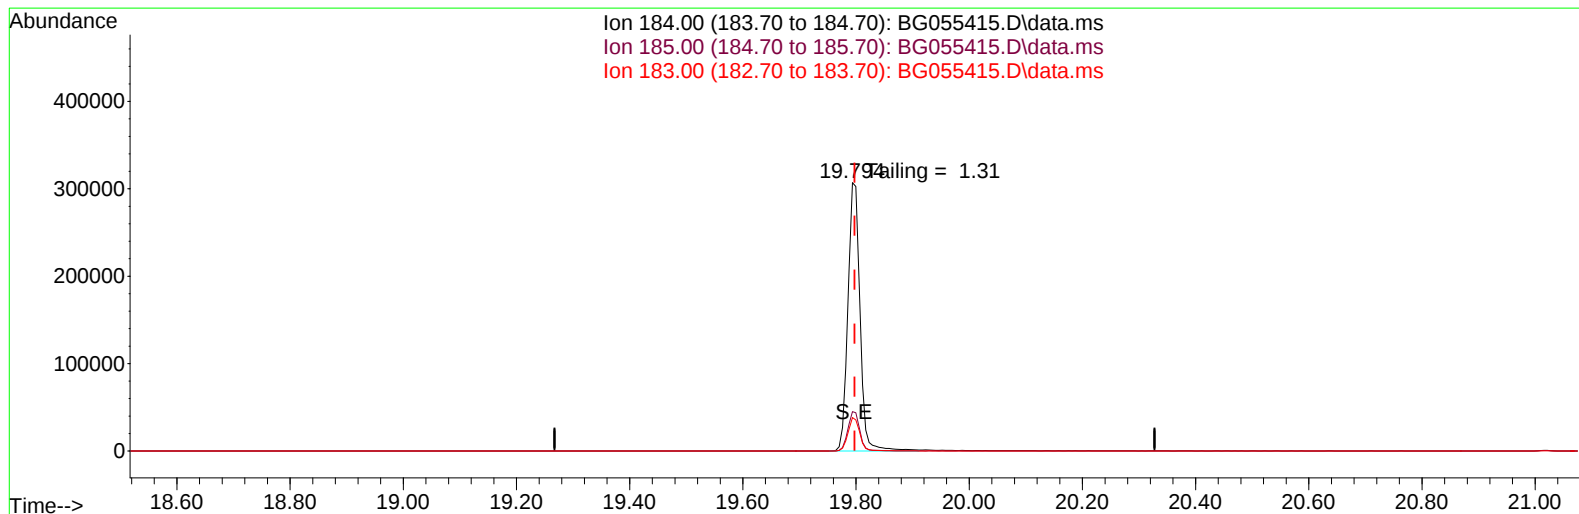

TIC: BG055415.D\data.ms

(77) Benzidine

19.794min (-0.003) 0.00 ng

response 454698

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.69
183.00	12.30	12.50
0.00	0.00	0.00