


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110222\
 Data File : BG055407.D
 Acq On : 2 Nov 2022 9:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 07 00:51:08 2022

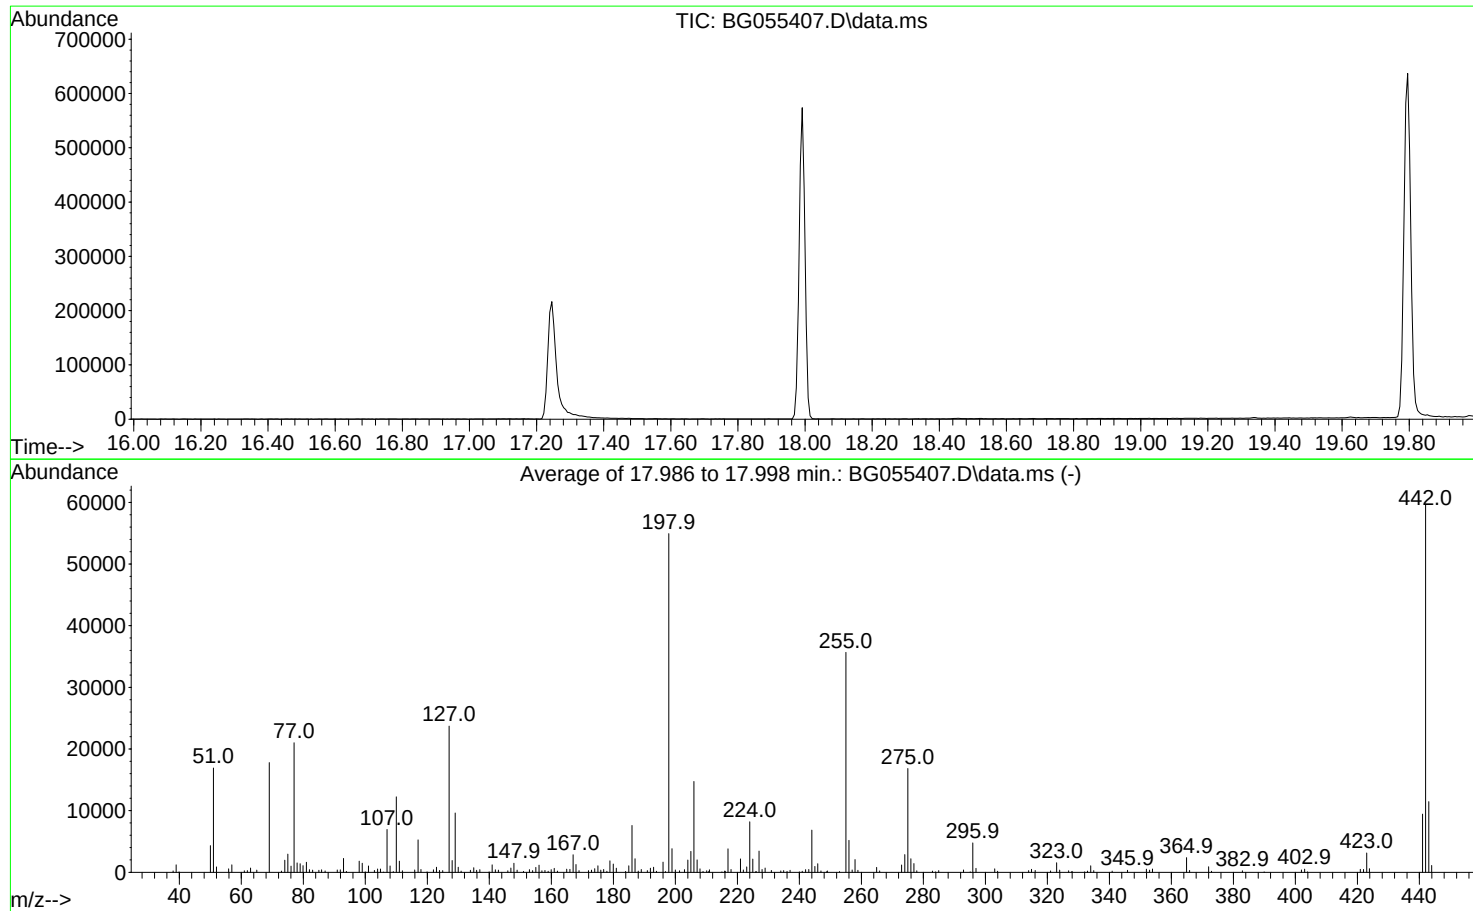




AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.8	16920	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.4	17786	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.2	23720	PASS
197	198	0.00	2	0.2	116	PASS
198	198	100	100	100.0	54939	PASS
199	198	5	9	7.0	3835	PASS
275	198	10	60	30.6	16821	PASS
365	198	1	100	4.3	2373	PASS
441	198	0.01	100	17.2	9449	PASS
442	442	50	100	100.0	59672	PASS
443	442	15	24	19.2	11464	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110222\
Data File : BG055407.D
Acq On : 2 Nov 2022 9:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 03 09:07:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 02 05:05:12 2022
Response via : Initial Calibration

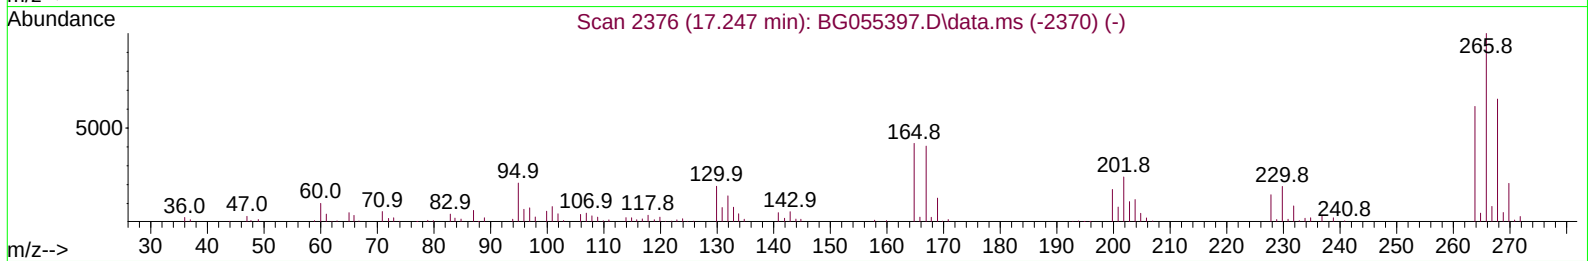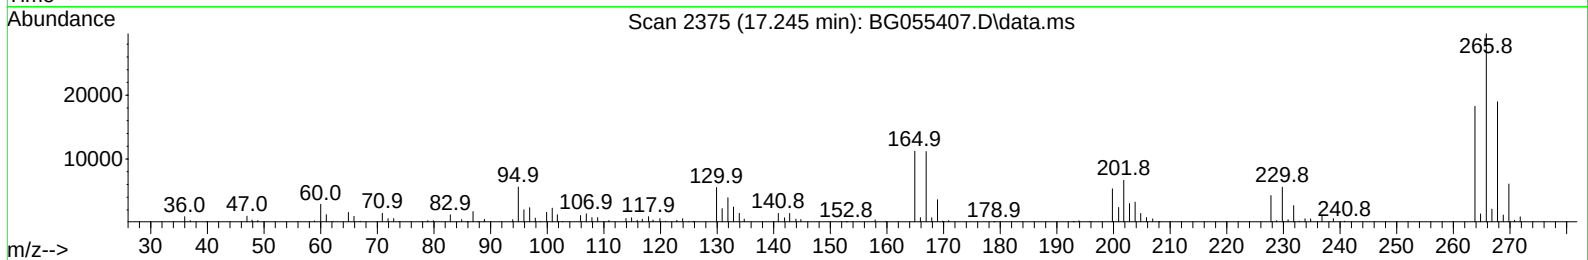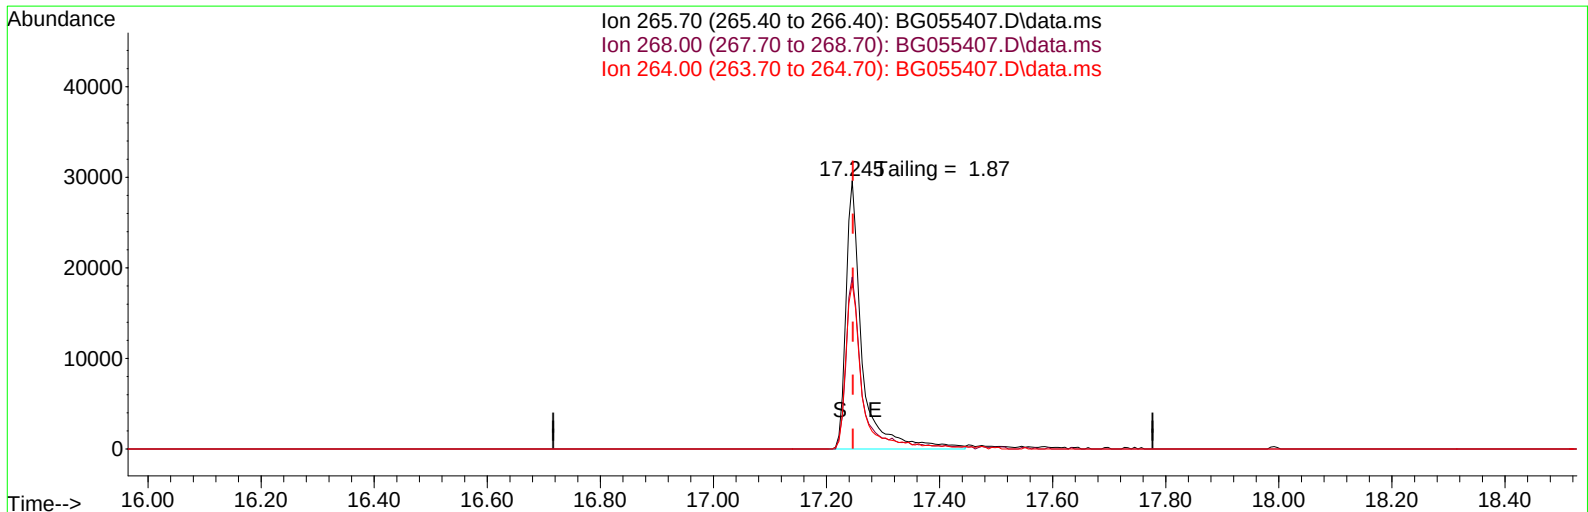

TIC: BG055407.D\data.ms

(70) Pentachlorophenol (C)

17.245min (-0.002) 37144.97 ng




response 58888

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.01
264.00	61.50	61.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110222\
Data File : BG055407.D
Acq On : 2 Nov 2022 9:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 03 09:07:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 02 05:05:12 2022
Response via : Initial Calibration

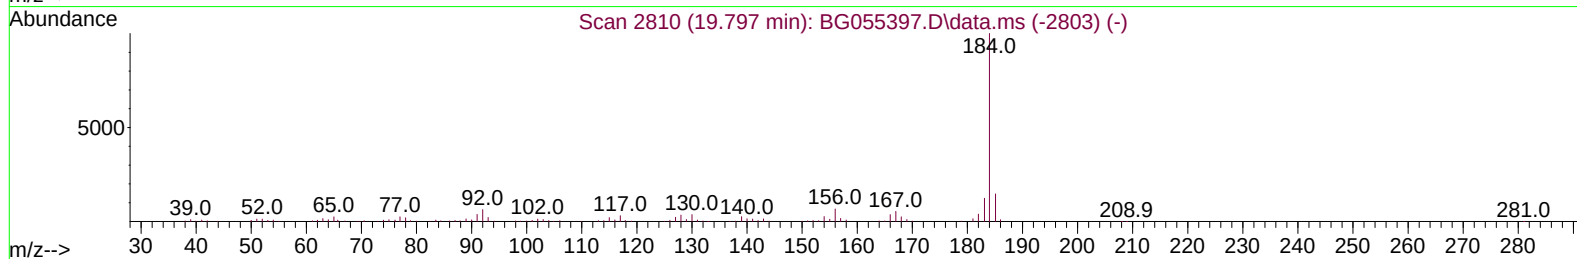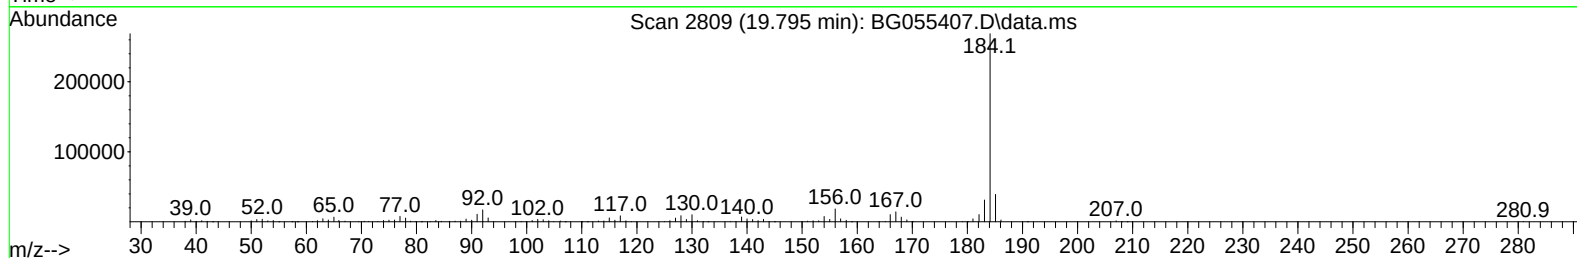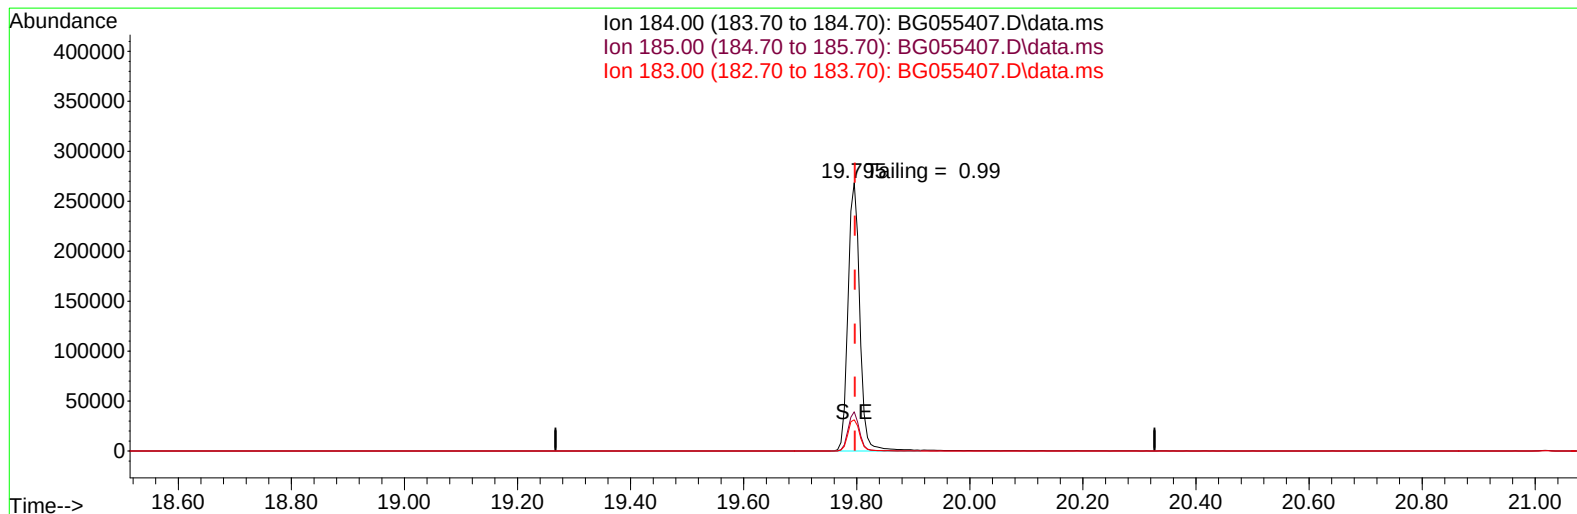

TIC: BG055407.D\data.ms

(77) Benzidine

19.795min (-0.002) 33811.28 ng

response 388568

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.63
183.00	12.30	11.66
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/2/2022	BNA_G	BG055407.D
Compound Name	Response	Retention Time
DDT	190459	21.017
DDD	3698	20.571
DDE	65	20.072
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3763	194222	1.94

Instrument :
BNA_G
ClientSampleId :
DFTPP