


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110222\
Data File : BG055415.D
Acq On : 2 Nov 2022 14:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Nov 07 00:51:08 2022

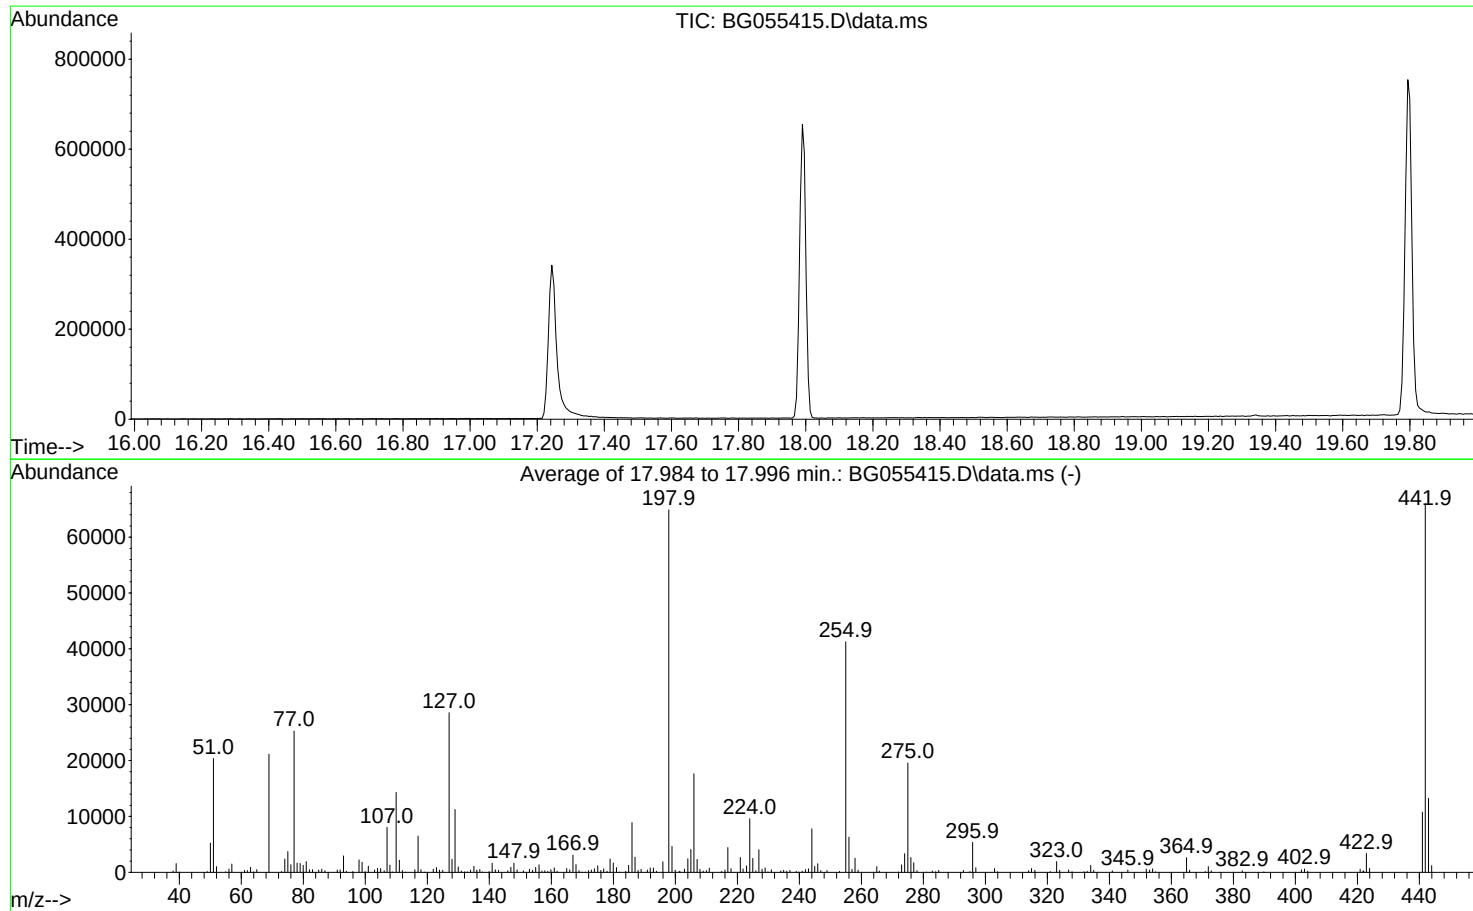




AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	20371	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.6	21149	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.0	28571	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	64891	PASS
199	198	5	9	7.1	4621	PASS
275	198	10	60	30.2	19574	PASS
365	198	1	100	4.0	2626	PASS
441	198	0.01	100	16.6	10755	PASS
442	442	50	100	100.0	65861	PASS
443	442	15	24	20.1	13217	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110222\
Data File : BG055415.D
Acq On : 2 Nov 2022 14:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 03 09:09:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 02 05:05:12 2022
Response via : Initial Calibration

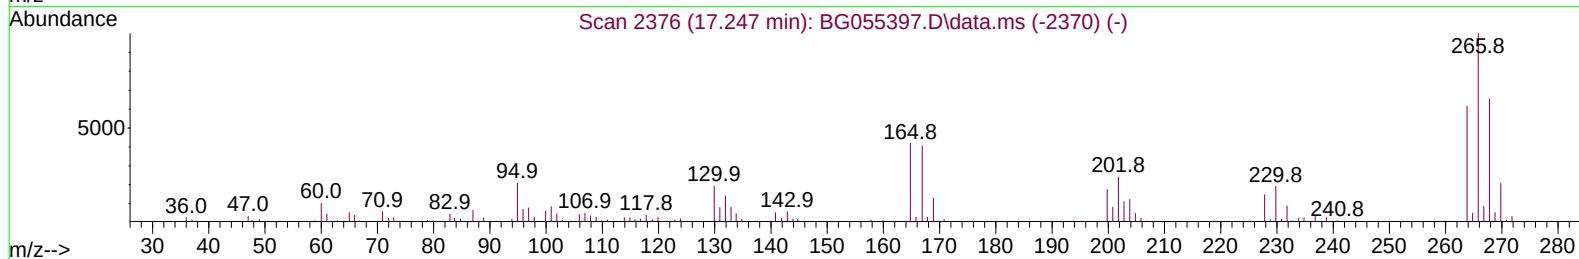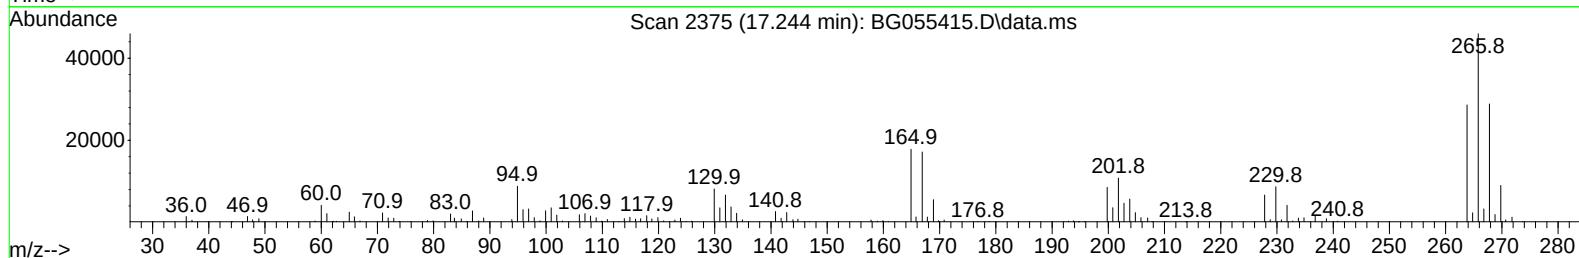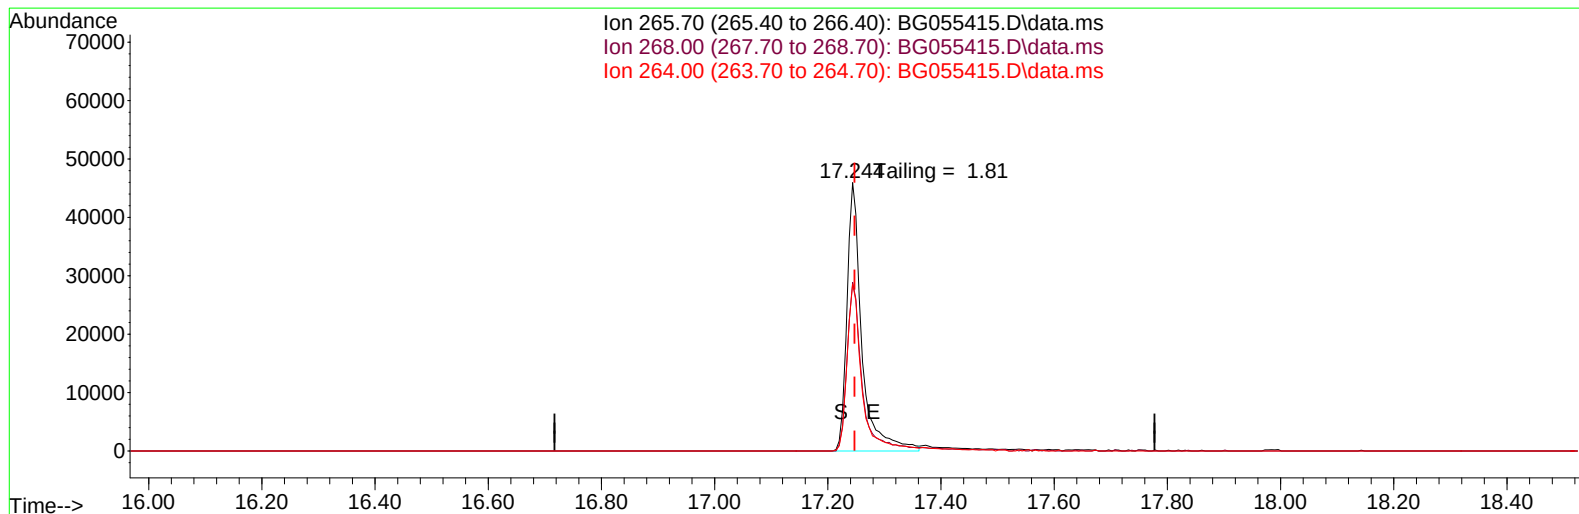

TIC: BG055415.D\data.ms

(70) Pentachlorophenol (C)

17.244min (-0.003) 31619.87 ng




response 84168

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	62.80
264.00	61.50	62.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110222\
Data File : BG055415.D
Acq On : 2 Nov 2022 14:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 03 09:09:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 02 05:05:12 2022
Response via : Initial Calibration

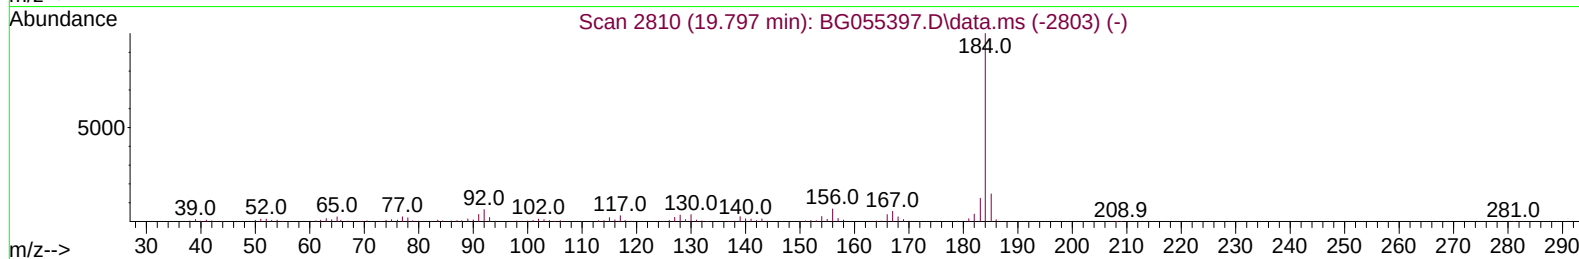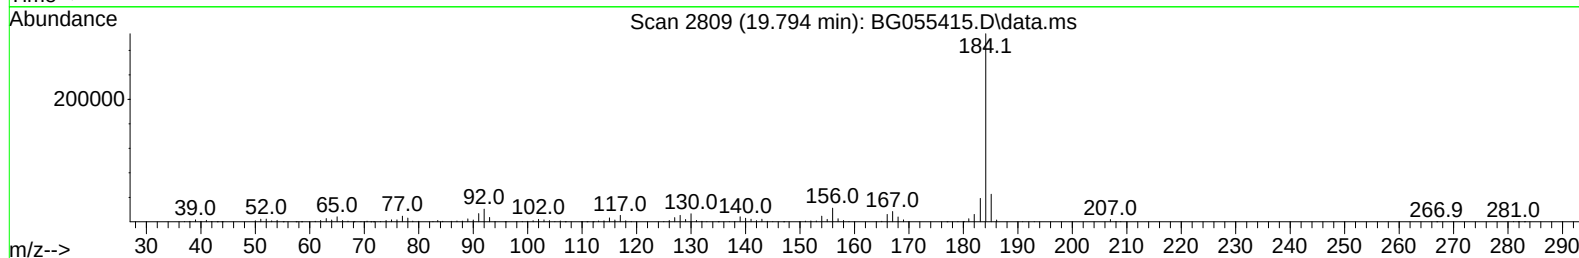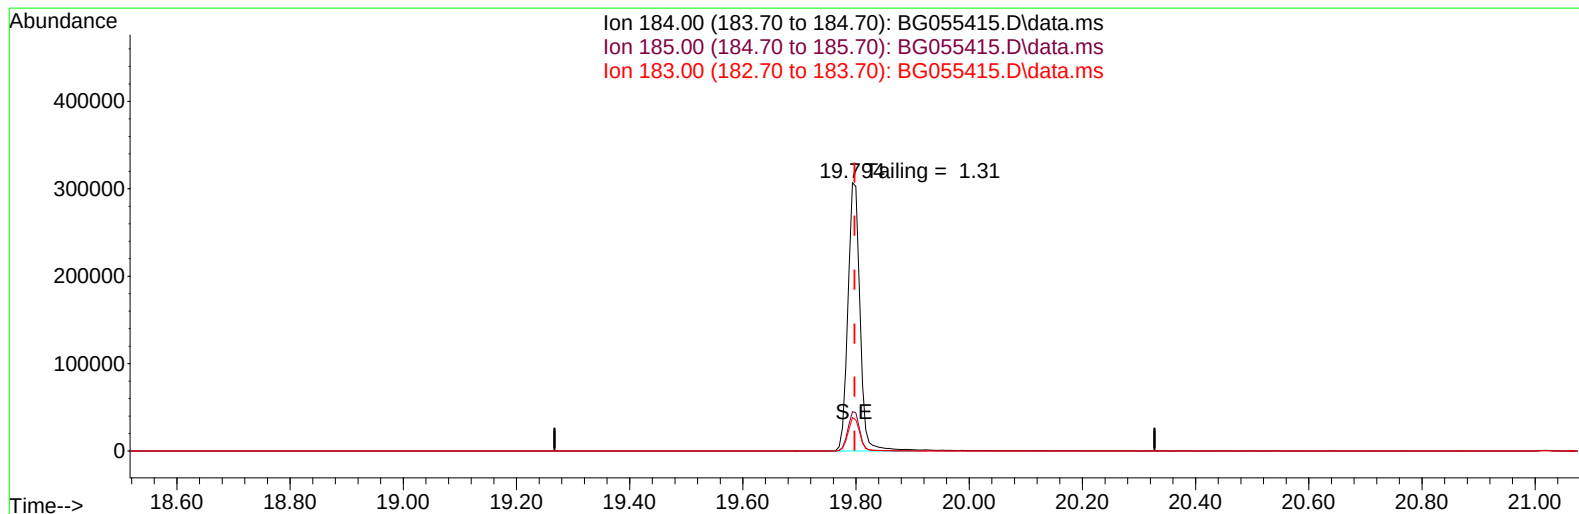

TIC: BG055415.D\data.ms

(77) Benzidine

19.794min (-0.003) 0.00 ng

response 454698

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.69
183.00	12.30	12.50
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/2/2022	BNA_G	<u>BG055415.D</u>
Compound Name	Response	Retention Time
DDT	225248	21.016
DDD	4428	20.622
DDE	253	20.07
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4681	229929	2.04

Instrument :
BNA_G
ClientSampleId :
DFTPP