

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110223\
 Data File : BG059599.D
 Acq On : 2 Nov 2023 10:55
 Operator : MA/JU
 Sample : PB156593BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK593

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059599.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.652	40	45	49	rBV2	18814	28720	0.90%	0.087%
2	3.793	66	69	71	rBV3	6032	6212	0.20%	0.019%
3	3.969	95	99	102	rBV4	7115	7683	0.24%	0.023%
4	4.081	113	118	126	rBV	206298	343044	10.79%	1.035%
5	4.422	171	176	180	rBV3	14239	23289	0.73%	0.070%
6	4.663	215	217	220	rVB3	7380	5657	0.18%	0.017%
7	5.168	301	303	305	rVB2	5759	5255	0.17%	0.016%
8	5.297	323	325	331	rBV3	3904	7434	0.23%	0.022%
9	5.426	344	347	349	rBV2	4760	5955	0.19%	0.018%
10	5.544	364	367	370	rBV2	5441	6227	0.20%	0.019%
11	5.655	383	386	388	rVB2	6509	6520	0.21%	0.020%
12	5.749	399	402	405	rBV2	6240	9418	0.30%	0.028%
13	6.026	442	449	453	rBV3	3155	6698	0.21%	0.020%
14	6.214	479	481	484	rVB3	7622	6477	0.20%	0.020%
15	6.690	559	562	564	rBV	5611	7616	0.24%	0.023%
16	6.819	577	584	586	rVB	6559	11730	0.37%	0.035%
17	7.295	664	665	668	rBV	5341	6273	0.20%	0.019%
18	7.465	687	694	703	rVV	348461	624782	19.66%	1.884%
19	7.547	705	708	710	rBV	4582	6021	0.19%	0.018%
20	7.671	722	729	735	rBV2	245055	407187	12.81%	1.228%
21	7.865	755	762	770	rVB	357999	628923	19.79%	1.897%
22	7.923	770	772	776	rBV	5649	7575	0.24%	0.023%
23	8.264	826	830	831	rVB	5526	5780	0.18%	0.017%
24	8.288	831	834	837	rBV	8214	10058	0.32%	0.030%
25	8.352	838	845	853	rVV2	247994	446372	14.05%	1.346%
26	8.511	866	872	874	rBV2	4344	8035	0.25%	0.024%
27	9.034	954	961	970	rVB2	486753	856910	26.96%	2.584%
28	9.298	1004	1006	1009	rBV2	6080	8657	0.27%	0.026%
29	9.551	1040	1049	1057	rBV	348166	613632	19.31%	1.851%
30	10.274	1163	1172	1179	rVB	308926	559589	17.61%	1.688%
31	10.432	1195	1199	1202	rBV2	11364	19268	0.61%	0.058%
32	10.456	1202	1203	1206	rVV	8620	7765	0.24%	0.023%
33	10.479	1206	1207	1210	rVB3	7736	5704	0.18%	0.017%
34	10.503	1210	1211	1213	rBV	9142	6397	0.20%	0.019%
35	10.620	1229	1231	1233	rBV2	7174	5994	0.19%	0.018%
36	10.738	1249	1251	1253	rBV	11552	7289	0.23%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110223\
 Data File : BG059599.D
 Acq On : 2 Nov 2023 10:55
 Operator : MA/JU
 Sample : PB156593BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK593

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

37	10.796	1253	1261	1268	rVV2	695505	1240936	39.05%	3.743%
38	10.914	1279	1281	1285	rBV3	6521	6284	0.20%	0.019%
39	10.979	1290	1292	1295	rVB3	6992	5521	0.17%	0.017%
40	11.002	1295	1296	1299	rBV2	7667	7244	0.23%	0.022%

41	11.202	1321	1330	1339	rBV	524723	971469	30.57%	2.930%
42	11.343	1347	1354	1361	rVV	689893	1234015	38.83%	3.722%
43	11.519	1381	1384	1388	rBV4	7268	10869	0.34%	0.033%
44	11.766	1424	1426	1428	rBV2	5334	5841	0.18%	0.018%
45	11.995	1463	1465	1467	rVB	7325	5749	0.18%	0.017%

46	12.177	1491	1496	1497	rBV	10257	12554	0.40%	0.038%
47	12.353	1524	1526	1529	rVB2	9636	9925	0.31%	0.030%
48	12.377	1529	1530	1534	rBV	11798	11605	0.37%	0.035%
49	12.759	1591	1595	1600	rVB4	15896	29910	0.94%	0.090%
50	13.012	1635	1638	1639	rBV	5217	6410	0.20%	0.019%

51	13.082	1647	1650	1651	rBV2	8623	9184	0.29%	0.028%
52	13.382	1698	1701	1703	rBV2	6355	6622	0.21%	0.020%
53	13.440	1709	1711	1715	rVB3	7530	9631	0.30%	0.029%
54	13.493	1718	1720	1723	rBV	8748	7208	0.23%	0.022%
55	13.599	1735	1738	1741	rBV3	7953	11383	0.36%	0.034%

56	13.740	1760	1762	1764	rVB2	8465	5702	0.18%	0.017%
57	13.816	1772	1775	1780	rVB5	18849	25538	0.80%	0.077%
58	14.104	1820	1824	1825	rBV5	5304	6618	0.21%	0.020%
59	14.375	1864	1870	1876	rBV	1300537	1890435	59.49%	5.702%
60	14.492	1888	1890	1892	rBV2	7715	6656	0.21%	0.020%

61	14.686	1916	1923	1930	rVB	1493099	2354389	74.09%	7.101%
62	14.739	1930	1932	1934	rVV3	7354	5630	0.18%	0.017%
63	14.757	1934	1935	1937	rVB2	9682	5606	0.18%	0.017%
64	14.780	1937	1939	1941	rBV	5791	5330	0.17%	0.016%
65	14.804	1941	1943	1946	rVV3	7546	6117	0.19%	0.018%

66	14.839	1946	1949	1950	rVV2	6334	5947	0.19%	0.018%
67	14.921	1961	1963	1965	rVB3	8931	5775	0.18%	0.017%
68	14.980	1967	1973	1981	rVB	883337	1354150	42.61%	4.084%
69	15.056	1983	1986	1987	rBV	7875	6126	0.19%	0.018%
70	15.097	1991	1993	1995	rBV	9496	6715	0.21%	0.020%

71	15.150	1995	2002	2009	rBV	710172	1084867	34.14%	3.272%
72	15.326	2030	2032	2036	rBV3	9438	14354	0.45%	0.043%
73	15.462	2054	2055	2058	rBV2	5980	6744	0.21%	0.020%
74	15.679	2091	2092	2094	rBV2	7477	5453	0.17%	0.016%
75	15.755	2104	2105	2109	rBV3	7655	7457	0.23%	0.022%

76	15.973	2135	2142	2150	rBV	1757788	2793714	87.91%	8.426%
----	--------	------	------	------	-----	---------	---------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110223\
 Data File : BG059599.D
 Acq On : 2 Nov 2023 10:55
 Operator : MA/JU
 Sample : PB156593BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK593

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
 Title : SVOA CALIBRATION

77	16.073	2153	2159	2165	rBV	557413	817157	25.71%	2.465%
78	16.208	2180	2182	2184	rVB3	12501	9690	0.30%	0.029%
79	16.866	2292	2294	2297	rBV3	7237	6184	0.19%	0.019%
80	17.236	2355	2357	2361	rBV3	6906	5865	0.18%	0.018%
81	17.330	2372	2373	2376	rVB3	8921	6653	0.21%	0.020%
82	17.406	2384	2386	2387	rVB2	12509	6620	0.21%	0.020%
83	17.512	2402	2404	2406	rBV3	5886	6071	0.19%	0.018%
84	17.577	2413	2415	2417	rBV2	5596	5725	0.18%	0.017%
85	17.735	2435	2442	2451	rVB	1053584	1655859	52.11%	4.994%
86	17.835	2451	2459	2467	rBV	2034737	3138801	98.77%	9.467%
87	17.941	2474	2477	2479	rBV4	8352	9752	0.31%	0.029%
88	18.247	2527	2529	2531	rBV3	7728	9448	0.30%	0.028%
89	18.558	2578	2582	2588	rVB8	10230	20260	0.64%	0.061%
90	18.805	2623	2624	2625	rBV	14032	5278	0.17%	0.016%
91	19.040	2662	2664	2667	rBV4	8199	7250	0.23%	0.022%
92	19.093	2671	2673	2677	rBV5	12424	19377	0.61%	0.058%
93	19.292	2705	2707	2709	rBV3	11513	8176	0.26%	0.025%
94	19.328	2712	2713	2715	rBV2	9630	5660	0.18%	0.017%
95	19.663	2767	2770	2774	rBV3	37869	56689	1.78%	0.171%
96	19.733	2780	2782	2785	rVB3	26679	22287	0.70%	0.067%
97	20.103	2839	2845	2852	rVB	2182714	3177916	100.00%	9.585%
98	22.066	3173	3179	3186	rVB2	871116	1566694	49.30%	4.725%
99	25.426	3741	3751	3763	rVB	987213	3046526	95.87%	9.188%
100	25.673	3785	3793	3807	rVB3	515196	1606676	50.56%	4.846%




Sum of corrected areas: 33156443

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110223\
Data File : BG059599.D
Acq On : 2 Nov 2023 10:55
Operator : MA/JU
Sample : PB156593BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK593

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

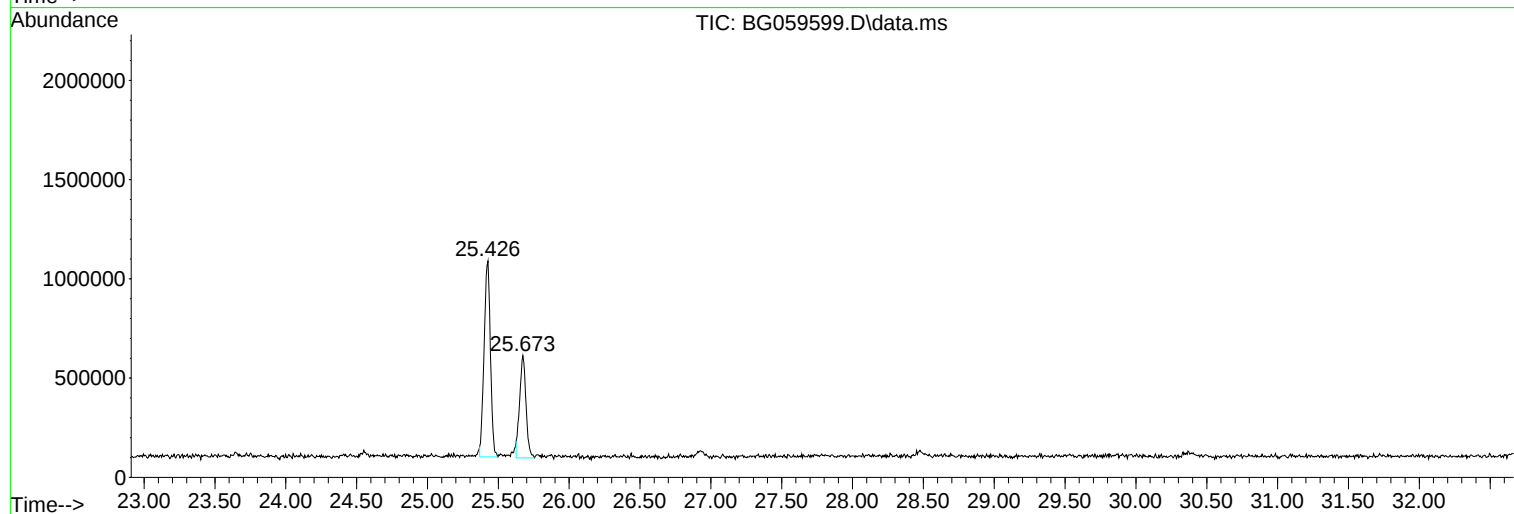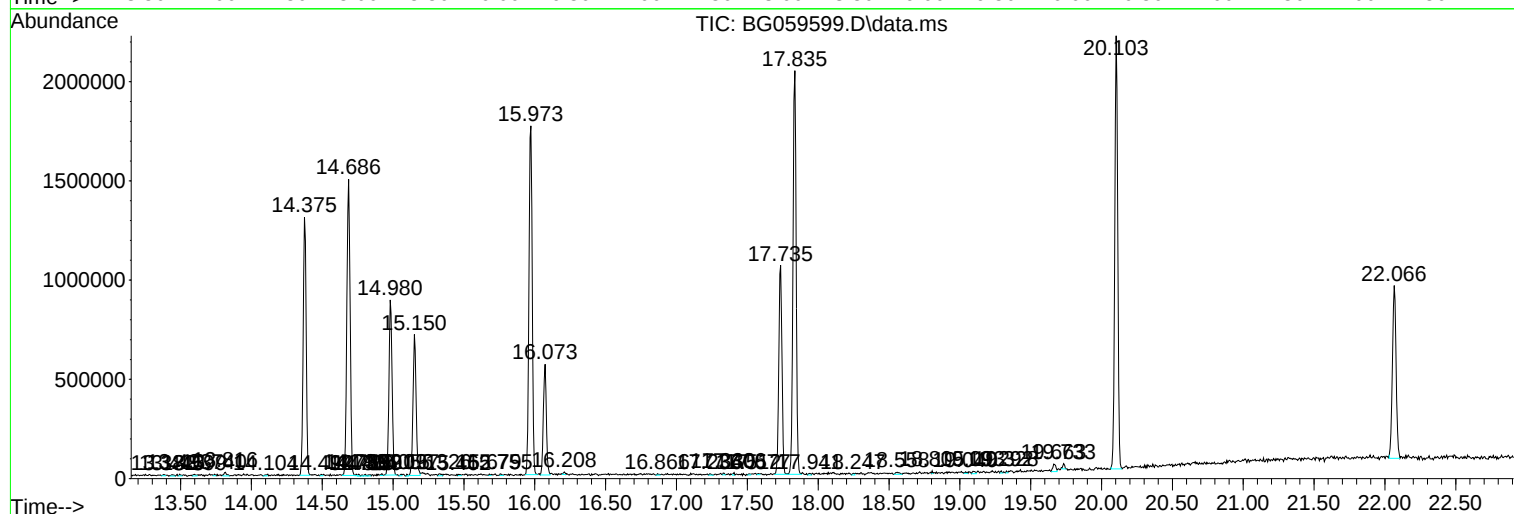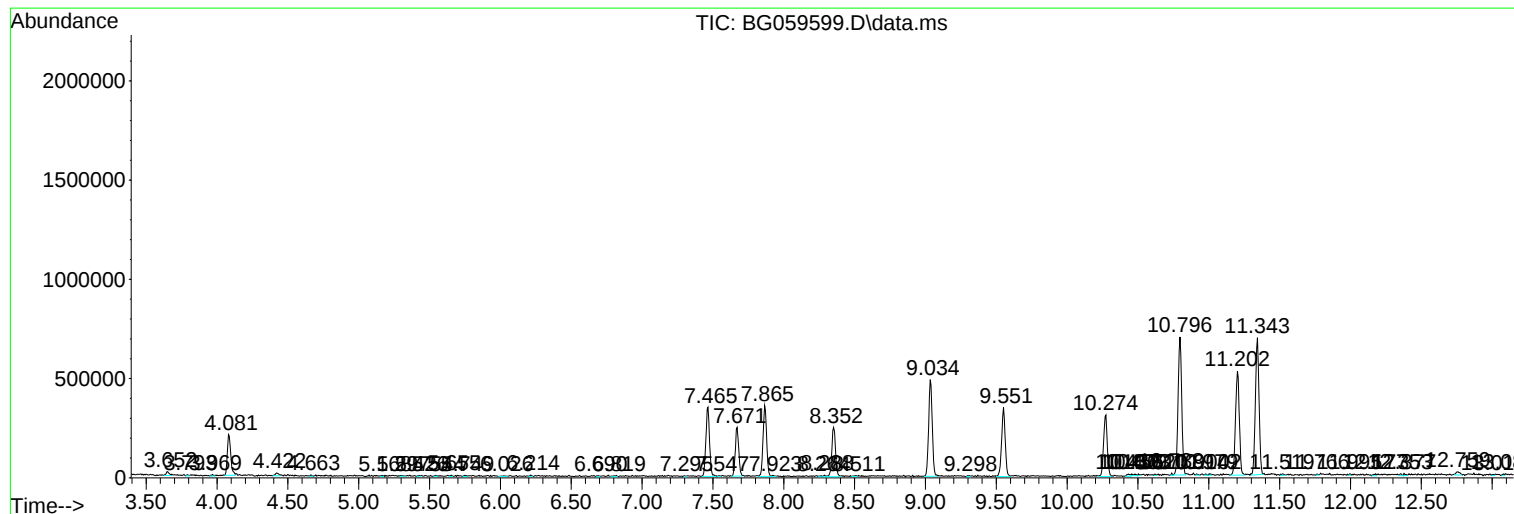

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110223\
Data File : BG059599.D
Acq On : 2 Nov 2023 10:55
Operator : MA/JU
Sample : PB156593BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK593

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110223\
Data File : BG059599.D
Acq On : 2 Nov 2023 10:55
Operator : MA/JU
Sample : PB156593BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK593

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG102723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc