
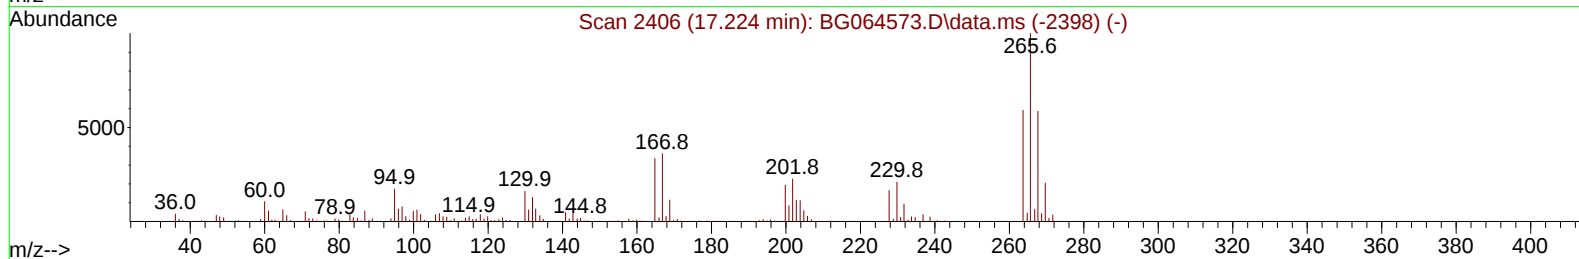
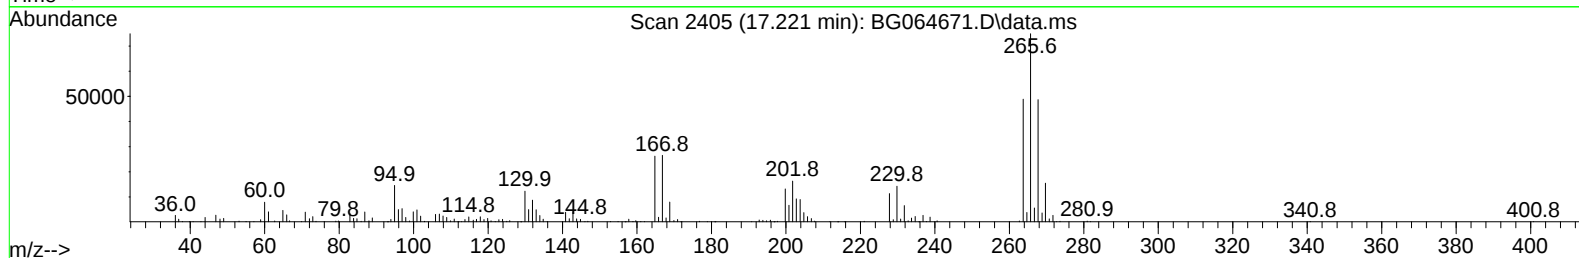


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110325\
Data File : BG064671.D
Acq On : 3 Nov 2025 13:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 01:35:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 03 18:16:26 2025
Response via : Initial Calibration

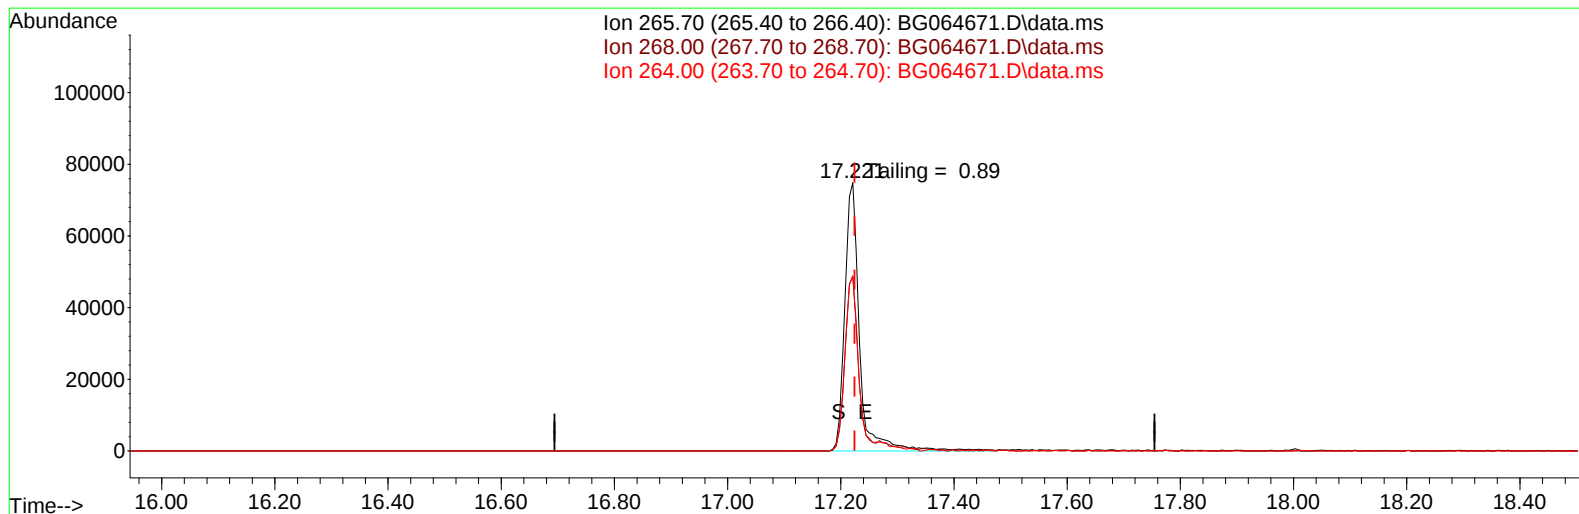

TIC: BG064671.D\data.ms

(70) Pentachlorophenol (C)




17.221min (-0.003) 285068.28 ng

response 132179

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	65.04
264.00	59.10	70.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110325\
Data File : BG064671.D
Acq On : 3 Nov 2025 13:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 01:35:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 03 18:16:26 2025
Response via : Initial Calibration

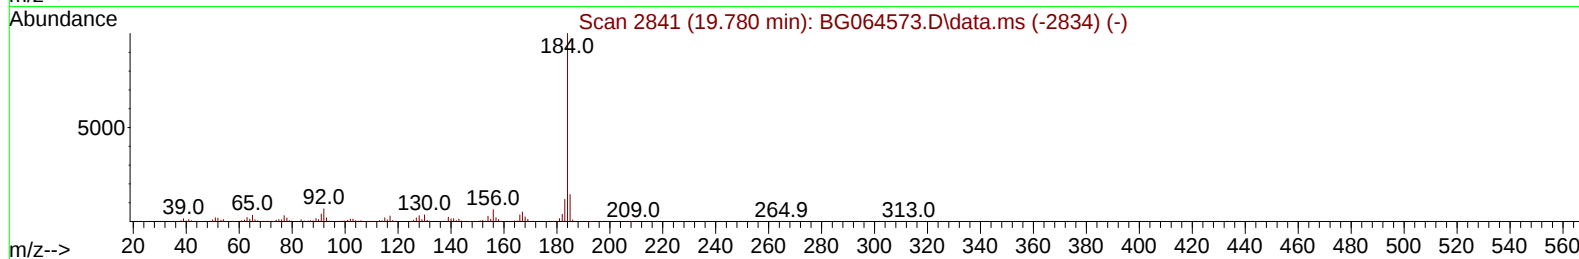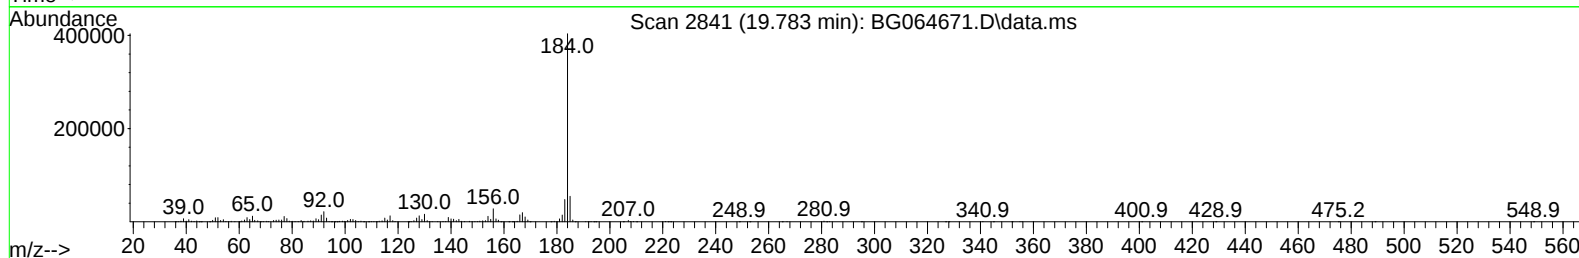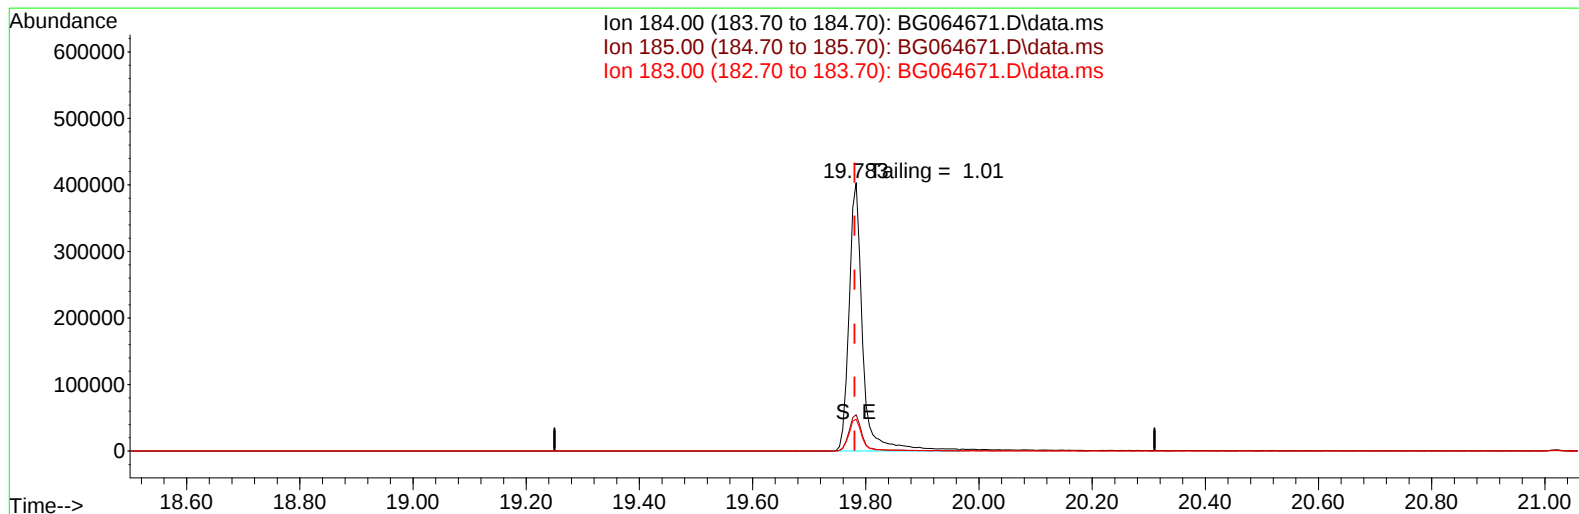

TIC: BG064671.D\data.ms

(77) Benzidine

19.783min (+ 0.003) 139043.84 ng

response 672874

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.55
183.00	11.80	11.90
0.00	0.00	0.00