

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG110518\
 Data File : BG037832.D
 Acq On : 6 Nov 2018 10:16
 Operator : JU/SJ
 Sample : J5764-20
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Nov 06 12:29:47 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 18 14:06:42 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.09	152	59815	20.00	ng	-0.02
21) Naphthalene-d8	10.91	136	265559	20.00	ng	-0.02
39) Acenaphthene-d10	14.73	164	171852	20.00	ng	-0.02
64) Phenanthrene-d10	17.48	188	375120	20.00	ng	0.00
76) Chrysene-d12	21.76	240	327327	20.00	ng	-0.02
87) Perylene-d12	25.09	264	272914	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	383562	107.21	ng	0.00
7) Phenol-d6	7.24	99	482784	89.24	ng	0.00
23) Nitrobenzene-d5	9.27	82	385558	81.33	ng	0.00
42) 2,4,6-Tribromophenol	16.22	330	187400	99.98	ng	0.00
45) 2-Fluorobiphenyl	13.35	172	948215	83.20	ng	-0.02
79) Terphenyl-d14	20.07	244	1292921	84.40	ng	-0.02
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.27	70	48932	13.135	ng	# 70
51) 2,6-Dinitrotoluene	14.73	165	22632	7.695	ng	# 26
57) 2,4-Dinitrotoluene	14.73	165	22632	5.862	ng	# 26
65) 4,6-Dinitro-2-methylphenol	16.21	198	430	8.687	ng	# 70
67) 4-Bromophenyl-phenylether	16.22	248	13173	3.198	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG110518\
Data File : BG037832.D
Acq On : 6 Nov 2018 10:16
Operator : JU/SJ
Sample : J5764-20
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Nov 06 12:29:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

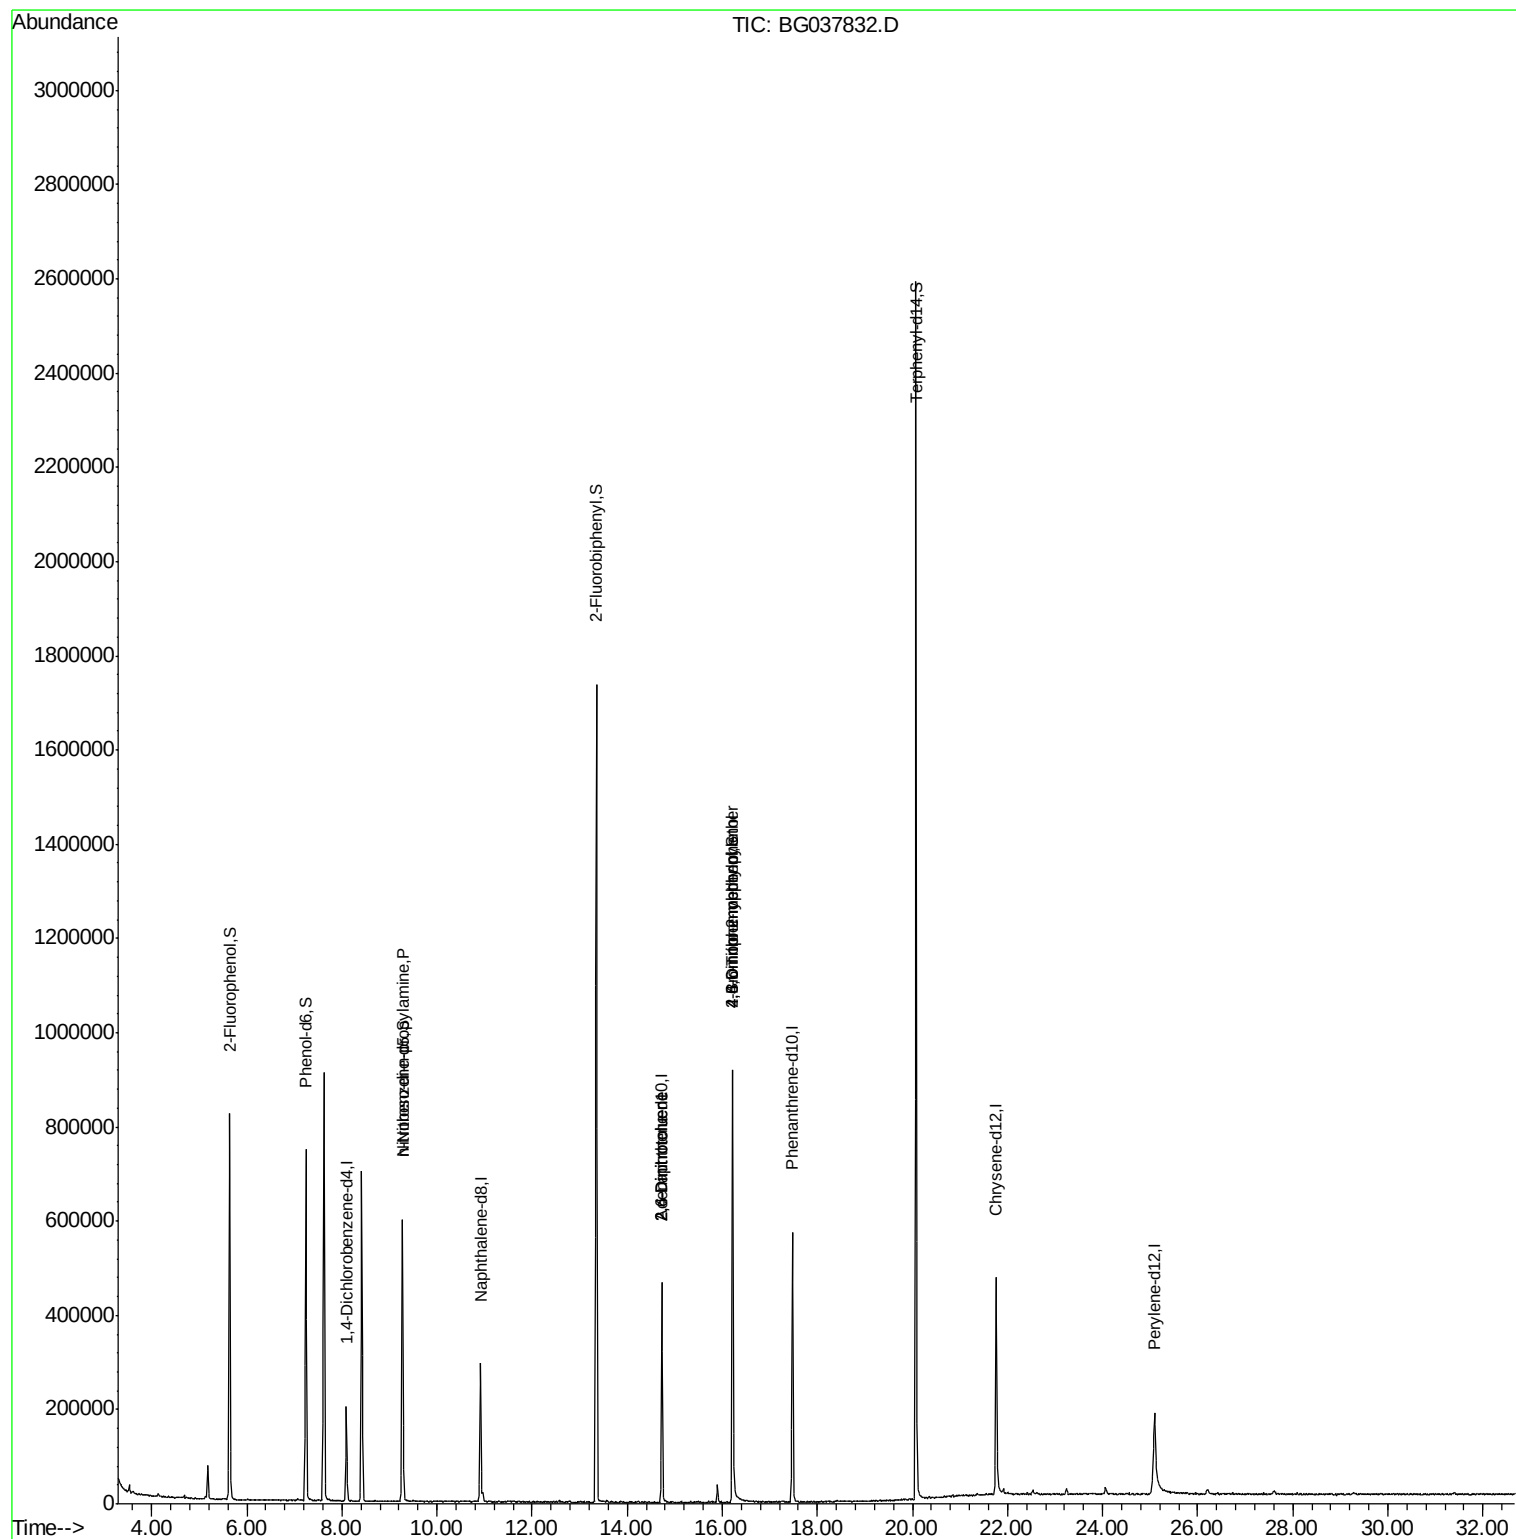




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.09 min Scan# 818
Delta R.T. -0.02 min
Lab File: BG037832.D
Acq: 6 Nov 2018 10:16

Instrument :
BNA_G
ClientSampleId :

Tot Ion:152 Resp: 59815
Ion Ratio Lower Upper
152 100
150 150.4 126.0 189.0
115 55.8 45.5 68.3

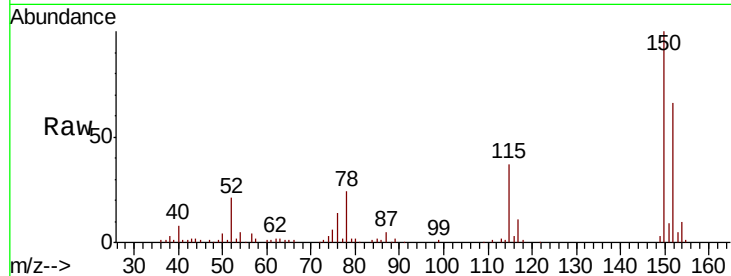


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

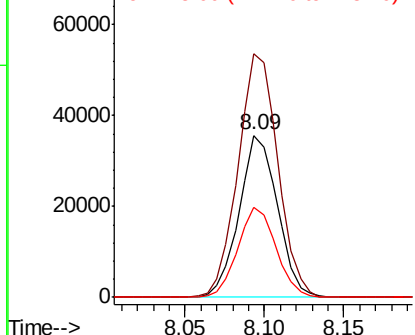



#5


2-Fluorophenol
Concen: 107.207 ng
RT: 5.64 min Scan# 400
Delta R.T. -0.01 min
Lab File: BG037832.D
Acq: 6 Nov 2018 10:16

Tgt Ion:112 Resp: 383562
Ion Ratio Lower Upper
112 100
64 66.0 53.1 79.7
63 33.2 27.3 40.9

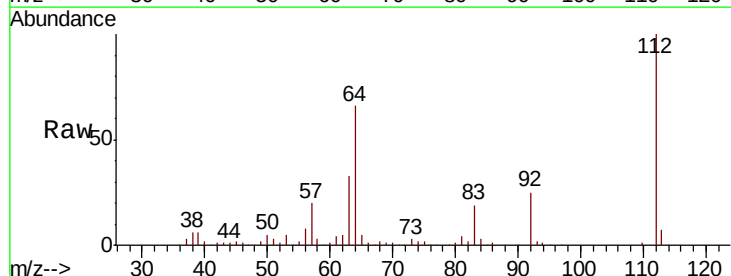

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

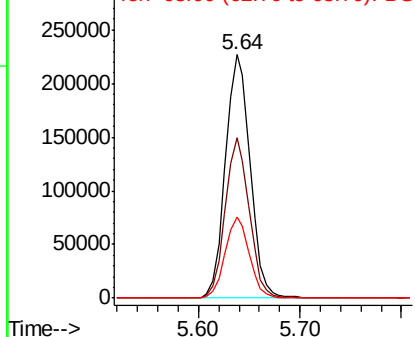

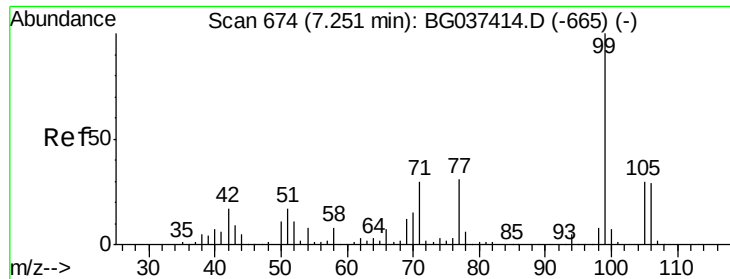

#7

Phenol-d6

Concen: 89.239 ng

RT: 7.24 min Scan# 673

Delta R.T. -0.01 min

Lab File: BG037832.D

Acq: 6 Nov 2018 10:16

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 482784

Ion Ratio Lower Upper




99 100

42 17.7 15.0 22.4

71 30.0 25.5 38.3

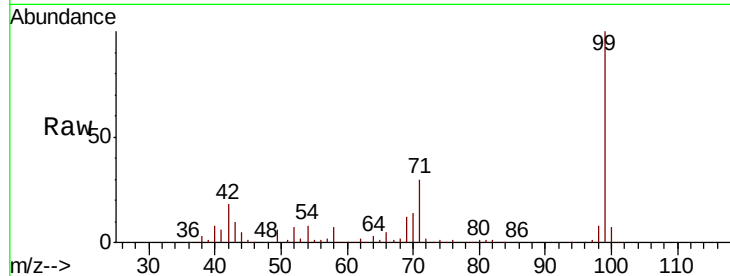

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

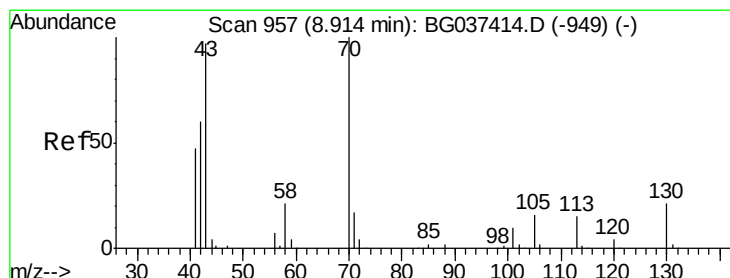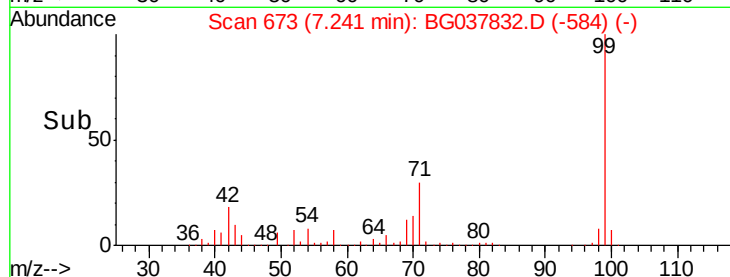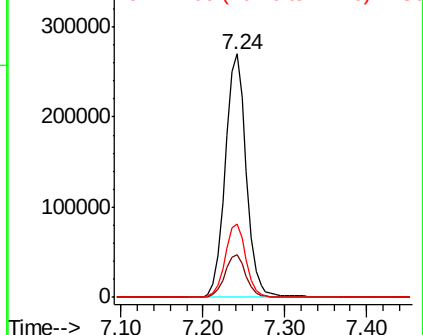

#19

n-Nitroso-di-n-propylamine

Concen: 13.135 ng

RT: 9.27 min Scan# 1018

Delta R.T. 0.35 min

Lab File: BG037832.D

Acq: 6 Nov 2018 10:16

Tgt Ion: 70 Resp: 48932


Ion Ratio Lower Upper

70 100



42 46.0 53.9 80.9#


101 0.0 8.2 12.2#

130 3.0 18.2 27.4#

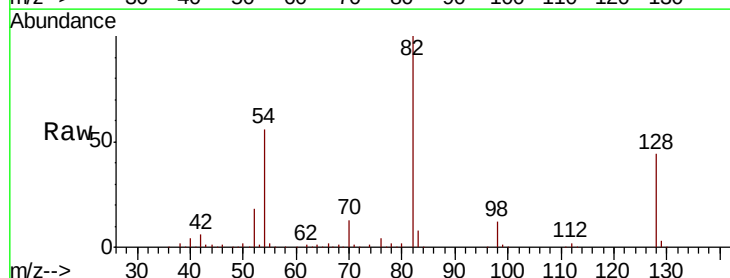

Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

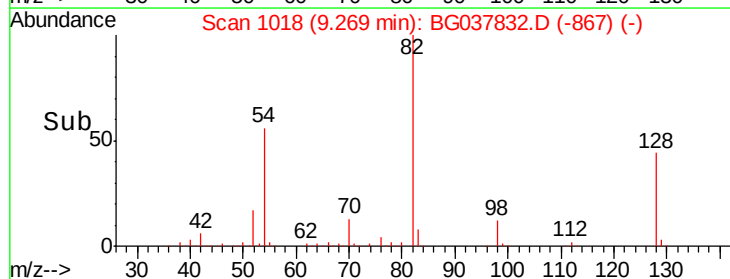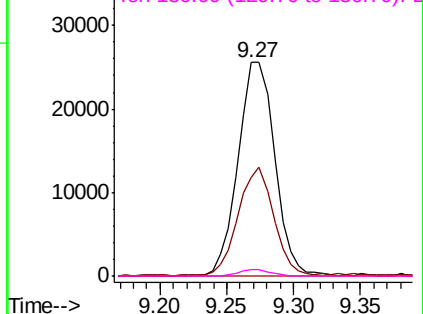


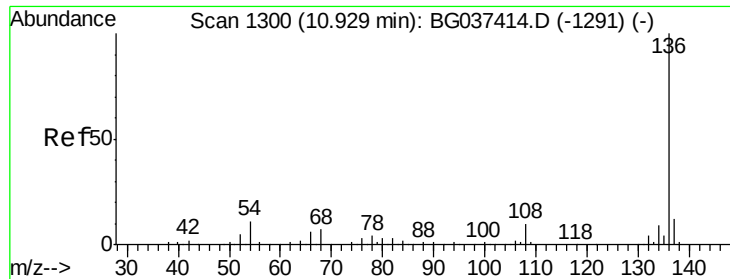




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.91 min Scan# 1298
Delta R.T. -0.02 min
Lab File: BG037832.D
Acq: 6 Nov 2018 10:16

Instrument :
BNA_G
ClientSampleId :

Tot Ion:136	Resp:	265559
Ion	Ratio	Lower Upper
136	100	
137	11.5	9.6 14.4
54	9.3	7.9 11.9
68	6.3	4.8 7.2

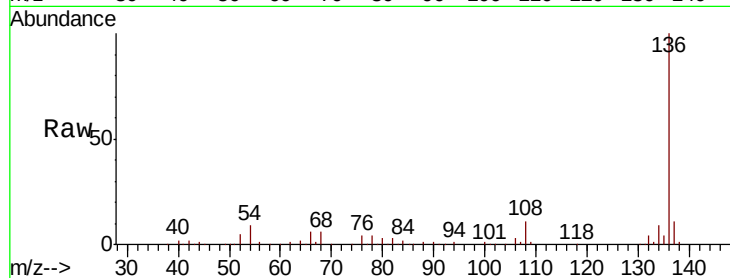


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

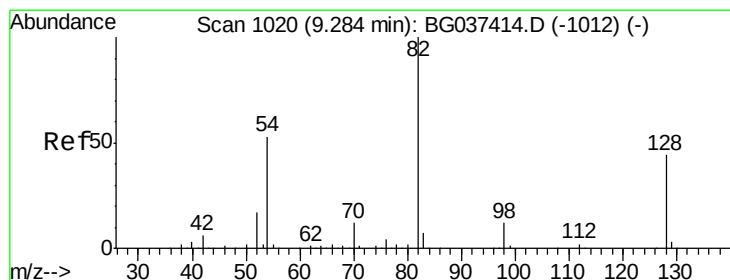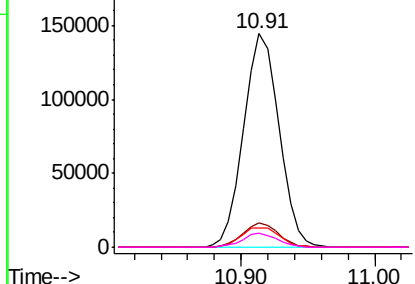
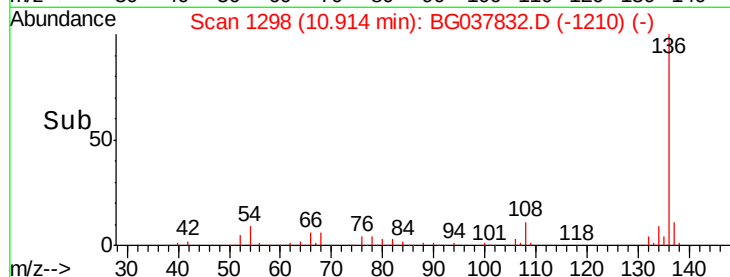



#23
Nitrobenzene-d5
Concen: 81.332 ng
RT: 9.27 min Scan# 1019
Delta R.T. -0.01 min
Lab File: BG037832.D
Acq: 6 Nov 2018 10:16

Tgt Ion: 82	Resp:	385558
Ion	Ratio	Lower Upper
82	100	
128	46.2	34.6 51.8
54	53.7	45.3 67.9

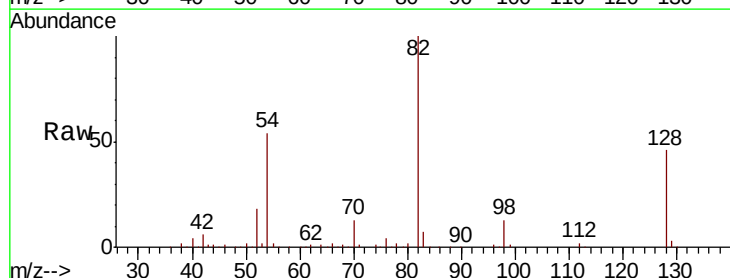

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

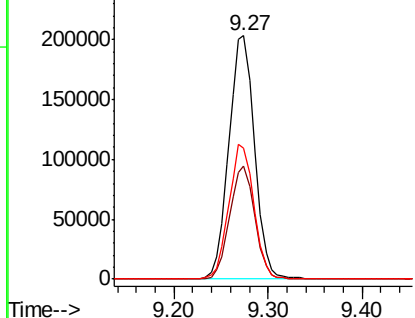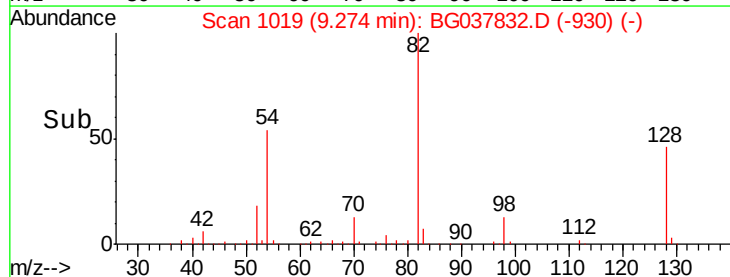

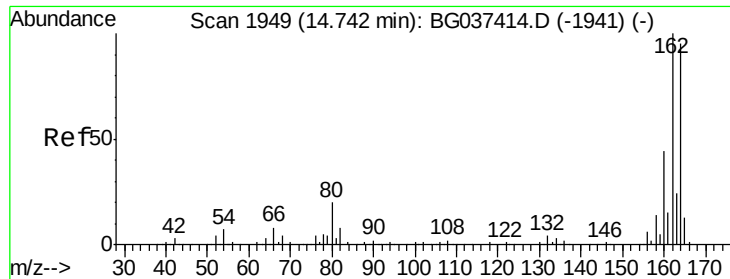

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.73 min Scan# 1947

Delta R.T. -0.02 min

Lab File: BG037832.D

Acq: 6 Nov 2018 10:16

Instrument :

BNA_G

ClientSampleId :


Tot Ion:164 Resp: 171852

Ion Ratio Lower Upper

164 100

162 101.5 81.3 121.9




160 44.7 36.3 54.5

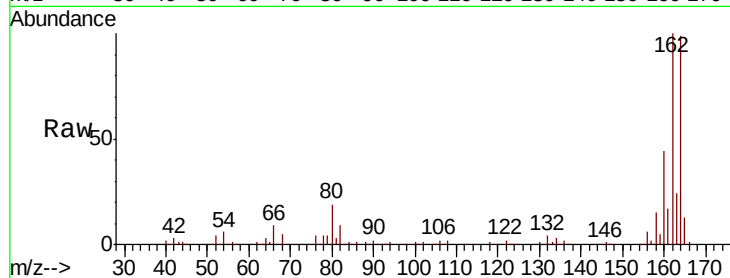

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

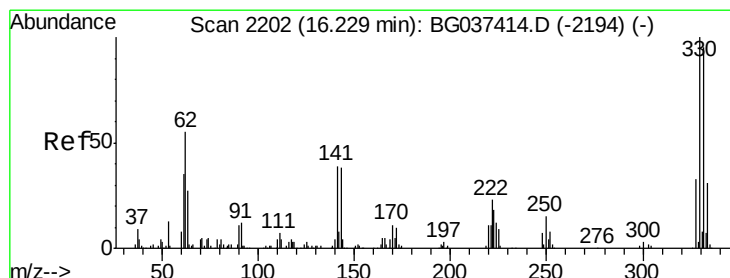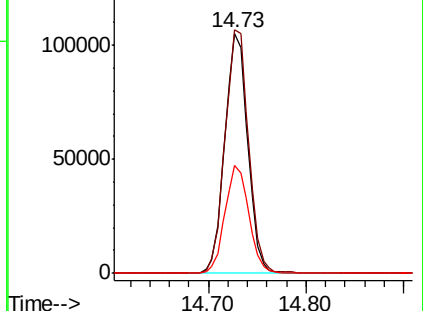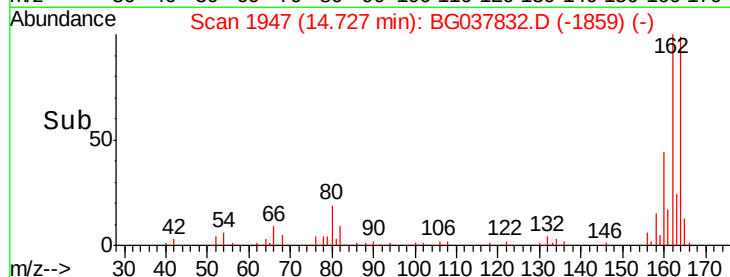

#42

2,4,6-Tribromophenol

Concen: 99.980 ng

RT: 16.22 min Scan# 2201

Delta R.T. -0.01 min

Lab File: BG037832.D

Acq: 6 Nov 2018 10:16


Tgt Ion:330 Resp: 187400

Ion Ratio Lower Upper

330 100

332 97.1 78.4 117.6



141 40.1 32.2 48.2

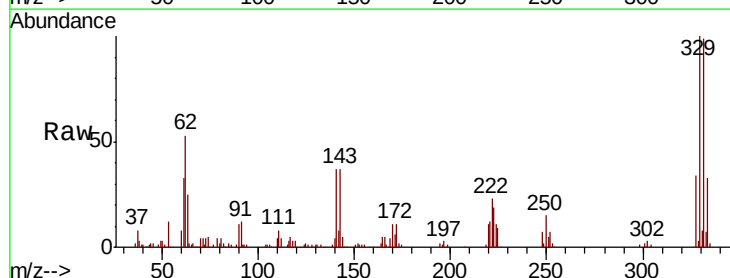


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

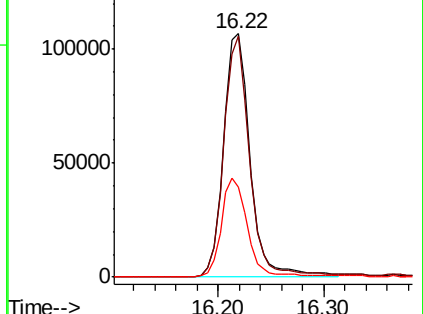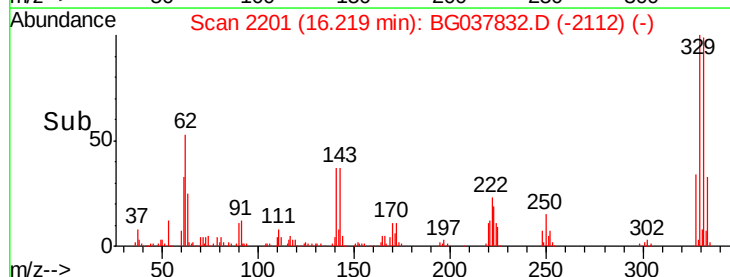





#45
 2-Fluorobiphenyl
 Concen: 83.203 ng
 RT: 13.35 min Scan# 1713
 Delta R.T. -0.02 min
 Lab File: BG037832.D
 Acq: 6 Nov 2018 10:16

Instrument :
 BNA_G
 ClientSampleId :



Tot Ion:	172	Resp:	948215
Ion	Ratio	Lower	Upper
172	100		
171	38.3	31.0	46.4
170	25.1	20.2	30.2



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

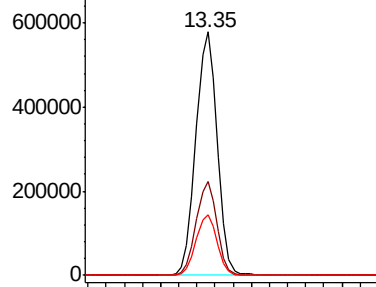


Time-->




#51
 2,6-Dinitrotoluene
 Concen: 7.695 ng
 RT: 14.73 min Scan# 1947
 Delta R.T. 0.41 min
 Lab File: BG037832.D
 Acq: 6 Nov 2018 10:16


Tgt Ion:	165	Resp:	22632
Ion	Ratio	Lower	Upper
165	100		
63	2.6	43.4	65.2#
89	1.6	45.8	68.6#




Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BGC
 Ion 89.00 (88.70 to 89.70): BGC

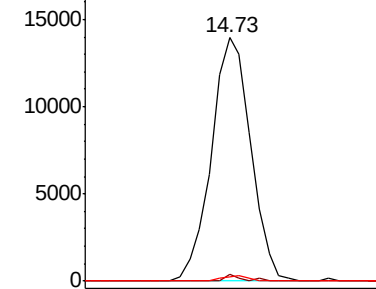

Time-->









#57
 2,4-Dinitrotoluene
 Concen: 5.862 ng
 RT: 14.73 min Scan# 1947
 Delta R.T. -0.37 min
 Lab File: BG037832.D
 Acq: 6 Nov 2018 10:16




Instrument :
 BNA_G
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
165	100		
63	2.6	33.4	50.0#
89	1.6	57.2	85.8#
182	0.0	2.6	4.0#

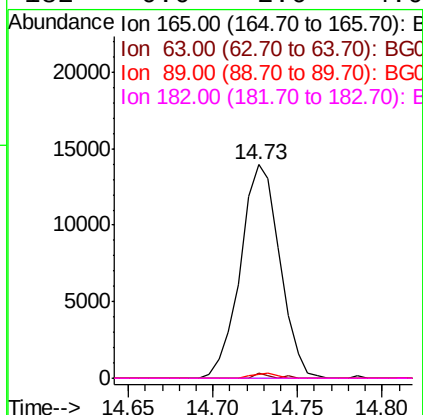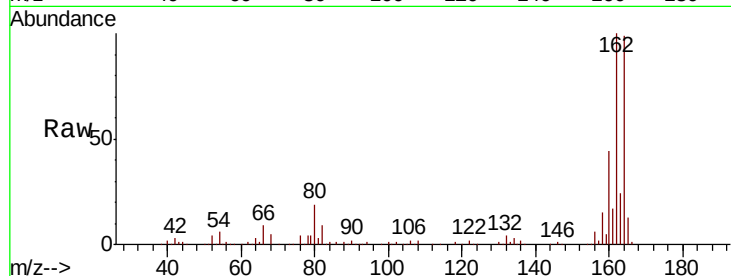

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.48 min Scan# 2415
 Delta R.T. -0.01 min
 Lab File: BG037832.D
 Acq: 6 Nov 2018 10:16

Tgt Ion	Ratio	Lower	Upper
188	100		
94	9.2	7.2	10.8
80	9.5	7.7	11.5

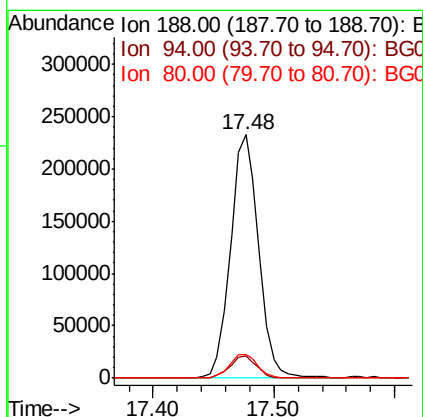

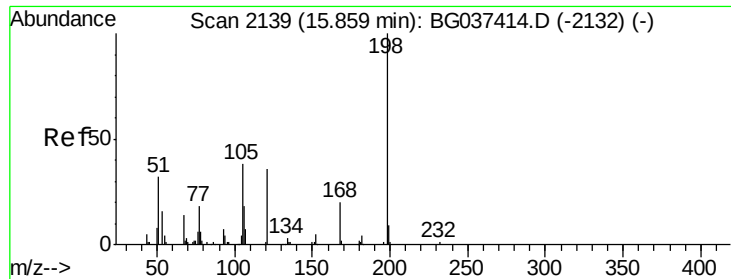

#65

4,6-Dinitro-2-methylphenol

Concen: 8.687 ng

RT: 16.21 min Scan# 2200

Delta R.T. 0.36 min

Lab File: BG037832.D

Acq: 6 Nov 2018 10:16

Instrument :

BNA_G

ClientSampled :


Tot Ion:198 Resp: 430

Ion Ratio Lower Upper

198 100

51 21.5 22.7 62.7#




105 23.9 19.7 59.7

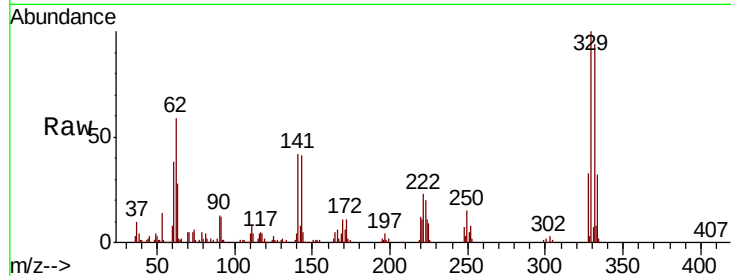

Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BG0

Ion 105.00 (104.70 to 105.70): E

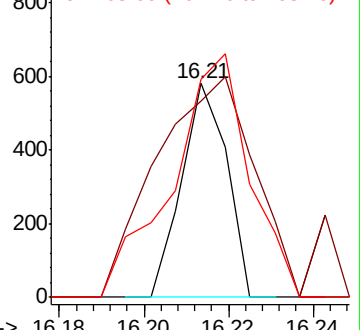

#67

4-Bromophenyl-phenylether

Concen: 3.198 ng

RT: 16.22 min Scan# 2201

Delta R.T. -0.45 min

Lab File: BG037832.D

Acq: 6 Nov 2018 10:16


Tgt Ion:248 Resp: 13173

Ion Ratio Lower Upper

248 100

250 199.9 77.0 115.6#



141 387.6 55.5 83.3#




Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E




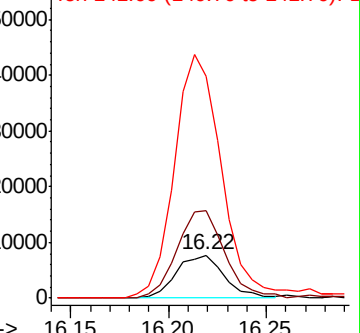




#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.76 min Scan# 3144
Delta R.T. -0.02 min
Lab File: BG037832.D
Acq: 6 Nov 2018 10:16




Instrument :
BNA_G
ClientSampleId :


Tot Ion:240 Resp: 327327
Ion Ratio Lower Upper
240 100
120 11.2 8.1 12.1
236 26.8 21.4 32.0

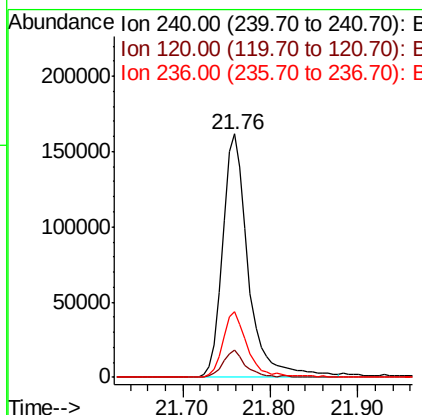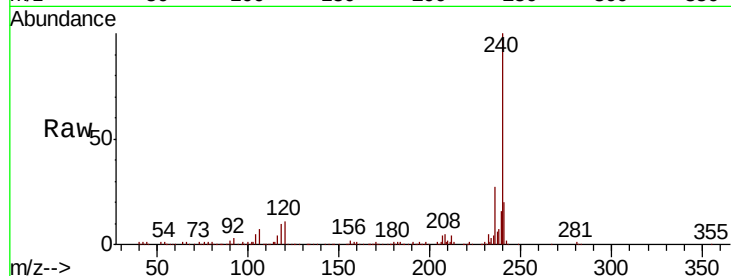

#79
Terphenyl-d14
Concen: 84.401 ng
RT: 20.07 min Scan# 2857
Delta R.T. -0.02 min
Lab File: BG037832.D
Acq: 6 Nov 2018 10:16

Tgt Ion:244 Resp: 1292921
Ion Ratio Lower Upper
244 100
212 8.3 6.5 9.7
122 11.3 9.0 13.4

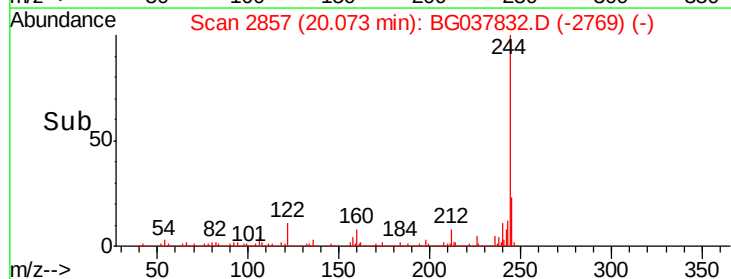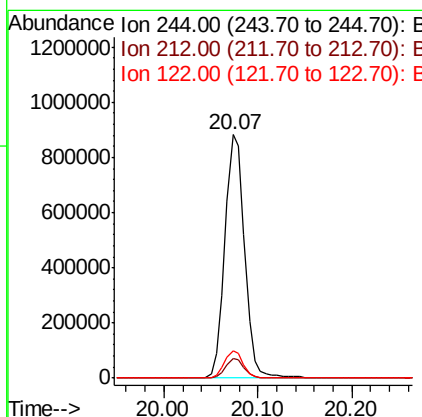


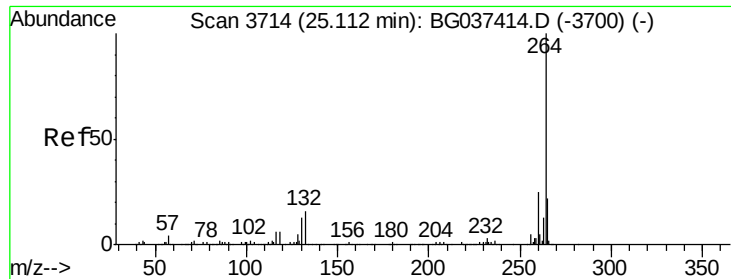

#87
Pervlene-d12
Concen: 20.000 ng
RT: 25.09 min Scan# 3711
Delta R.T. -0.02 min
Lab File: BG037832.D
Acq: 6 Nov 2018 10:16

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	22.6	18.2	27.4
265	20.3	17.9	26.9



Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

