

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG110518\
 Data File : BG037823.D
 Acq On : 6 Nov 2018 4:11
 Operator : JU/SJ
 Sample : PB114495BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB114495BL

Quant Time: Nov 06 06:05:17 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 18 14:06:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	64721	20.00	ng	-0.01
21) Naphthalene-d8	10.92	136	293118	20.00	ng	-0.01
39) Acenaphthene-d10	14.73	164	194060	20.00	ng	-0.01
64) Phenanthrene-d10	17.47	188	426239	20.00	ng	-0.01
76) Chrysene-d12	21.76	240	382774	20.00	ng	-0.02
87) Perylene-d12	25.09	264	337025	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	559007	144.40	ng	0.00
7) Phenol-d6	7.24	99	809257	138.25	ng	0.00
23) Nitrobenzene-d5	9.27	82	483447	92.39	ng	-0.01
42) 2,4,6-Tribromophenol	16.22	330	263209	124.36	ng	-0.01
45) 2-Fluorobiphenyl	13.35	172	1194202	92.80	ng	-0.02
79) Terphenyl-d14	20.08	244	1662346	92.80	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG110518\
Data File : BG037823.D
Acq On : 6 Nov 2018 4:11
Operator : JU/SJ
Sample : PB114495BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB114495BL

Quant Time: Nov 06 06:05:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

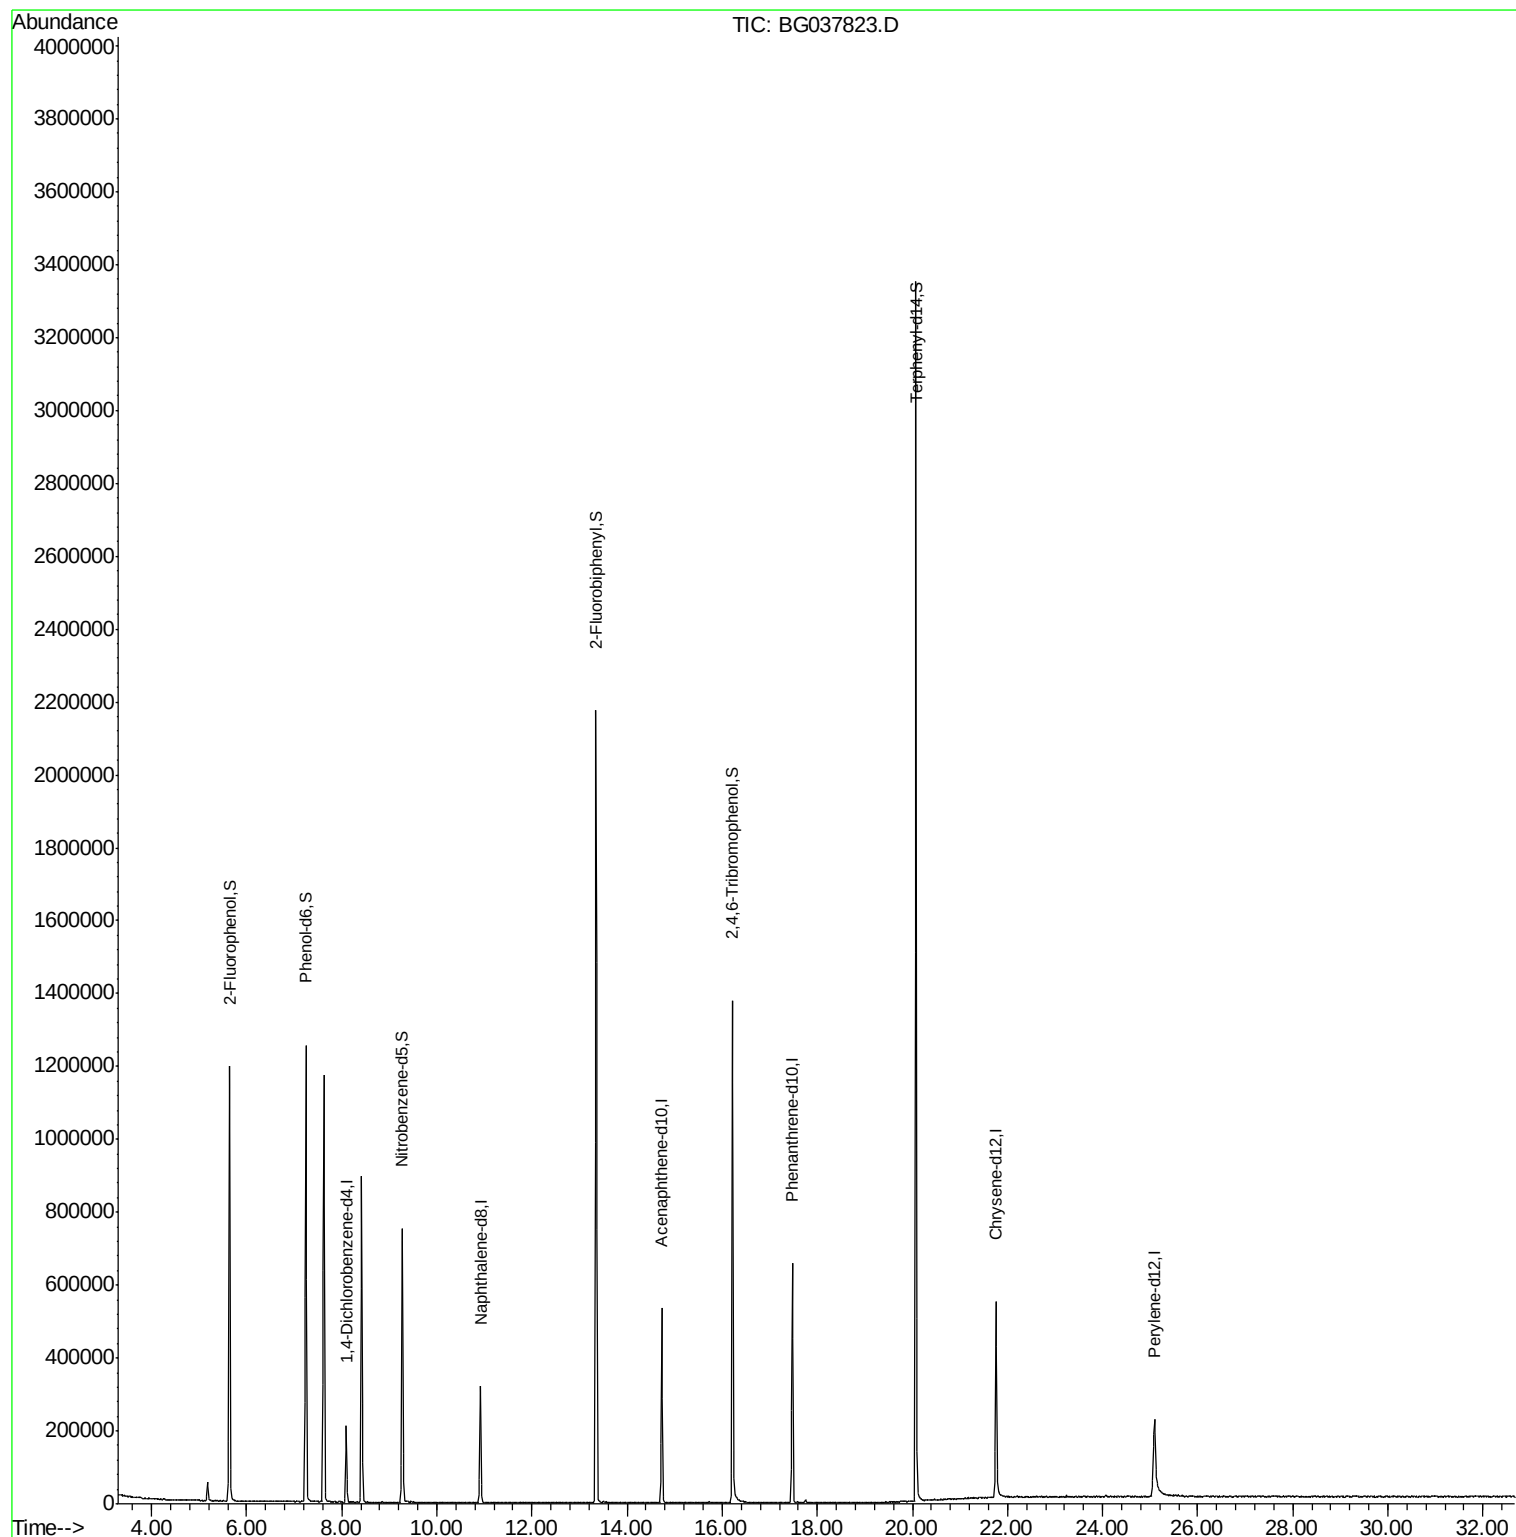

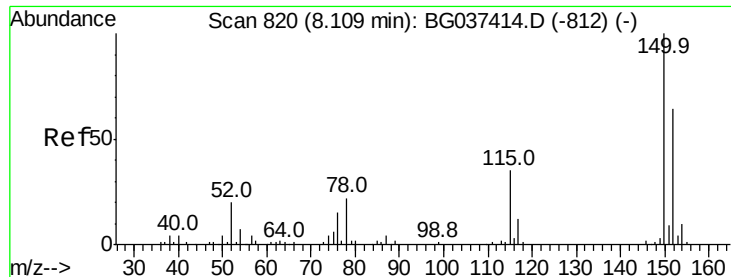


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.10 min Scan# 818
Delta R.T. -0.01 min
Lab File: BG037823.D
Acq: 6 Nov 2018 4:11

Instrument :
BNA_G
ClientSampleId :
PB114495BL

Tot Ion:152 Resp: 64721
Ion Ratio Lower Upper
152 100
150 155.3 126.0 189.0
115 57.4 45.5 68.3

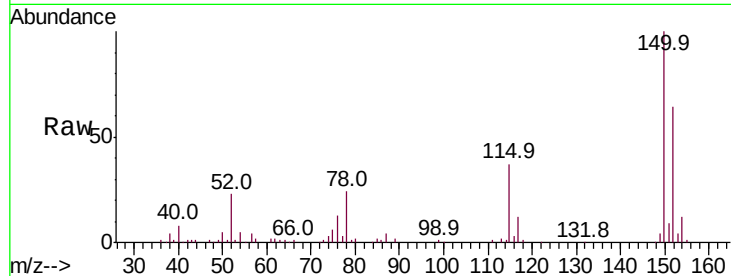


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

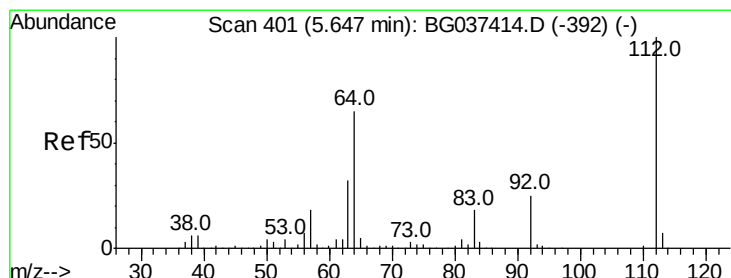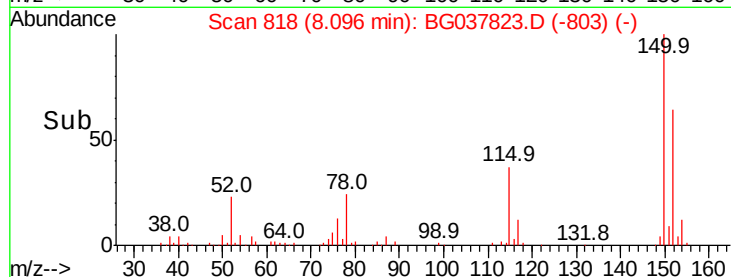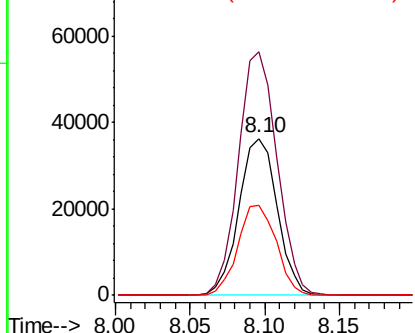



#5


2-Fluorophenol
Concen: 144.401 ng
RT: 5.64 min Scan# 400
Delta R.T. -0.01 min
Lab File: BG037823.D
Acq: 6 Nov 2018 4:11

Tgt Ion:112 Resp: 559007
Ion Ratio Lower Upper
112 100
64 65.5 53.1 79.7
63 33.1 27.3 40.9

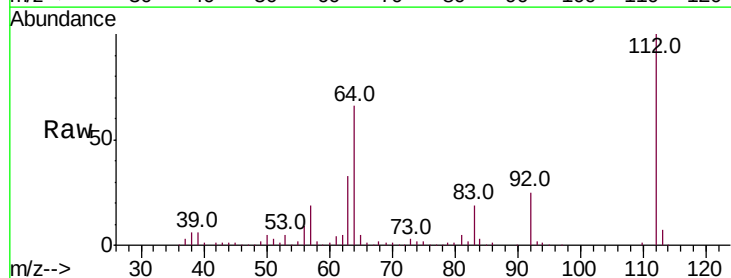

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

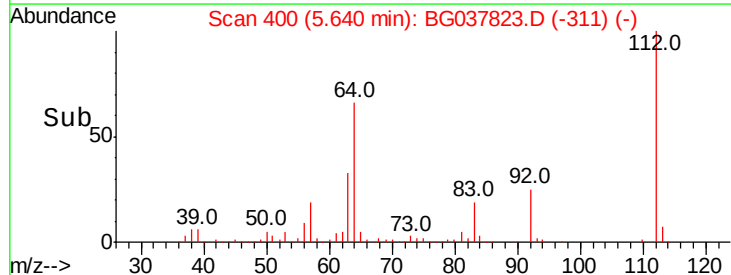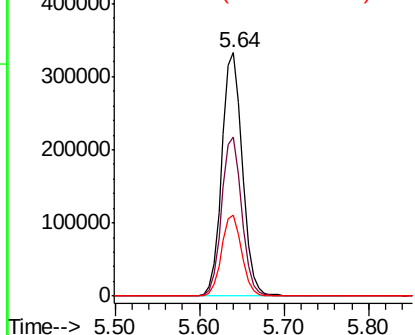

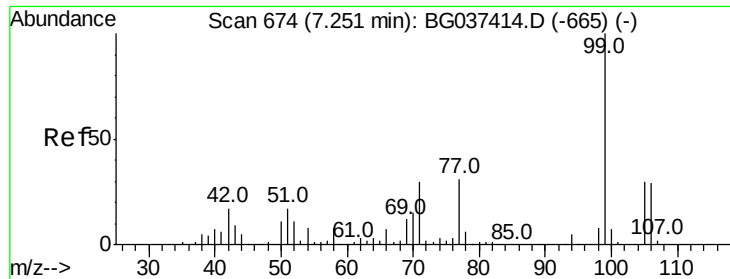

#7

Phenol-d6

Concen: 138.246 ng

RT: 7.24 min Scan# 673

Delta R.T. -0.01 min

Lab File: BG037823.D

Acq: 6 Nov 2018 4:11

Instrument :

BNA_G

ClientSampleId :

PB114495BL


Tot Ion: 99 Resp: 809257

Ion Ratio Lower Upper




99 100

42 17.8 15.0 22.4

71 31.2 25.5 38.3

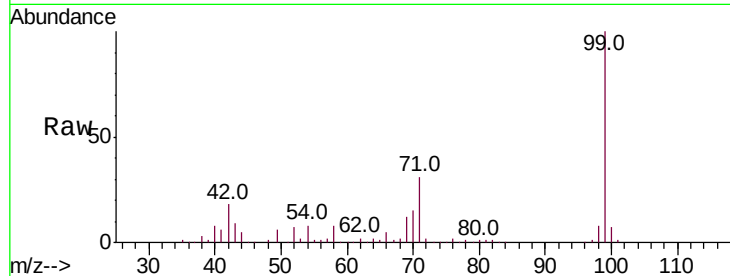

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

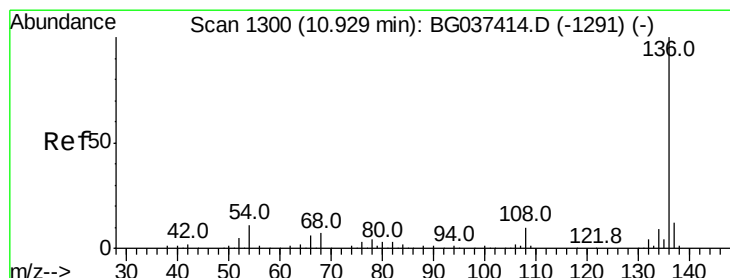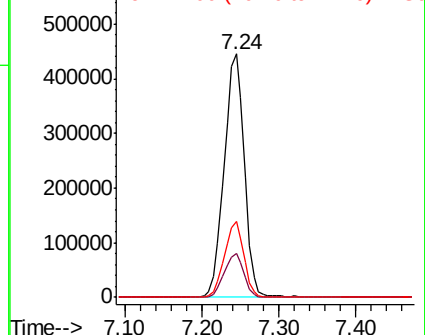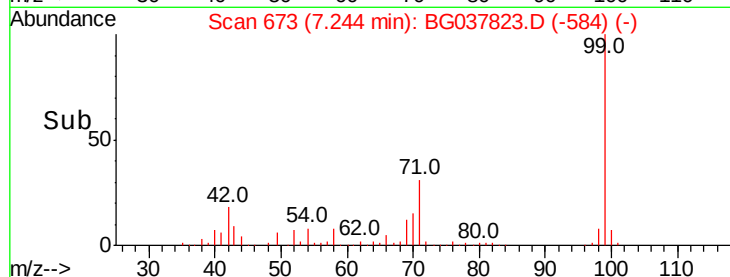

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.92 min Scan# 1298

Delta R.T. -0.01 min

Lab File: BG037823.D

Acq: 6 Nov 2018 4:11

Tgt Ion: 136 Resp: 293118


Ion Ratio Lower Upper

136 100



137 11.6 9.6 14.4


54 9.8 7.9 11.9

68 6.3 4.8 7.2

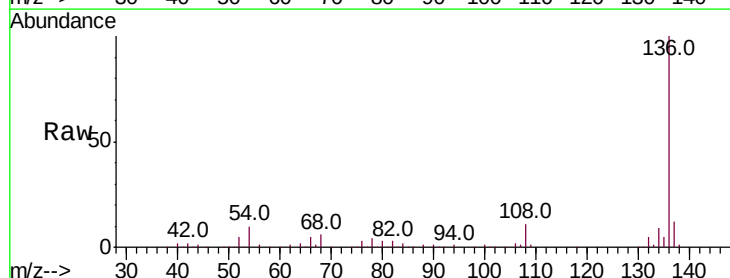

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



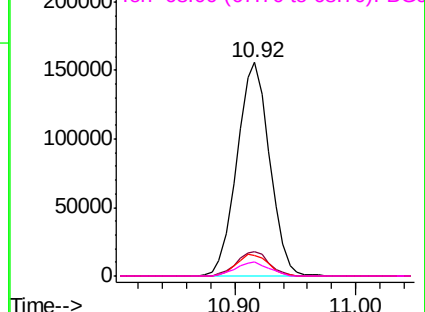
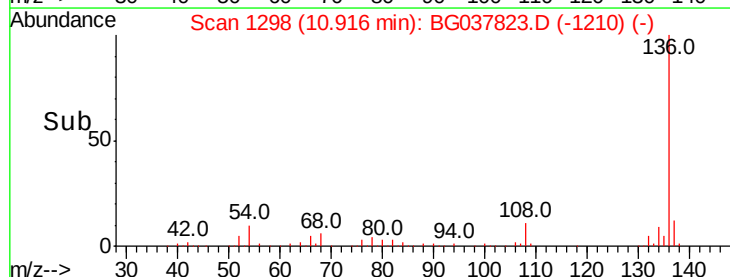


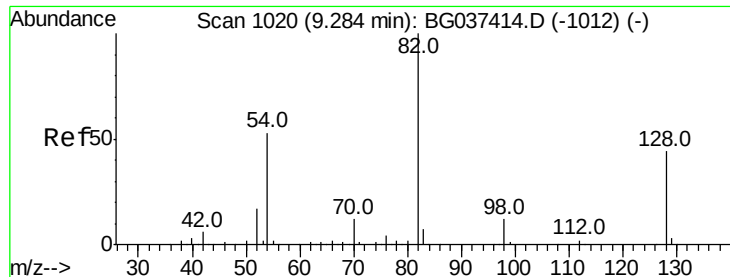

#23
Nitrobenzene-d5
Concen: 92.394 ng
RT: 9.27 min Scan# 1018
Delta R.T. -0.01 min
Lab File: BG037823.D
Acq: 6 Nov 2018 4:11




Instrument :
BNA_G
ClientSampleId :
PB114495BL


Tot Ion	Ratio	Lower	Upper
82	100		
128	46.0	34.6	51.8
54	53.7	45.3	67.9

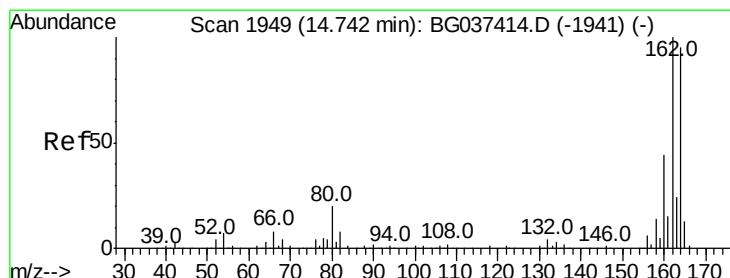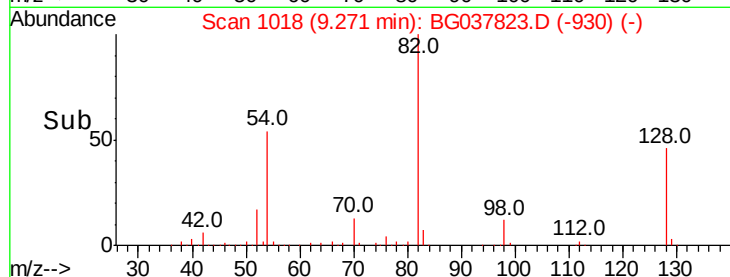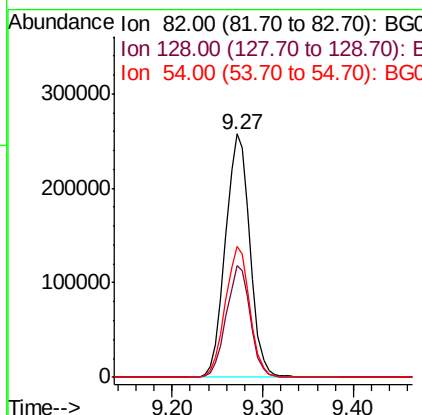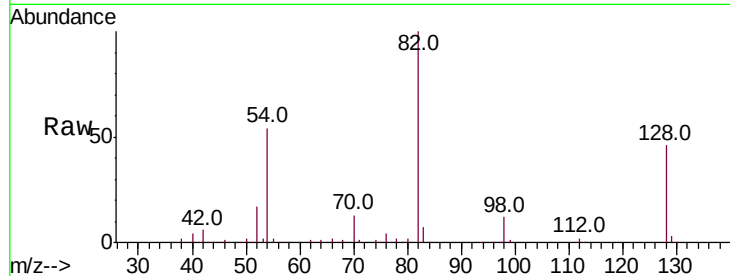

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.73 min Scan# 1947
Delta R.T. -0.01 min
Lab File: BG037823.D
Acq: 6 Nov 2018 4:11

Tgt Ion	Ratio	Lower	Upper
164	100		
162	107.1	81.3	121.9
160	45.6	36.3	54.5

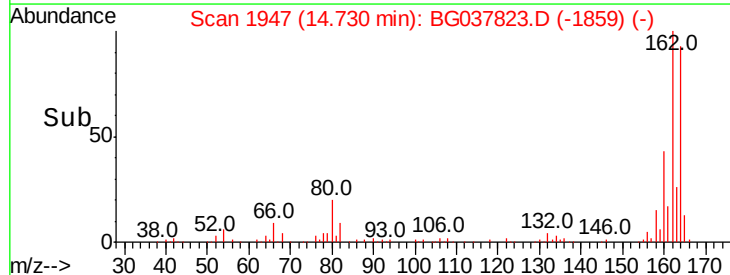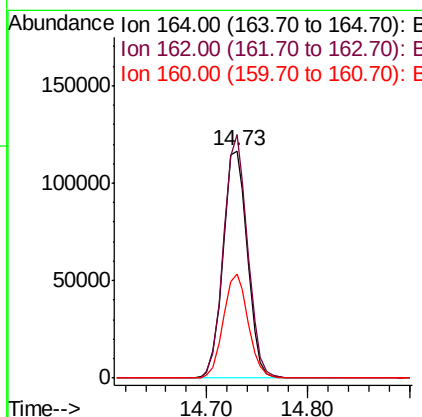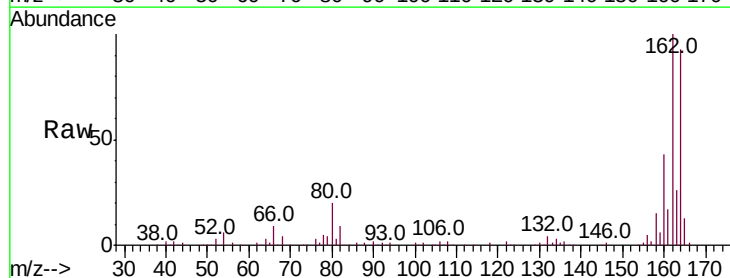


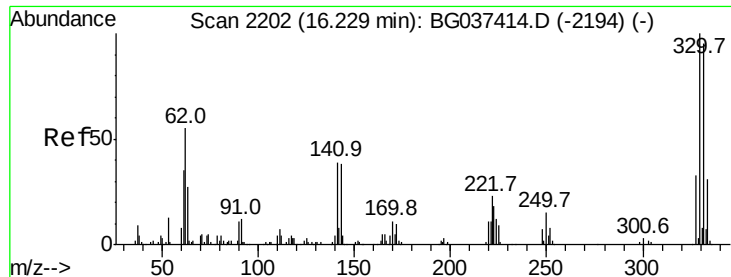




#42
 2,4,6-Tribromophenol
 Concen: 124.355 ng
 RT: 16.22 min Scan# 2200
 Delta R.T. -0.01 min
 Lab File: BG037823.D
 Acq: 6 Nov 2018 4:11

Instrument :
 BNA_G
 ClientSampleId :
 PB114495BL

Tot Ion:330 Resp: 263209
 Ion Ratio Lower Upper
 330 100
 332 94.4 78.4 117.6
 141 38.0 32.2 48.2

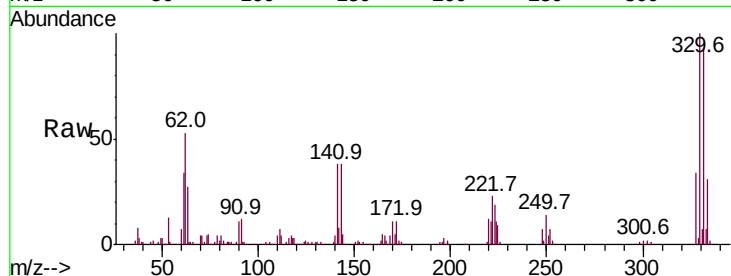


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

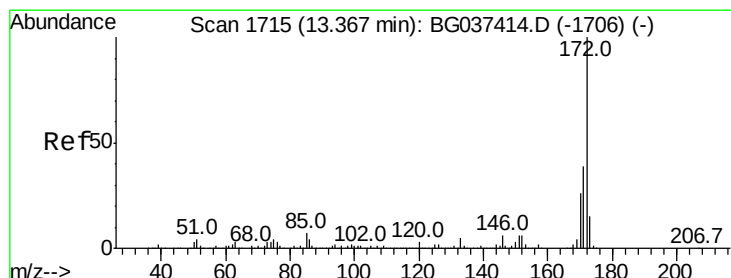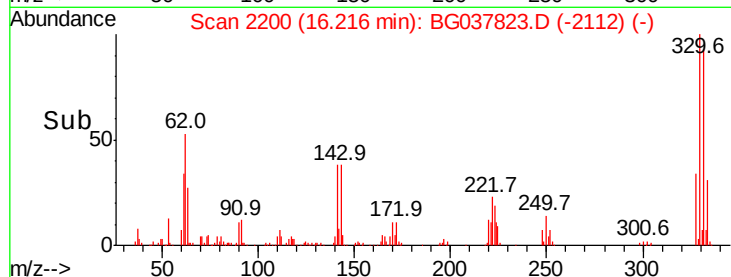
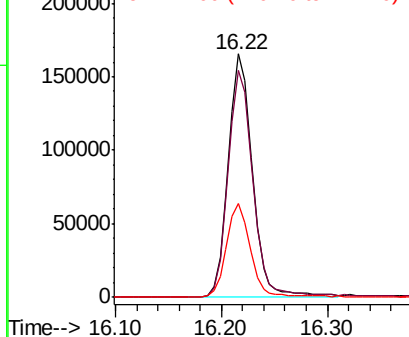



#45
 2-Fluorobiphenyl
 Concen: 92.796 ng
 RT: 13.35 min Scan# 1712
 Delta R.T. -0.02 min
 Lab File: BG037823.D
 Acq: 6 Nov 2018 4:11

Tgt Ion:172 Resp: 1194202
 Ion Ratio Lower Upper
 172 100
 171 39.0 31.0 46.4
 170 25.5 20.2 30.2

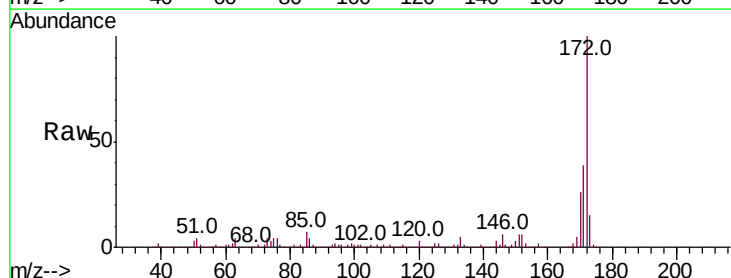

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

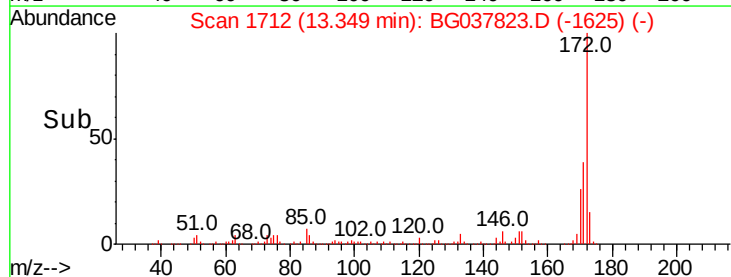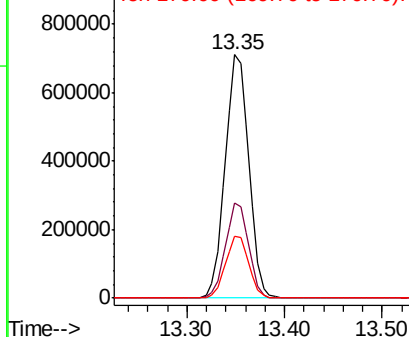

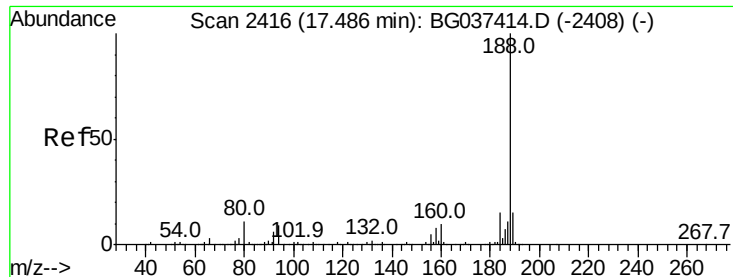

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.47 min Scan# 2414

Delta R.T. -0.01 min

Lab File: BG037823.D

Acq: 6 Nov 2018 4:11

Instrument :

BNA_G

ClientSampleId :

PB114495BL


Tot Ion:188 Resp: 426239

Ion Ratio Lower Upper

188 100

94 9.8 7.2 10.8




80 10.0 7.7 11.5

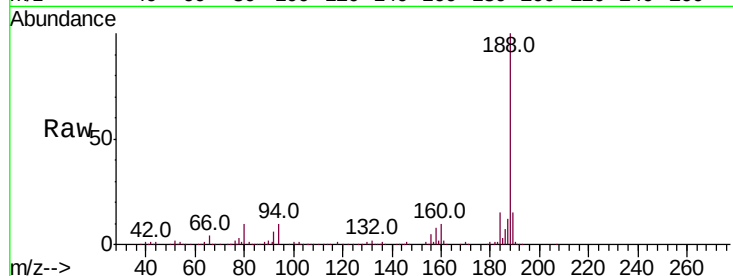

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

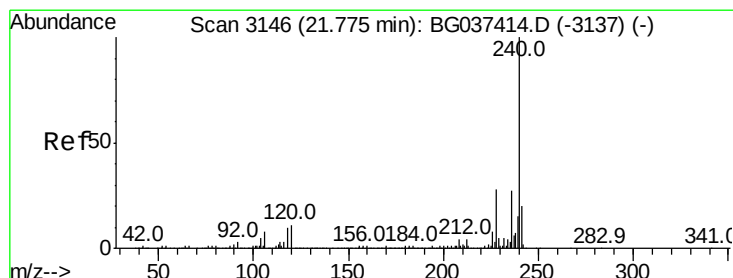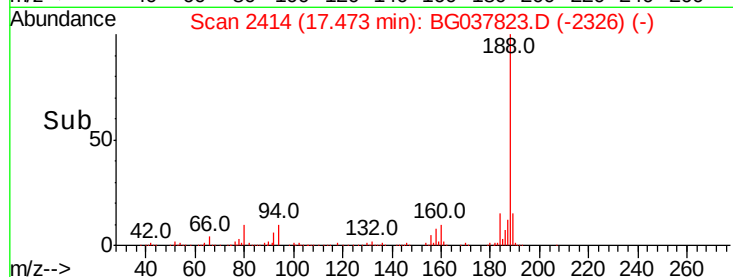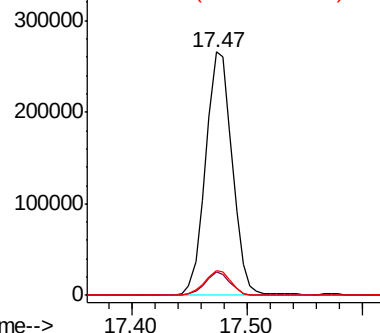

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.76 min Scan# 3143

Delta R.T. -0.02 min

Lab File: BG037823.D

Acq: 6 Nov 2018 4:11


Tgt Ion:240 Resp: 382774

Ion Ratio Lower Upper

240 100

120 11.0 8.1 12.1



236 26.9 21.4 32.0

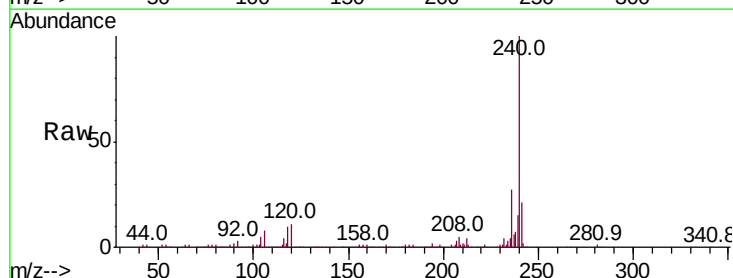


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

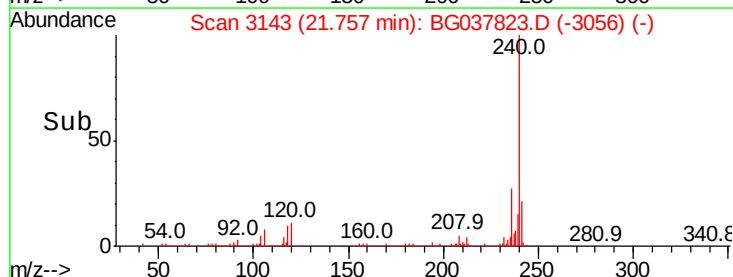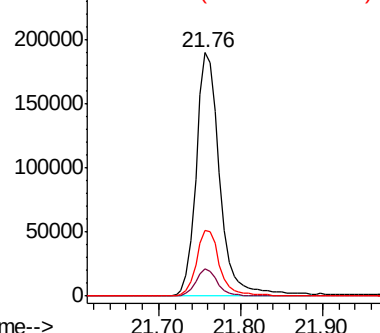

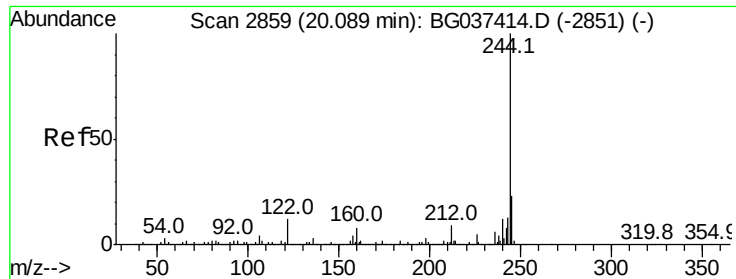

#79

Terphenyl-d14

Concen: 92.797 ng

RT: 20.08 min Scan# 2857

Delta R.T. -0.01 min

Lab File: BG037823.D

Acq: 6 Nov 2018 4:11

Instrument :


BNA_G

ClientSampleId :

PB114495BL

Tot Ion:244 Resp: 1662346




Ion	Ratio	Lower	Upper
244	100		
212	8.8	6.5	9.7
122	11.6	9.0	13.4

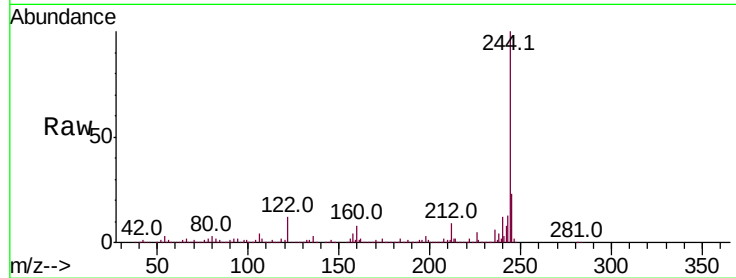

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

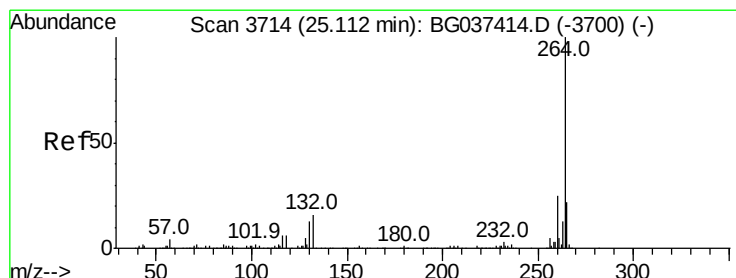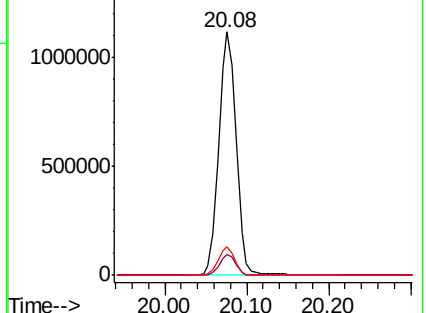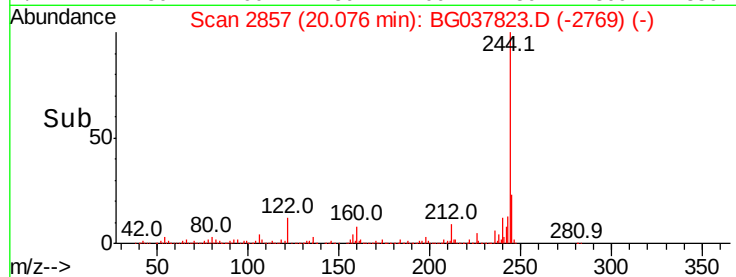

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.09 min Scan# 3710


Delta R.T. -0.02 min

Lab File: BG037823.D

Acq: 6 Nov 2018 4:11

Tgt Ion:264 Resp: 337025

Ion	Ratio	Lower	Upper
264	100		
260	22.9	18.2	27.4
265	19.8	17.9	26.9

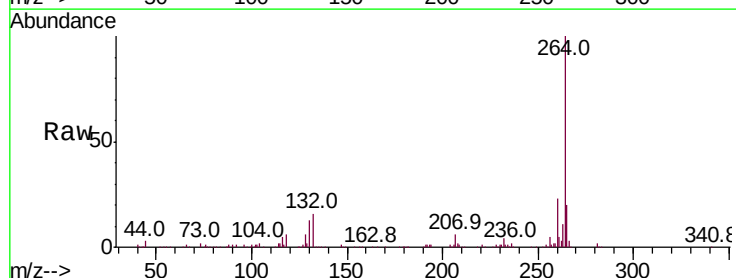

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

